

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
 Data File : PD068463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2022 17:19
 Operator : AR\AJ
 Sample : N1847-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CG-B1-030722-0-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/11/2022
 Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 22:49:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.175	12369292	106.1E6	10.552m	11.056
28) SA Decachlor...	8.210	9.371	15951573	82214002	13.708	13.867

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
Data File : PD068463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2022 17:19
Operator : AR\AJ
Sample : N1847-08
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CG-B1-030722-0-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 22:49:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

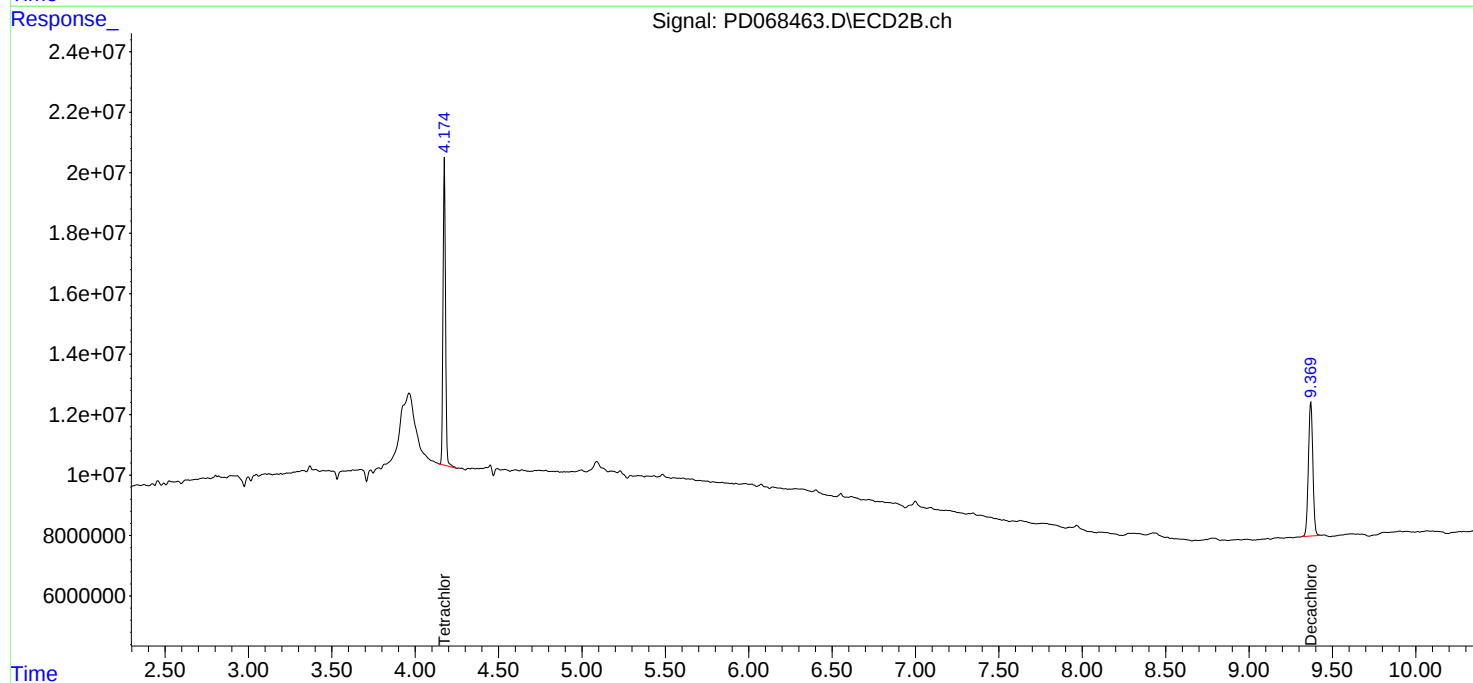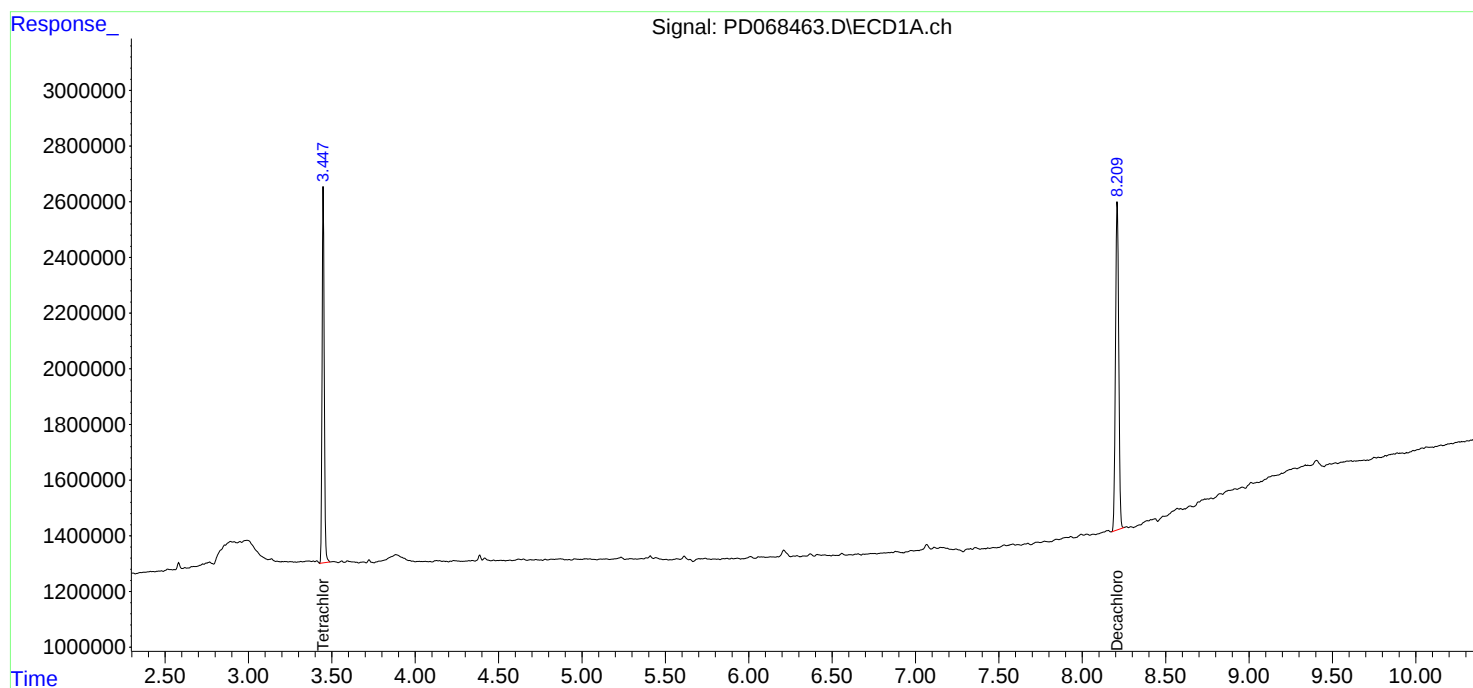

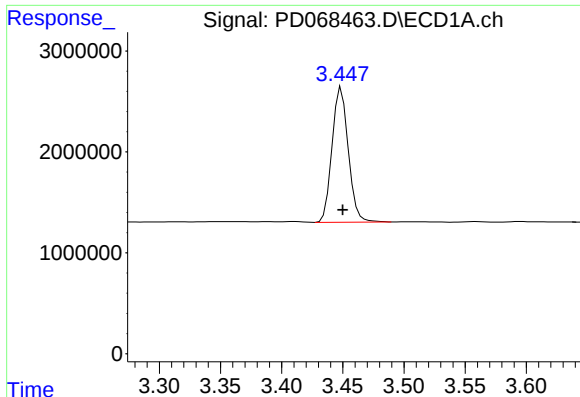


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.003 min
Response: 12369292
Conc: 10.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
CG-B1-030722-0-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

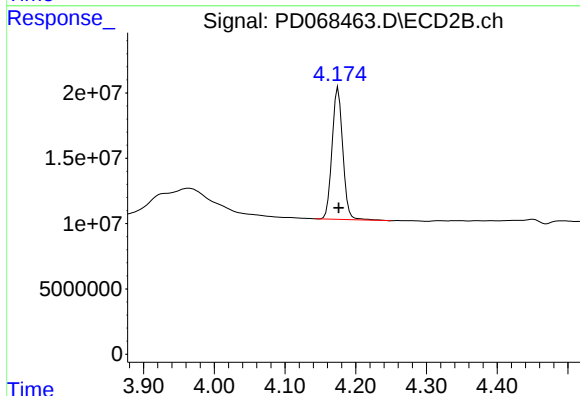


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 106112932
Conc: 11.06 ng/ml

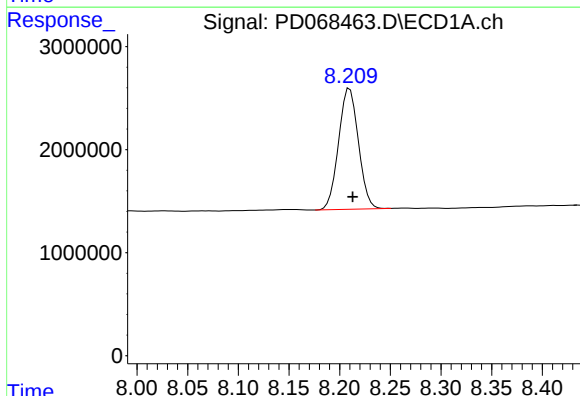

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.003 min
Response: 15951573
Conc: 13.71 ng/ml

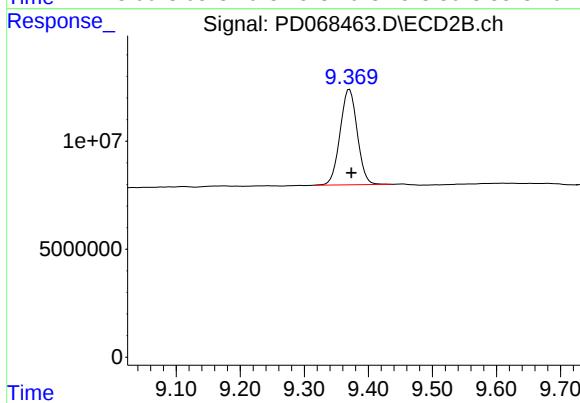

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.003 min
Response: 82214002
Conc: 13.87 ng/ml