

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
 Data File : PD068474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2022 19:52
 Operator : AR\AJ
 Sample : N1848-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CG-B2-030722-2-5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/11/2022
 Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 22:57:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.175	13248971	109.8E6	11.302m	11.441
28)	SA Decachlor...	8.210	9.371	18781233	92567844	16.139	15.613
Target Compounds							
12)	B 4,4'-DDE	5.612	6.551	3756763	30784426	2.754m	3.149

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
Data File : PD068474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2022 19:52
Operator : AR\AJ
Sample : N1848-10
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CG-B2-030722-2-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 22:57:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

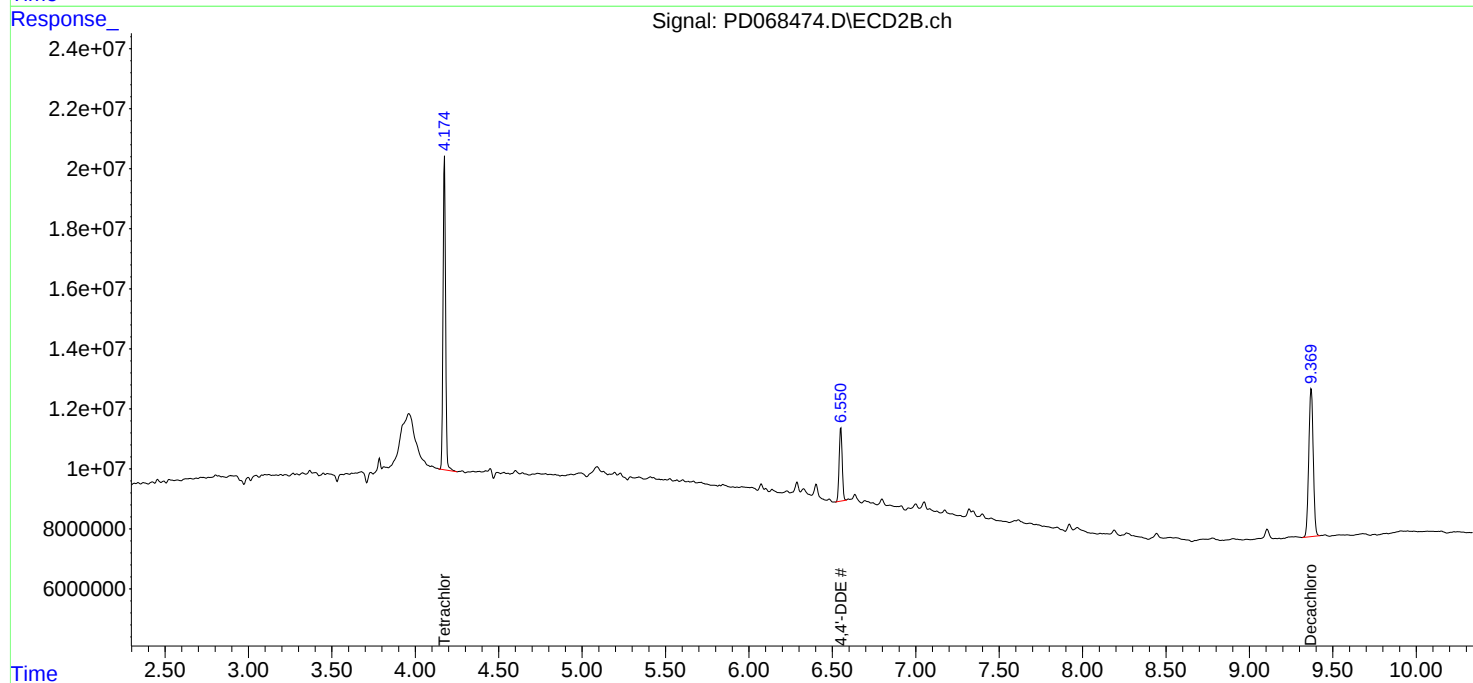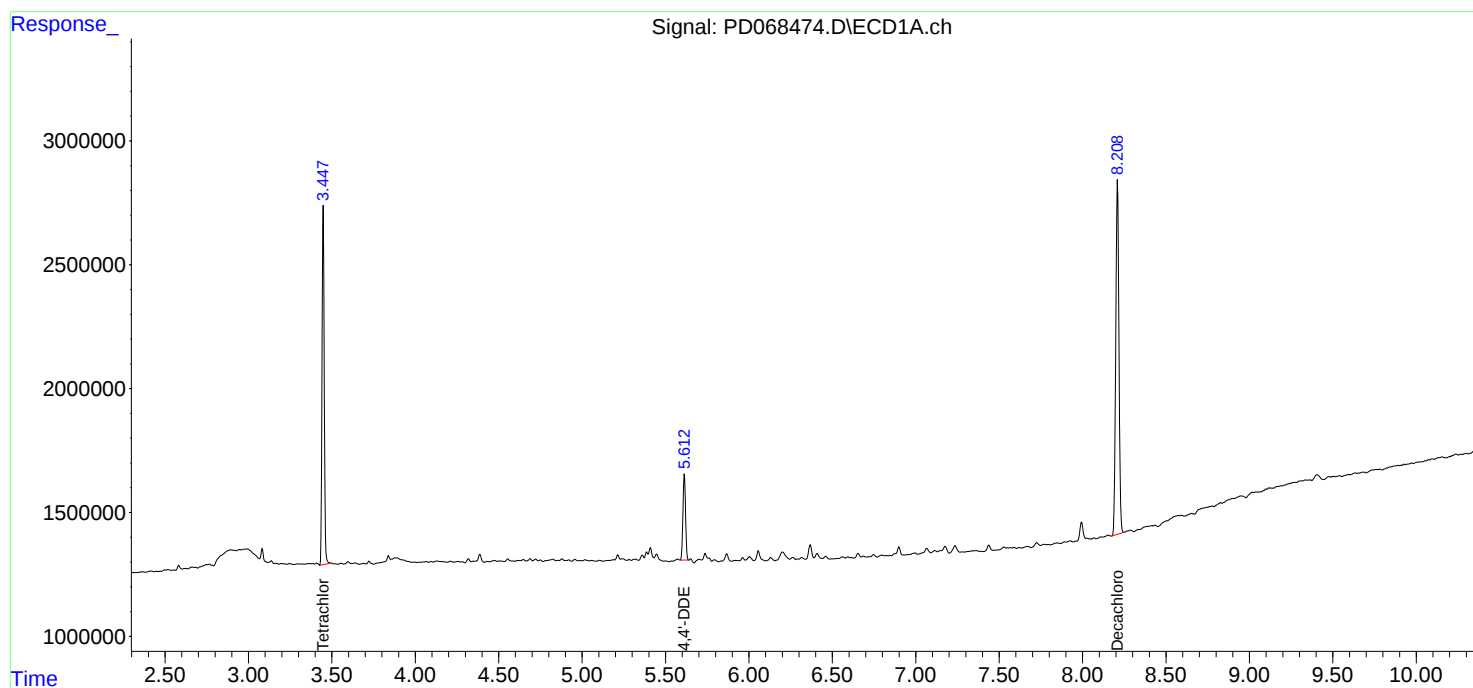

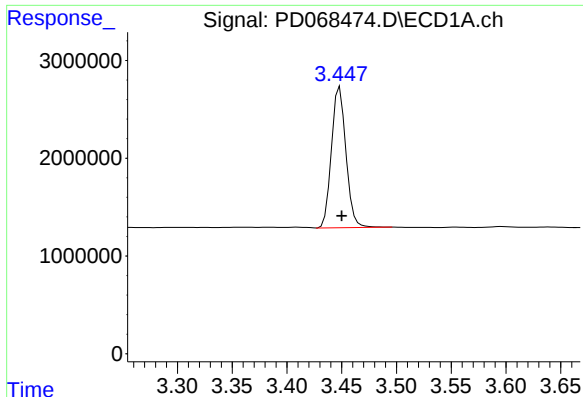


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.003 min
Response: 13248971
Conc: 11.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
CG-B2-030722-2-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

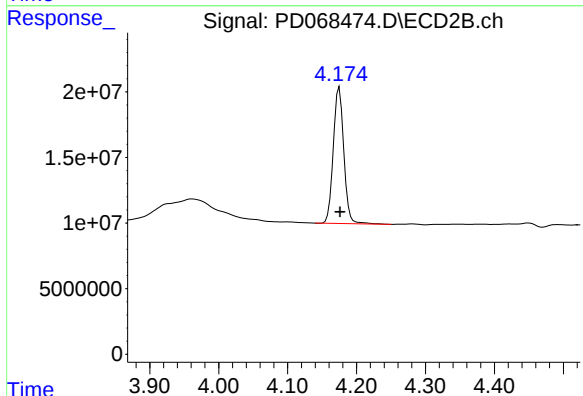


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 109812625
Conc: 11.44 ng/ml

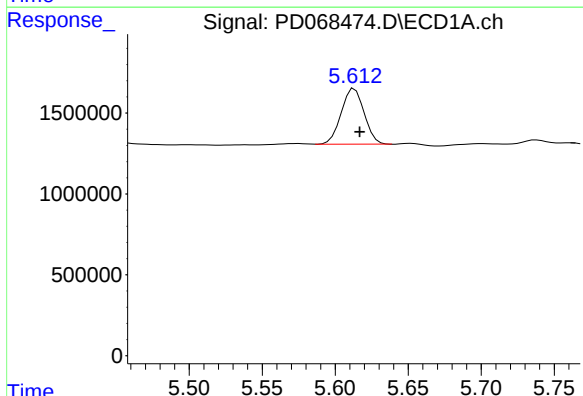


#12 4,4'-DDE

R.T.: 5.612 min
Delta R.T.: -0.005 min
Response: 3756763
Conc: 2.75 ng/ml m

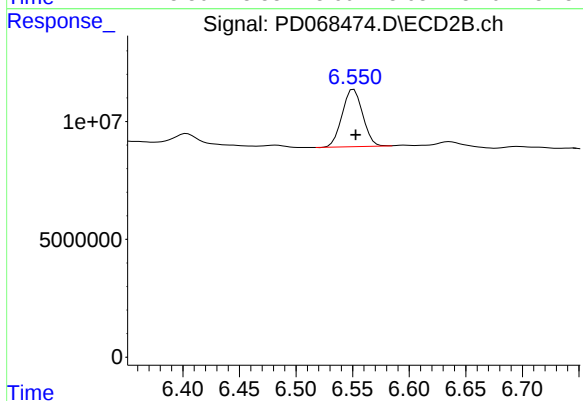

#12 4,4'-DDE

R.T.: 6.551 min
Delta R.T.: -0.002 min
Response: 30784426
Conc: 3.15 ng/ml

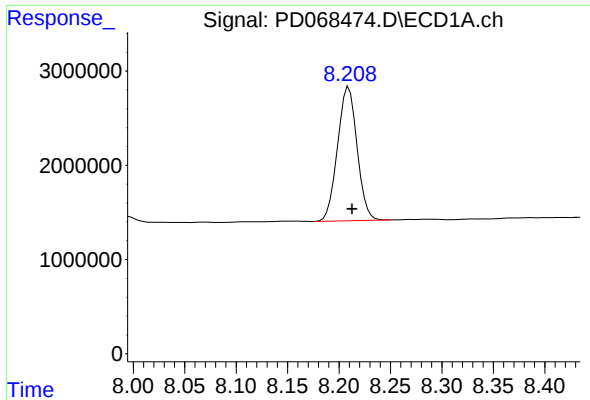


#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.003 min
Response: 18781233
Conc: 16.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
CG-B2-030722-2-5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

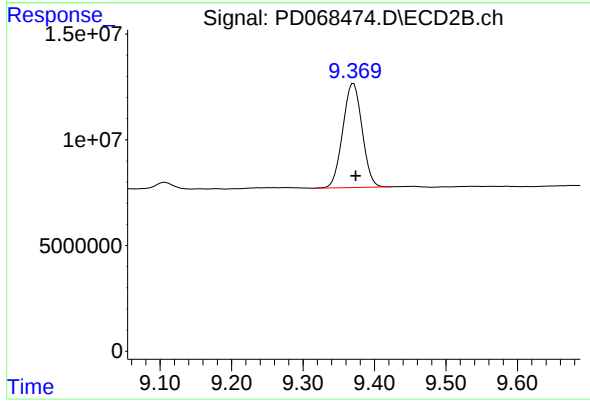

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.003 min
Response: 92567844
Conc: 15.61 ng/ml