

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
 Data File : PD051704.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 9:52
 Operator : AJ\SJ
 Sample : PB117661BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK61

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:55:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	28349371	632.4E6	19.728	20.469
27)	SA Decachlor...	7.824	9.157	48186966	614.1E6	40.068	32.393
Target Compounds							
15)	B Endosulfa...	0.000	6.977	0	18745544	N.D.	0.683


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
Data File : PD051704.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 9:52
Operator : AJ\SJ
Sample : PB117661BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:55:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

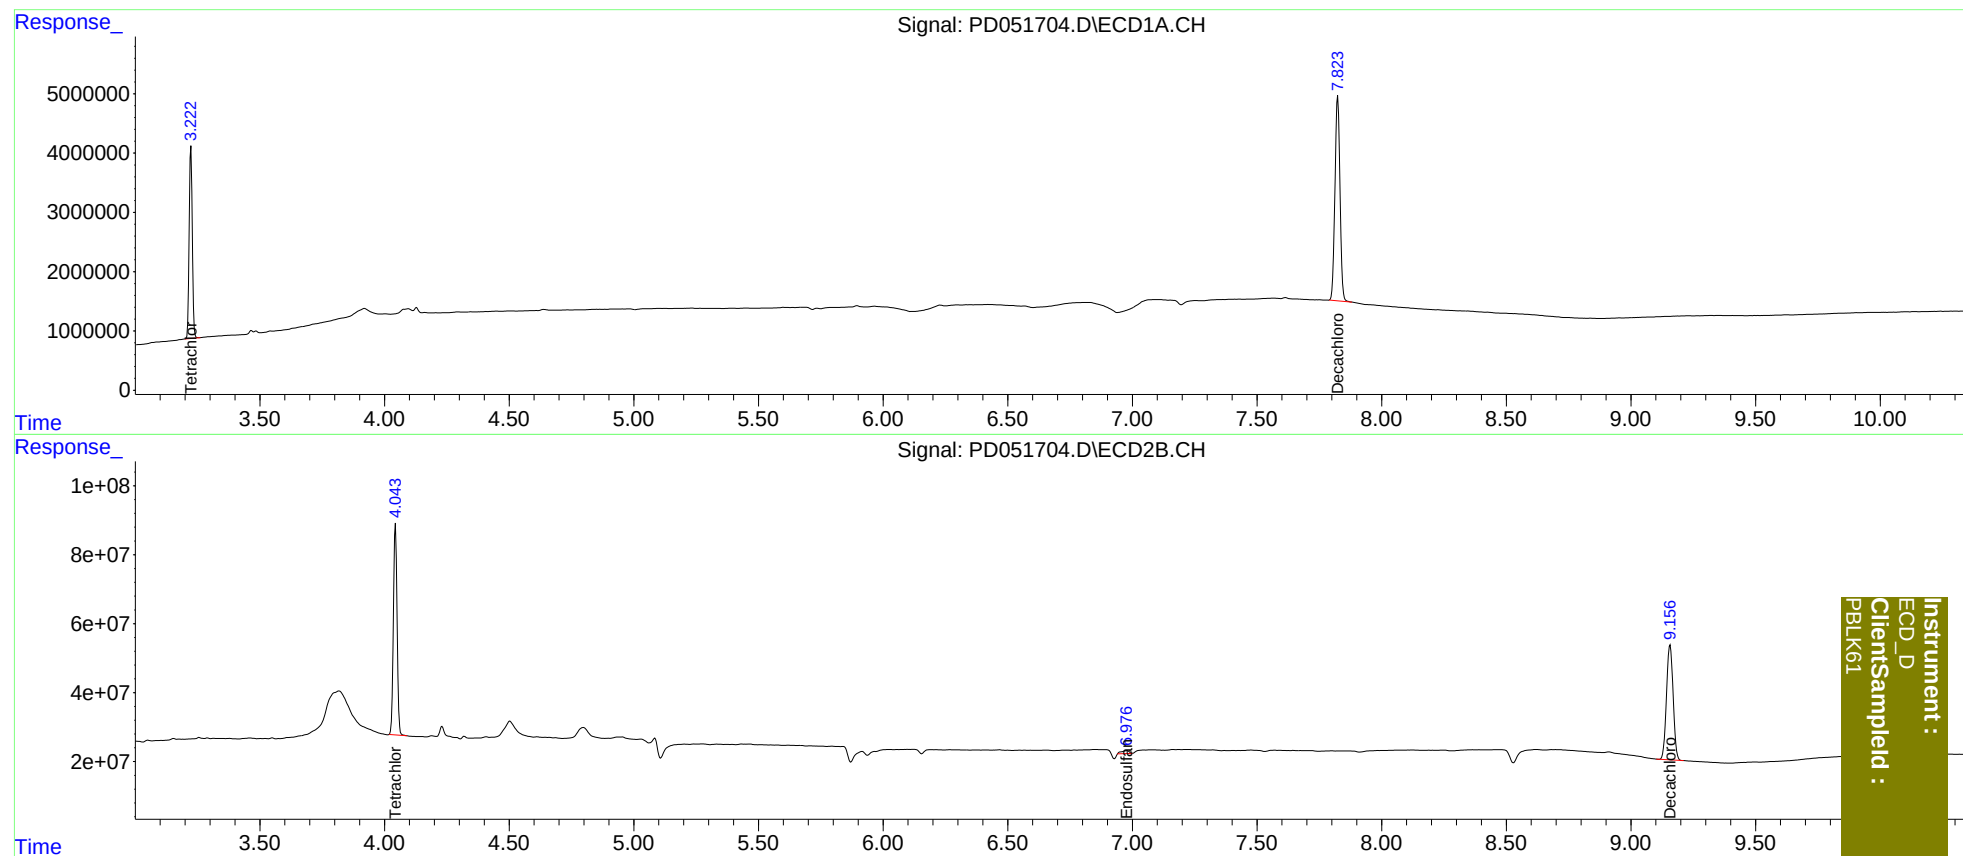


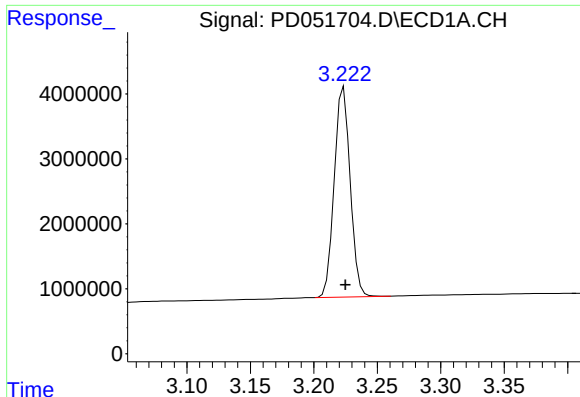

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 28349371
Conc: 19.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK61

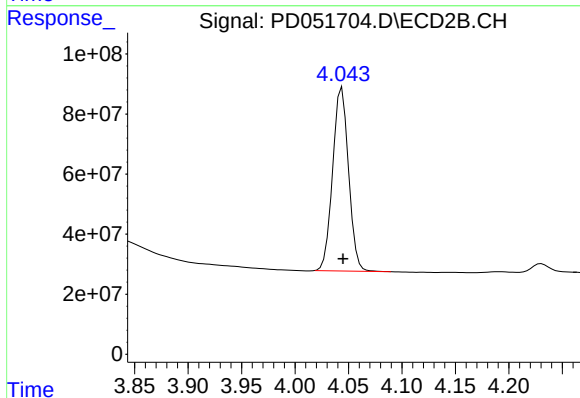


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 632410973
Conc: 20.47 ng/ml

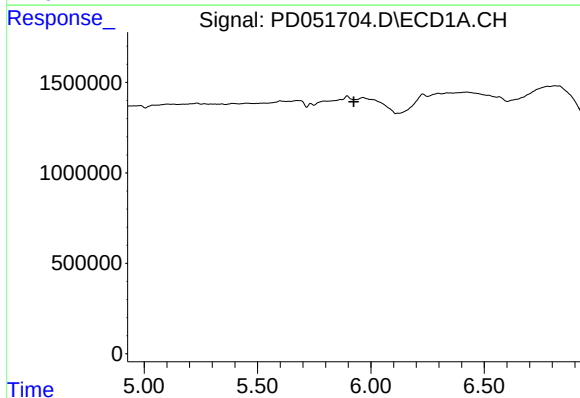


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

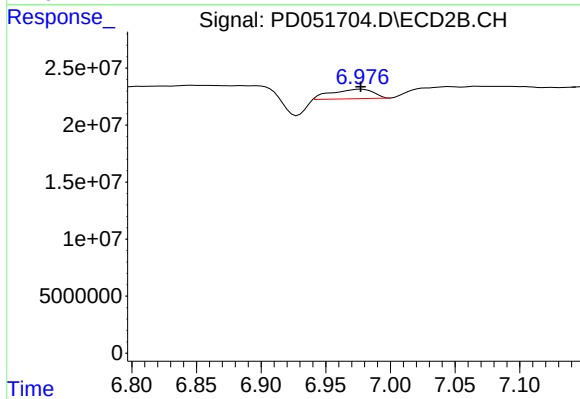

#15 Endosulfan II

R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 18745544
Conc: 0.68 ng/ml

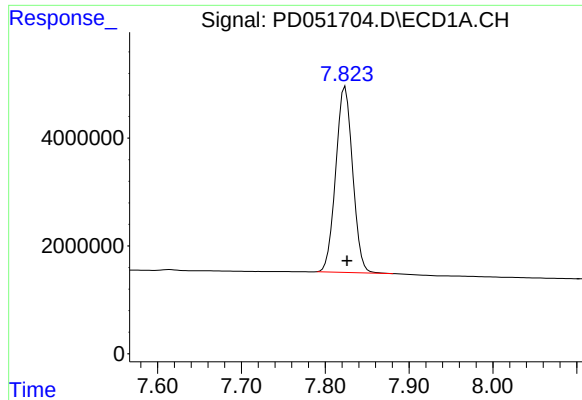

#27 Decachlorobiphenyl


R.T.: 7.824 min

Delta R.T.: -0.002 min

Response: 48186966

Conc: 40.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK61

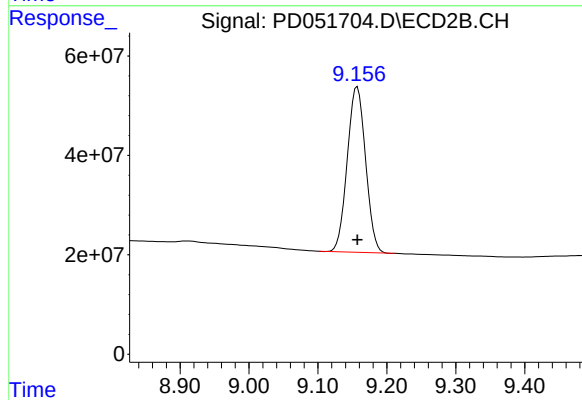

#27 Decachlorobiphenyl

R.T.: 9.157 min

Delta R.T.: 0.000 min

Response: 614087977

Conc: 32.39 ng/ml