

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
 Data File : PD051716.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 13:14
 Operator : AJ\SJ
 Sample : K1736-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF622

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:57:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	18770453	414.2E6	13.062	13.406
27)	SA Decachlor...	7.823	9.156	21144327	317.1E6	17.582	16.728
Target Compounds							
3)	MA gamma-BHC...	0.000	4.746	0 15295048	N.D.	0.358	
6)	B beta-BHC	0.000	4.942f	0 18257215	N.D.	0.920	
8)	B Heptachlo...	0.000	5.915	0 71741732	N.D.	2.004	
10)	B trans-Chl...	0.000	6.176	0 14608267	N.D.	0.404	
11)	B cis-Chlor...	0.000	6.176f	0 14608267	N.D.	0.422	
15)	B Endosulfa...	0.000	6.986	0 8983014	N.D.	0.327	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
Data File : PD051716.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 13:14
Operator : AJ\SJ
Sample : K1736-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:57:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

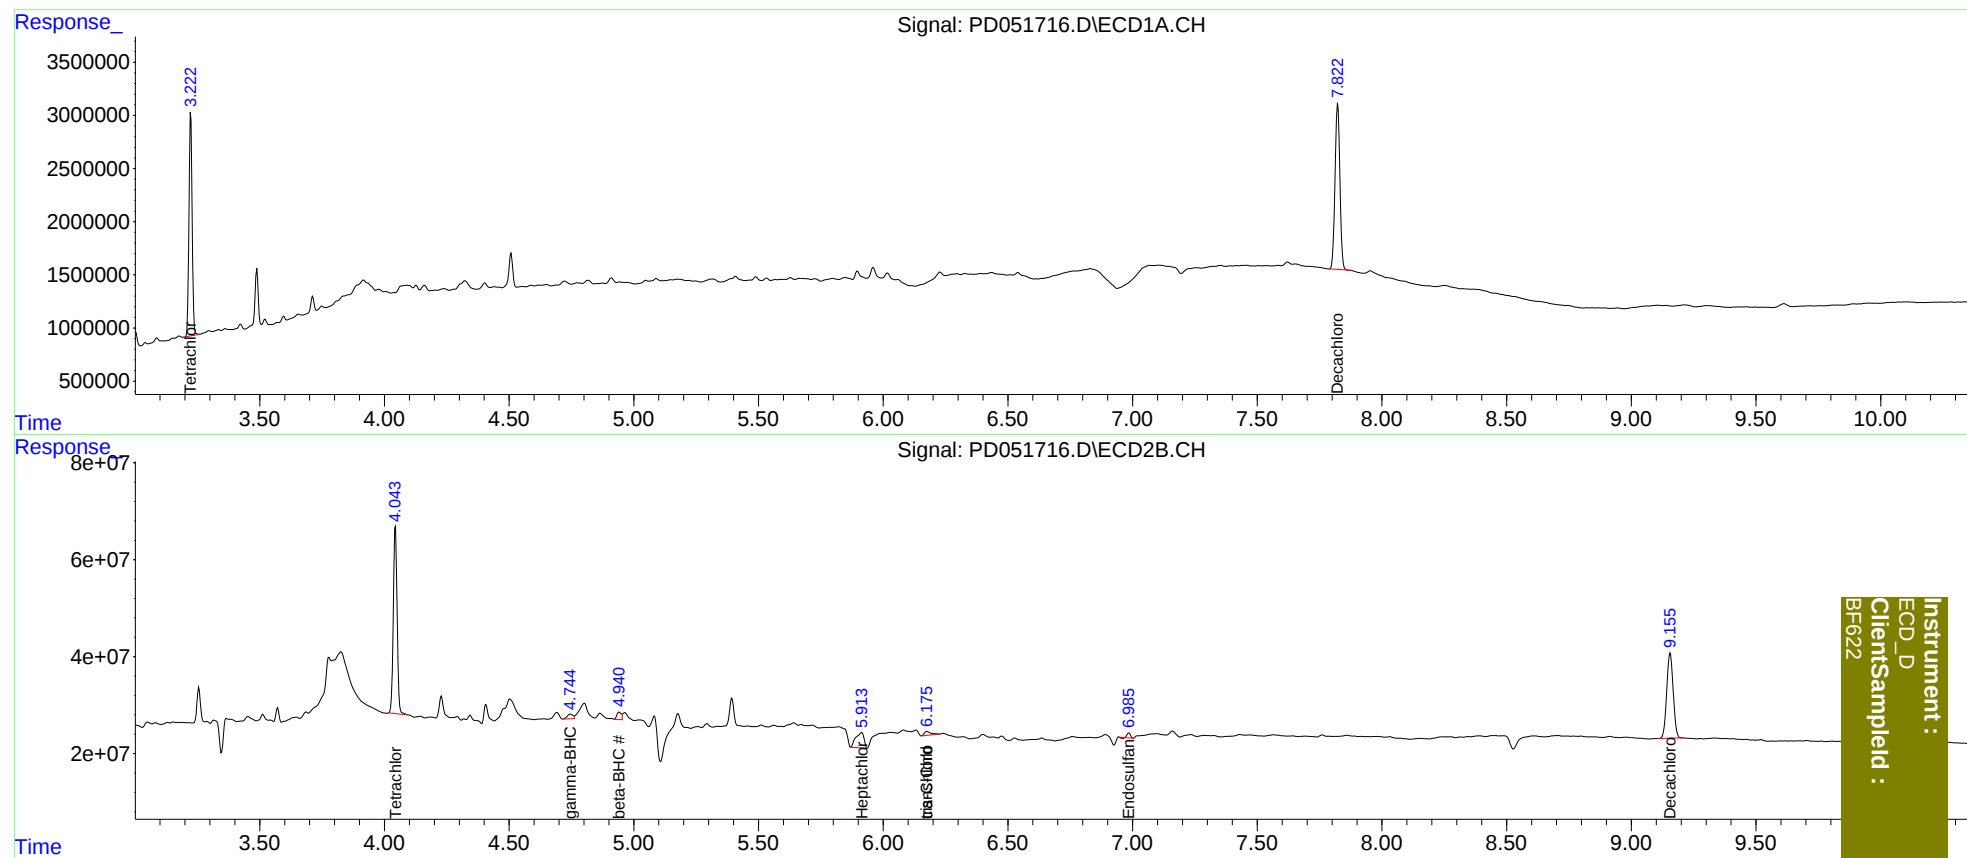


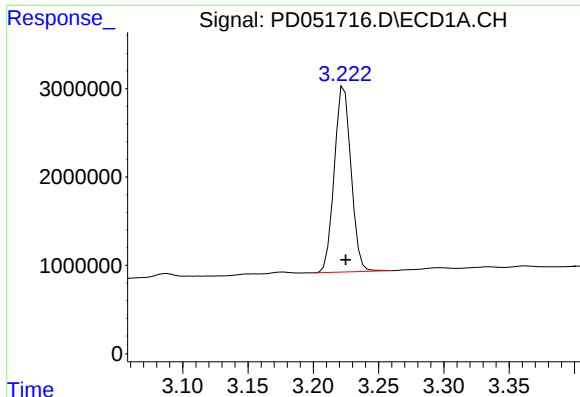

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 18770453
Conc: 13.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF622

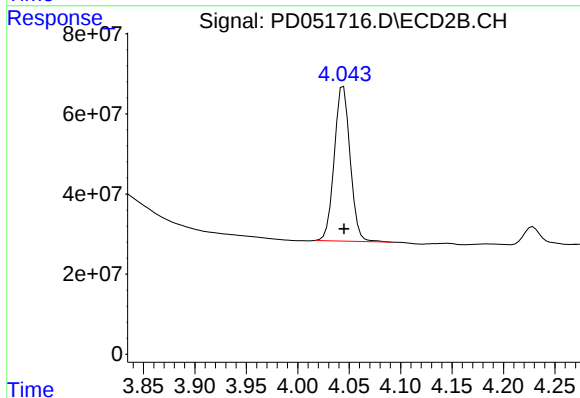


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 414203099
Conc: 13.41 ng/ml

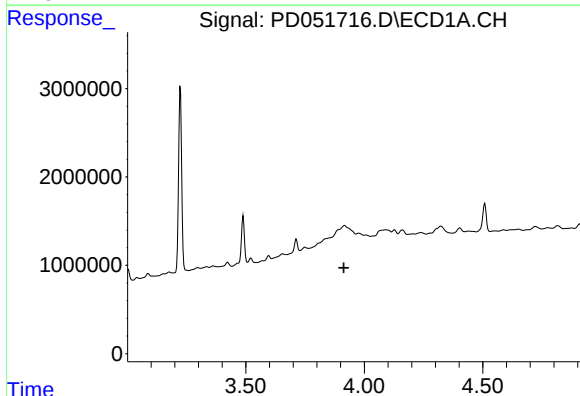


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.913 min
Response: 0
Conc: N.D.

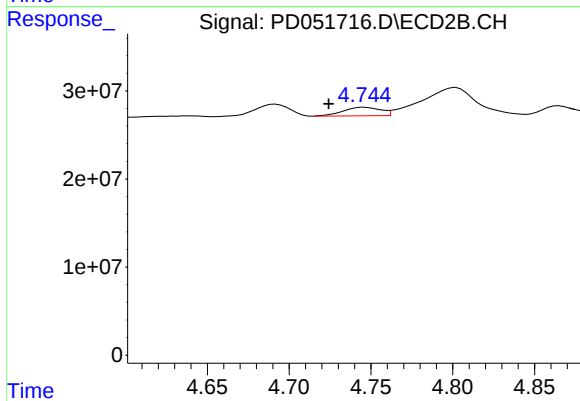

#3 gamma-BHC (Lindane)


R.T.: 4.746 min
Delta R.T.: 0.022 min
Response: 15295048
Conc: 0.36 ng/ml

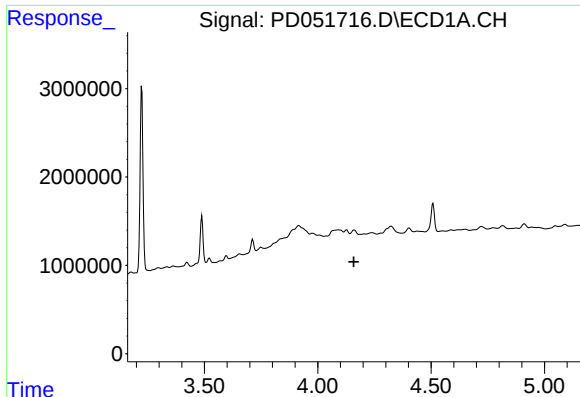

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF622

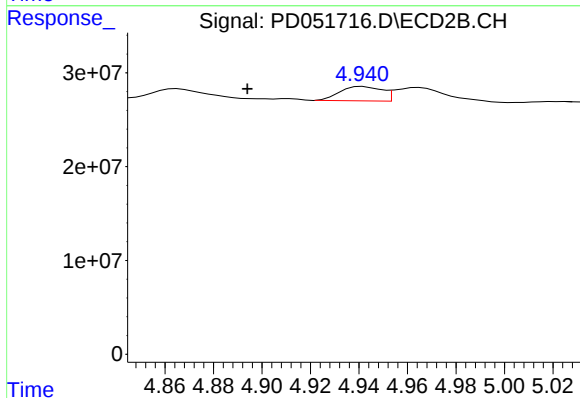


#6 beta-BHC

R.T.: 4.942 min
Delta R.T.: 0.048 min
Response: 18257215
Conc: 0.92 ng/ml

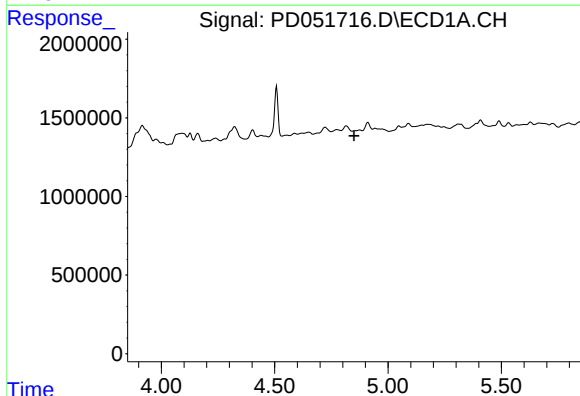


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

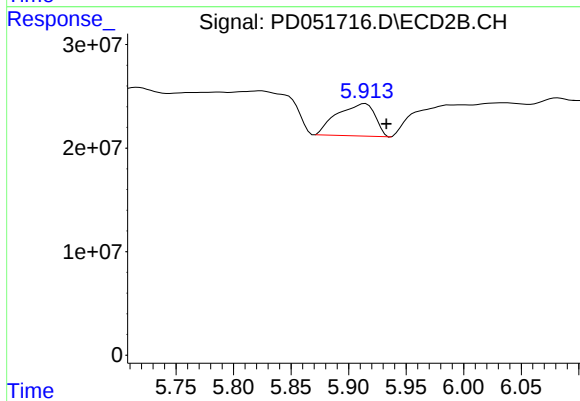

#8 Heptachlor epoxide


R.T.: 5.915 min
Delta R.T.: -0.018 min
Response: 71741732
Conc: 2.00 ng/ml

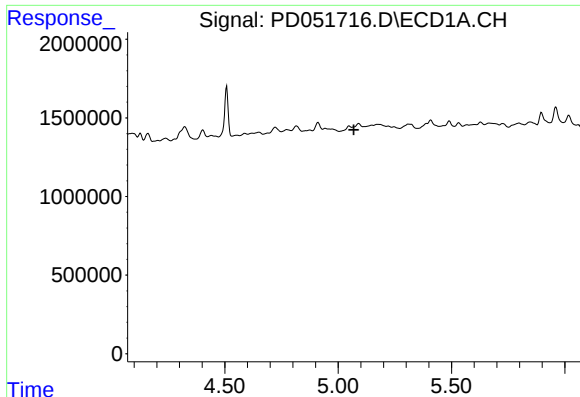

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF622

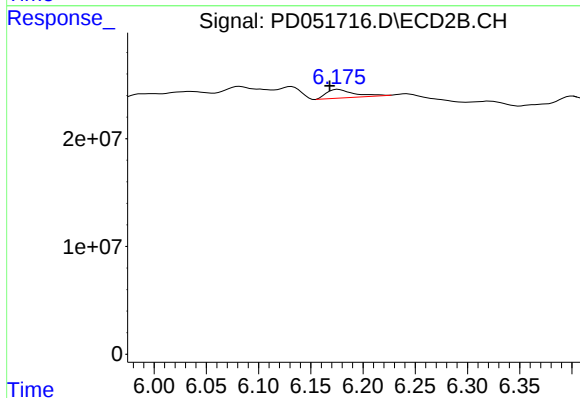


#10 trans-Chlordane

R.T.: 6.176 min
Delta R.T.: 0.008 min
Response: 14608267
Conc: 0.40 ng/ml

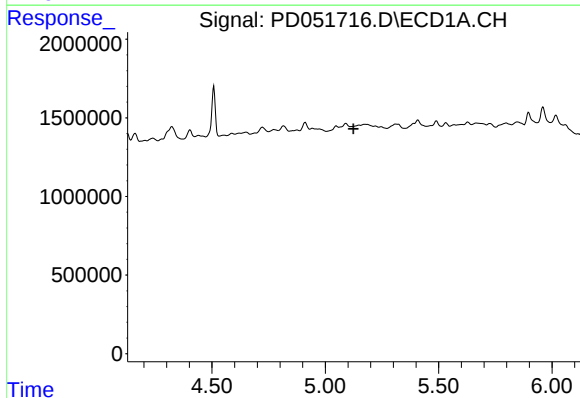


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

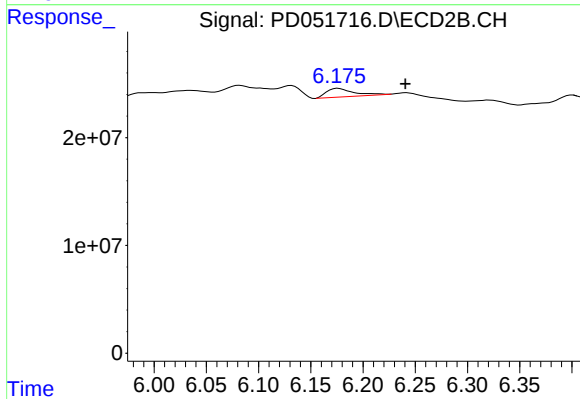

#11 cis-Chlordane


R.T.: 6.176 min
Delta R.T.: -0.064 min
Response: 14608267
Conc: 0.42 ng/ml

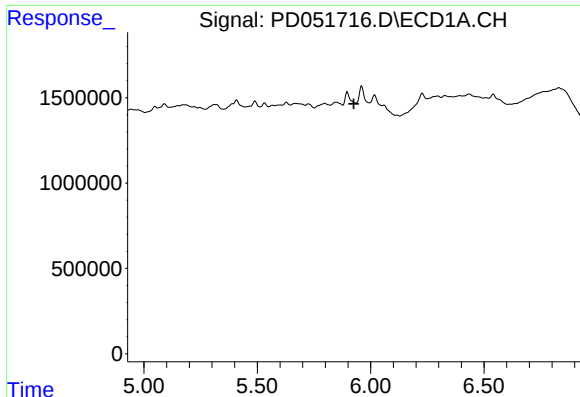

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF622

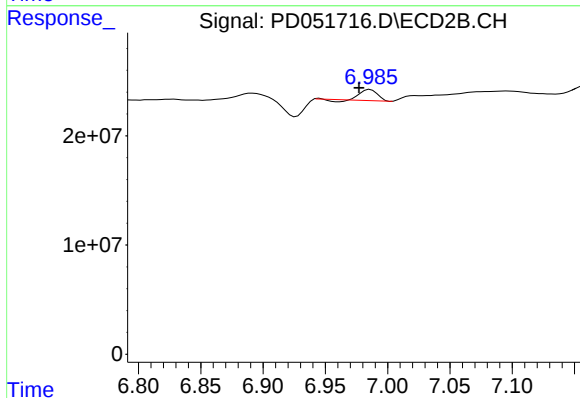


#15 Endosulfan II

R.T.: 6.986 min
Delta R.T.: 0.009 min
Response: 8983014
Conc: 0.33 ng/ml

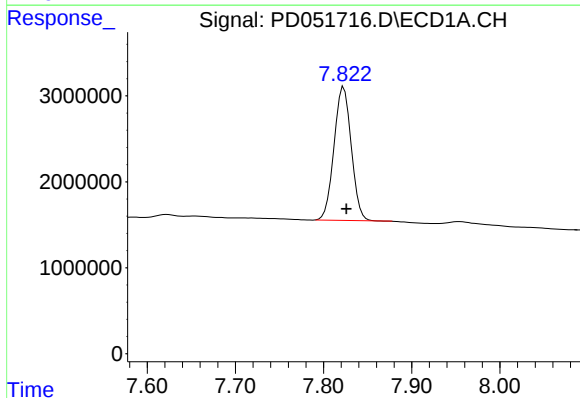

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 21144327
Conc: 17.58 ng/ml

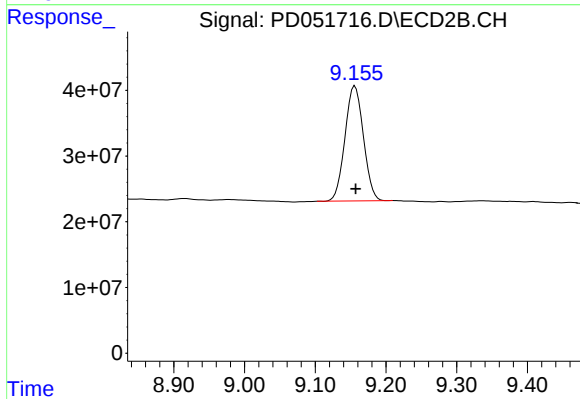

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 317127875
Conc: 16.73 ng/ml