

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
 Data File : PD051720.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 14:10
 Operator : AJ\SJ
 Sample : K1736-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:58:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	15311737	333.6E6	10.655	10.796
27)	SA Decachlor...	7.824	9.158	15586382	233.1E6	12.960	12.298
Target Compounds							
3)	MA gamma-BHC...	0.000	4.695f	0 11332628	N.D.	0.265	
6)	B beta-BHC	0.000	4.939f	0 26054956	N.D.	1.313	
7)	B delta-BHC	0.000	5.083f	0 3822386	N.D.	<MDL	
8)	B Heptachlo...	0.000	5.916	0 57088291	N.D.	1.594	
10)	B trans-Chl...	0.000	6.176	0 23399954	N.D.	0.648	
11)	B cis-Chlor...	0.000	6.176f	0 23399954	N.D.	0.676	
15)	B Endosulfa...	0.000	6.987	0 24964530	N.D.	0.909	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
Data File : PD051720.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 14:10
Operator : AJ\SJ
Sample : K1736-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:58:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

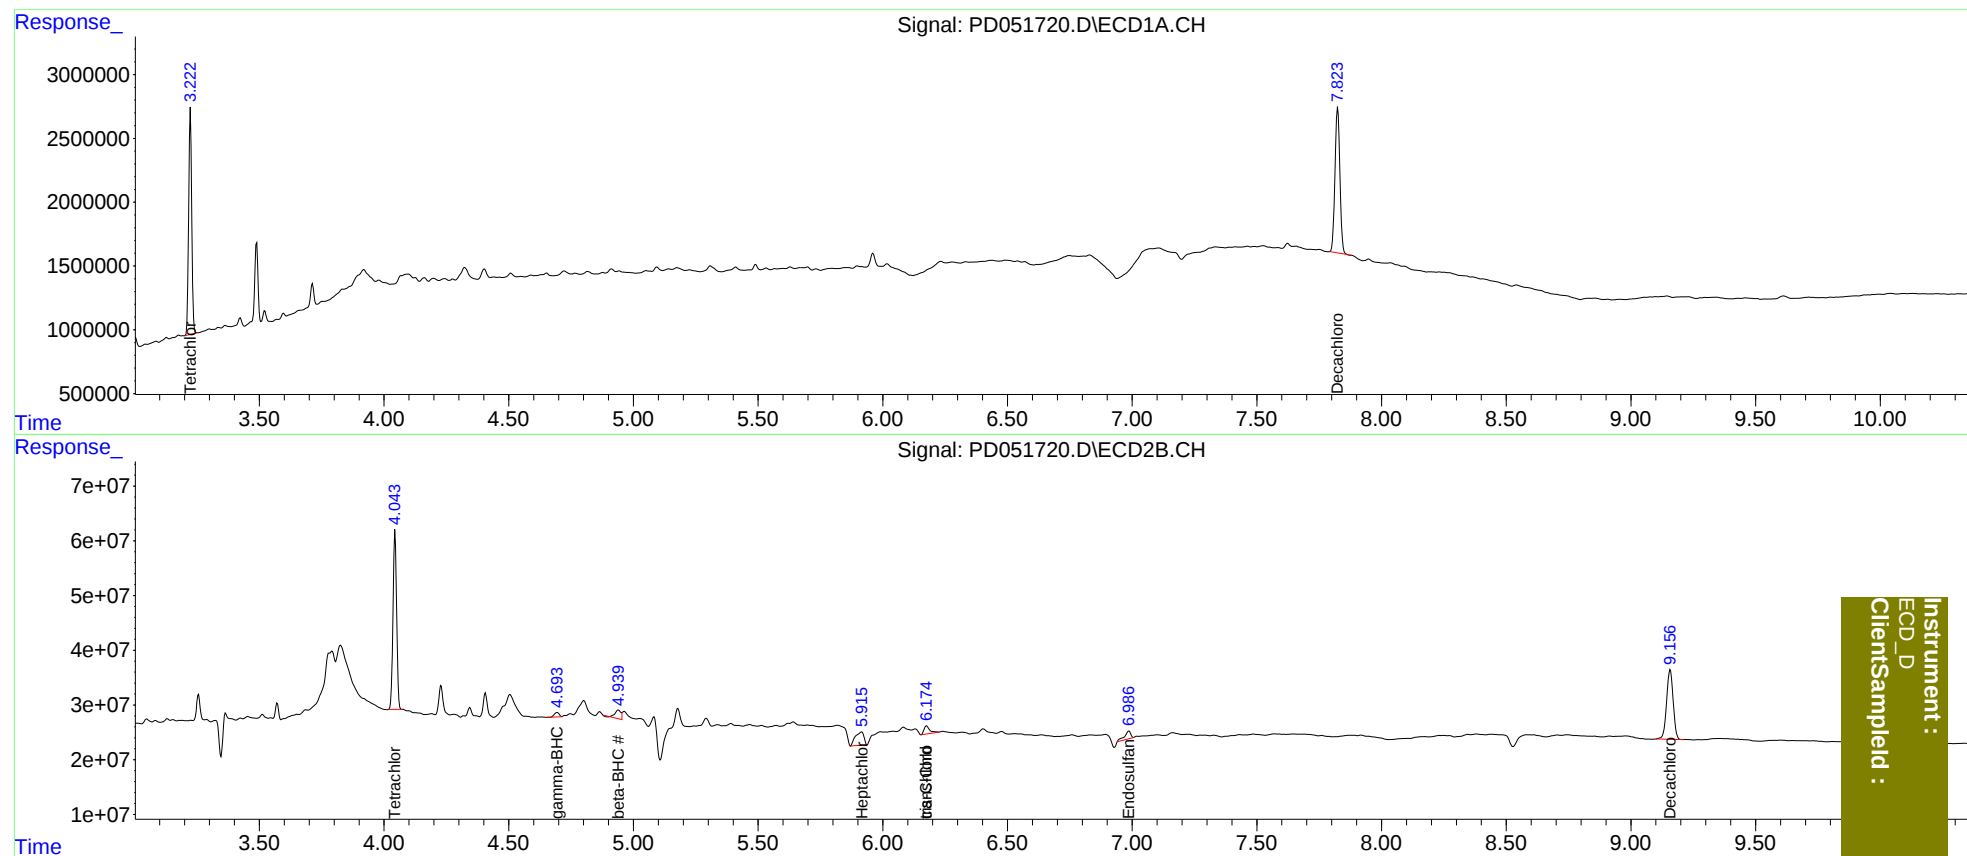


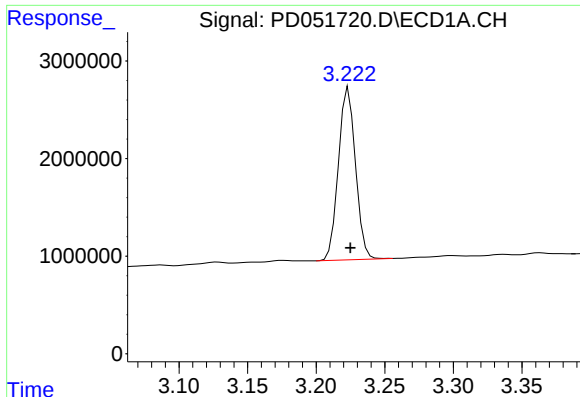

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 15311737
Conc: 10.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

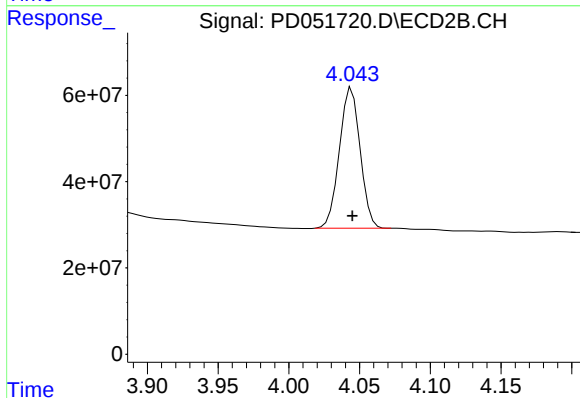


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 333556315
Conc: 10.80 ng/ml

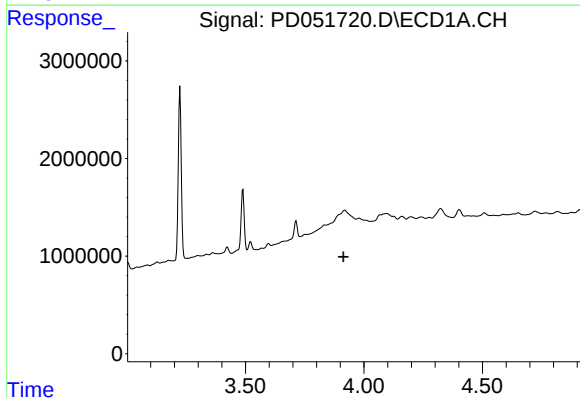


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.913 min
Response: 0
Conc: N.D.

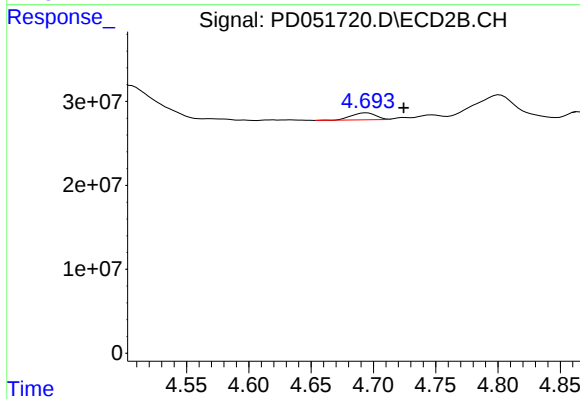

#3 gamma-BHC (Lindane)


R.T.: 4.695 min
Delta R.T.: -0.029 min
Response: 11332628
Conc: 0.27 ng/ml

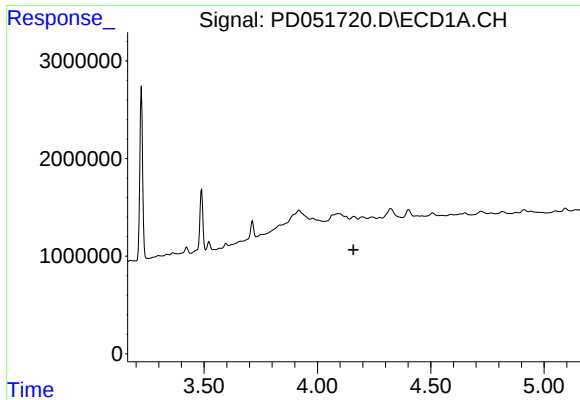

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

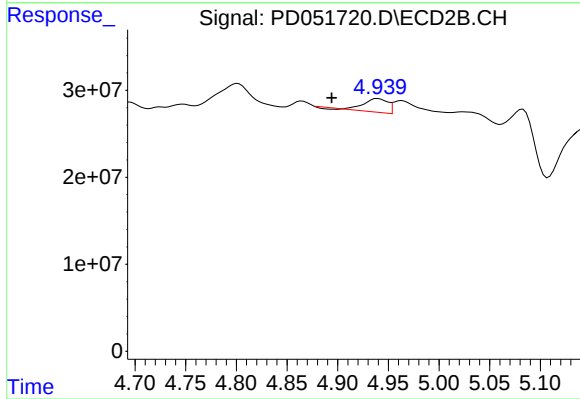


#6 beta-BHC

R.T.: 4.939 min
Delta R.T.: 0.046 min
Response: 26054956
Conc: 1.31 ng/ml

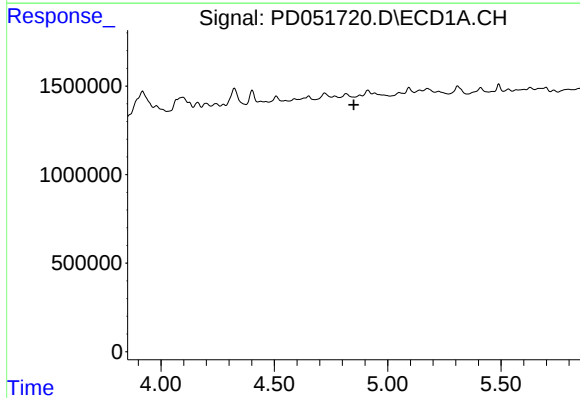


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

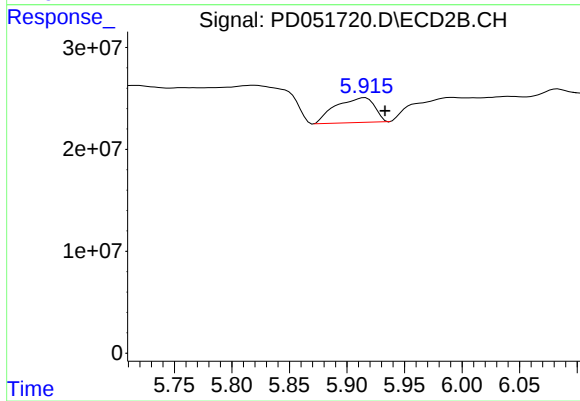

#8 Heptachlor epoxide


R.T.: 5.916 min
Delta R.T.: -0.017 min
Response: 57088291
Conc: 1.59 ng/ml

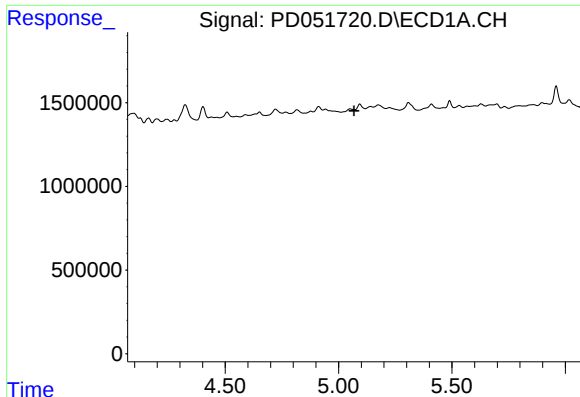

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

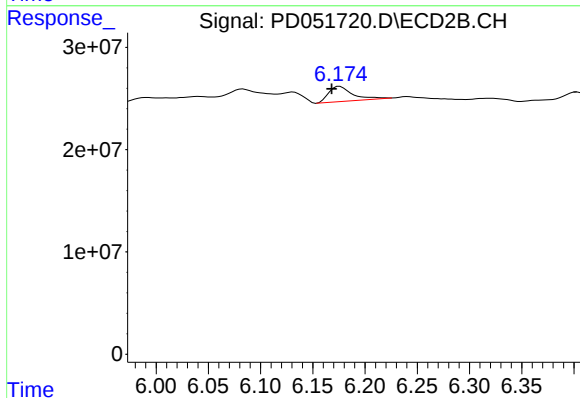


#10 trans-Chlordane

R.T.: 6.176 min
Delta R.T.: 0.008 min
Response: 23399954
Conc: 0.65 ng/ml

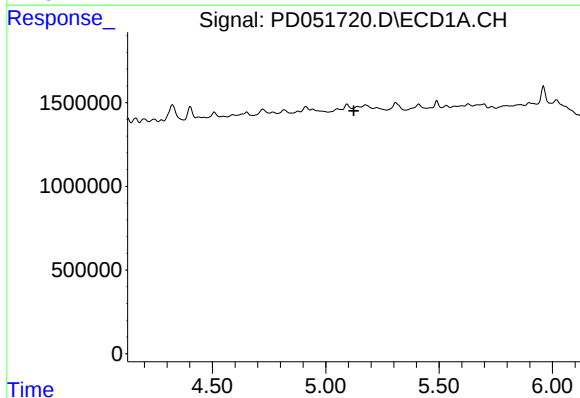


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

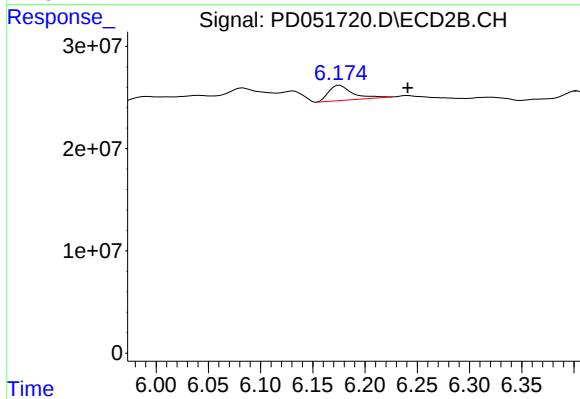

#11 cis-Chlordane


R.T.: 6.176 min
Delta R.T.: -0.065 min
Response: 23399954
Conc: 0.68 ng/ml

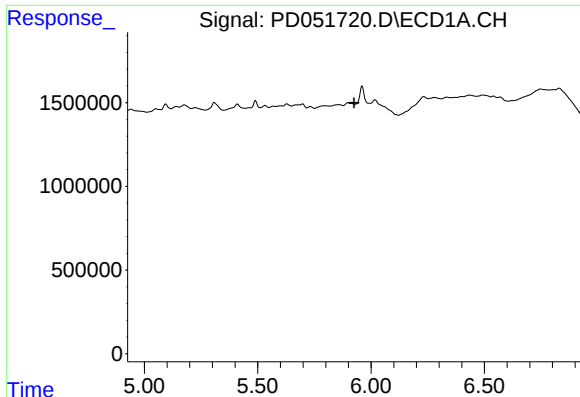

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

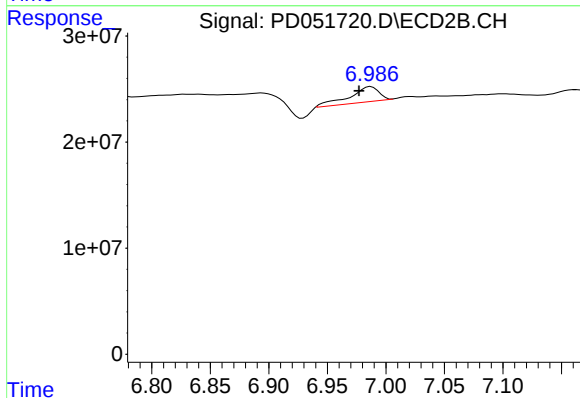


#15 Endosulfan II

R.T.: 6.987 min
Delta R.T.: 0.010 min
Response: 24964530
Conc: 0.91 ng/ml

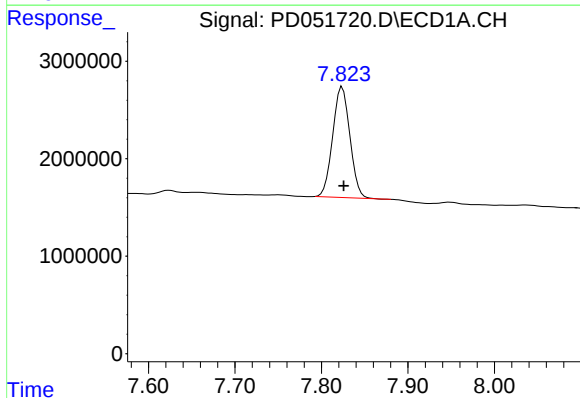

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 15586382
Conc: 12.96 ng/ml

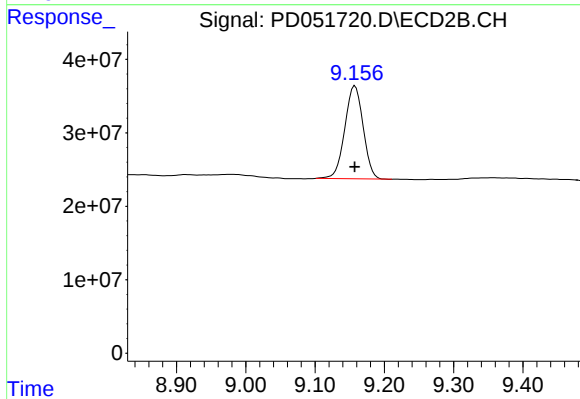

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 233142367
Conc: 12.30 ng/ml