

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
 Data File : PD051724.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 15:06
 Operator : AJ\SJ
 Sample : K1736-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF627

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:59:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.044	10733574	251.3E6	7.469	8.134
27) SA Decachlor...	7.824	9.158	10477851	156.4E6	8.712	8.249
Target Compounds						
8) B Heptachlo...	0.000	5.916	0	68386998	N.D.	1.910


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
Data File : PD051724.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 15:06
Operator : AJ\SJ
Sample : K1736-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:59:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

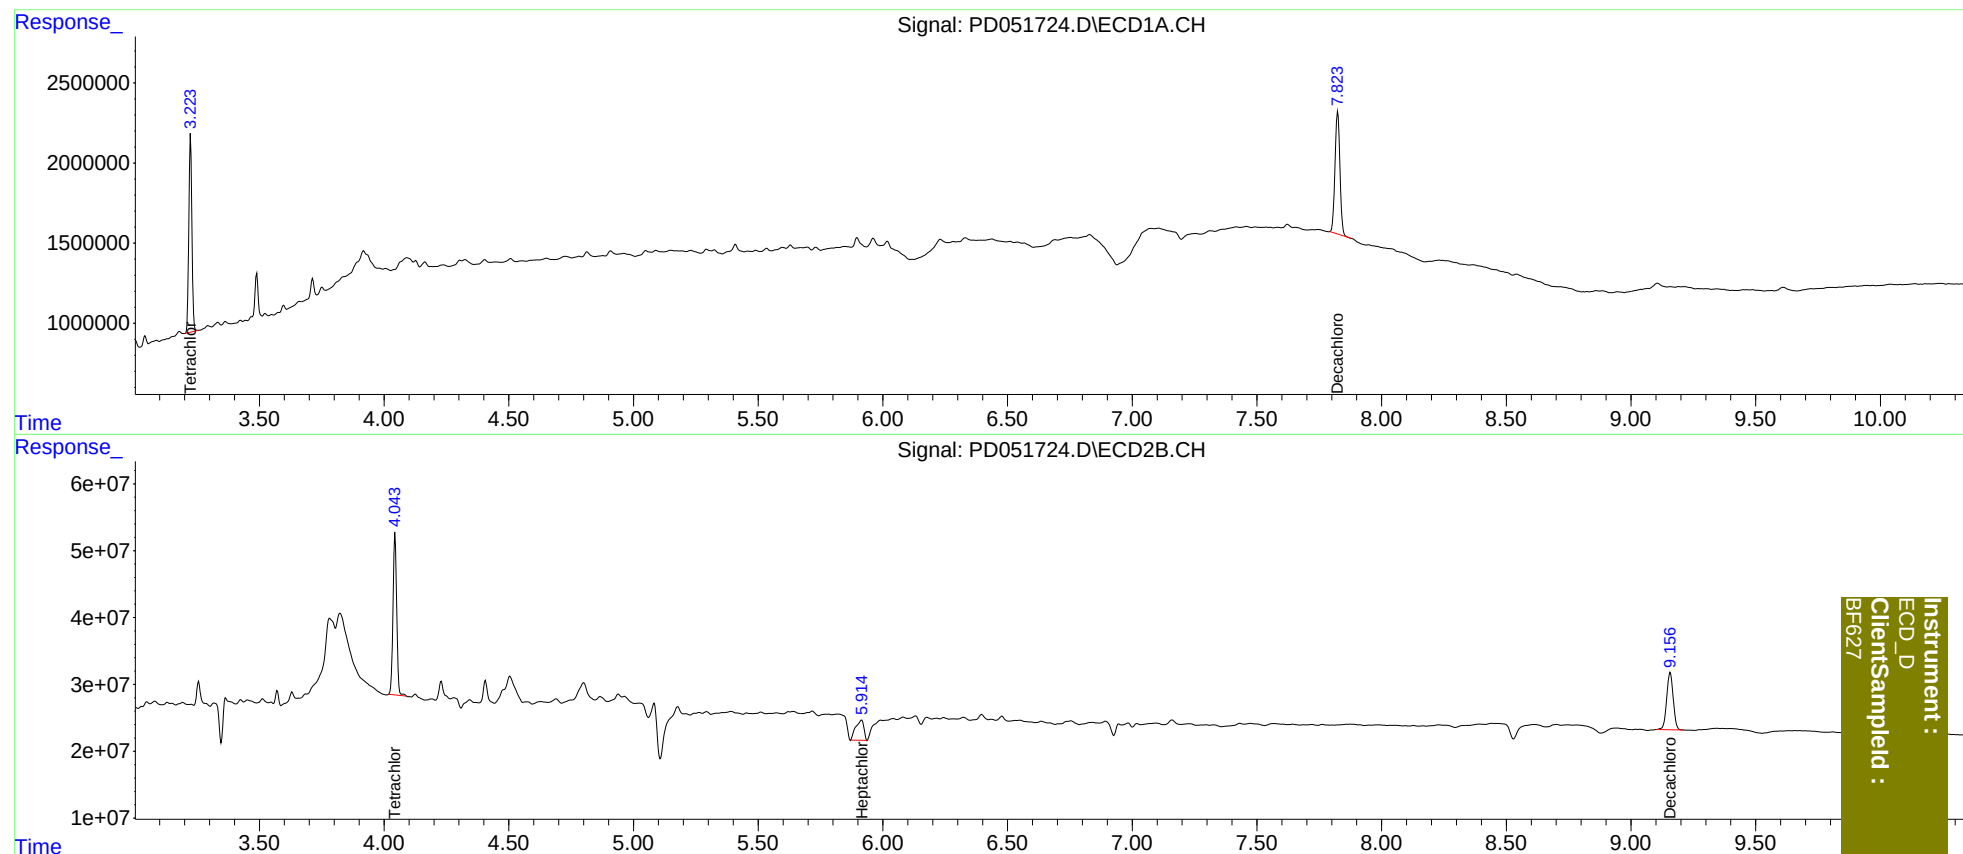


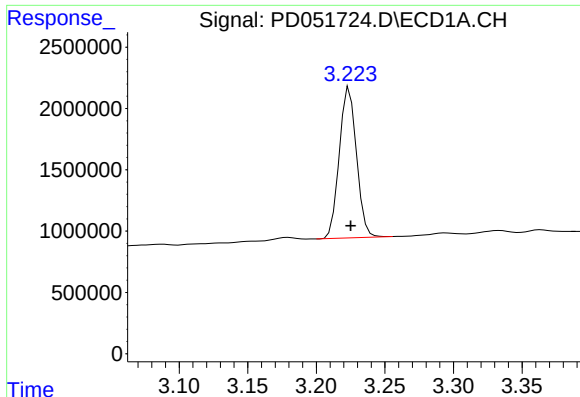

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 10733574
Conc: 7.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF627

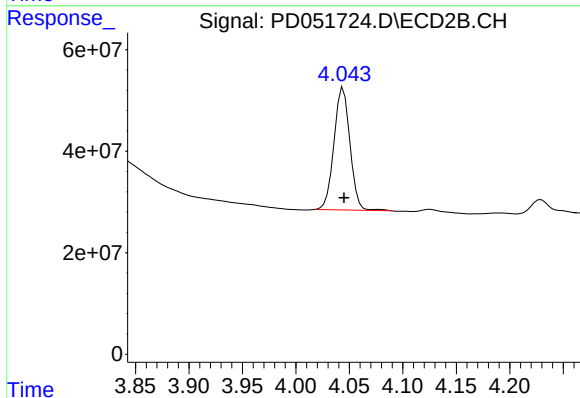


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 251294073
Conc: 8.13 ng/ml

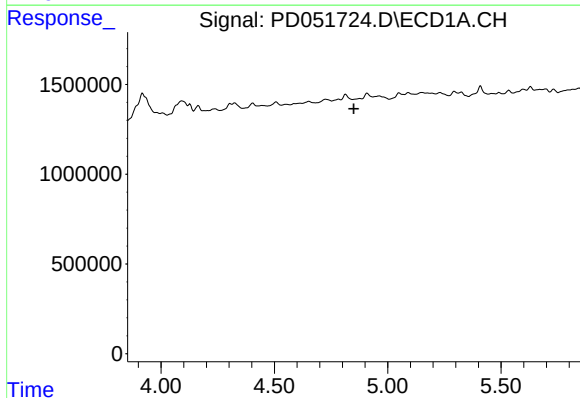


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

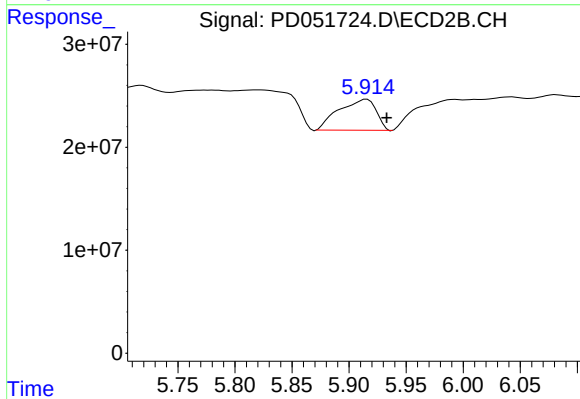

#8 Heptachlor epoxide


R.T.: 5.916 min
Delta R.T.: -0.017 min
Response: 68386998
Conc: 1.91 ng/ml

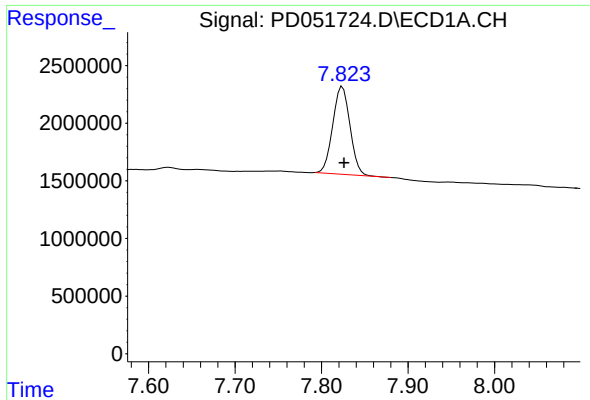

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 10477851
Conc: 8.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF627

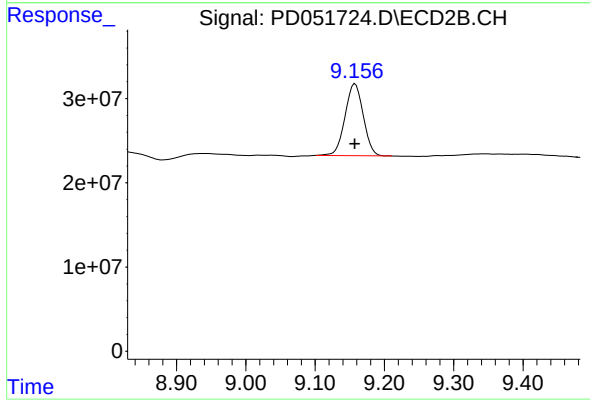

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 156376693
Conc: 8.25 ng/ml