

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
 Data File : PD051733.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 17:12
 Operator : AJ\SJ
 Sample : PB117796BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK96

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 07:01:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	28497380	620.3E6	19.831	20.078
27)	SA Decachlor...	7.824	9.158	45331606	658.0E6	37.693	34.708
Target Compounds							
6)	B beta-BHC	0.000	4.943f	0 54214447	N.D.		2.732
8)	B Heptachlo...	0.000	5.920	0 53585050	N.D.		1.497
15)	B Endosulfa...	0.000	6.986	0 7251652	N.D.		0.264
19)	B Endosulfa...	0.000	7.348	0 32007154	N.D.		1.261
20)	A Methoxychlor	0.000	7.654	0 148.0E6	N.D.		13.985

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031119\
Data File : PD051733.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 17:12
Operator : AJ\SJ
Sample : PB117796BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 07:01:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

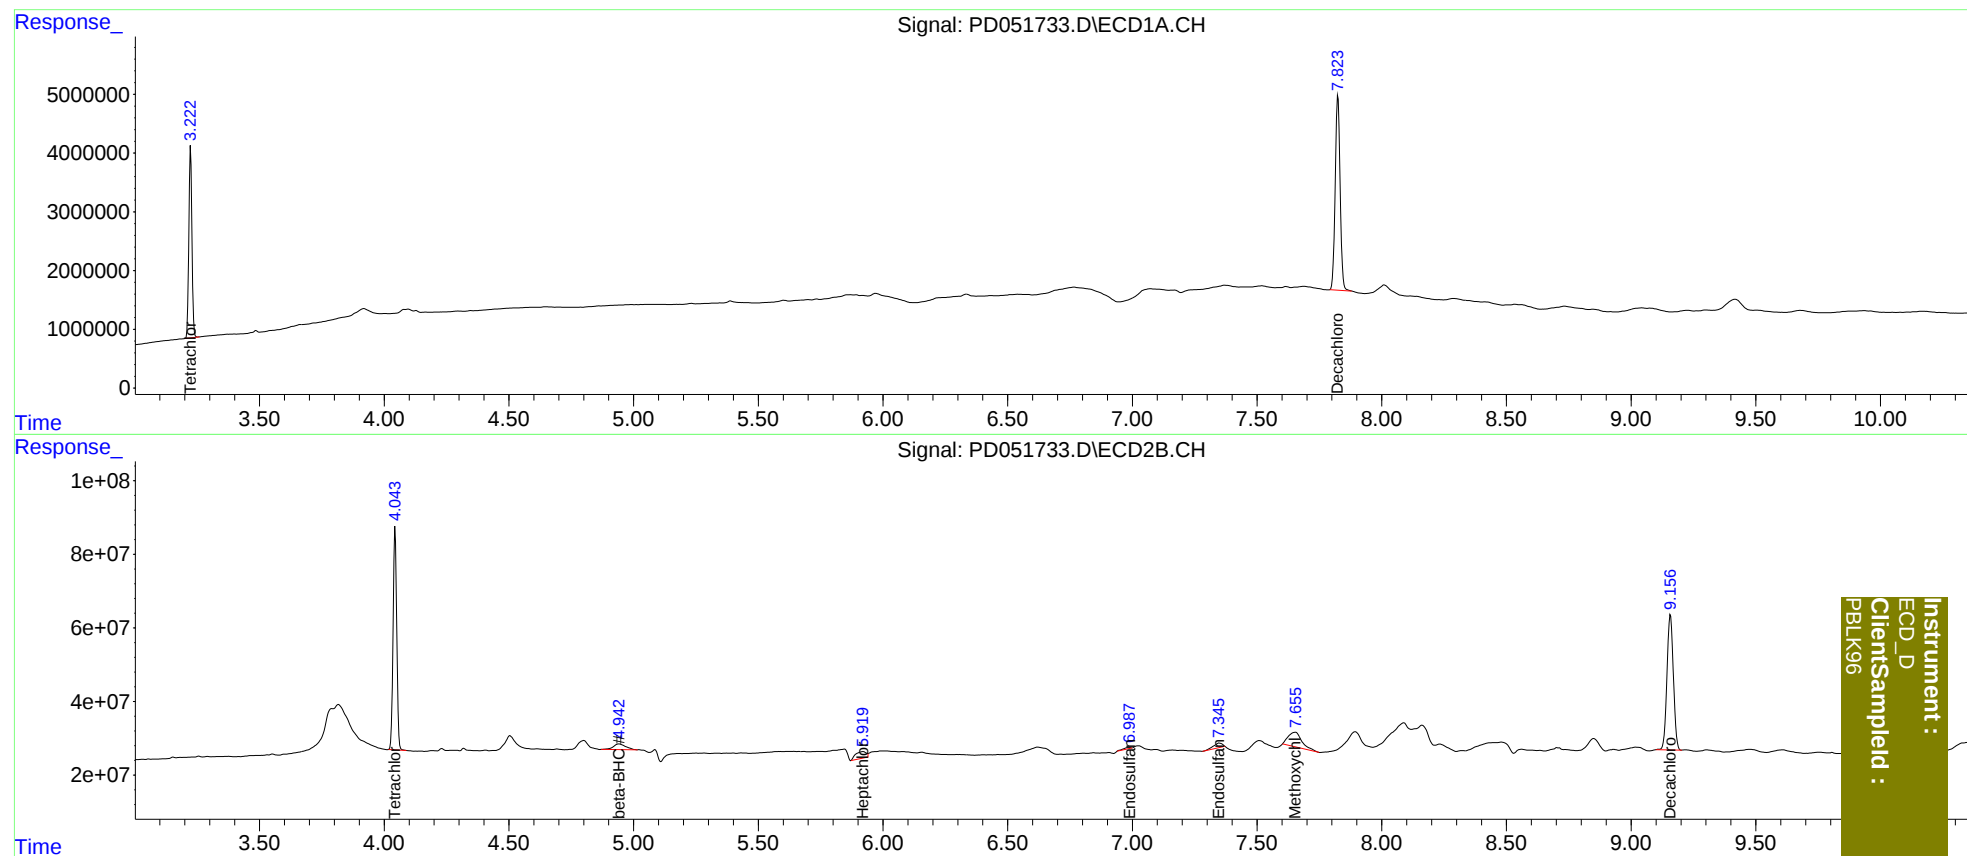


Instrument :
ECD_D
ClientSampleId :
PBLK96

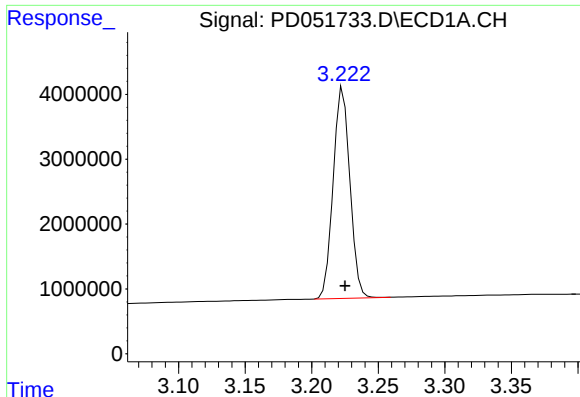

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 28497380
Conc: 19.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK96

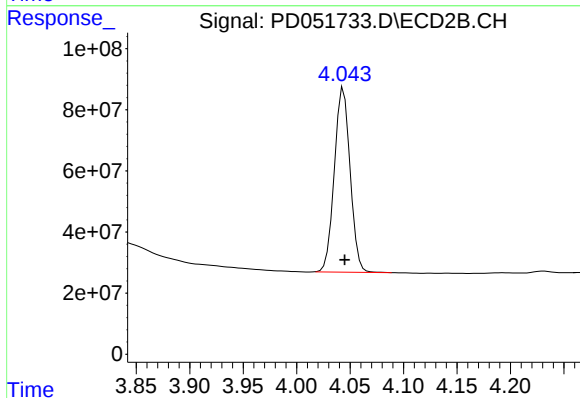


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 620333907
Conc: 20.08 ng/ml

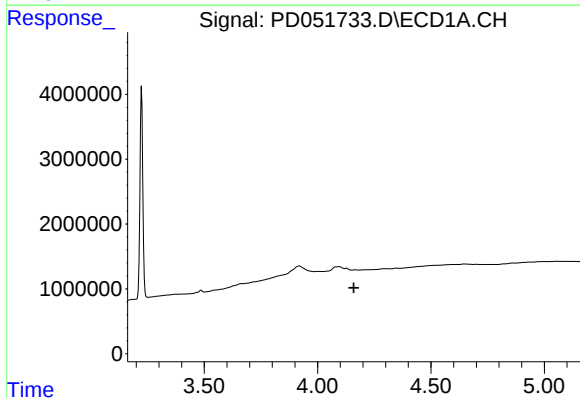


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

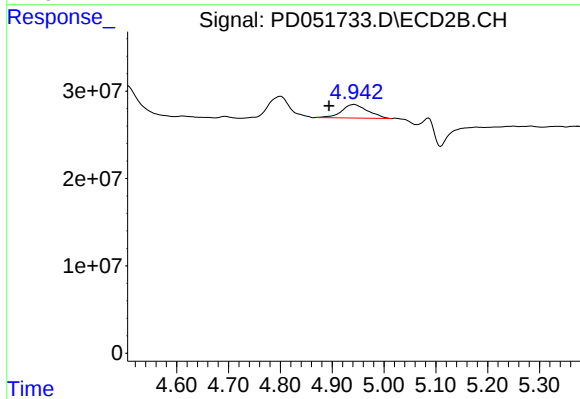

#6 beta-BHC


R.T.: 4.943 min
Delta R.T.: 0.049 min
Response: 54214447
Conc: 2.73 ng/ml

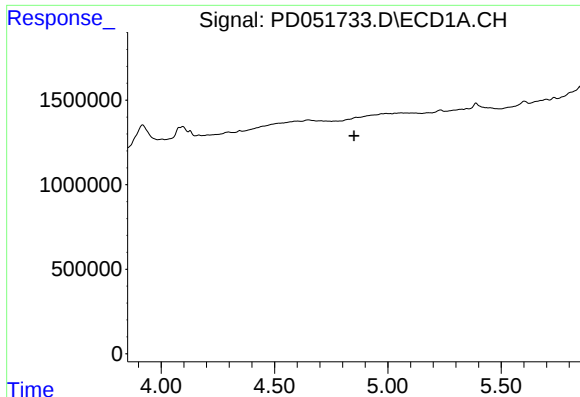

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK96

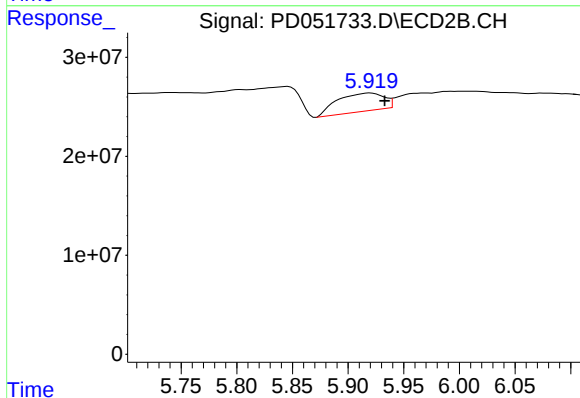


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: -0.013 min
Response: 53585050
Conc: 1.50 ng/ml

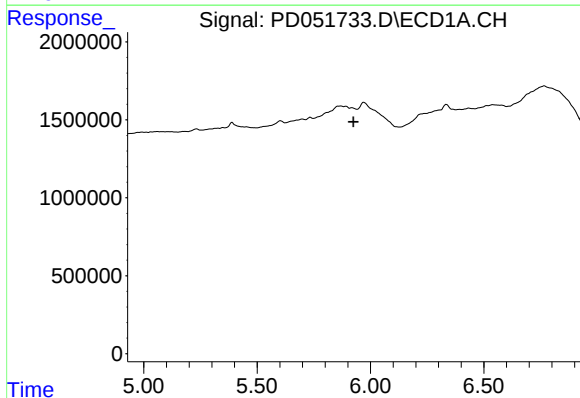


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

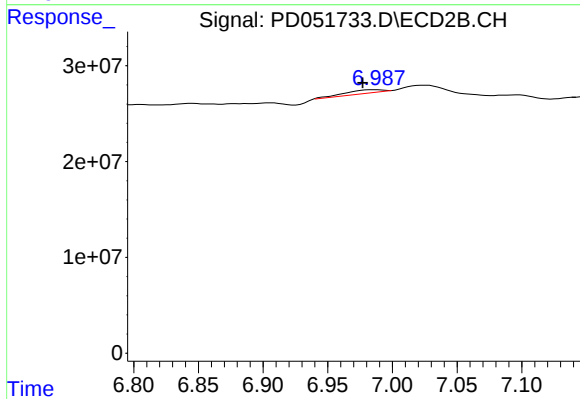

#15 Endosulfan II


R.T.: 6.986 min
Delta R.T.: 0.009 min
Response: 7251652
Conc: 0.26 ng/ml

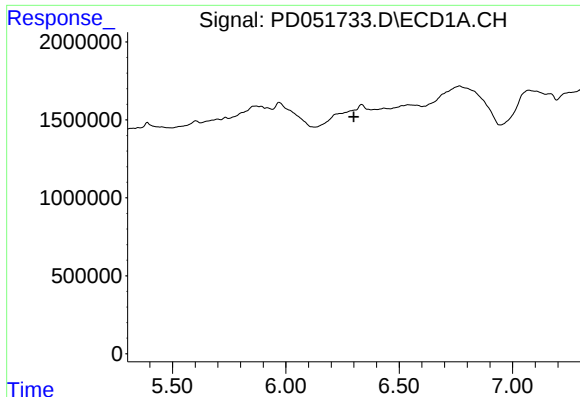

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK96

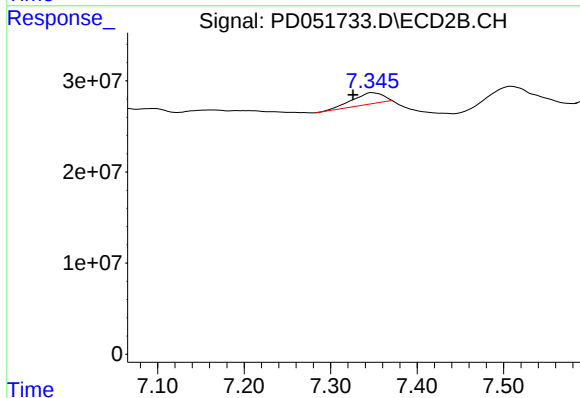


#19 Endosulfan Sulfate

R.T.: 7.348 min
Delta R.T.: 0.022 min
Response: 32007154
Conc: 1.26 ng/ml

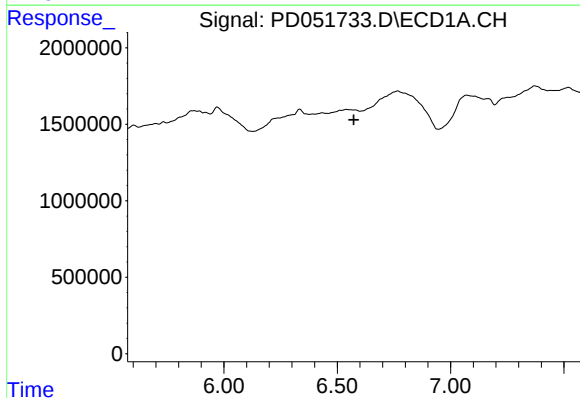


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.572 min
Response: 0
Conc: N.D.

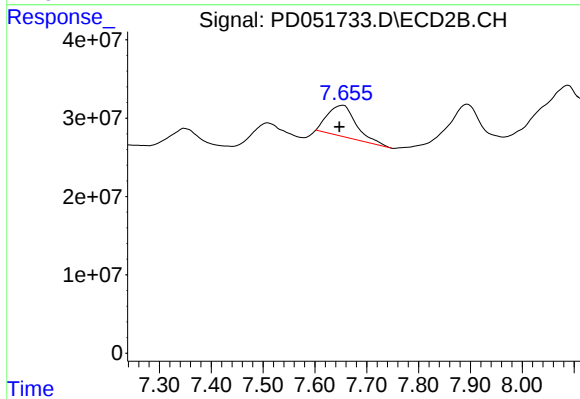

#20 Methoxychlor


R.T.: 7.654 min
Delta R.T.: 0.007 min
Response: 148043535
Conc: 13.99 ng/ml

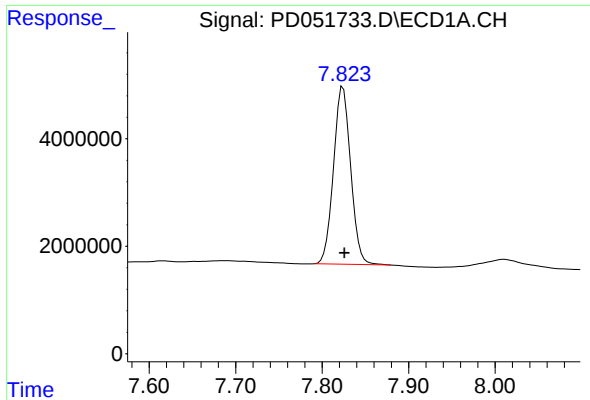

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 45331606
Conc: 37.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK96

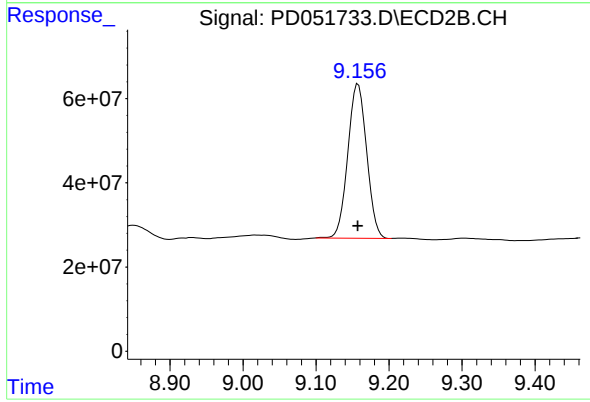

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 657982592
Conc: 34.71 ng/ml