

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
 Data File : PD057575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 21:05
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:21:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:17:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	4714065	4845907	5.207	4.857
27)	SA Decachlor...	7.867	8.897	10555508	11413107	10.870	10.713
Target Compounds							
2)	A alpha-BHC	3.650	4.281	6276523	6427971	4.807	4.560
3)	MA gamma-BHC...	3.922	4.561	6413871	6225614	5.285	4.605
4)	MA Heptachlor	4.202	5.062	4555924	6953802	5.047	5.280
9)	A Endosulfan I	5.197	6.099	4787651	6100924	4.971	4.970
13)	MA Dieldrin	5.435	6.354	7880541	12648300	10.073	9.401
14)	MA Endrin	5.686	6.569	7640331	10394021	10.113	9.646
16)	A 4,4'-DDD	5.823	6.696	6310811	10604380	10.299	9.742
17)	MA 4,4'-DDT	6.057	6.992	6302184	8781711	9.492	8.840
20)	A Methoxychlor	6.604	7.451	12902526	24441886	52.484	49.234


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
Data File : PD057575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 21:05
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:21:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:17:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

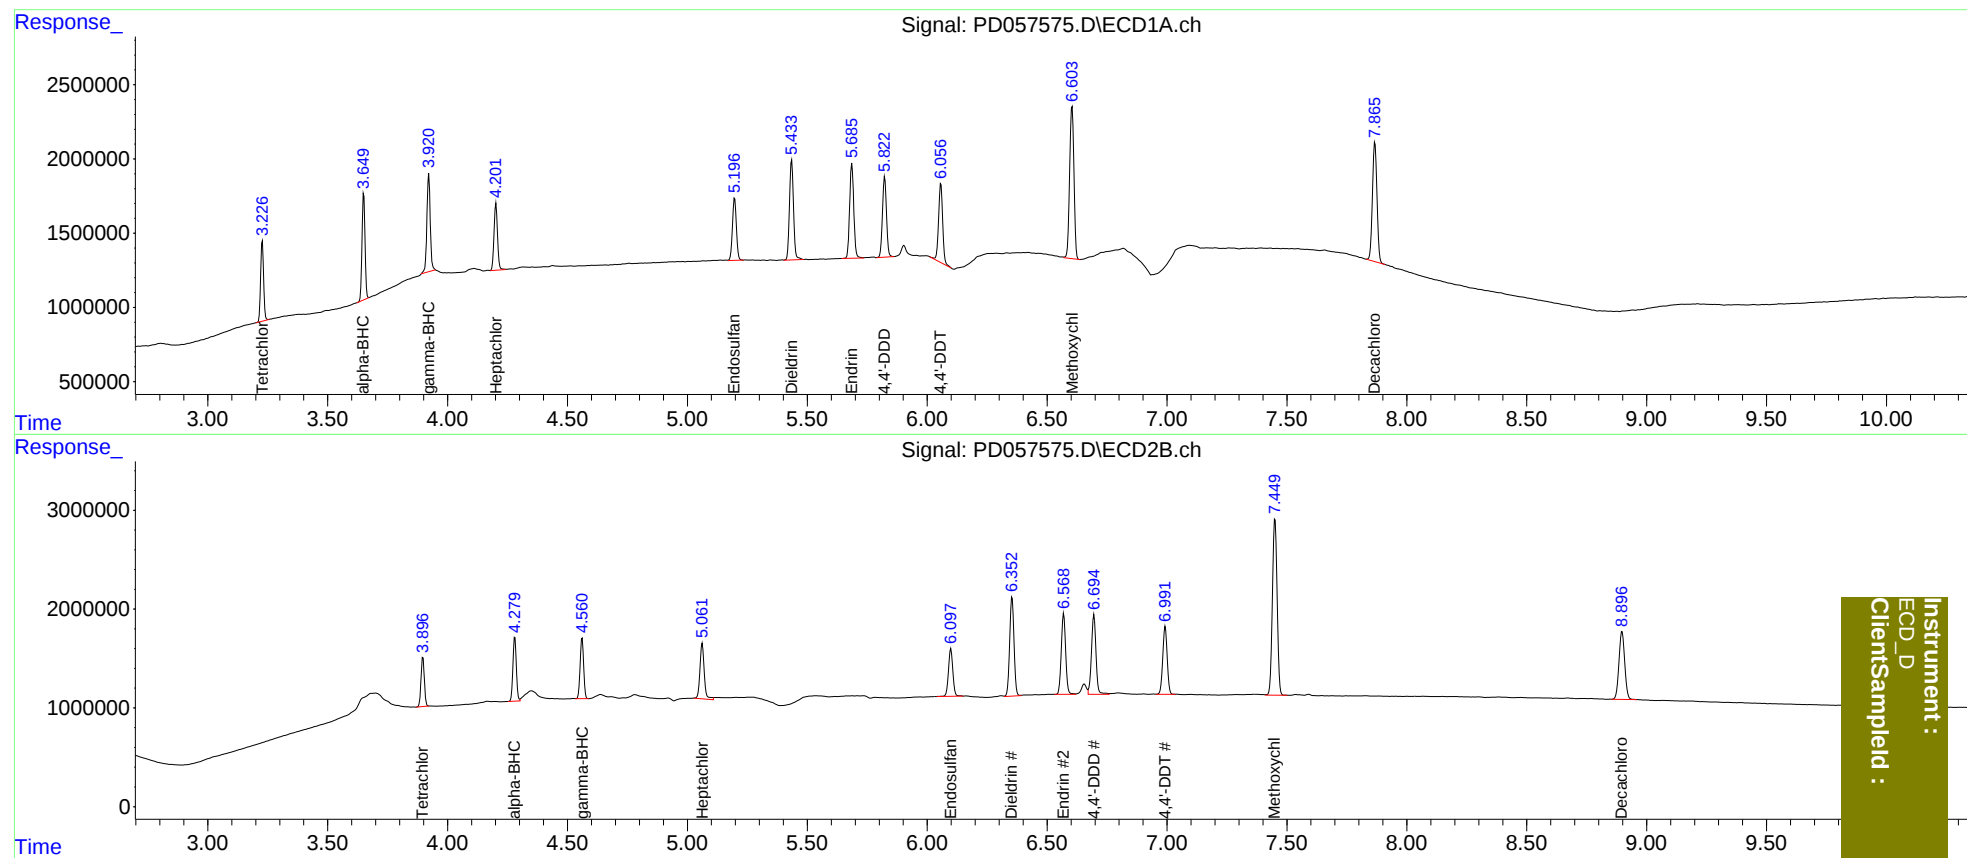


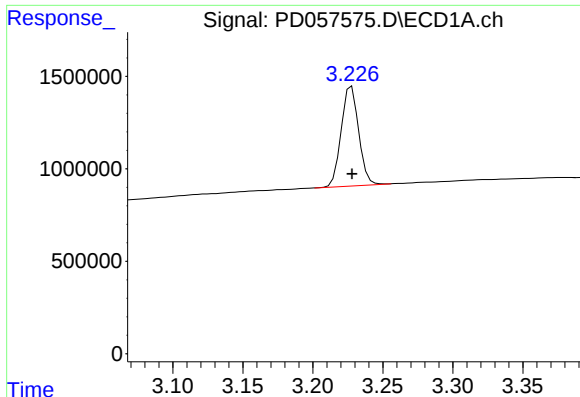

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 4714065
Conc: 5.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

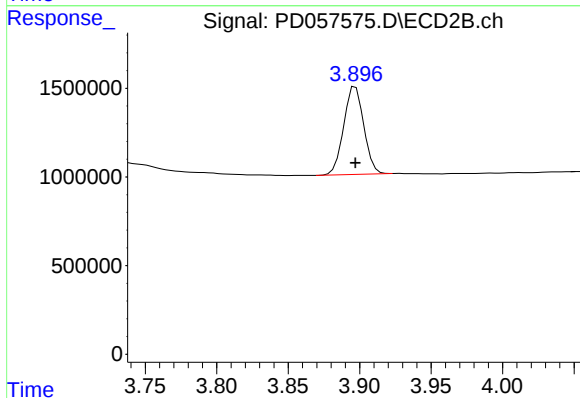


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 4845907
Conc: 4.86 ng/ml

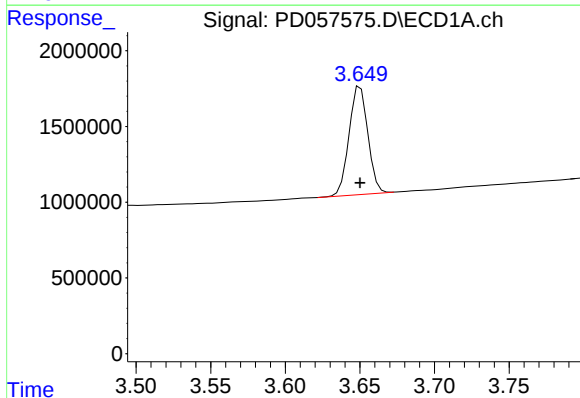


#2 alpha-BHC

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 6276523
Conc: 4.81 ng/ml

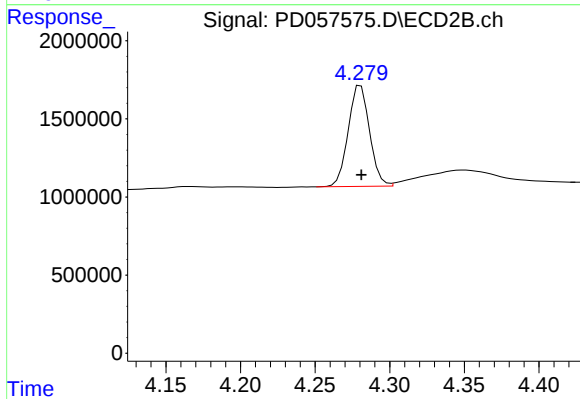

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 6427971
Conc: 4.56 ng/ml

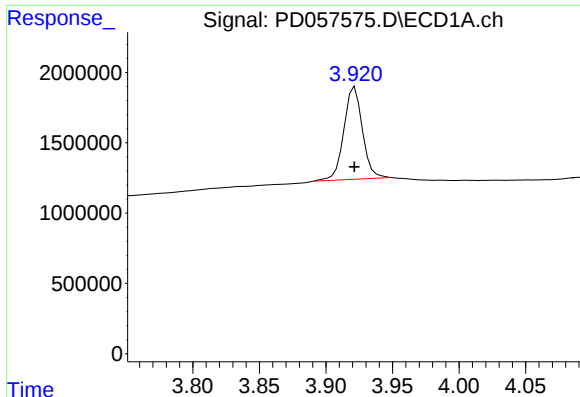

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 6413871
Conc: 5.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

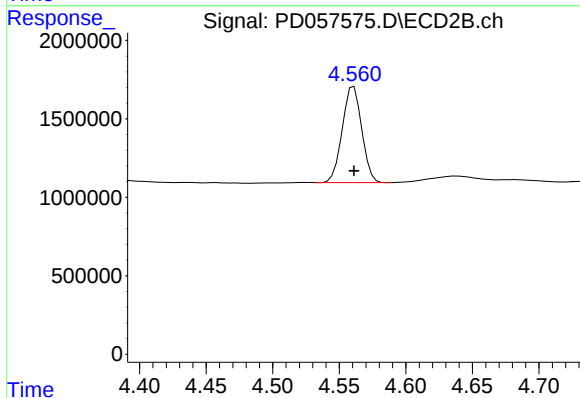


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 6225614
Conc: 4.61 ng/ml

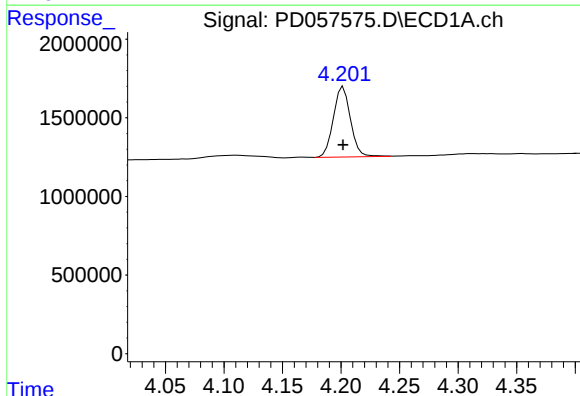


#4 Heptachlor

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 4555924
Conc: 5.05 ng/ml

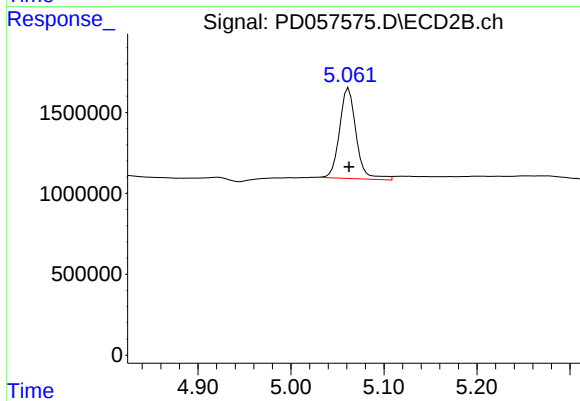

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 6953802
Conc: 5.28 ng/ml

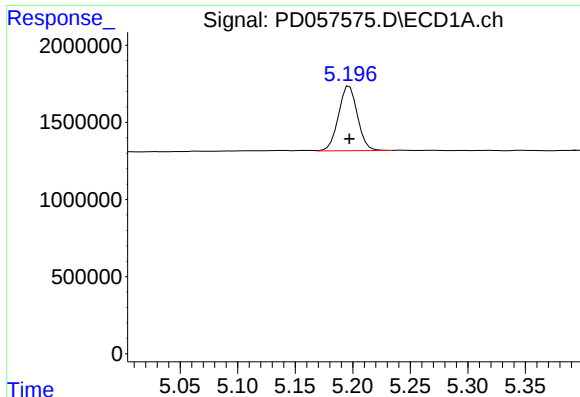

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 4787651
Conc: 4.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

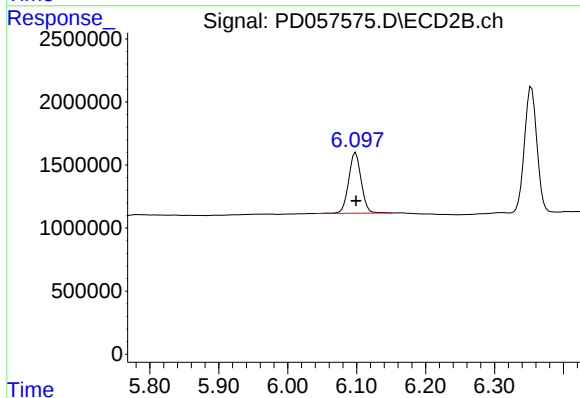


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 6100924
Conc: 4.97 ng/ml

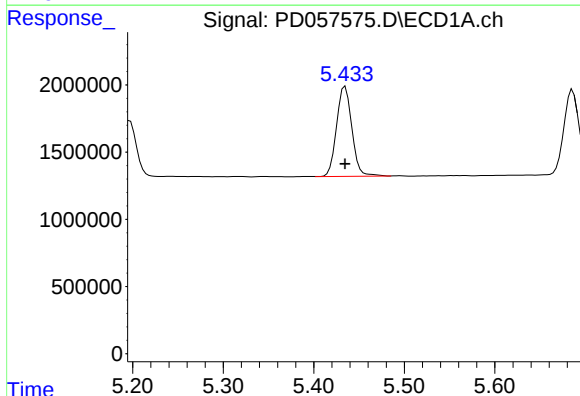


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 7880541
Conc: 10.07 ng/ml

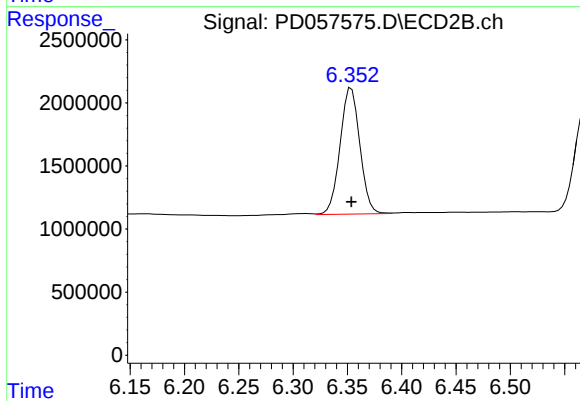

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 12648300
Conc: 9.40 ng/ml

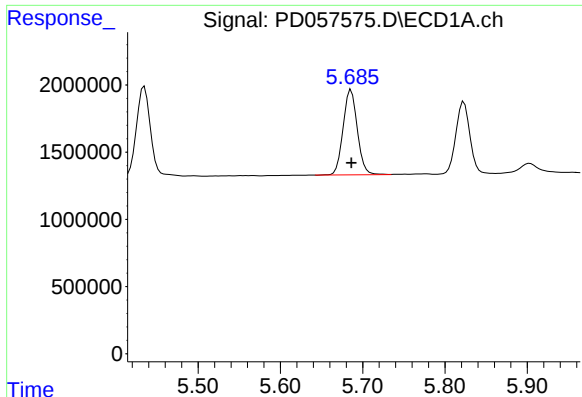

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 7640331
Conc: 10.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

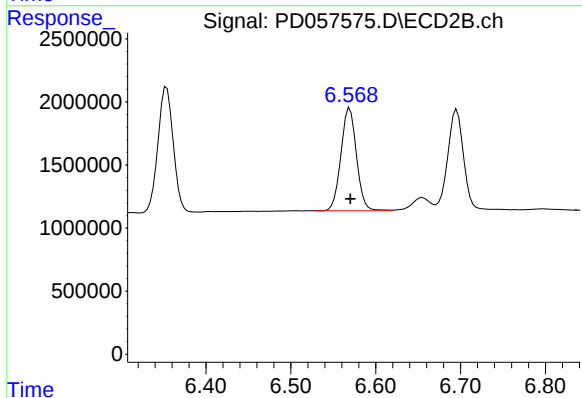


#14 Endrin

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 10394021
Conc: 9.65 ng/ml

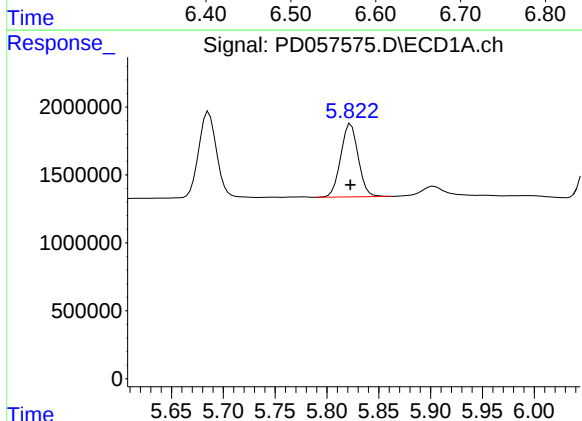


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 6310811
Conc: 10.30 ng/ml

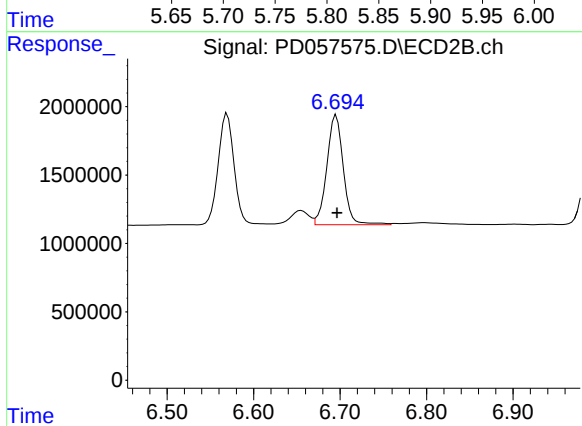

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: -0.001 min
Response: 10604380
Conc: 9.74 ng/ml

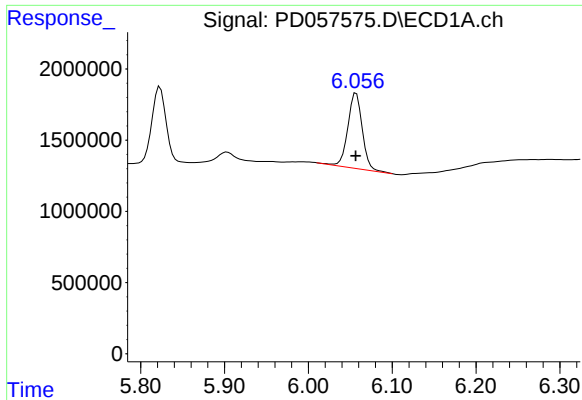

#17 4,4'-DDT


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 6302184
Conc: 9.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

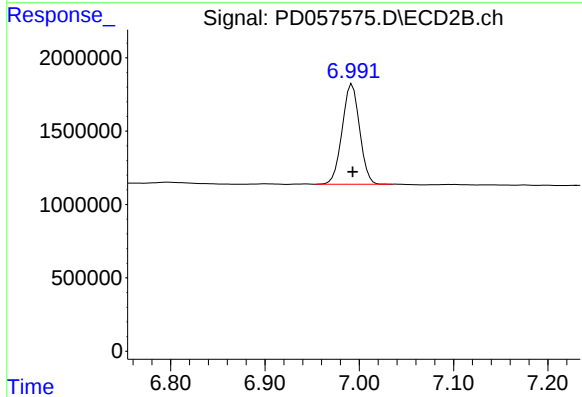


#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 8781711
Conc: 8.84 ng/ml

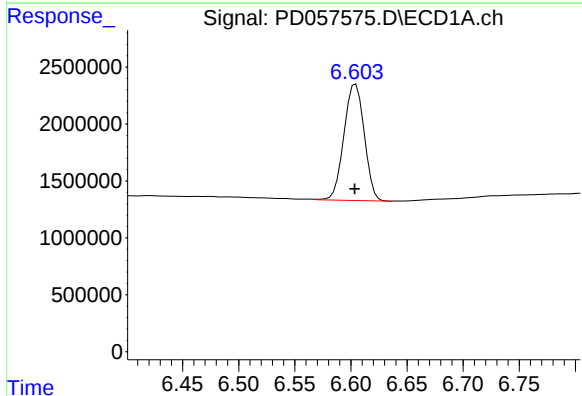


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 12902526
Conc: 52.48 ng/ml

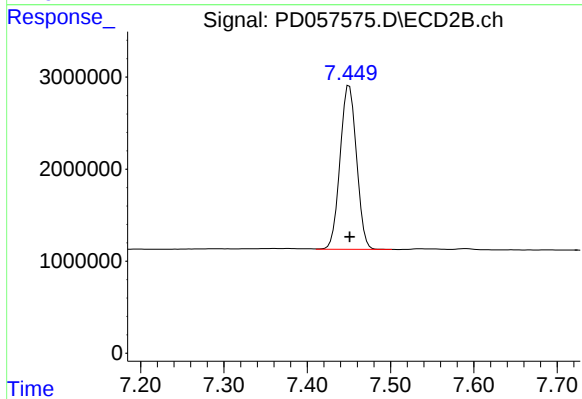

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 24441886
Conc: 49.23 ng/ml

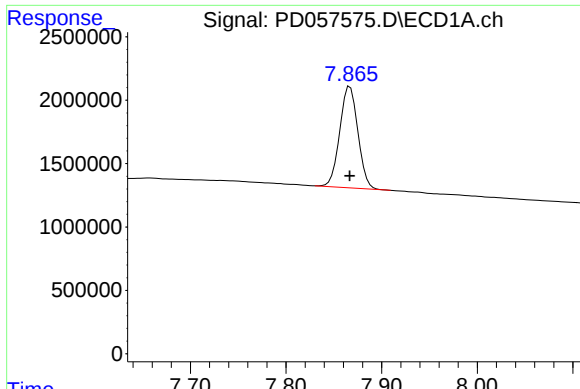

#27 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 10555508
Conc: 10.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

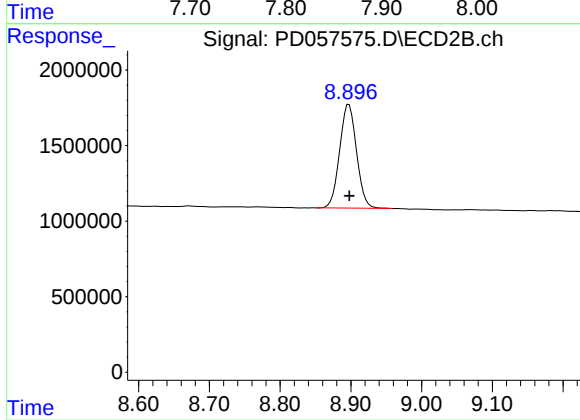

#27 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.000 min
Response: 11413107
Conc: 10.71 ng/ml