

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
 Data File : PD057579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 22:01
 Operator : AJ\MA
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:21:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:17:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	18105682	19955214	20.000	20.000
27)	SA Decachlor...	7.867	8.898	38842793	42612613	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.650	4.281	26112025	28190727	20.000	20.000
3)	MA gamma-BHC...	3.921	4.561	24270306	27036400	20.000	20.000
4)	MA Heptachlor	4.202	5.062	18054725	26340360	20.000	20.000
9)	A Endosulfan I	5.197	6.099	19263598	24549091	20.000	20.000
13)	MA Dieldrin	5.434	6.354	31295217	53814828	40.000	40.000
14)	MA Endrin	5.686	6.570	30220643	43102641	40.000	40.000
16)	A 4,4'-DDD	5.823	6.697	24509471	43541009	40.000	40.000
17)	MA 4,4'-DDT	6.057	6.993	26558520	39736699	40.000	40.000
20)	A Methoxychlor	6.604	7.451	49167557	99289536	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
Data File : PD057579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 22:01
Operator : AJ\MA
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:21:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:17:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

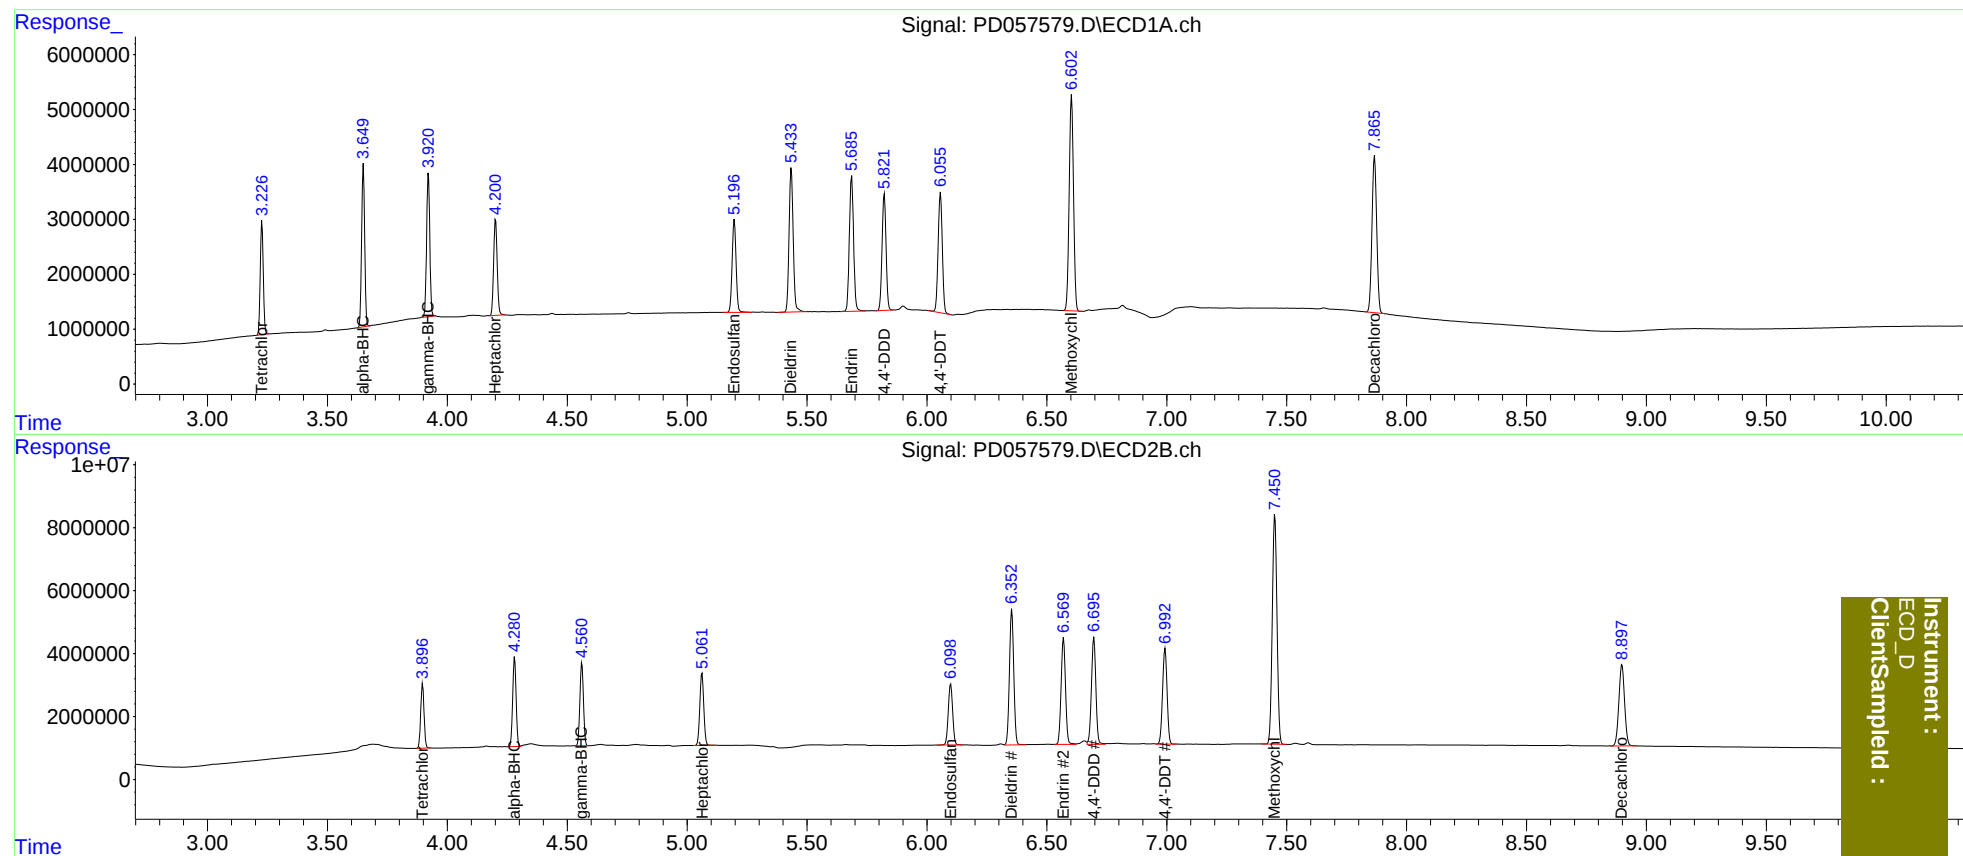


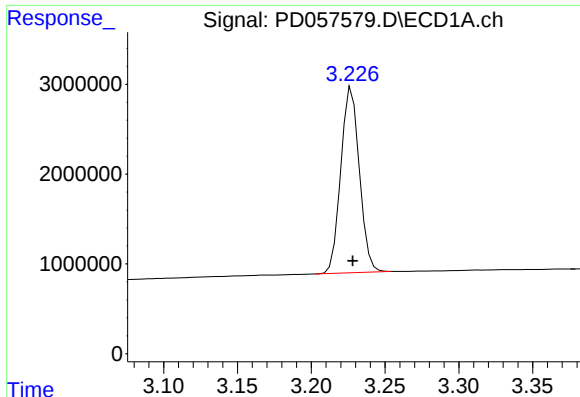

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 18105682
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

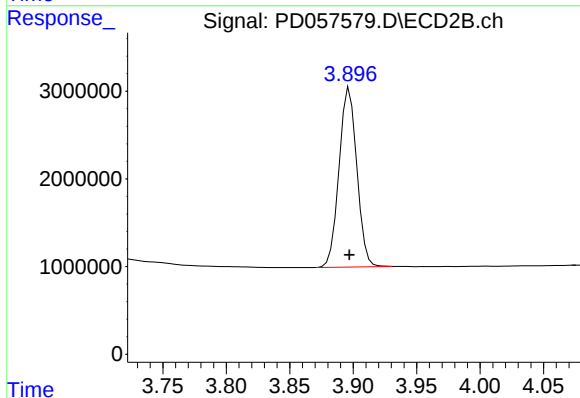


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 19955214
Conc: 20.00 ng/ml

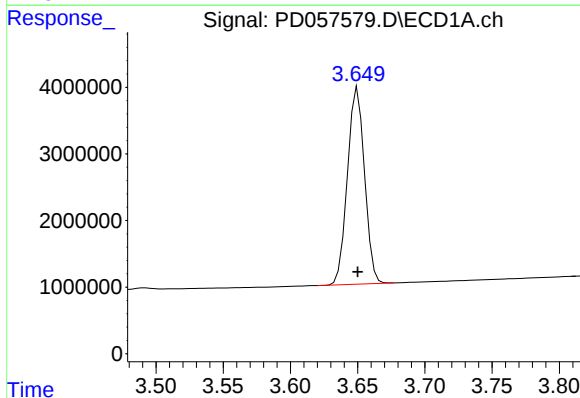


#2 alpha-BHC

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 26112025
Conc: 20.00 ng/ml

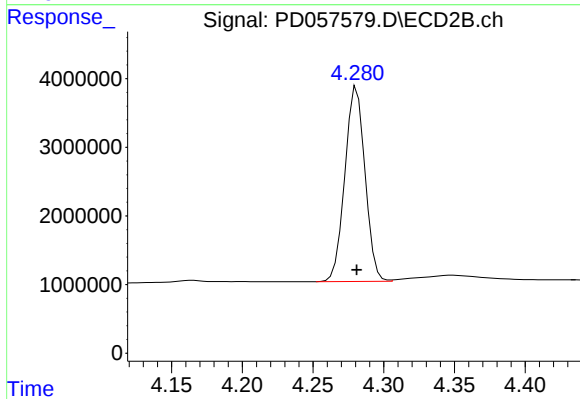

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 28190727
Conc: 20.00 ng/ml

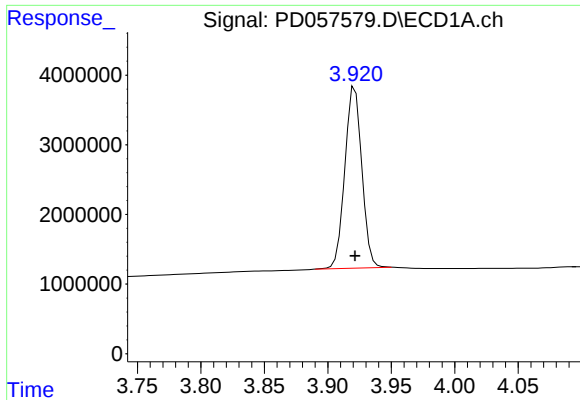

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 24270306
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

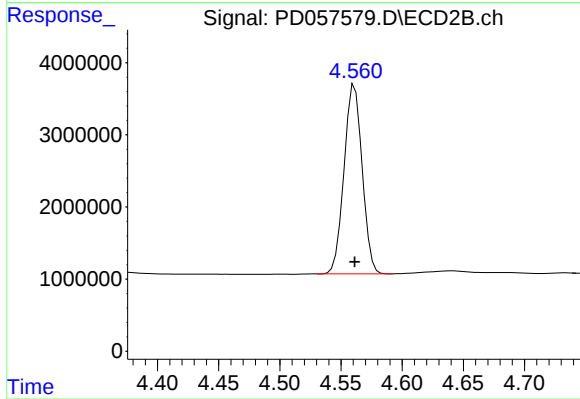


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 27036400
Conc: 20.00 ng/ml

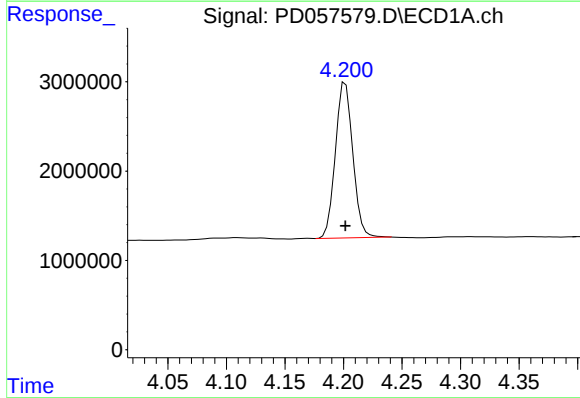


#4 Heptachlor

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 18054725
Conc: 20.00 ng/ml

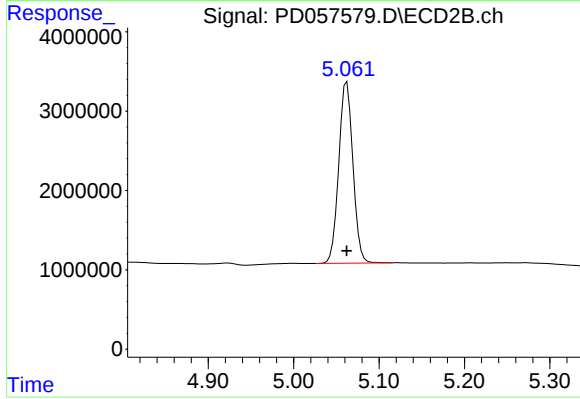

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 26340360
Conc: 20.00 ng/ml

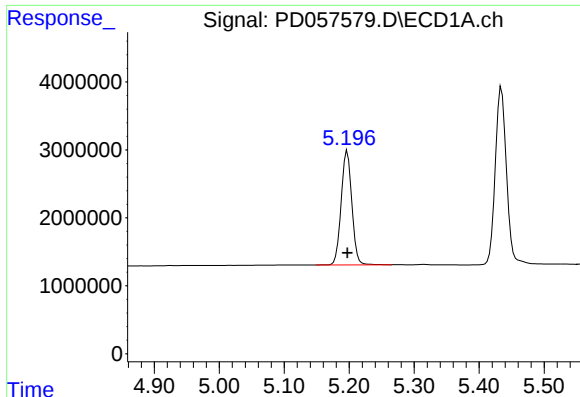

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 19263598
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

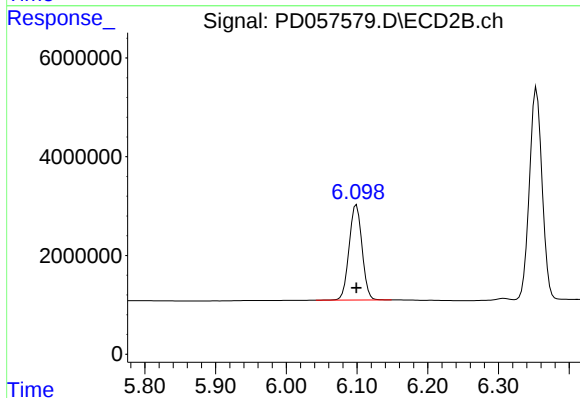


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 24549091
Conc: 20.00 ng/ml

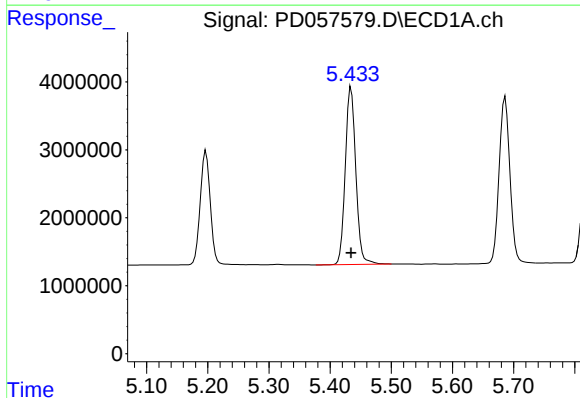


#13 Dieldrin

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 31295217
Conc: 40.00 ng/ml

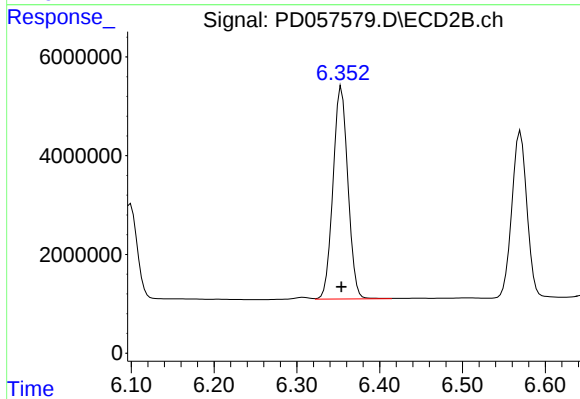

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 53814828
Conc: 40.00 ng/ml

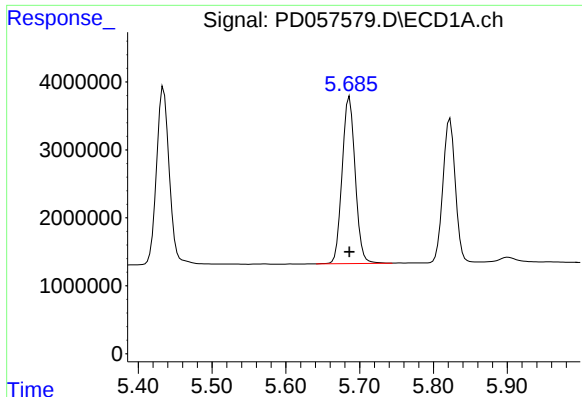

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 30220643
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

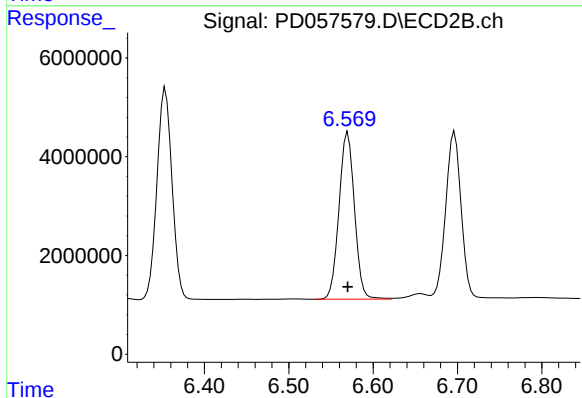


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 43102641
Conc: 40.00 ng/ml

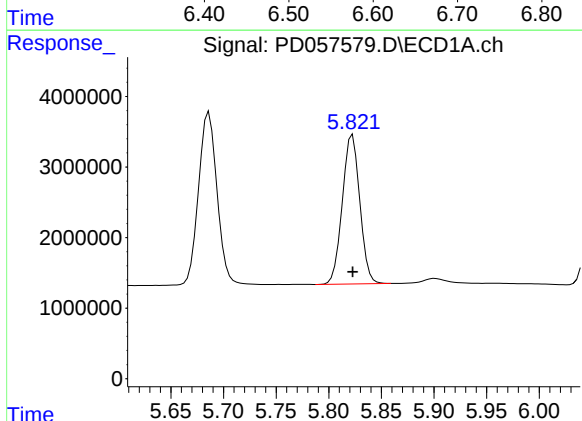


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 24509471
Conc: 40.00 ng/ml

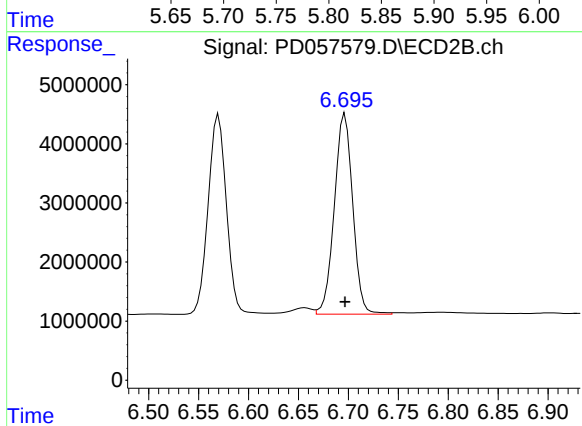

#16 4,4'-DDD


R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 43541009
Conc: 40.00 ng/ml

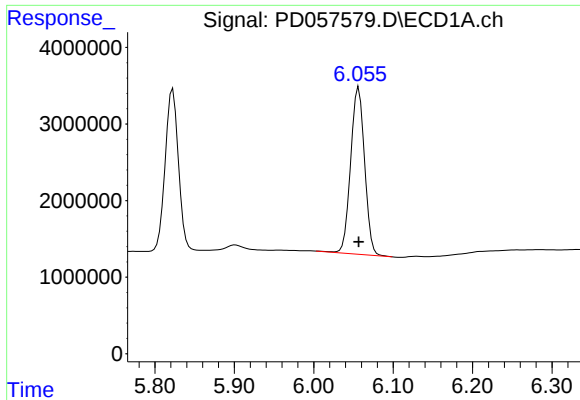

#17 4,4'-DDT


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 26558520
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

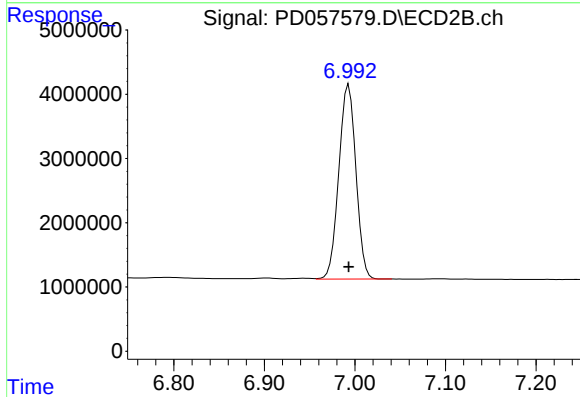


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 39736699
Conc: 40.00 ng/ml

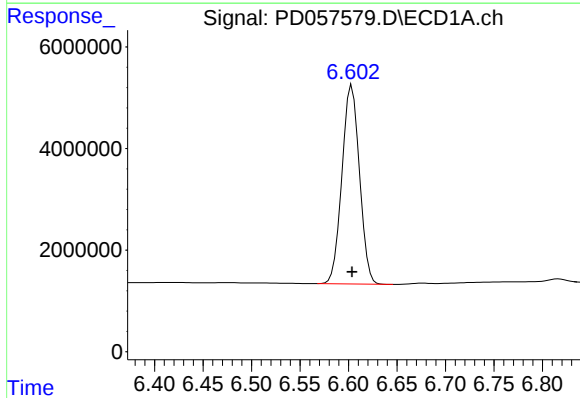


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 49167557
Conc: 200.00 ng/ml

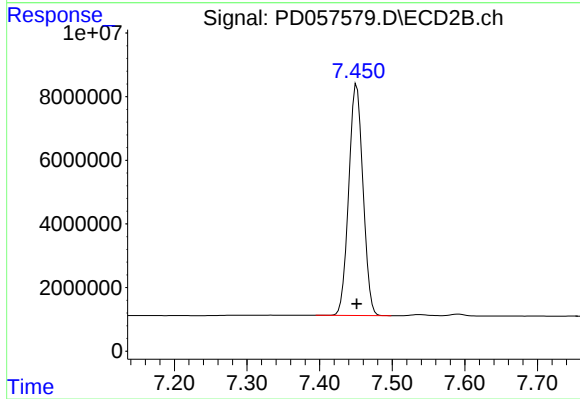

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 99289536
Conc: 200.00 ng/ml

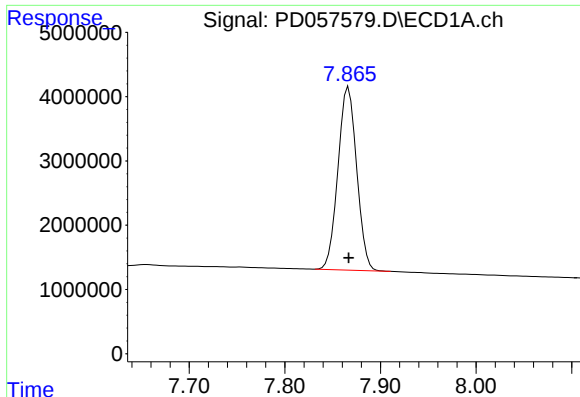

#27 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 38842793
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

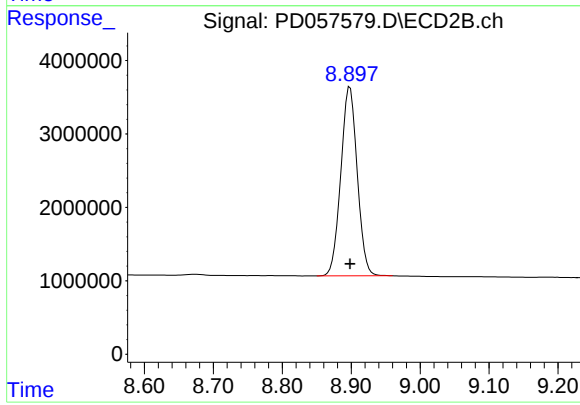

#27 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 42612613
Conc: 40.00 ng/ml