

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
 Data File : PD057581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 22:30
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:21:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:17:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	35059132	38969482	38.727	39.057
27)	SA Decachlor...	7.867	8.898	72720484	78630998	74.887	73.810
Target Compounds							
2)	A alpha-BHC	3.651	4.281	53062621	57526543	40.642	40.812
3)	MA gamma-BHC...	3.922	4.561	48252642	54695462	39.763	40.461
4)	MA Heptachlor	4.202	5.062	35734175	53680642	39.584	40.759
9)	A Endosulfan I	5.197	6.099	38097741	48131410	39.554	39.212
13)	MA Dieldrin	5.435	6.354	61912412	106.9E6	79.133	79.456
14)	MA Endrin	5.686	6.570	59046381	83564729	78.154	77.550
16)	A 4,4'-DDD	5.822	6.696	48136507	85701645	78.560	78.732
17)	MA 4,4'-DDT	6.056	6.993	53379807	79587350	80.396	80.115
20)	A Methoxychlor	6.604	7.451	93294638	191.4E6	379.497	385.562


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
Data File : PD057581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 22:30
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:21:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:17:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

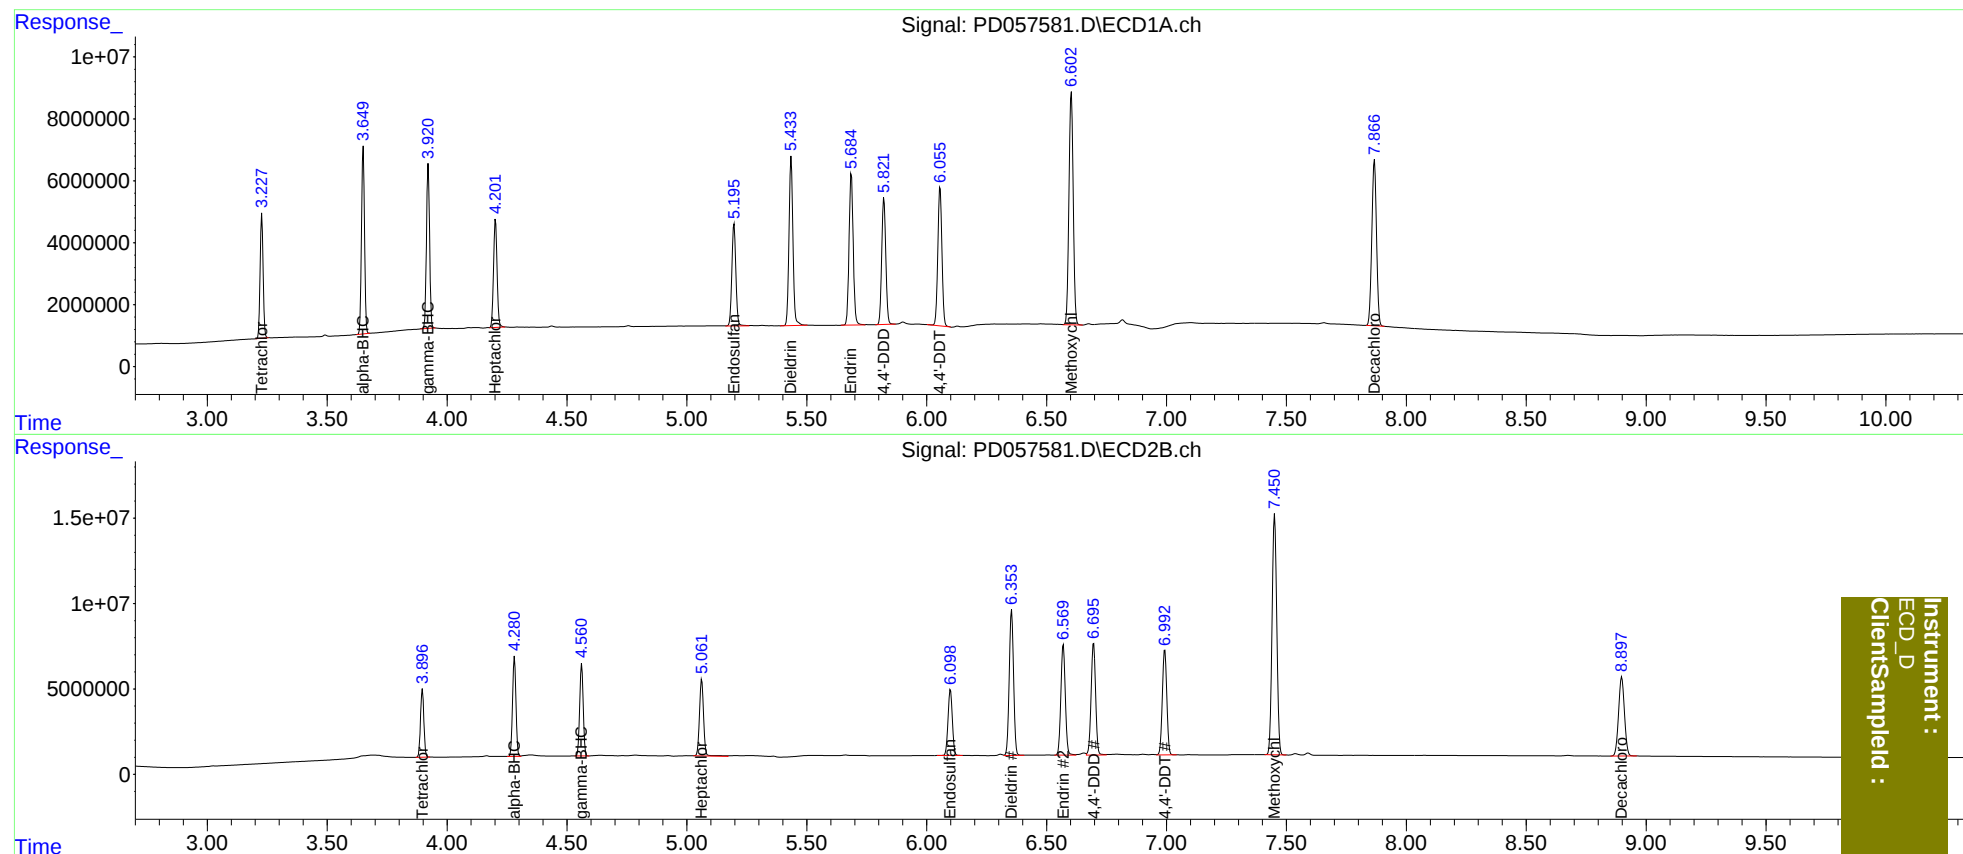


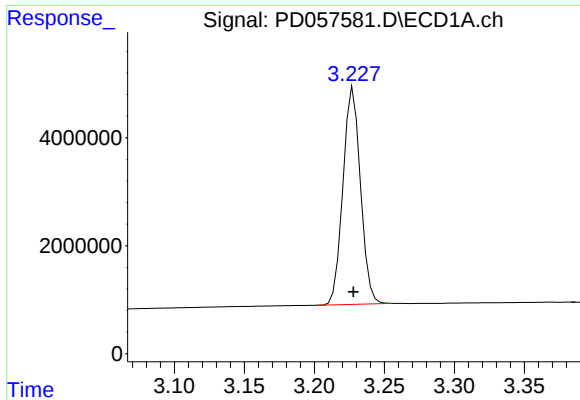

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 35059132
Conc: 38.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

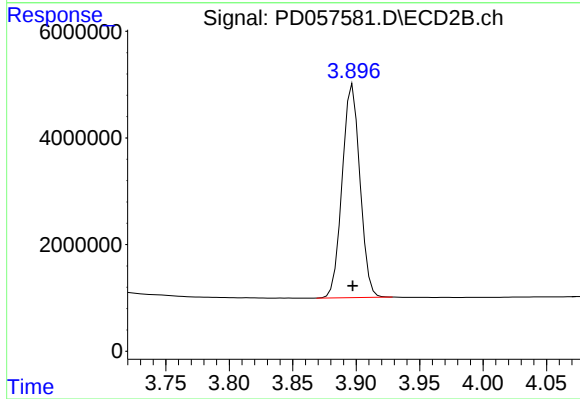


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 38969482
Conc: 39.06 ng/ml

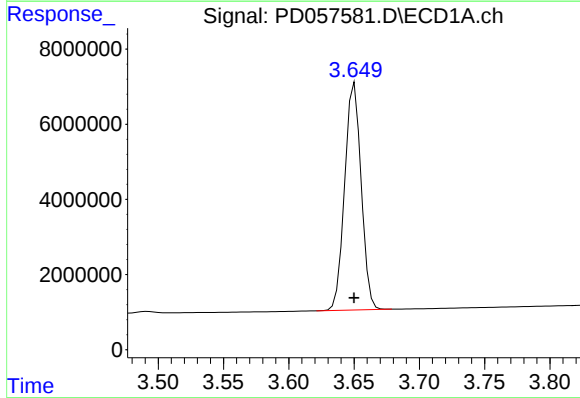


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.000 min
Response: 53062621
Conc: 40.64 ng/ml

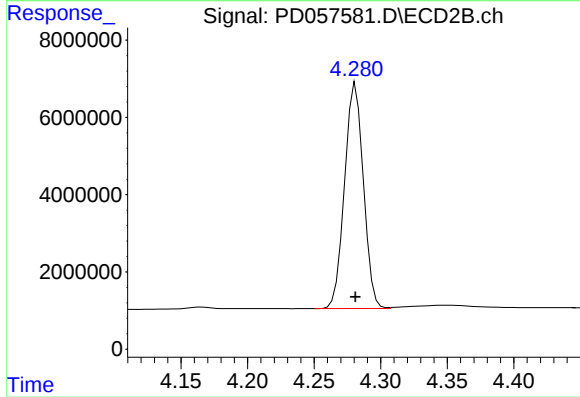

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 57526543
Conc: 40.81 ng/ml

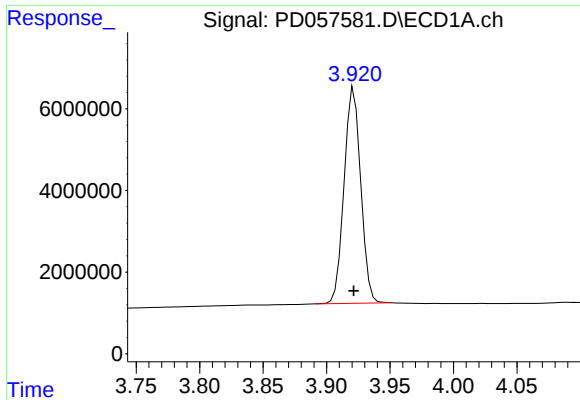

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 48252642
Conc: 39.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

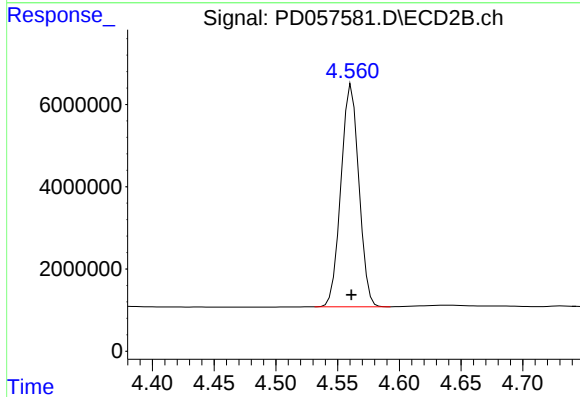


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 54695462
Conc: 40.46 ng/ml

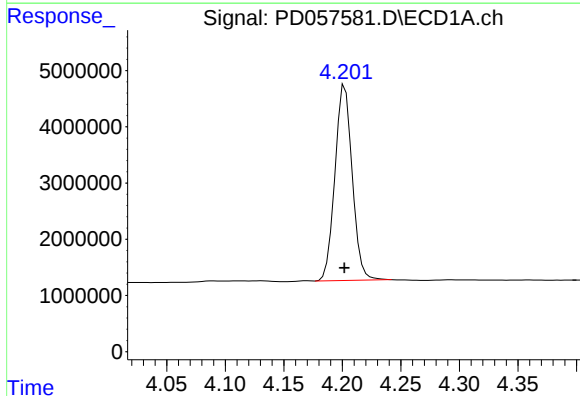


#4 Heptachlor

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 35734175
Conc: 39.58 ng/ml

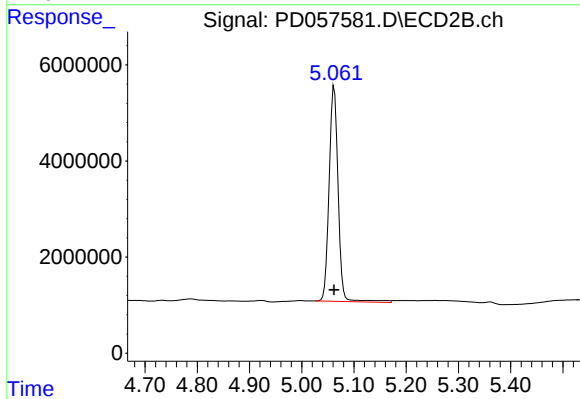

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 53680642
Conc: 40.76 ng/ml

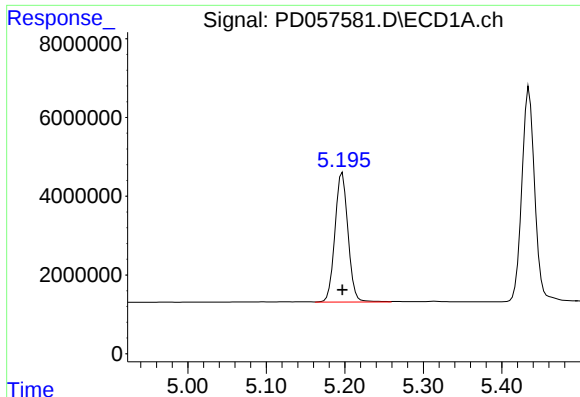

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 38097741
Conc: 39.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

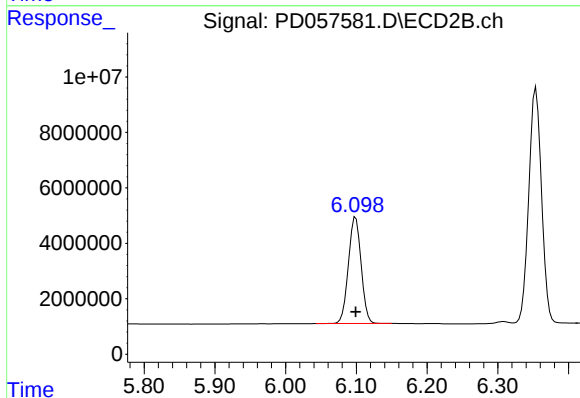


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 48131410
Conc: 39.21 ng/ml

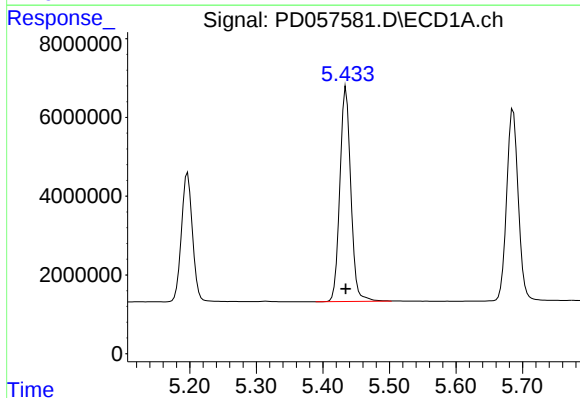


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 61912412
Conc: 79.13 ng/ml

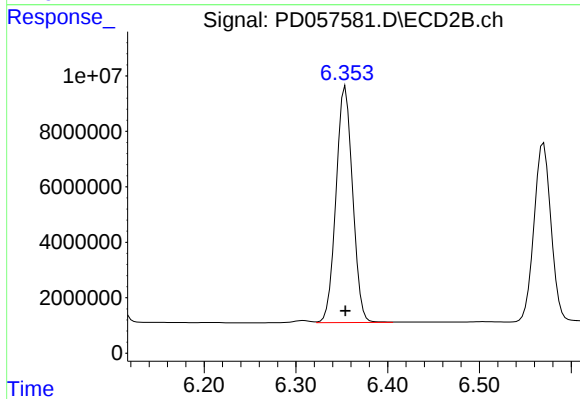

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 106897375
Conc: 79.46 ng/ml

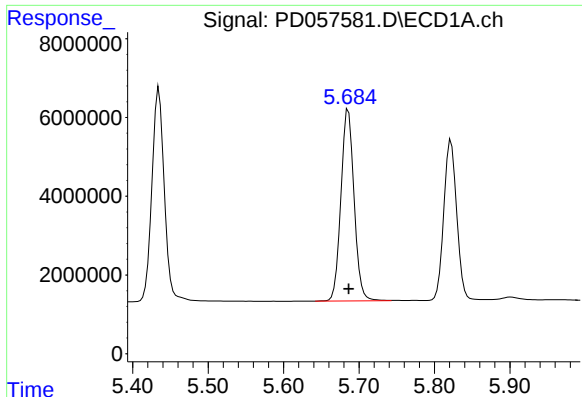

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 59046381
Conc: 78.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

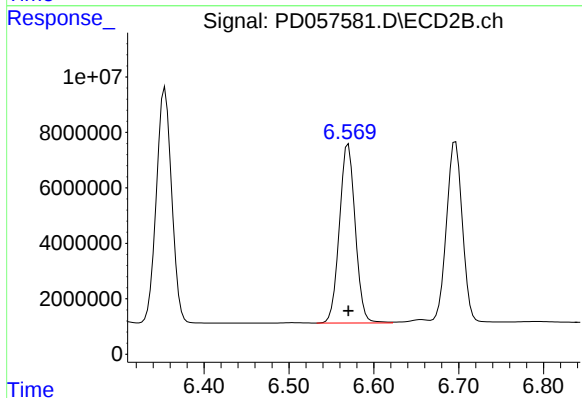


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 83564729
Conc: 77.55 ng/ml

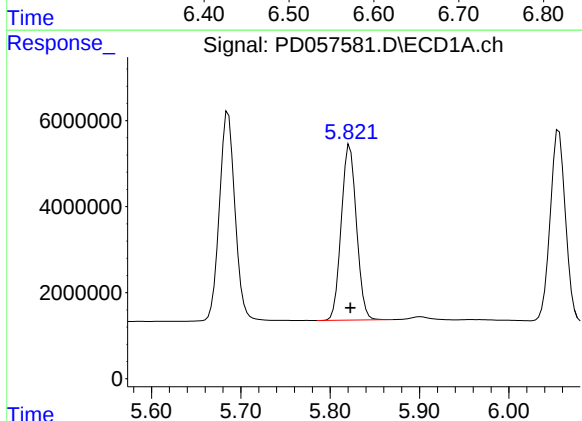


#16 4,4'-DDD

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 48136507
Conc: 78.56 ng/ml

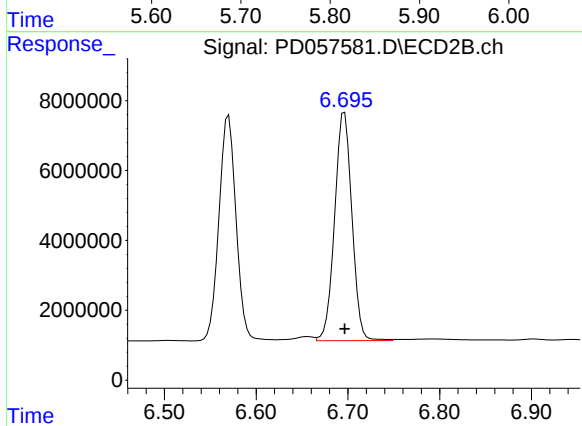

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 85701645
Conc: 78.73 ng/ml

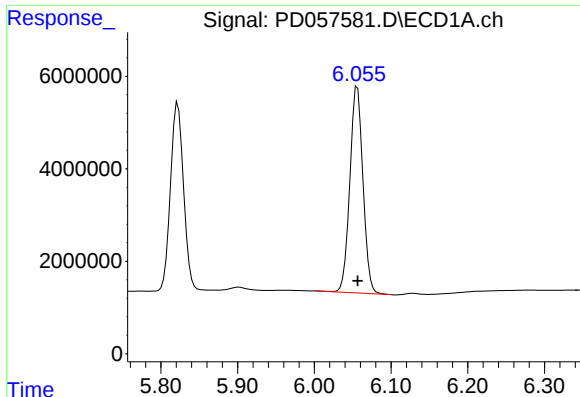

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 53379807
Conc: 80.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

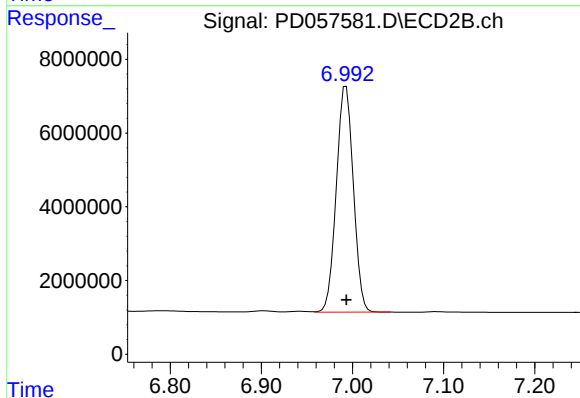


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 79587350
Conc: 80.11 ng/ml

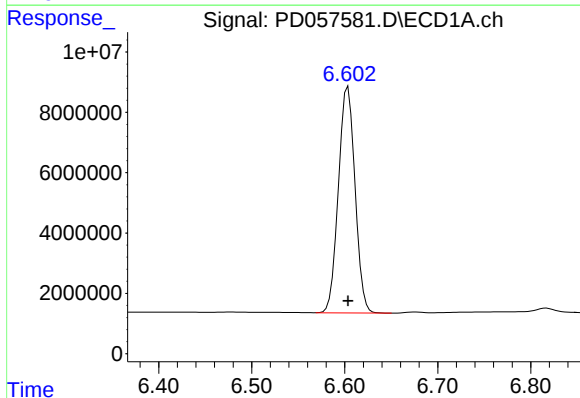


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 93294638
Conc: 379.50 ng/ml

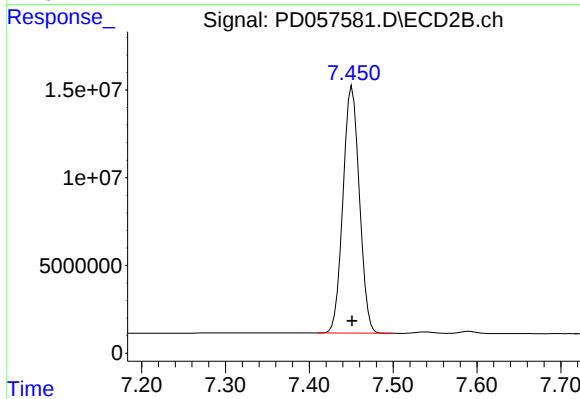

#20 Methoxychlor


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 191411465
Conc: 385.56 ng/ml

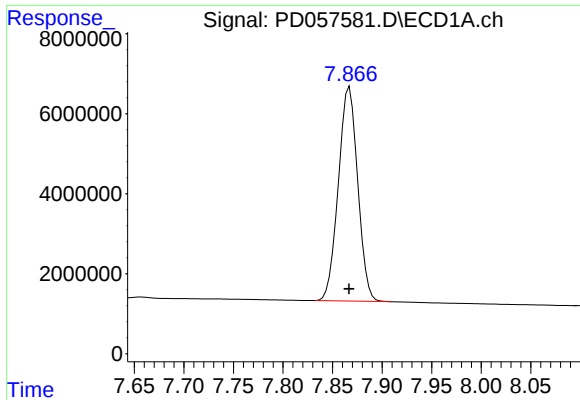

#27 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 72720484
Conc: 74.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

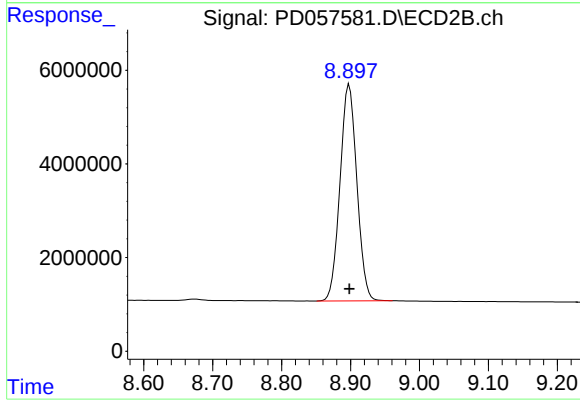

#27 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 78630998
Conc: 73.81 ng/ml