

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
 Data File : PD057583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 22:58
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:21:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:17:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	71129460	79312945	78.571	79.491
27)	SA Decachlor...	7.868	8.898	144.9E6	154.6E6	149.231	145.074
Target Compounds							
2)	A alpha-BHC	3.651	4.281	112.0E6	122.2E6	85.796	86.682
3)	MA gamma-BHC...	3.922	4.561	101.0E6	115.4E6	83.231	85.382
4)	MA Heptachlor	4.202	5.062	74038094	109.0E6	82.015	82.726
9)	A Endosulfan I	5.197	6.099	78860399	99963697	81.875	81.440
13)	MA Dieldrin	5.435	6.354	127.7E6	224.4E6	163.160	166.776
14)	MA Endrin	5.686	6.570	121.8E6	172.9E6	161.156	160.473
16)	A 4,4'-DDD	5.823	6.696	98424284	179.3E6	160.631	164.721
17)	MA 4,4'-DDT	6.056	6.993	112.4E6	171.0E6	169.296	172.085
20)	A Methoxychlor	6.604	7.452	184.1E6	389.5E6	749.014	784.527

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031120\
Data File : PD057583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 22:58
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:21:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:17:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

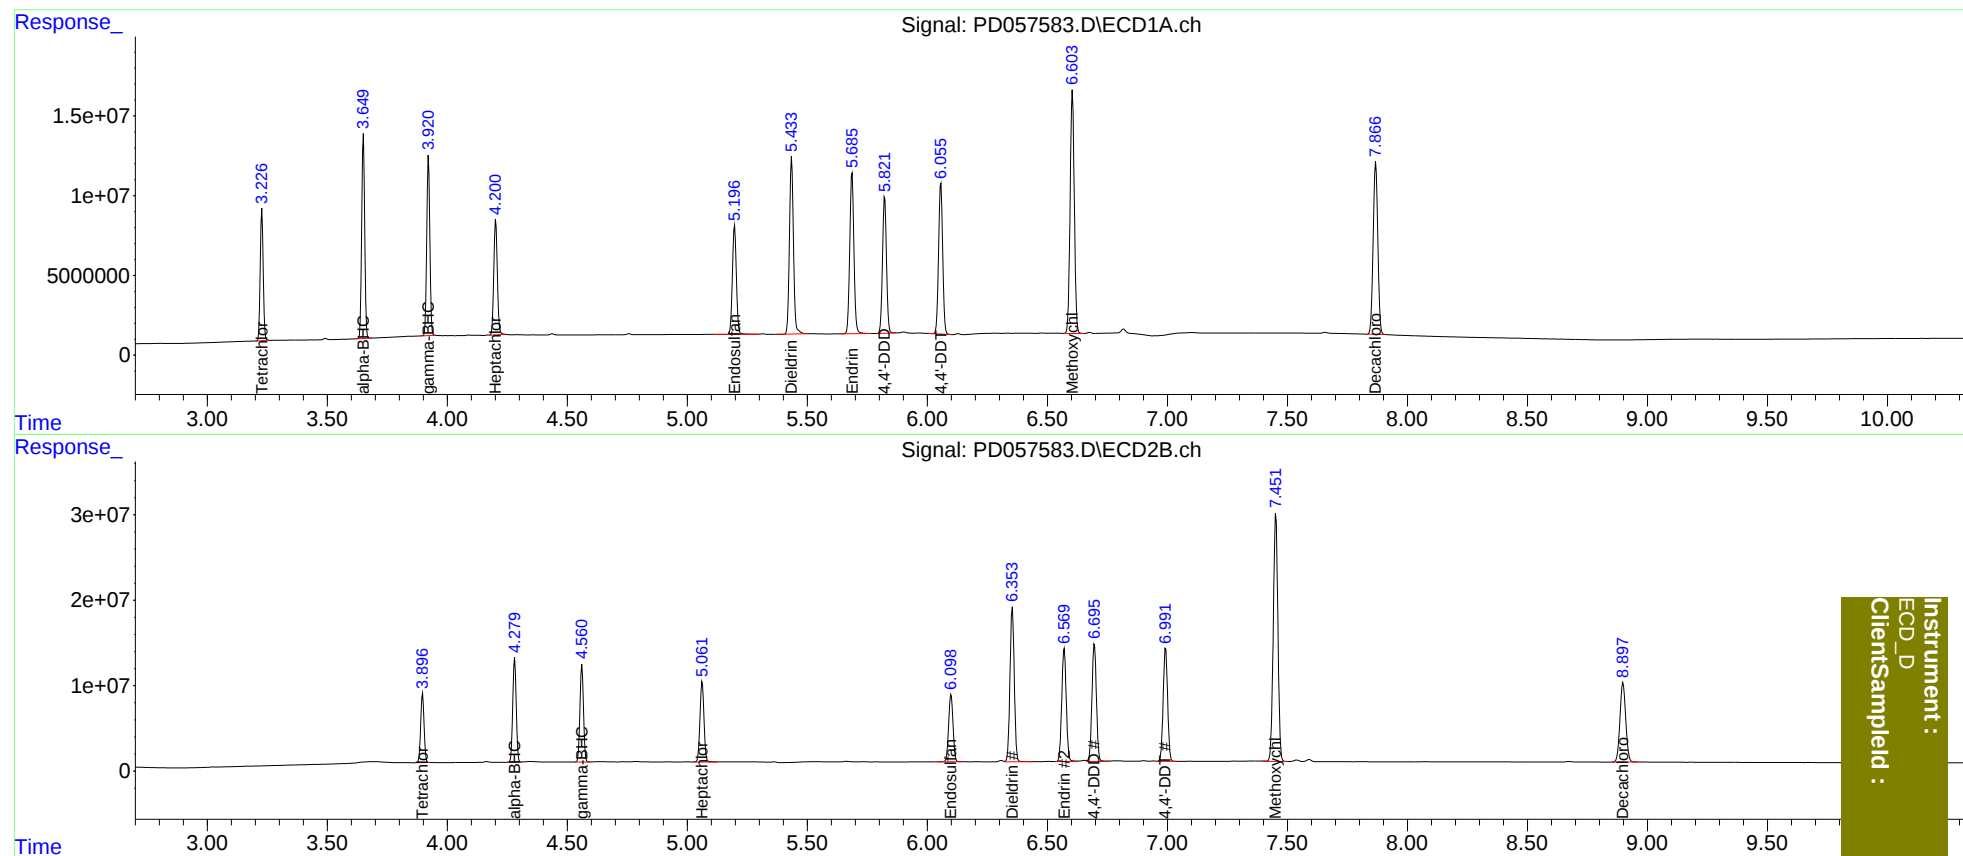


Instrument :
ECD_D
ClientSampled :

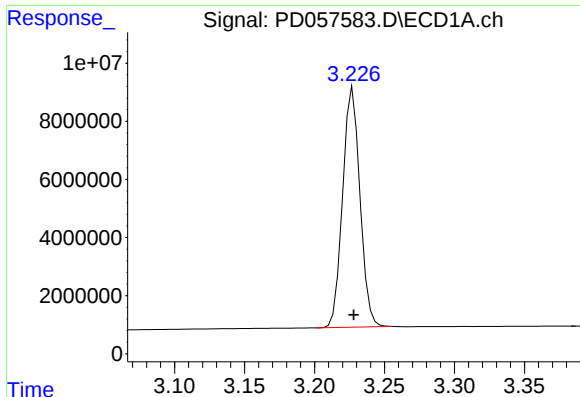

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 71129460
Conc: 78.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

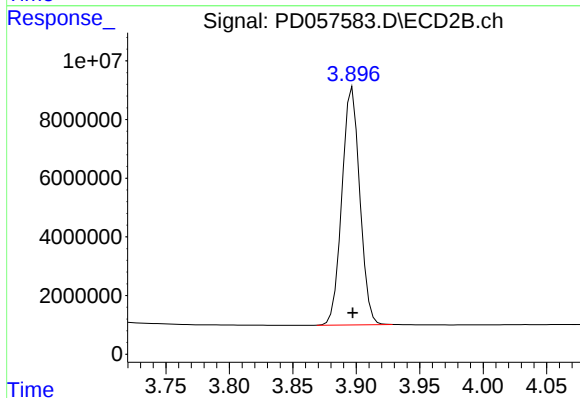


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 79312945
Conc: 79.49 ng/ml

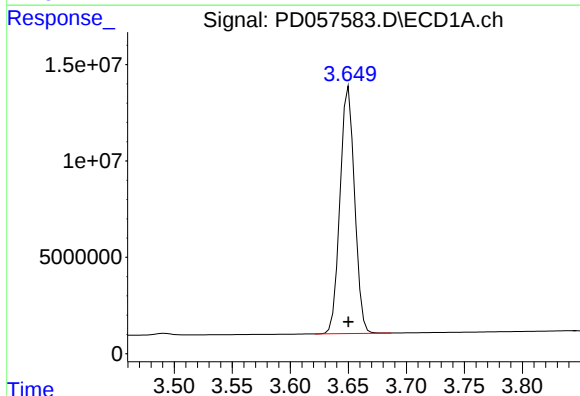


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.000 min
Response: 112015105
Conc: 85.80 ng/ml

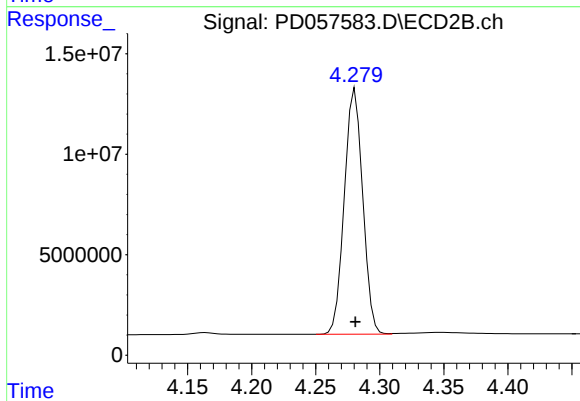

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 122181622
Conc: 86.68 ng/ml

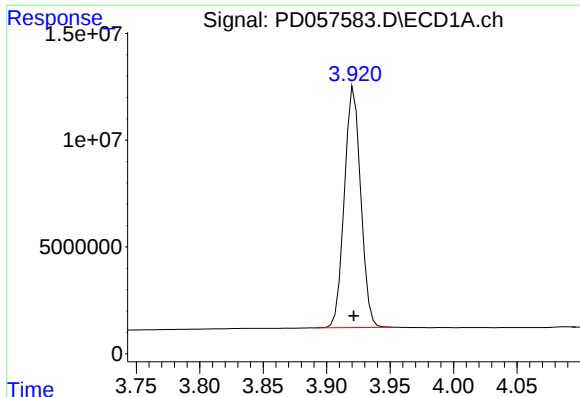

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.000 min
Response: 101001565
Conc: 83.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

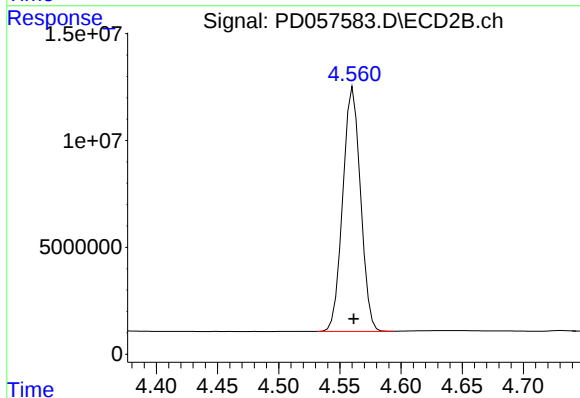


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 115421166
Conc: 85.38 ng/ml

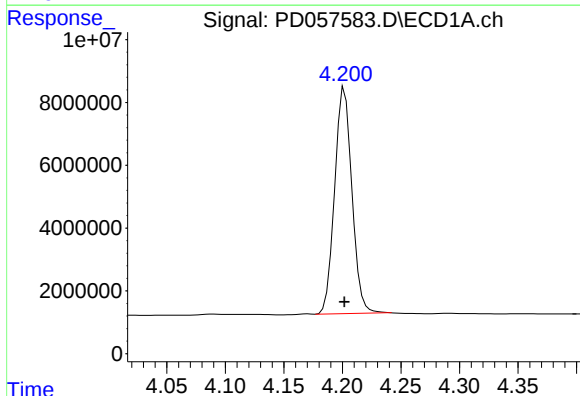


#4 Heptachlor

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 74038094
Conc: 82.02 ng/ml

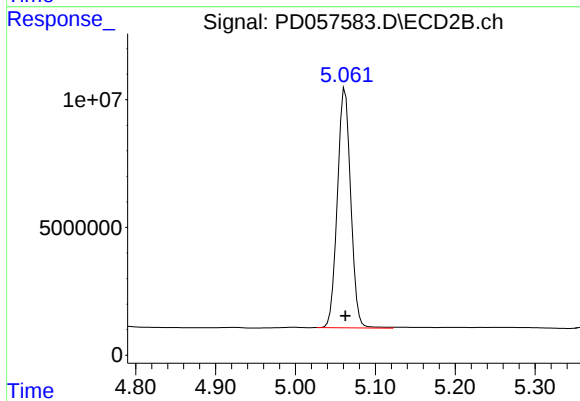

#4 Heptachlor


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 108951806
Conc: 82.73 ng/ml

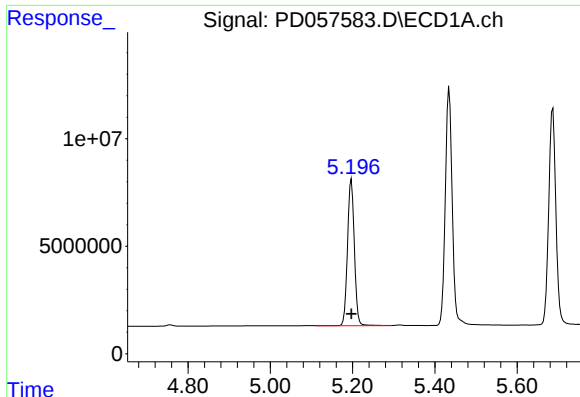

#9 Endosulfan I


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 78860399
Conc: 81.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

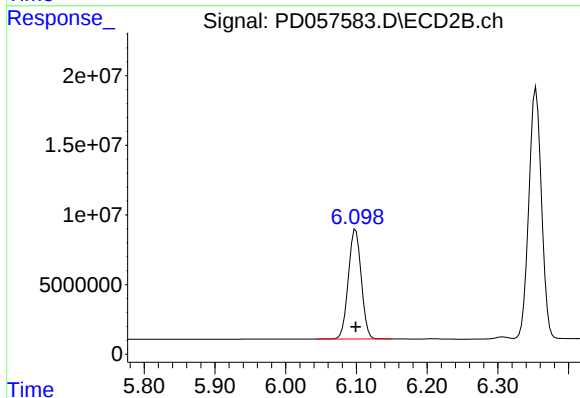


#9 Endosulfan I

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 99963697
Conc: 81.44 ng/ml

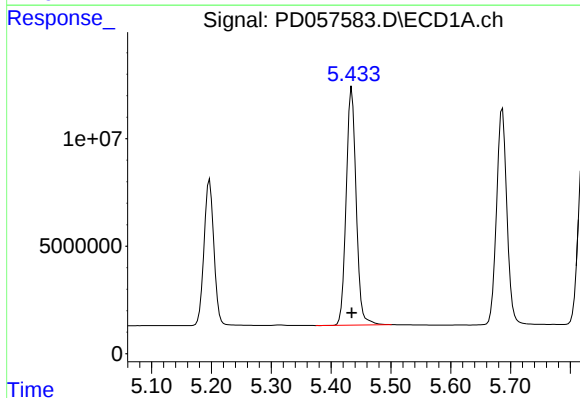


#13 Dieldrin

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 127653166
Conc: 163.16 ng/ml

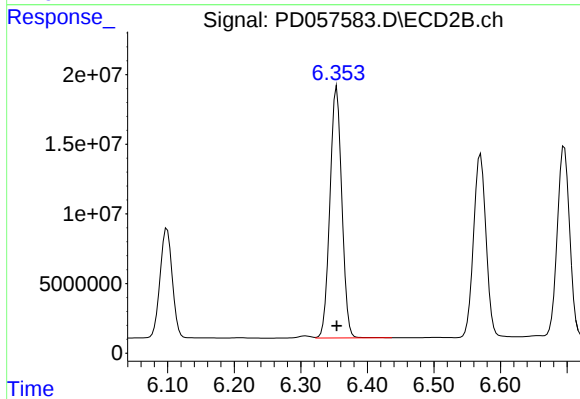

#13 Dieldrin


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 224376132
Conc: 166.78 ng/ml

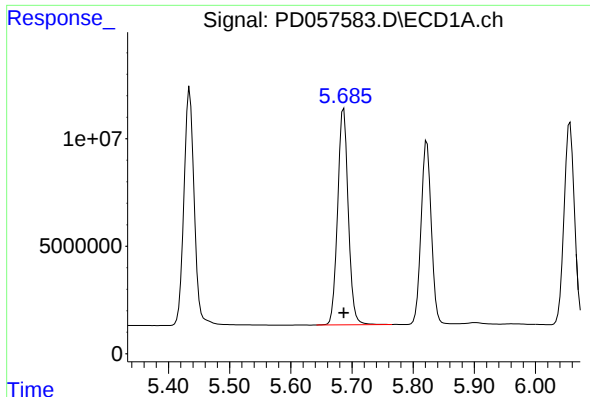

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 121755643
Conc: 161.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

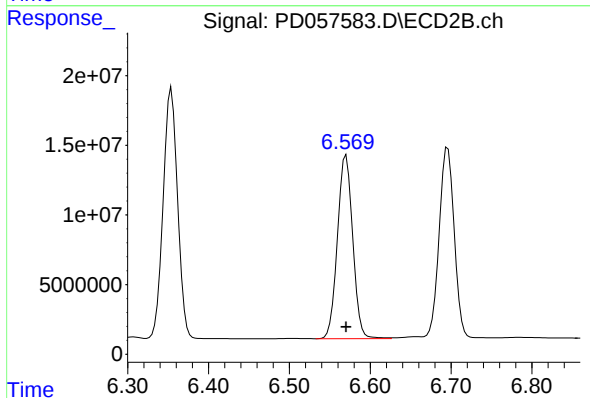


#14 Endrin

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 172919805
Conc: 160.47 ng/ml

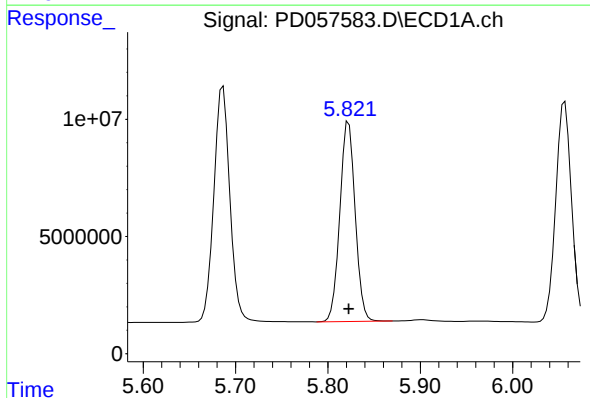


#16 4,4'-DDD

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 98424284
Conc: 160.63 ng/ml

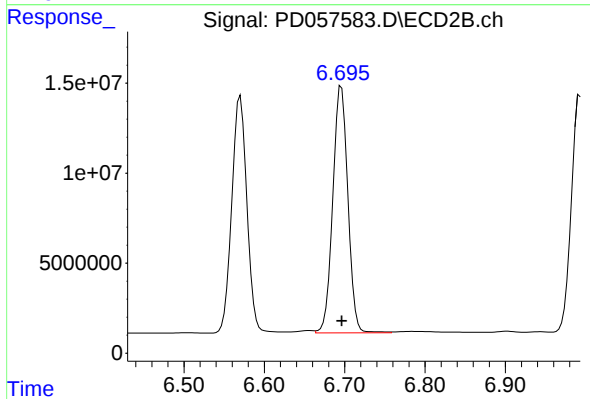

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 179302422
Conc: 164.72 ng/ml

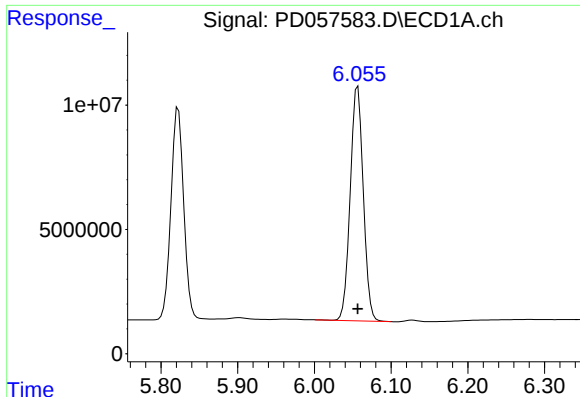

#17 4,4'-DDT


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 112406510
Conc: 169.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

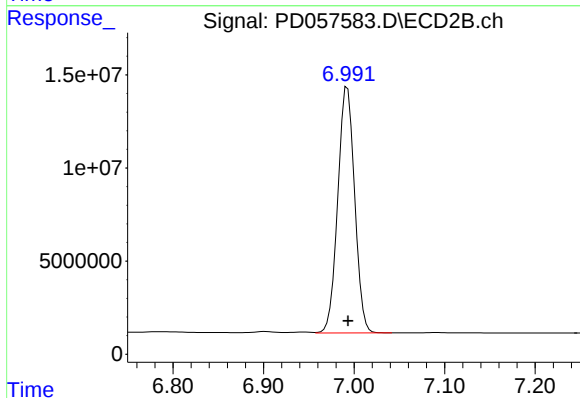


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 170952156
Conc: 172.08 ng/ml

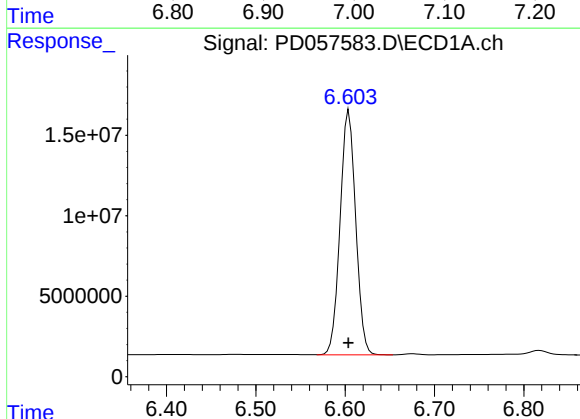


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 184135982
Conc: 749.01 ng/ml

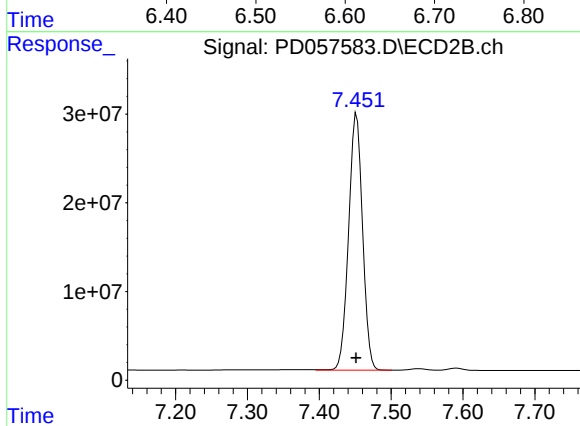

#20 Methoxychlor


R.T.: 7.452 min
Delta R.T.: 0.000 min
Response: 389476671
Conc: 784.53 ng/ml

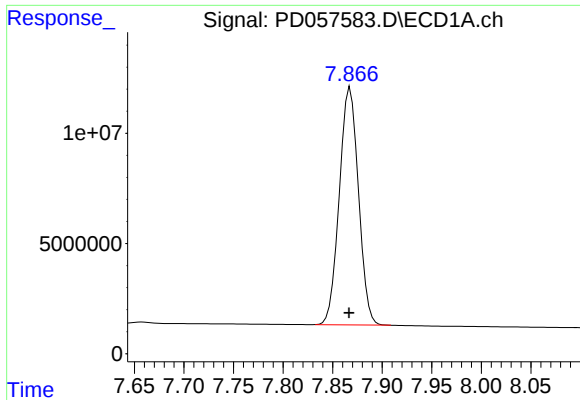

#27 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.001 min
Response: 144913494
Conc: 149.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

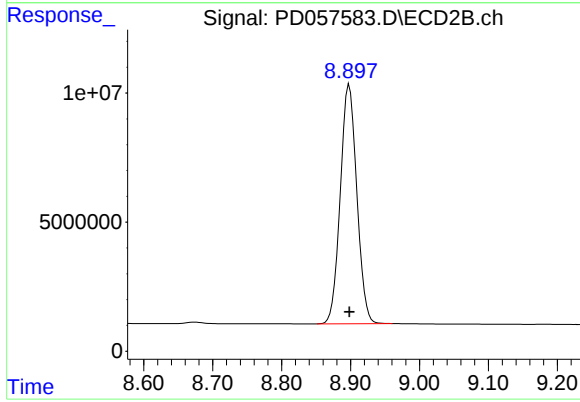

#27 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 154550047
Conc: 145.07 ng/ml