

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031121\
 Data File : PD061546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2021 15:31
 Operator : AR\AJ
 Sample : M1608-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HD-02-030921

Manual Integrations
 APPROVED

Ankita
 3/12/2021 11:36:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 07:38:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 04:34:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.981	11100417	95679310	13.848	11.468m
28)	SA Decachlor...	8.259	9.040	16443618	115.0E6	13.635	13.333

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031121\
Data File : PD061546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2021 15:31
Operator : AR\AJ
Sample : M1608-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HD-02-030921


Manual Integrations
APPROVED

Ankita
3/12/2021 11:36:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 07:38:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 04:34:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

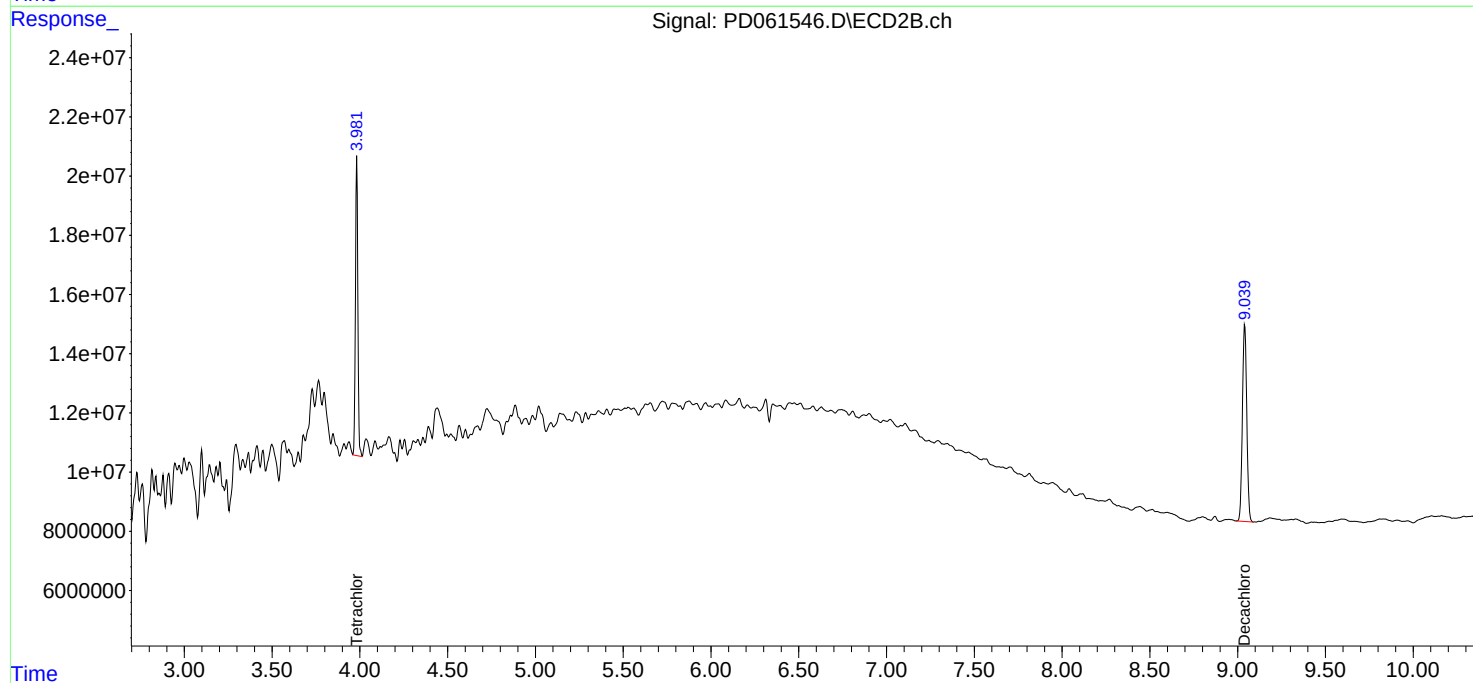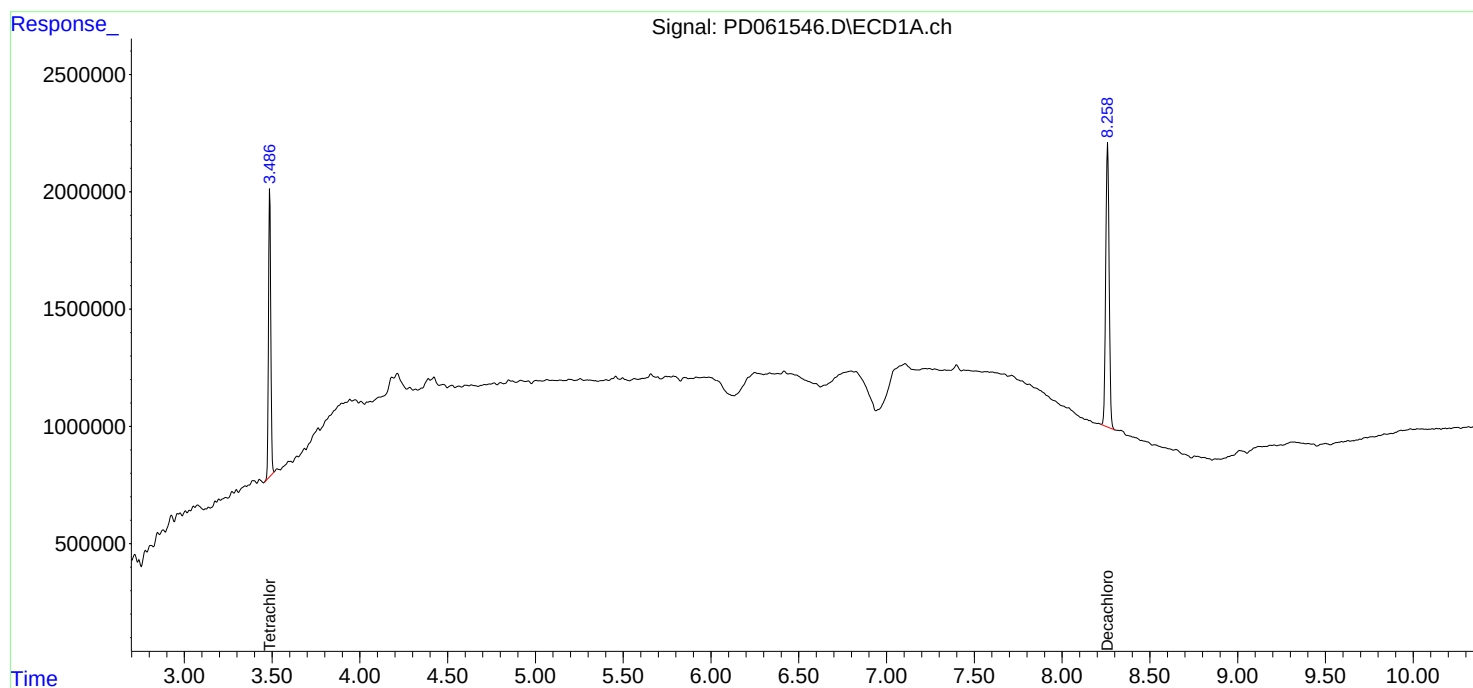

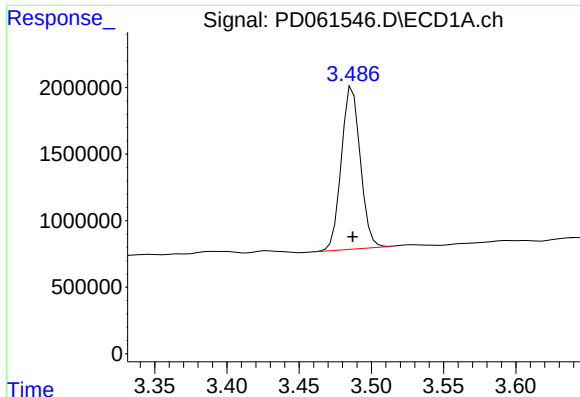


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 11100417
Conc: 13.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
HD-02-030921


Manual Integrations
APPROVED

Ankita
3/12/2021 11:36:38 AM

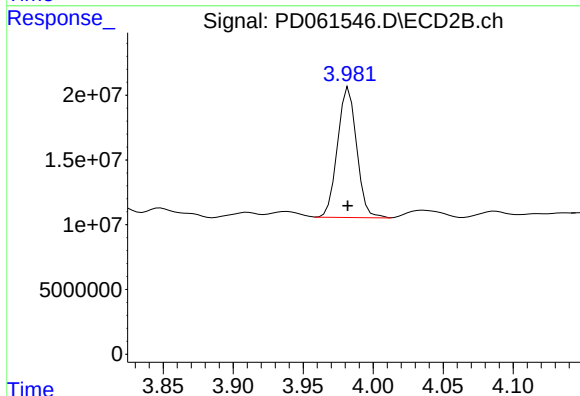


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 95679310
Conc: 11.47 ng/ml m

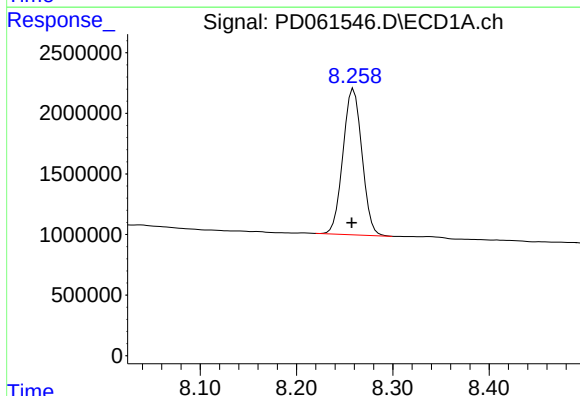

#28 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.002 min
Response: 16443618
Conc: 13.64 ng/ml

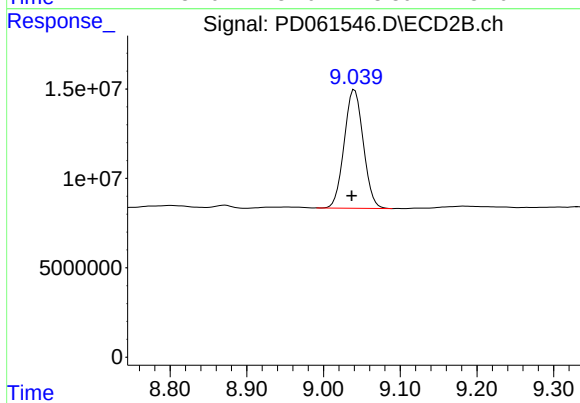

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.004 min
Response: 115040516
Conc: 13.33 ng/ml