

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031122\
 Data File : PD068492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 14:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/14/2022
 Supervised By : Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:13:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	27795487	218.7E6	23.711	22.785
28)	SA Decachlor...	8.210	9.371	26286823	121.6E6	22.589	20.504m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031122\
Data File : PD068492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 14:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/14/2022
Supervised By : Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:13:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

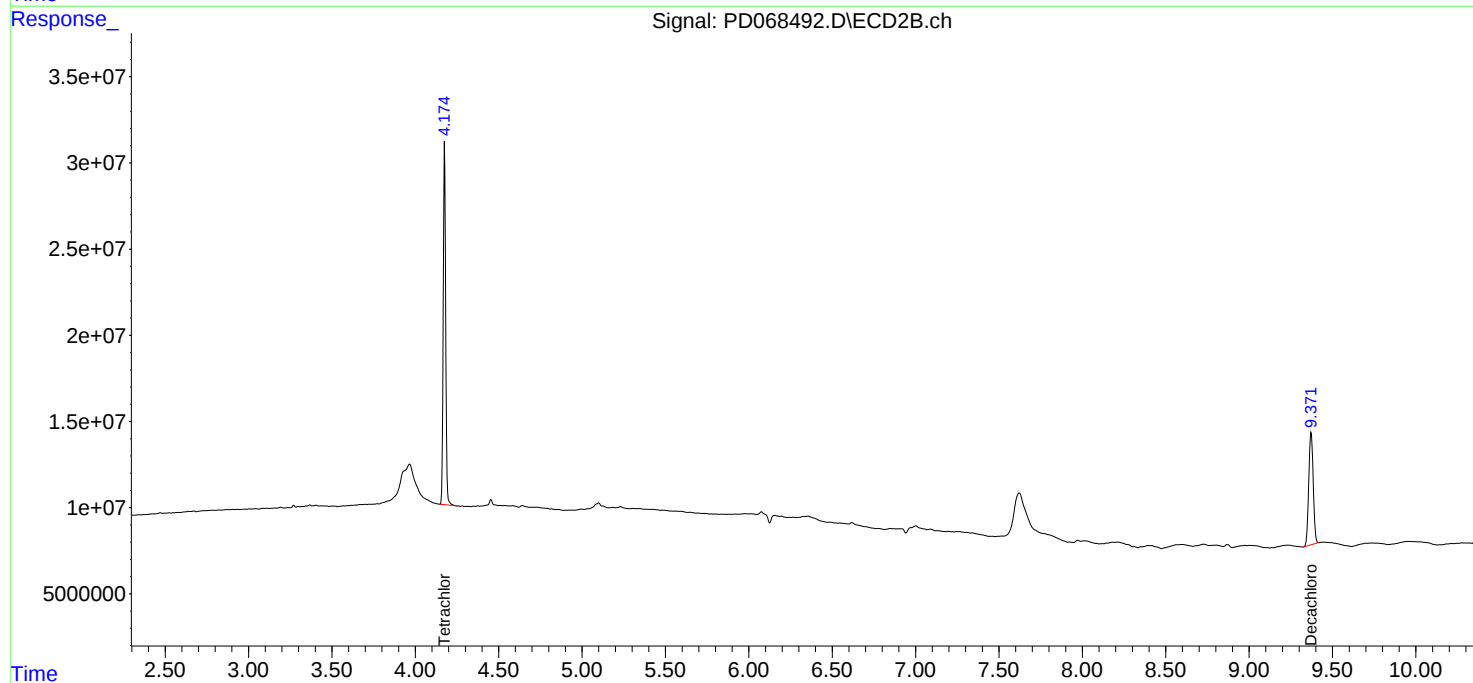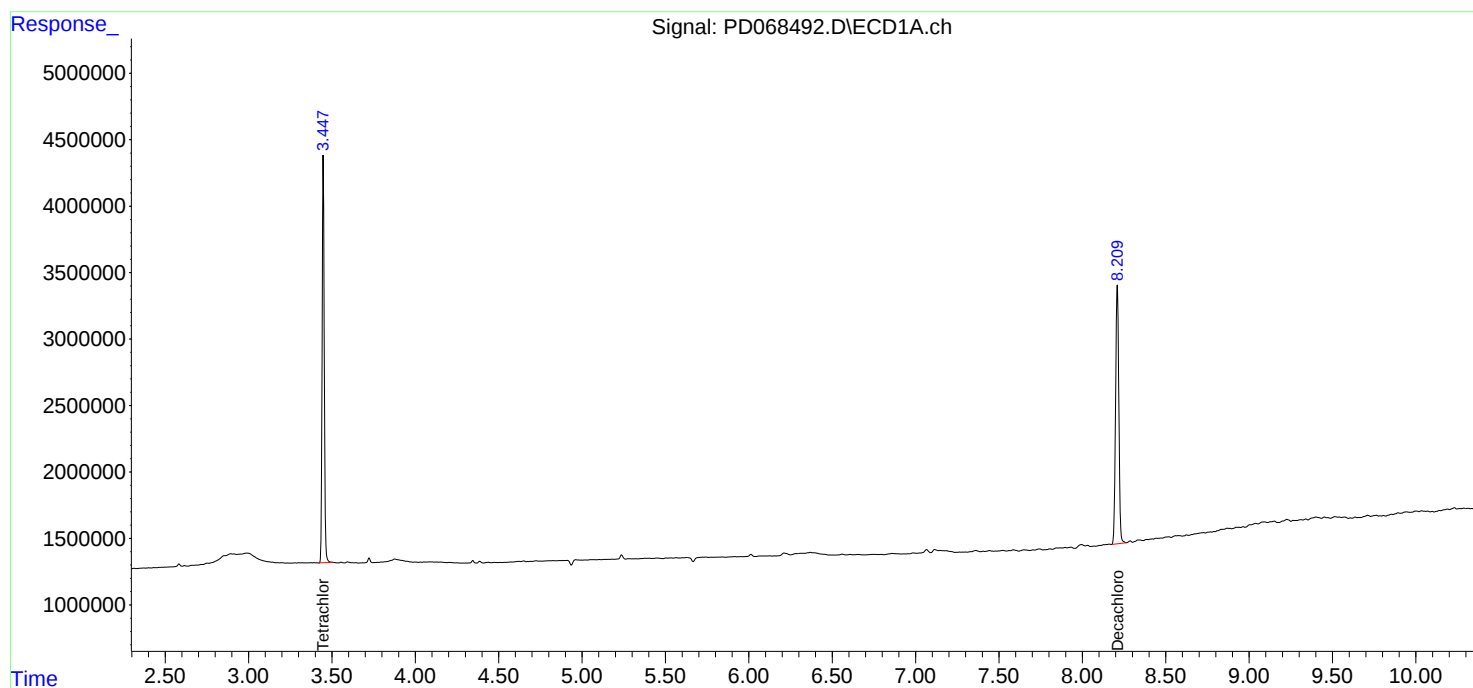

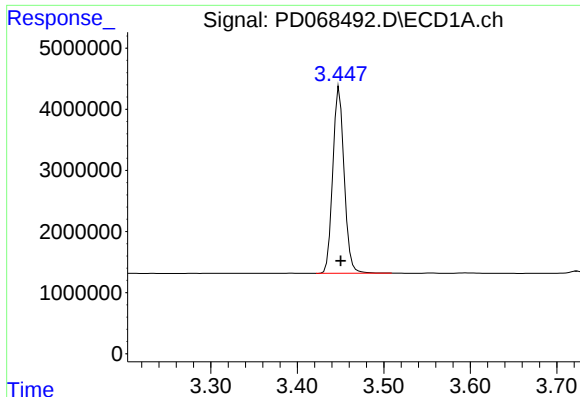


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: -0.001 min
Response: 27795487
Conc: 23.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

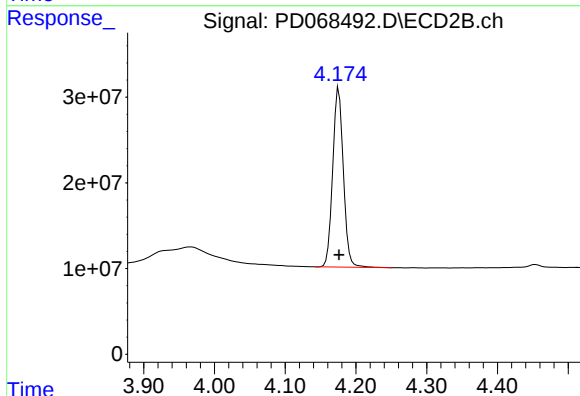


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 218694176
Conc: 22.79 ng/ml

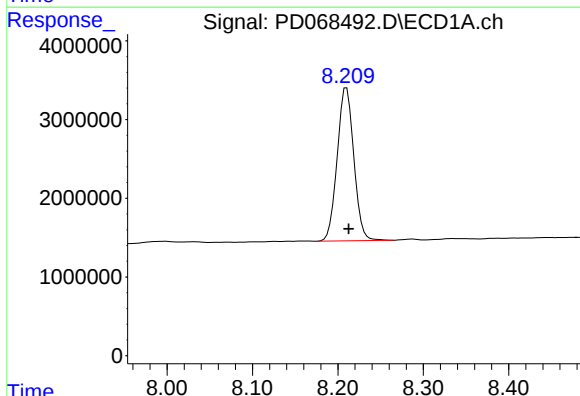

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.003 min
Response: 26286823
Conc: 22.59 ng/ml

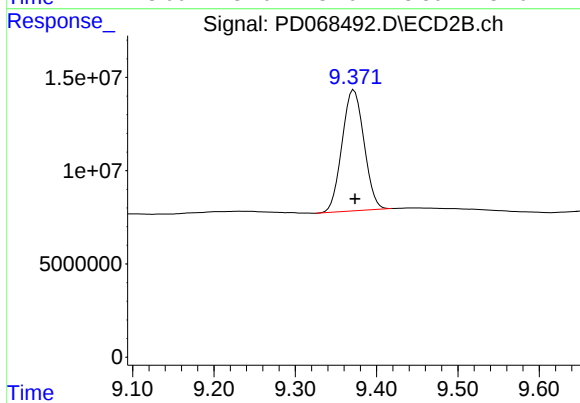

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.003 min
Response: 121566117
Conc: 20.50 ng/ml m