

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031220\
Data File : PD057606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 15:29
Operator : AJ\MA
Sample : INDA329
Misc :
ALS Vial : 99 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA329

Manual Integrations
APPROVED

mohammad
3/17/2020 12:05:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 03:27:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:32:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

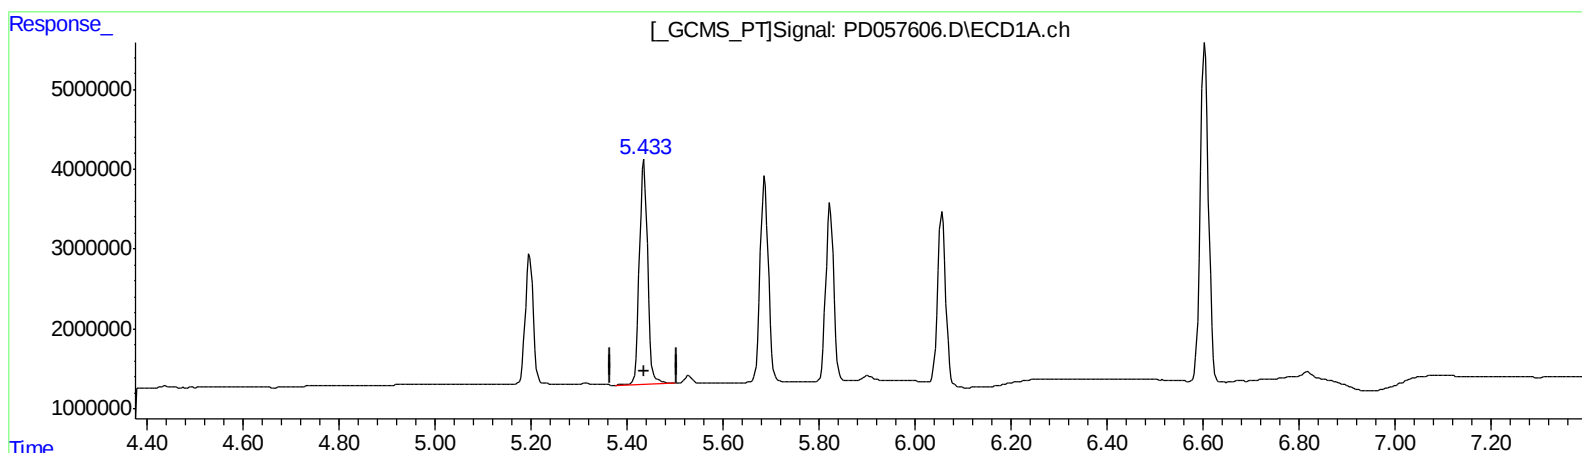

(13) Dieldrin (MA)
5.435min 42.712 ng/ml
response 33757627

(13) Dieldrin #2 (MA)
6.354min 37.736 ng/ml
response 50455978

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031220\
Data File : PD057606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 15:29
Operator : AJ\MA
Sample : INDA329
Misc :
ALS Vial : 99 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA329

Manual Integrations
APPROVED

mohammad
3/17/2020 12:05:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 03:27:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:32:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

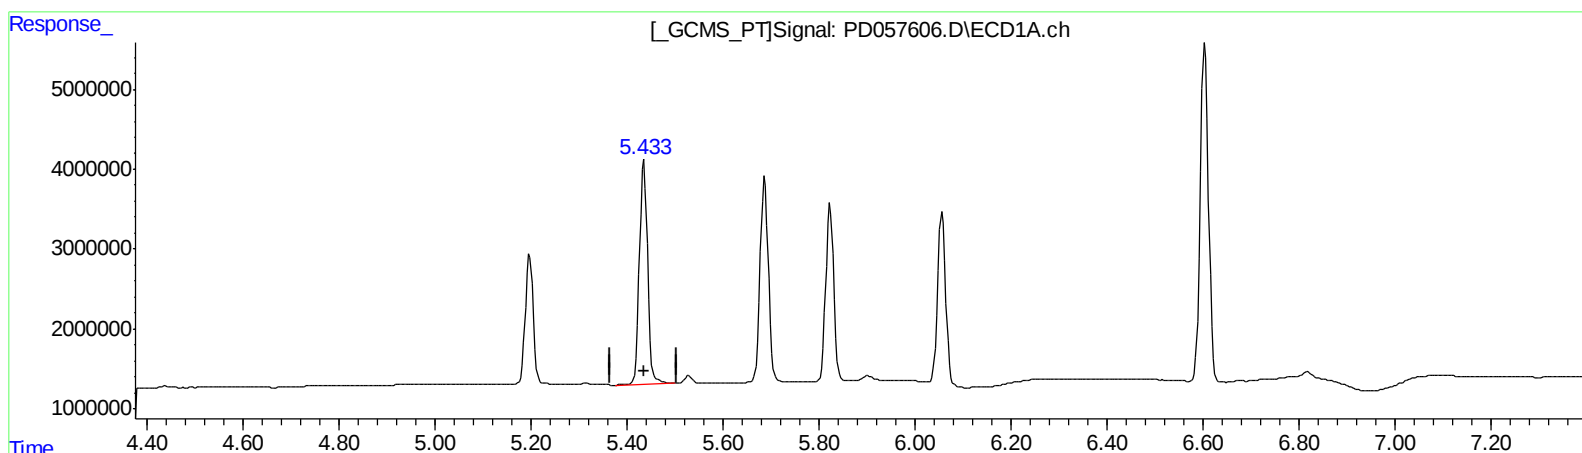

(13) Dieldrin (MA)
5.435min 42.712 ng/ml
response 33757627

(13) Dieldrin #2 (MA)
6.353min 38.060 ng/ml m
response 50889214

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031220\
 Data File : PD057606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 15:29
 Operator : AJ\MA
 Sample : INDA329
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA329

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 03:27:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:32:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

mohammad
 3/17/2020 12:05:43 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.227	3.897	16852608	18760799	18.456	18.906
27) SA Decachlor...	7.867	8.898	35360140	39721087	36.316	37.510
Target Compounds						
2) A alpha-BHC	3.650	4.280	24546882	26520453	18.574	18.819
3) MA gamma-BHC...	3.922	4.561	23183987	25778138	18.624	19.091
4) MA Heptachlor	4.202	5.062	18374441	25752480	20.074	19.518
9) A Endosulfan I	5.197	6.099	18634086	23383297	19.083	18.971
13) MA Dieldrin	5.435	6.353	33757627	50889214	42.712	38.060m
14) MA Endrin	5.686	6.570	31157401	41023039	40.970	38.508
16) A 4,4'-DDD	5.823	6.696	25574929	41870237	41.284	38.640
17) MA 4,4'-DDT	6.056	6.993	25506605	39313827	38.300	40.102
20) A Methoxychlor	6.603	7.452	50817545	103.6E6	207.543	210.504

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

2 SJ
 03/18/20