

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031221\
 Data File : PD061551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 08:56
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 00:39:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 04:34:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.970	0	307707	N.D.	0.037 #
Target Compounds							
2)	A alpha-BHC	3.927	0.000	181614	0	0.147	N.D. #
6)	B beta-BHC	4.471	0.000	539132	0	1.020	N.D. #
7)	B delta-BHC	0.000	5.055f	0	944307	N.D.	0.079 #
8)	B Heptachlo...	0.000	5.844	0	60231581	N.D.	5.534 #
9)	A Endosulfan I	0.000	6.188f	0	27444010	N.D.	2.638 #
11)	B alpha-Chl...	0.000	6.188f	0	27444010	N.D.	2.517 #
14)	MA Endrin	6.054	0.000	1214591	0	1.150	N.D. #
26)	Chlordane-4	0.000	6.188f	0	27444010	N.D.	13.608 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031221\
Data File : PD061551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 08:56
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 00:39:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 04:34:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

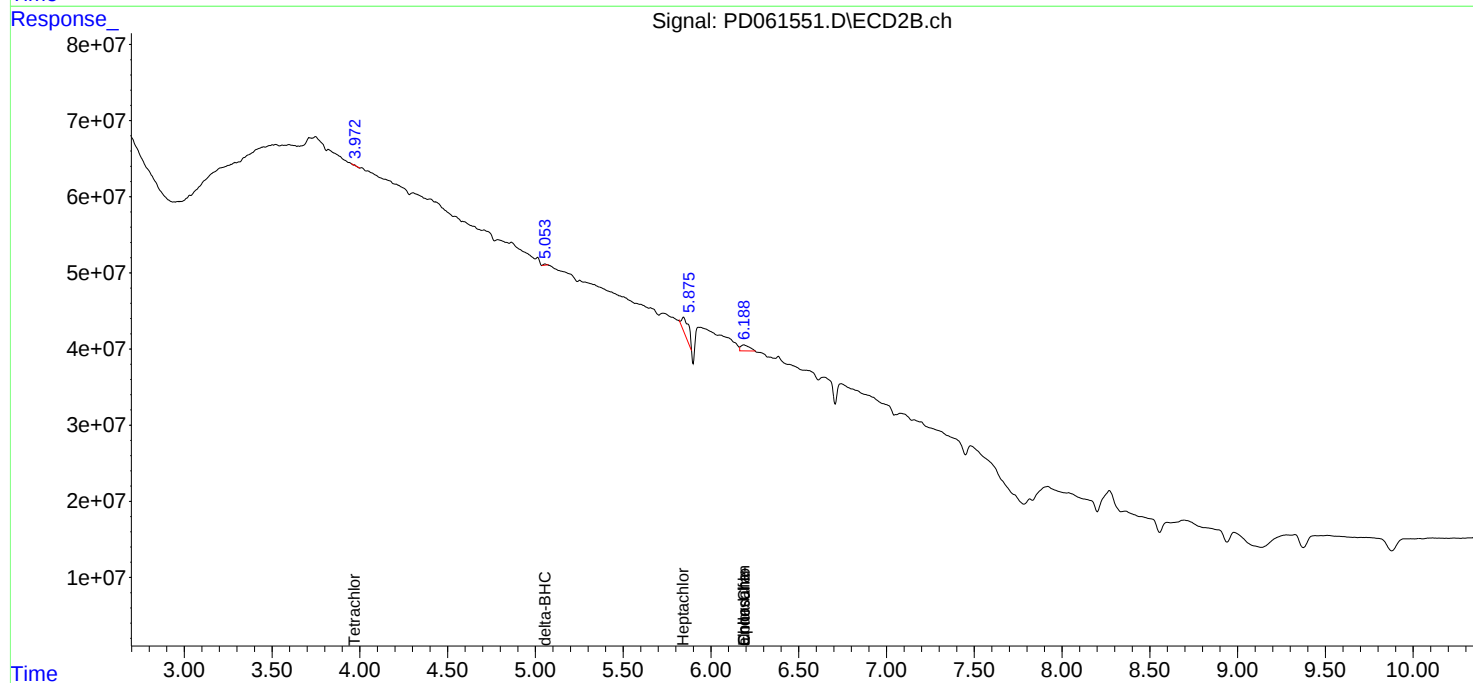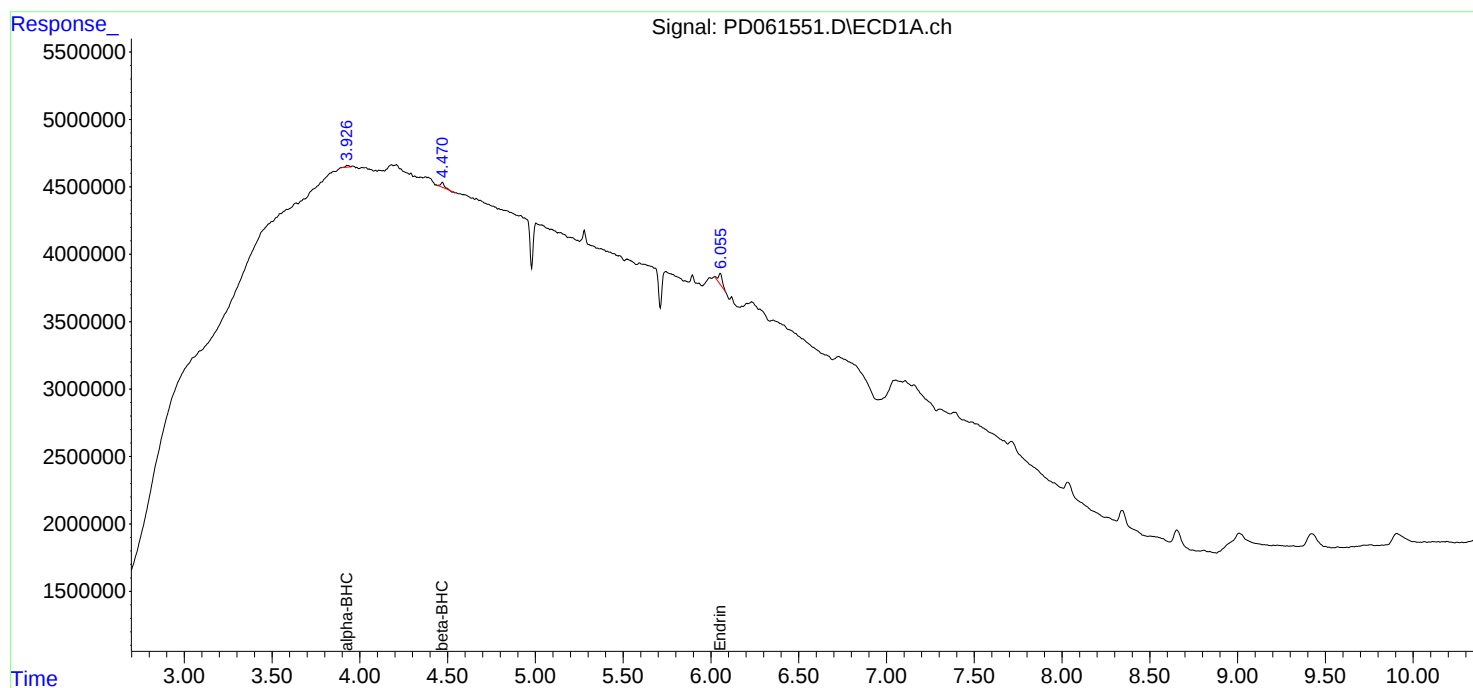


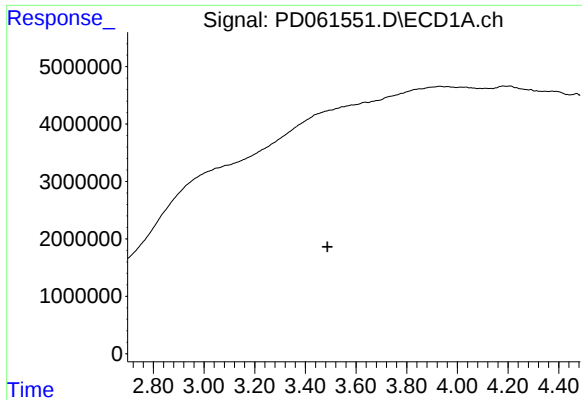

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

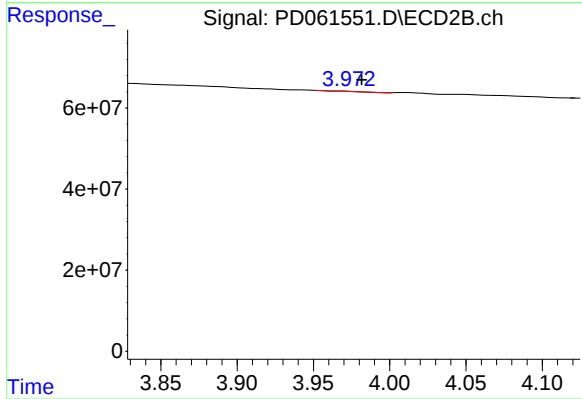


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.012 min
Response: 307707
Conc: 0.04 ng/ml

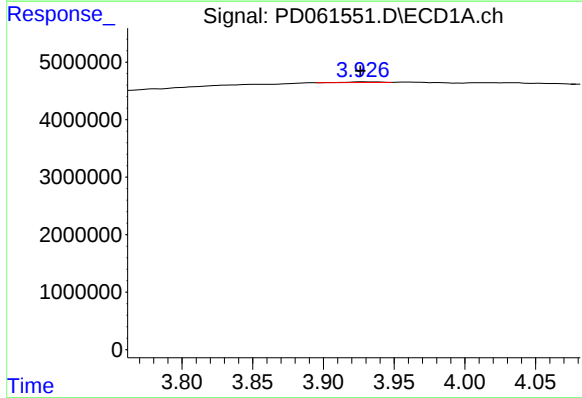


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.001 min
Response: 181614
Conc: 0.15 ng/ml

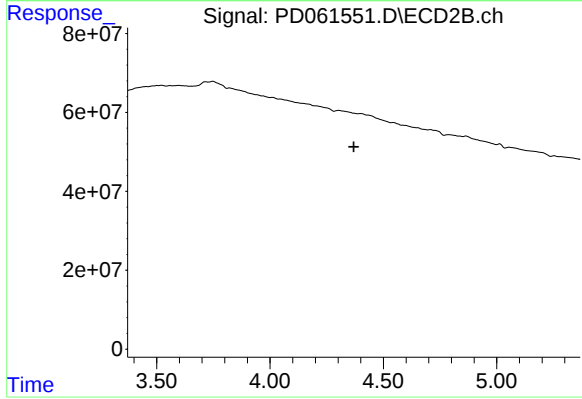

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.370 min
Response: 0
Conc: N.D.

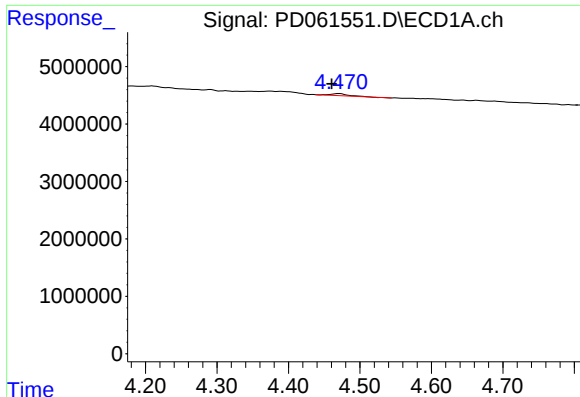

#6 beta-BHC


R.T.: 4.471 min
Delta R.T.: 0.010 min
Response: 539132
Conc: 1.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

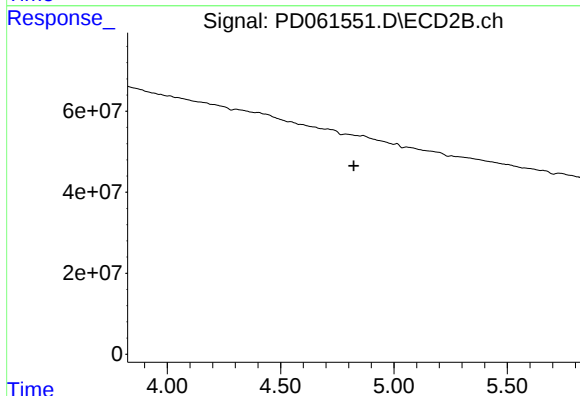


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.823 min
Response: 0
Conc: N.D.

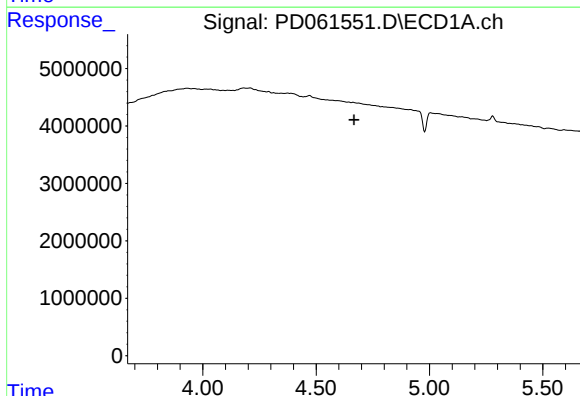


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.667 min
Response: 0
Conc: N.D.

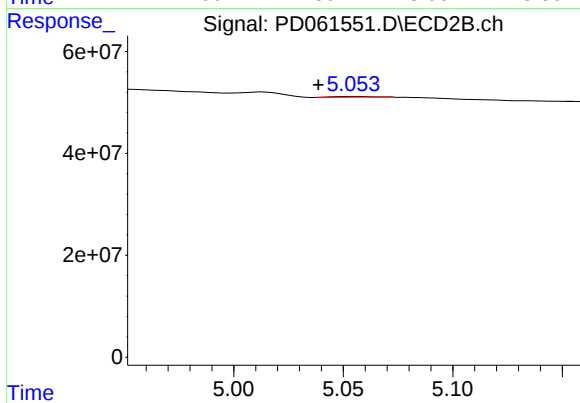

#7 delta-BHC


R.T.: 5.055 min
Delta R.T.: 0.017 min
Response: 944307
Conc: 0.08 ng/ml

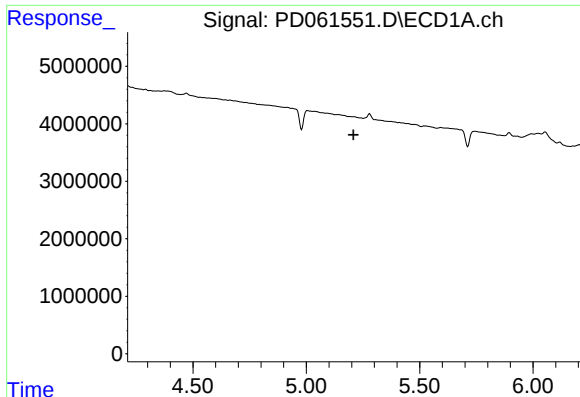

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.208 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

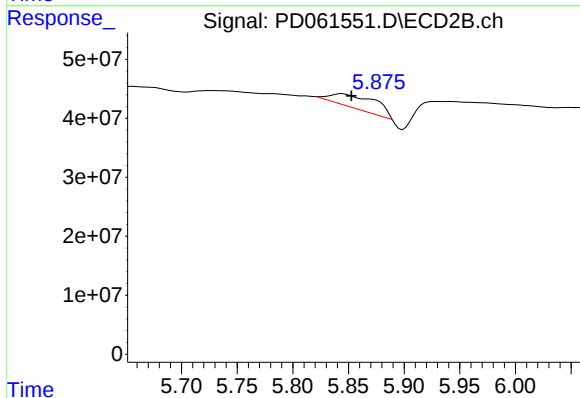


#8 Heptachlor epoxide

R.T.: 5.844 min
Delta R.T.: -0.008 min
Response: 60231581
Conc: 5.53 ng/ml

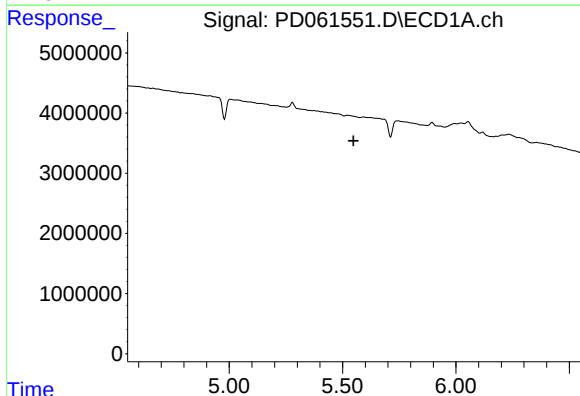


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

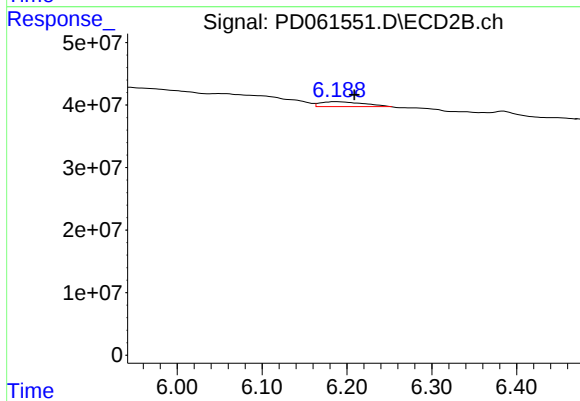

#9 Endosulfan I


R.T.: 6.188 min
Delta R.T.: -0.021 min
Response: 27444010
Conc: 2.64 ng/ml

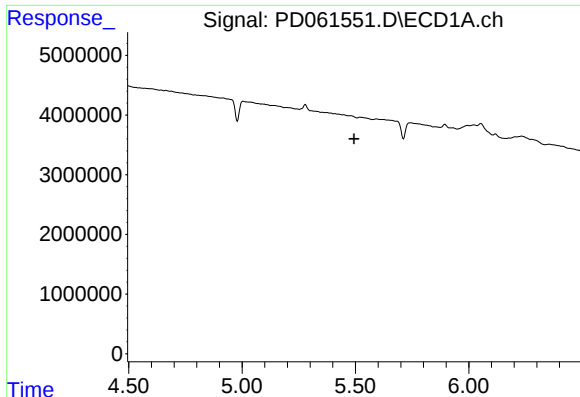

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

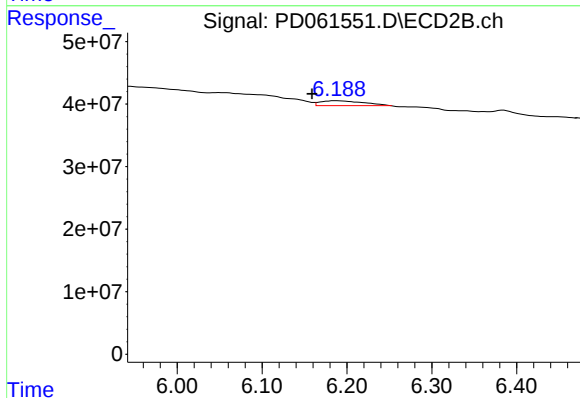


#11 alpha-Chlordane

R.T.: 6.188 min
Delta R.T.: 0.029 min
Response: 27444010
Conc: 2.52 ng/ml

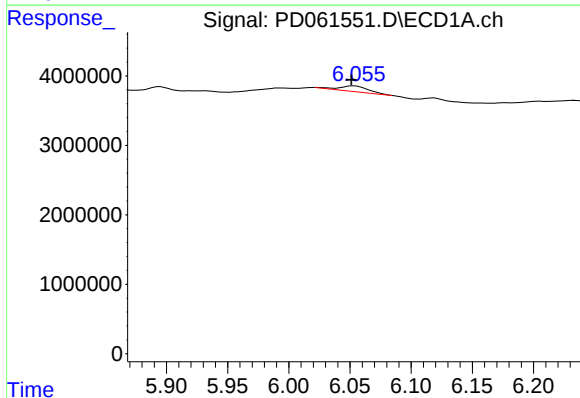


#14 Endrin

R.T.: 6.054 min
Delta R.T.: 0.002 min
Response: 1214591
Conc: 1.15 ng/ml

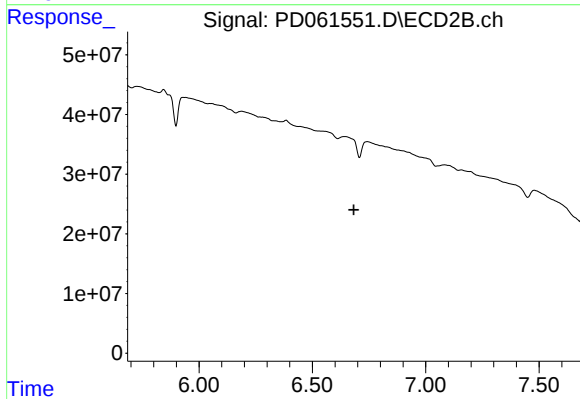

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.683 min
Response: 0
Conc: N.D.

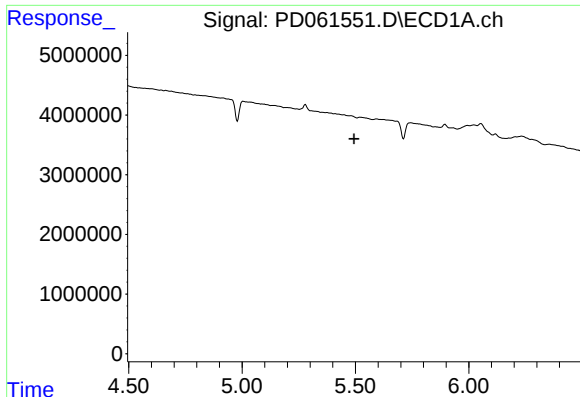

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T. : 5.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

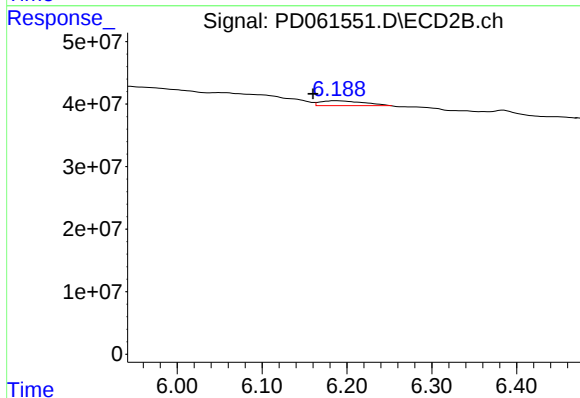


#26 Chlorodane-4

R.T.: 6.188 min
Delta R.T.: 0.028 min
Response: 27444010
Conc: 13.61 ng/ml

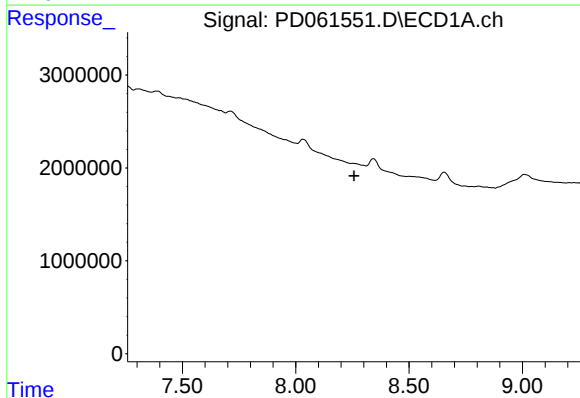

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.257 min
Response: 0
Conc: N.D.

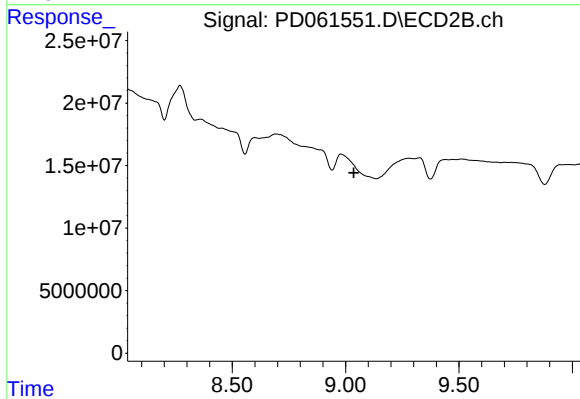

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.037 min
Response: 0
Conc: N.D.