

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
 Data File : PS014217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 09:45
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 03:34:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.466f	0.000	209.1E6	0	151.198	N.D. #
3) T	4-Nitroph...	6.998f	0.000	2416816	0	4.653	N.D. #
5) T	DICAMBA	0.000	7.137f	0	111.3E6	N.D.	68.812
6) T	MCP	0.000	7.137	0	111.3E6	N.D.	83.934
7) T	MCPA	7.744	0.000	5323078	0	1.228	N.D. #
15) T	Picloram	10.972f	11.064f	56852060	9503479	7.123	2.879 #
16) T	DCPA	0.000	10.859f	0	6165518	N.D.	1.837


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
Data File : PS014217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 09:45
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 03:34:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

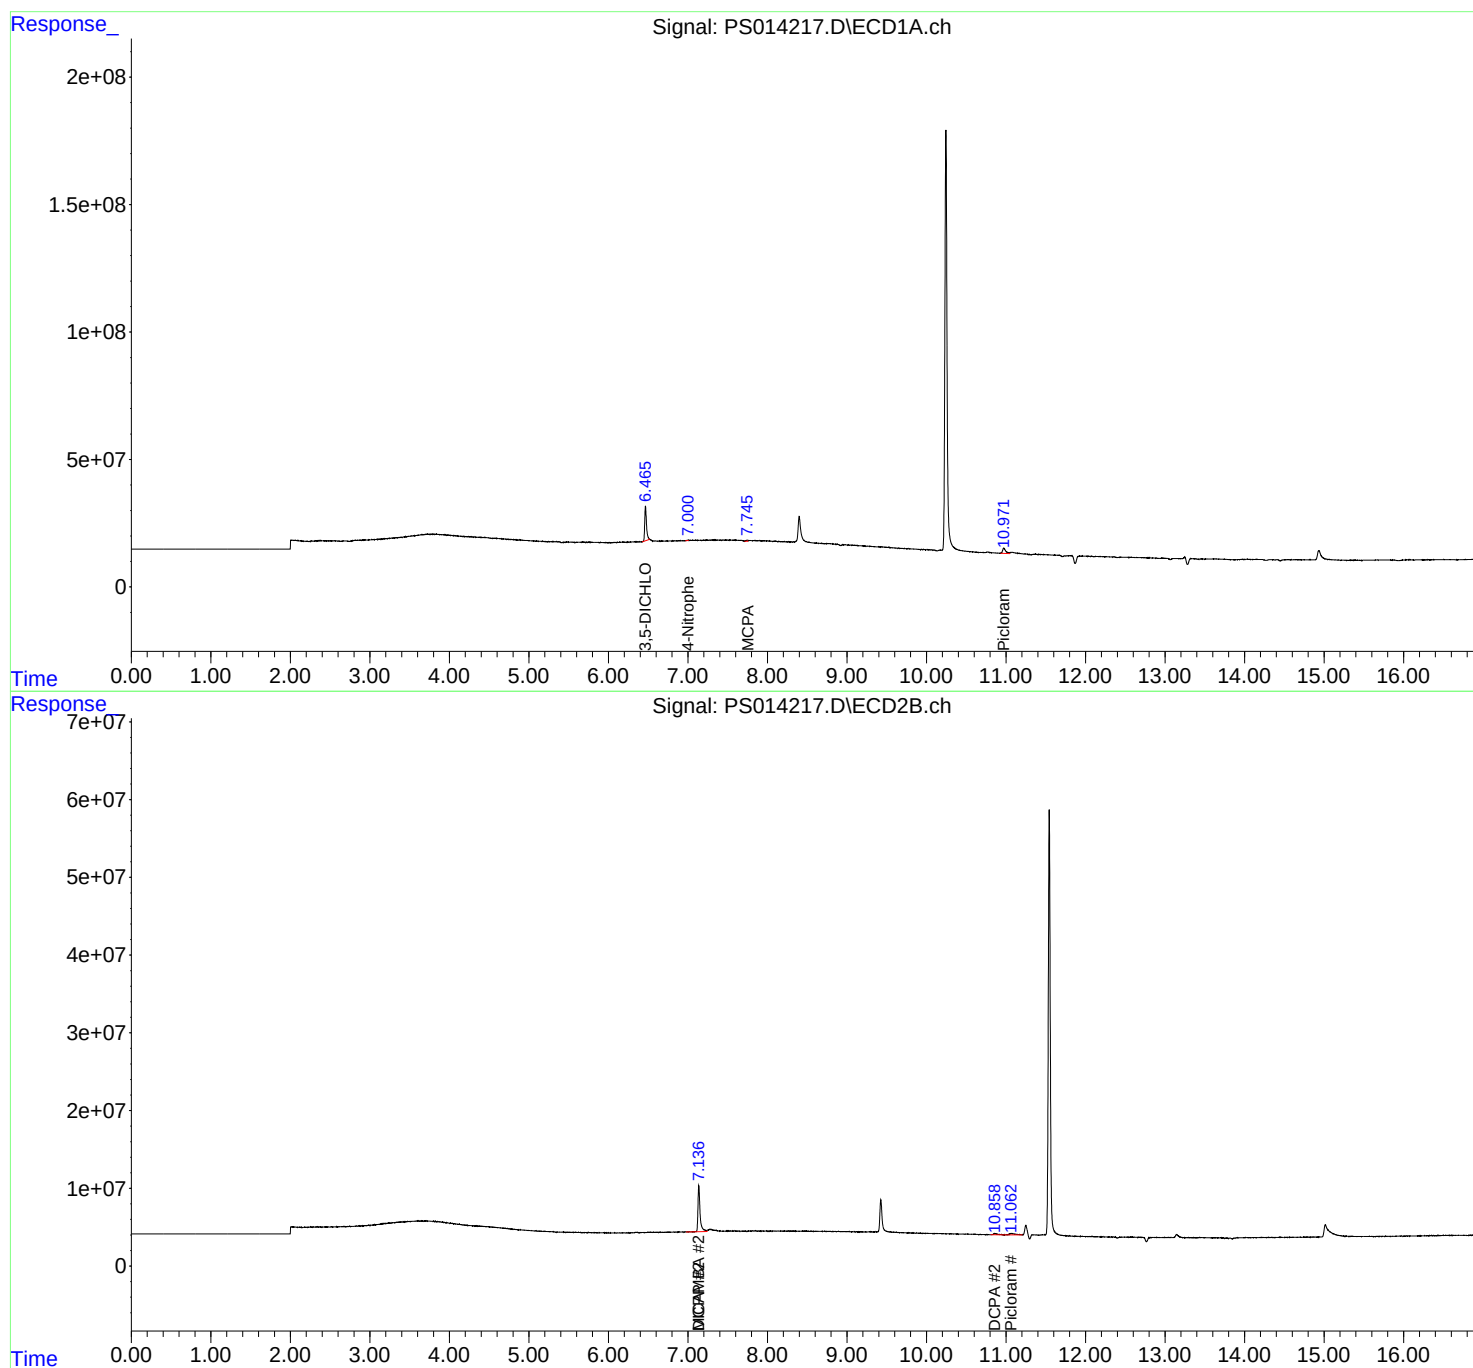


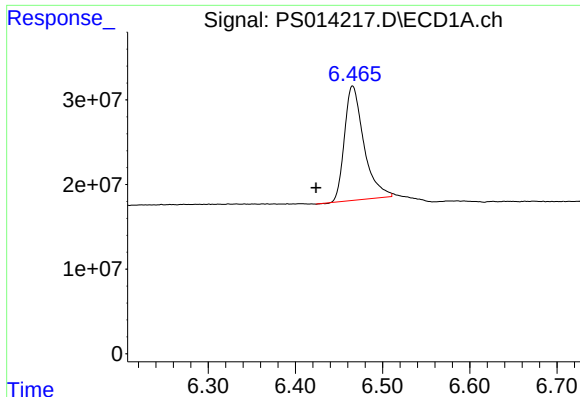

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.466 min
Delta R.T.: 0.042 min
Response: 209092076
Conc: 151.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

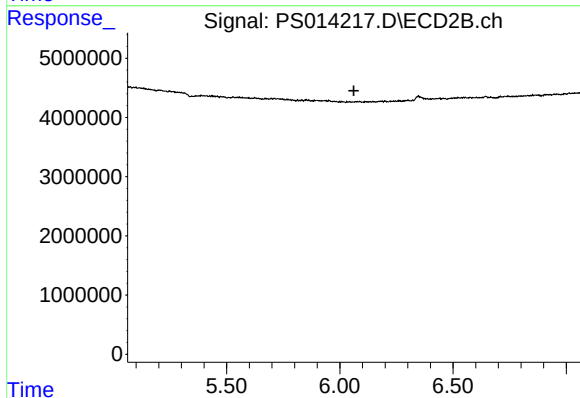


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

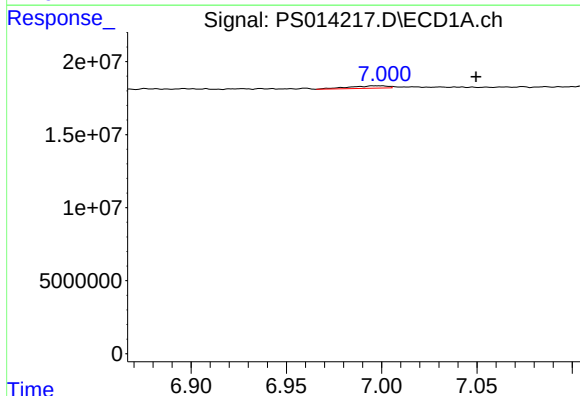


#3 4-Nitrophenol

R.T.: 6.998 min
Delta R.T.: -0.051 min
Response: 2416816
Conc: 4.65 ng/ml

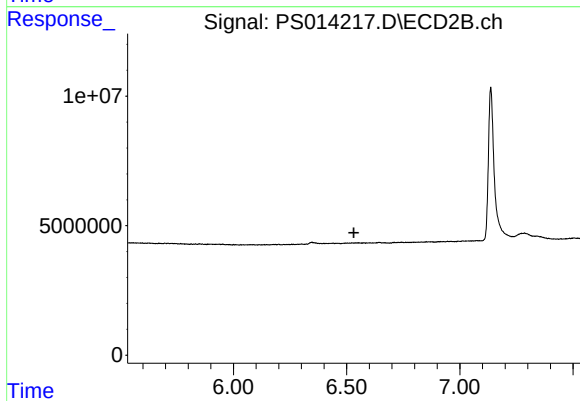

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.532 min
Response: 0
Conc: N.D.

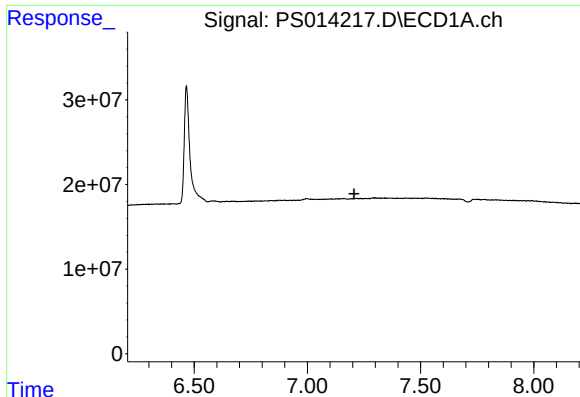

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

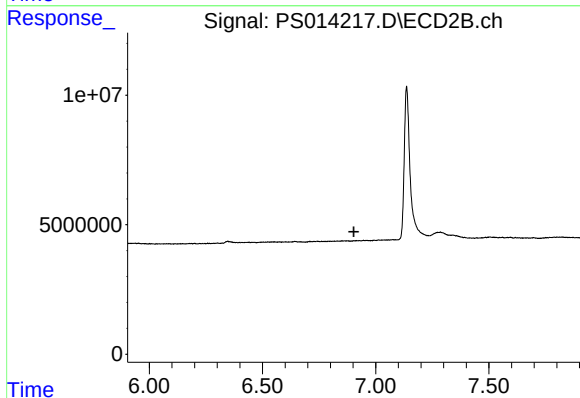


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.904 min
Response: 0
Conc: N.D.

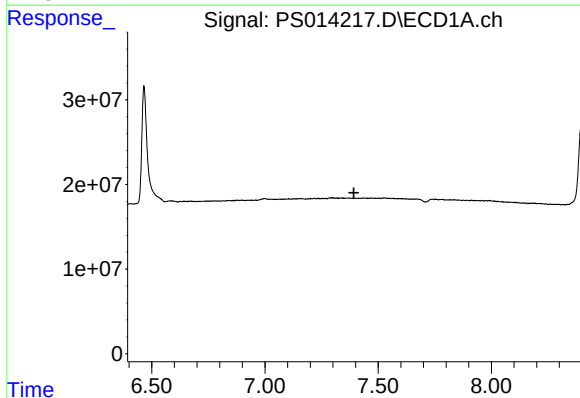


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.393 min
Response: 0
Conc: N.D.

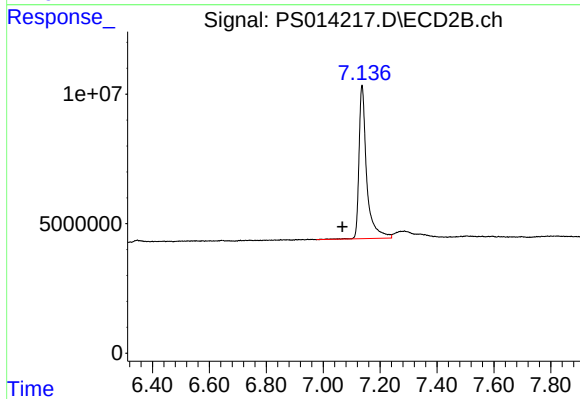

#5 DICAMBA


R.T.: 7.137 min
Delta R.T.: 0.069 min
Response: 111252048
Conc: 68.81 ng/ml

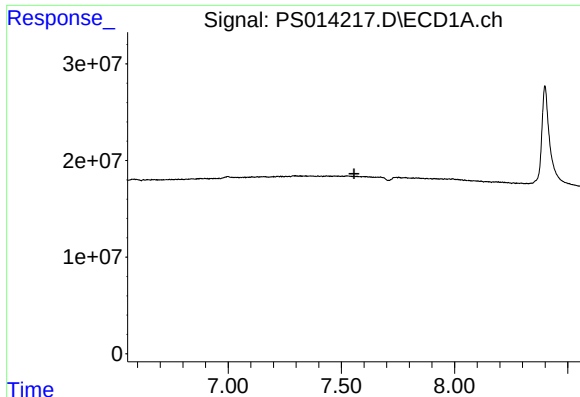

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

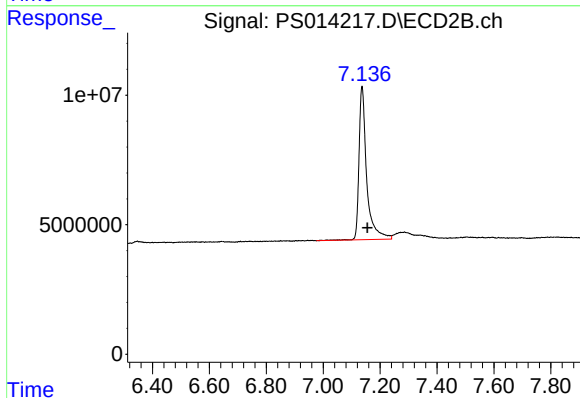


#6 MCPP

R.T.: 7.137 min
Delta R.T.: -0.019 min
Response: 111252048
Conc: 83.93 ug/ml

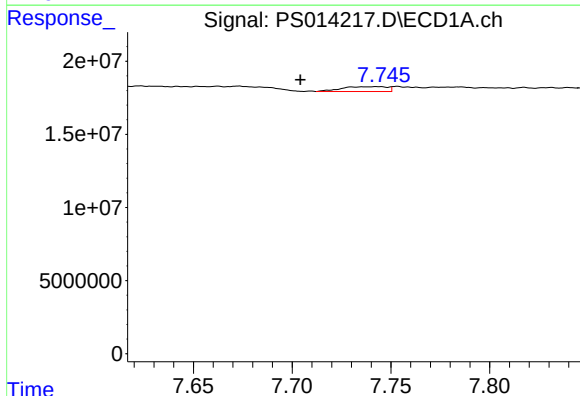


#7 MCPA

R.T.: 7.744 min
Delta R.T.: 0.039 min
Response: 5323078
Conc: 1.23 ug/ml

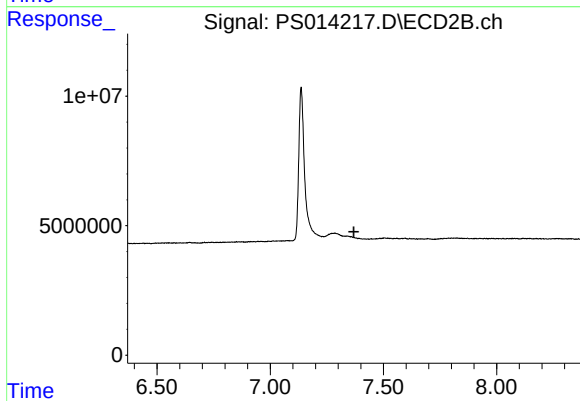

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

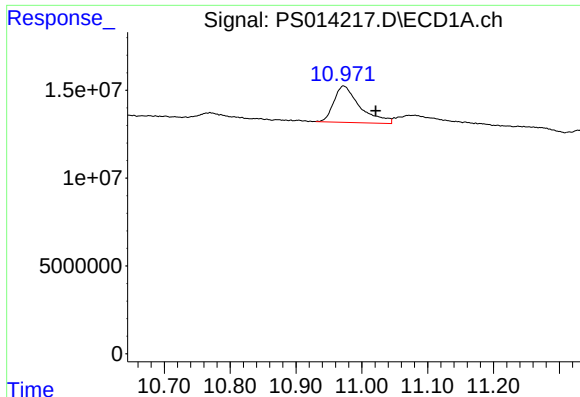

#15 Picloram


R.T.: 10.972 min
Delta R.T.: -0.049 min
Response: 56852060
Conc: 7.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

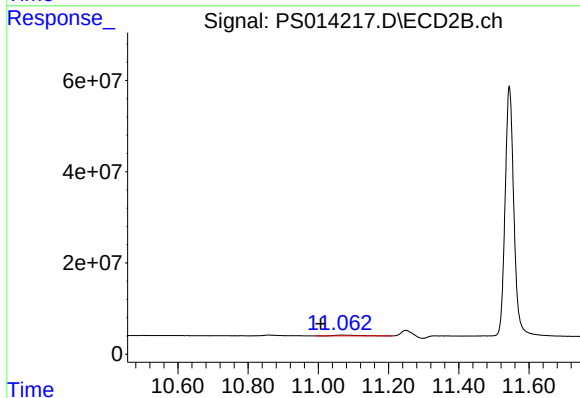


#15 Picloram

R.T.: 11.064 min
Delta R.T.: 0.057 min
Response: 9503479
Conc: 2.88 ng/ml

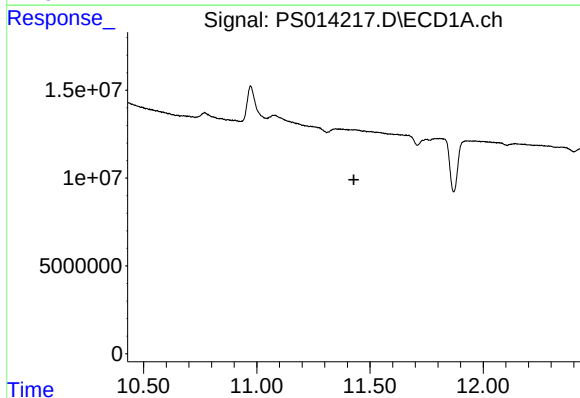

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.428 min
Response: 0
Conc: N.D.

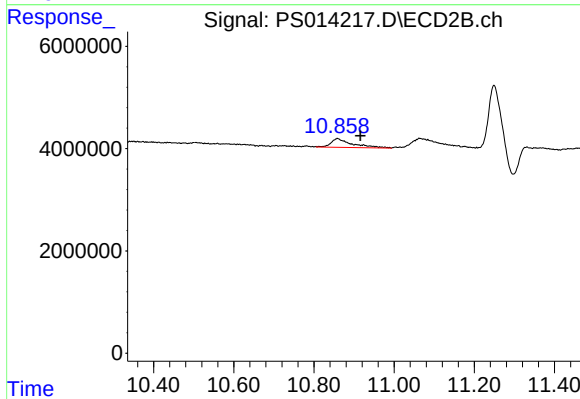

#16 DCPA

R.T.: 10.859 min
Delta R.T.: -0.057 min
Response: 6165518
Conc: 1.84 ng/ml