

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
 Data File : PS014239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2021 00:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 03:40:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.906	479.1E6	206.2E6	475.826	542.023
Target Compounds							
5) T	DICAMBA	0.000	7.051	0	2700005	N.D.	1.670
7) T	MCPA	0.000	7.362	0	1984589	N.D.	1.008
12) T	2,4,5-T	0.000	9.188	0	269493	N.D.	<MDL
14) T	DINOSEB	0.000	10.048f	0	513095	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
Data File : PS014239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2021 00:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 03:40:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

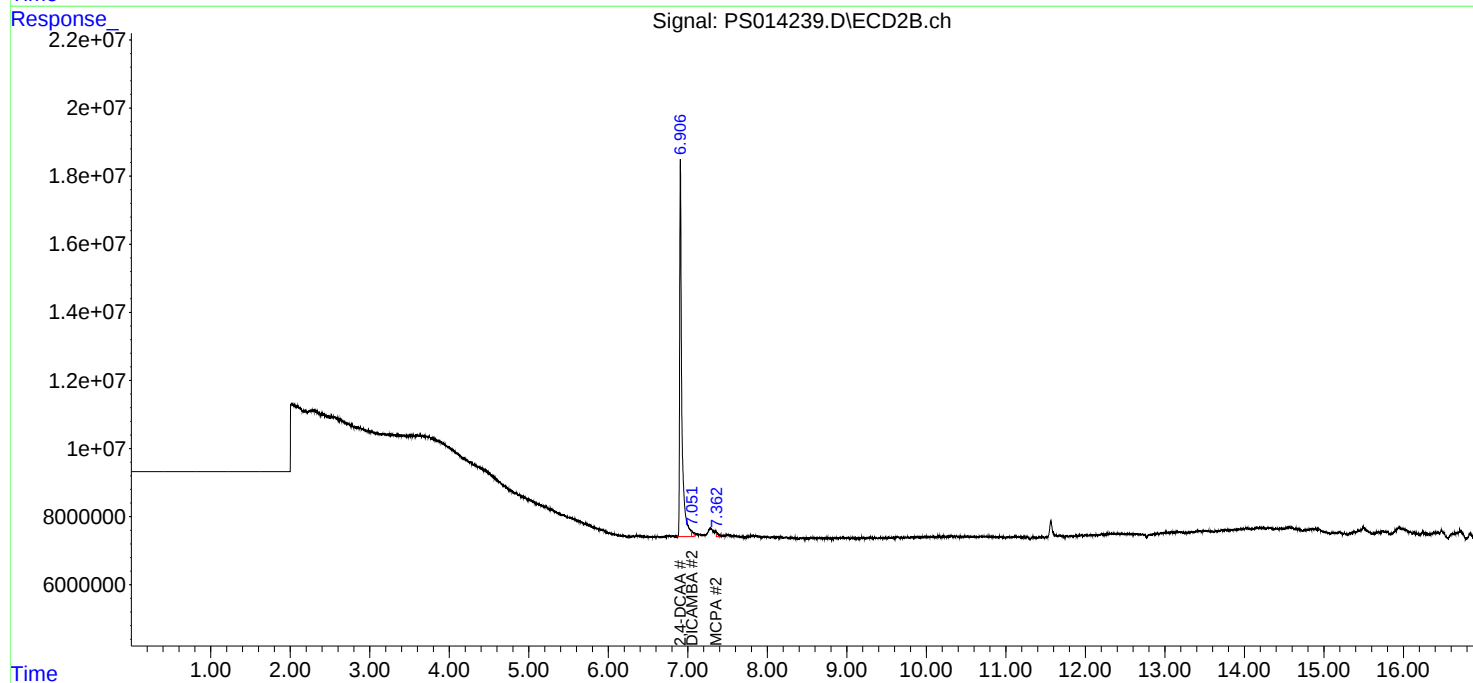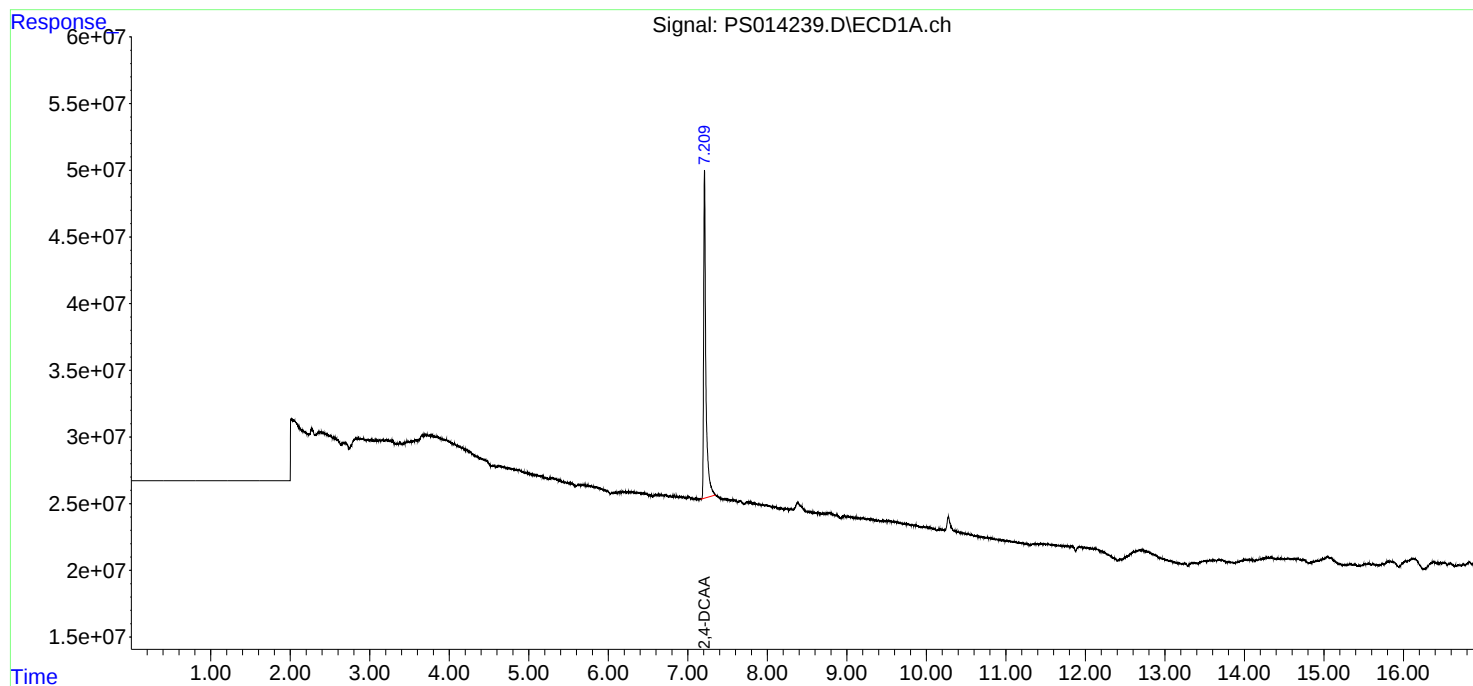


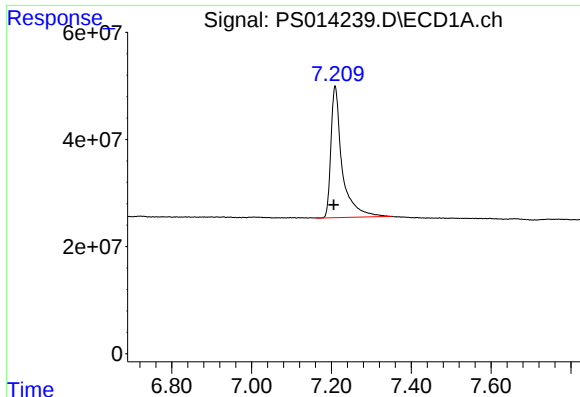

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.003 min
Response: 479143969
Conc: 475.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

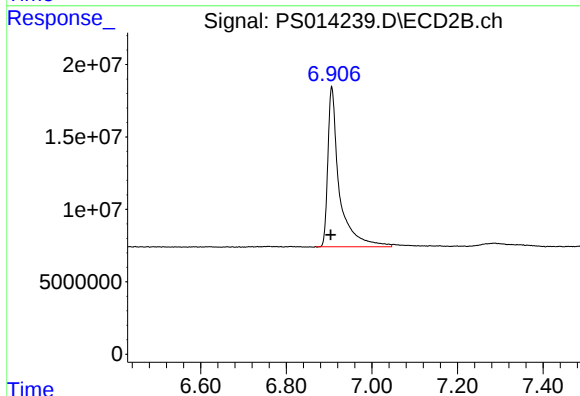


#4 2,4-DCAA

R.T.: 6.906 min
Delta R.T.: 0.002 min
Response: 206211189
Conc: 542.02 ng/ml

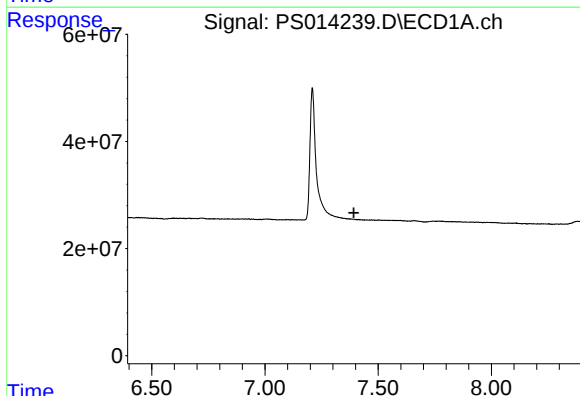


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.393 min
Response: 0
Conc: N.D.

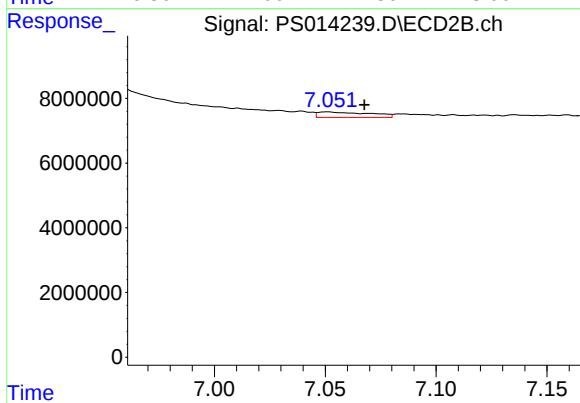

#5 DICAMBA


R.T.: 7.051 min
Delta R.T.: -0.017 min
Response: 2700005
Conc: 1.67 ng/ml

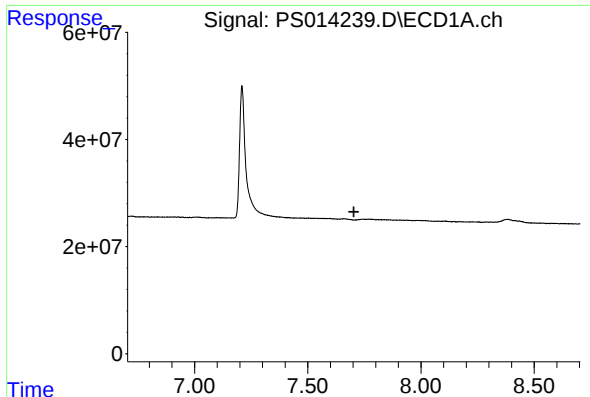

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

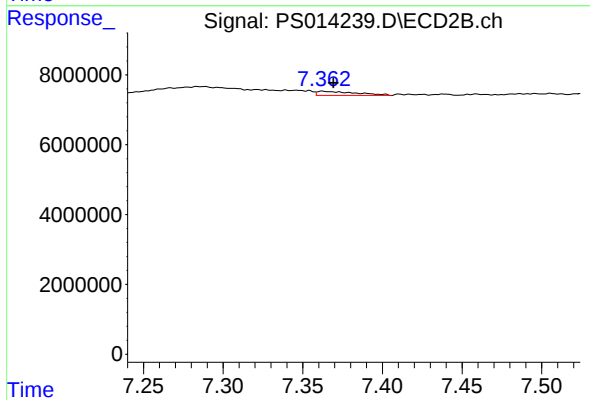

#7 MCPA

R.T.: 7.362 min
Delta R.T.: -0.007 min
Response: 1984589
Conc: 1.01 ug/ml