

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
 Data File : PD068505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 21:39
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:47:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 02:46:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	74128746	478.5E6	50.000	50.000
28)	SA Decachlor...	8.210	9.373	64078254	285.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.318	5.198	21494848	196.3E6	500.000	500.000
24)	Chlordane-2	4.820	5.671	25016386	187.9E6	500.000	500.000
25)	Chlordane-3	5.389	6.326	70043490	659.9E6	500.000	500.000
26)	Chlordane-4	5.447	6.404	58890589	762.1E6	500.000	500.000
27)	Chlordane-5	6.285	7.216	25315636	144.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 21:39
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:47:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 02:46:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

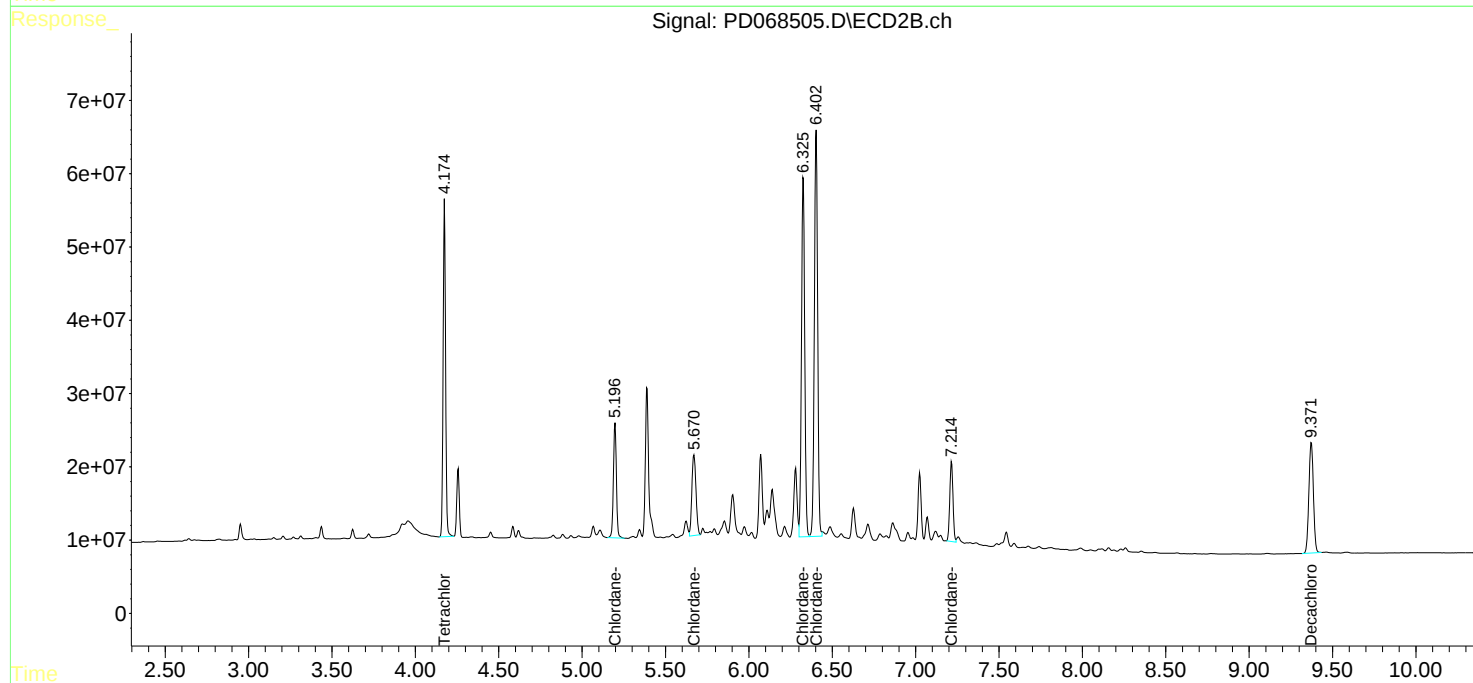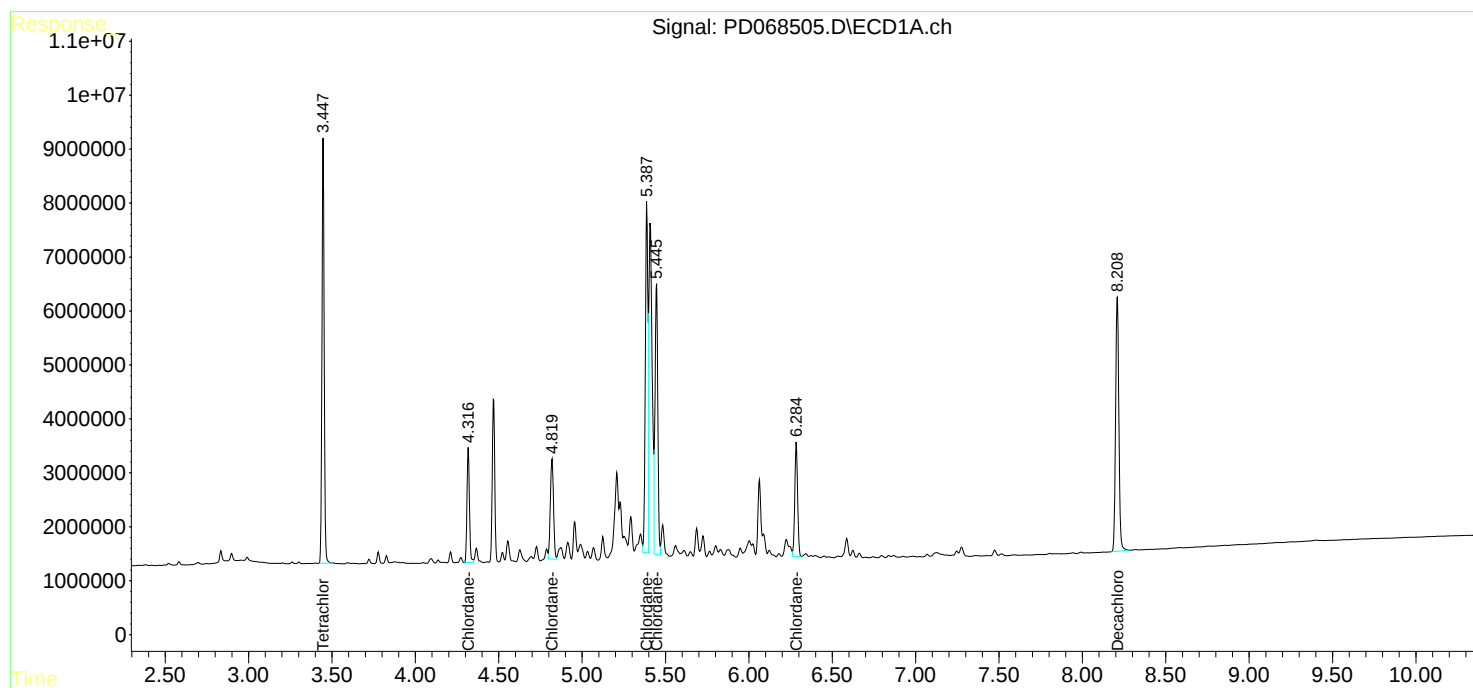


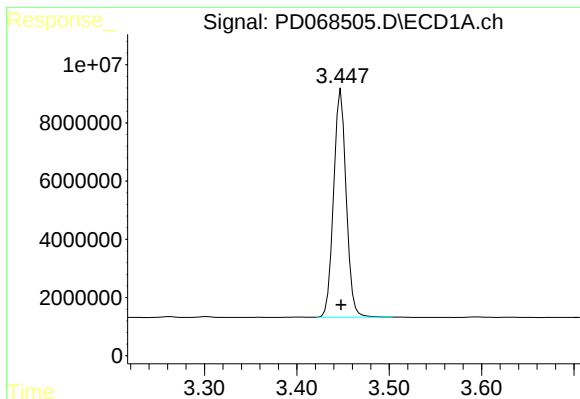

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 74128746
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

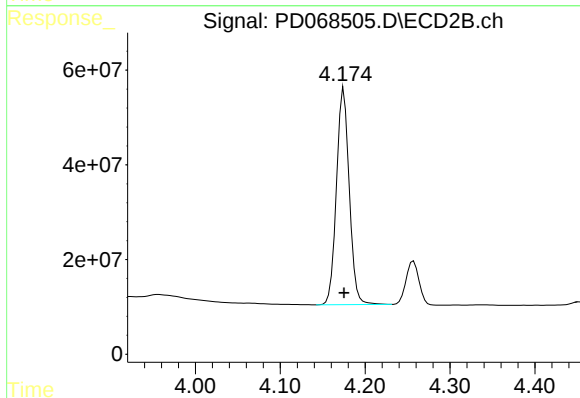


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 478480018
Conc: 50.00 ng/ml

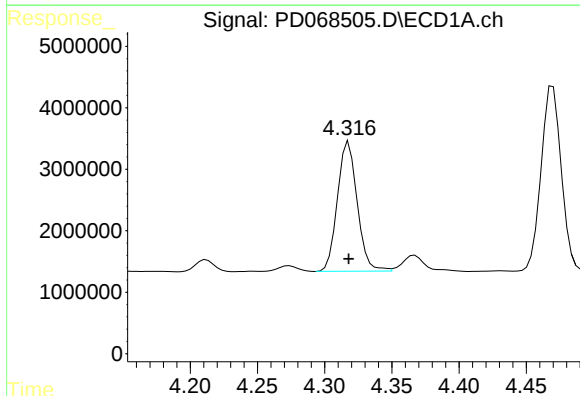


#23 Chlordane-1

R.T.: 4.318 min
Delta R.T.: 0.000 min
Response: 21494848
Conc: 500.00 ng/ml

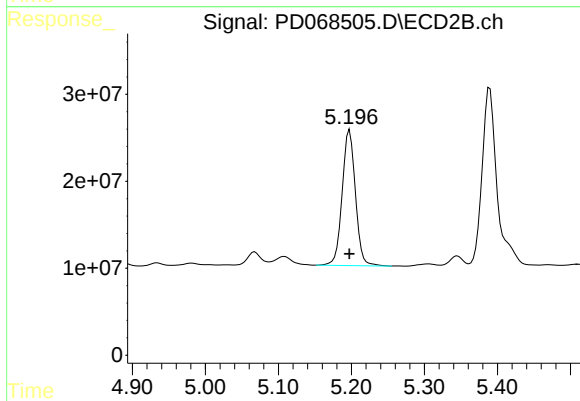

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 196334882
Conc: 500.00 ng/ml

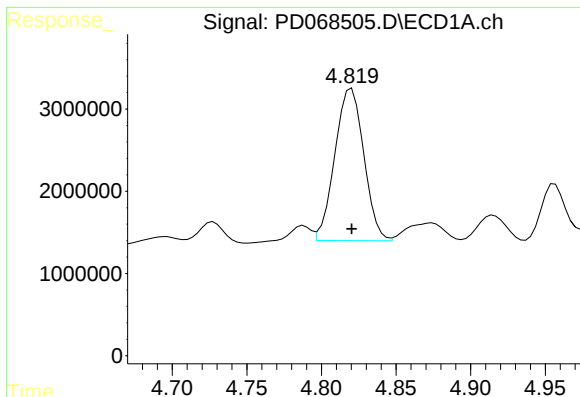

#24 Chlordane-2


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 25016386
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

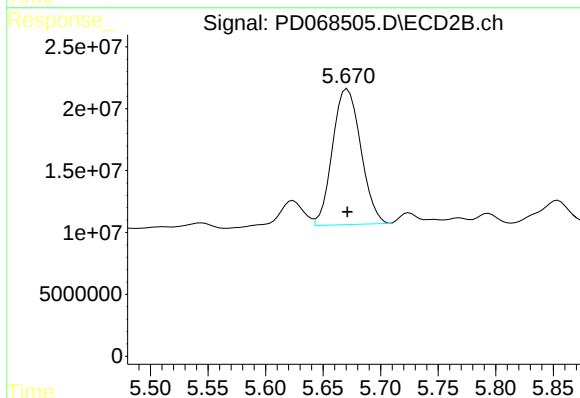


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 187949586
Conc: 500.00 ng/ml

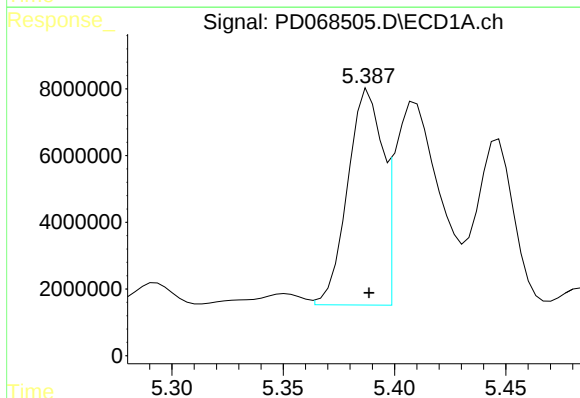


#25 Chlordane-3

R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 70043490
Conc: 500.00 ng/ml

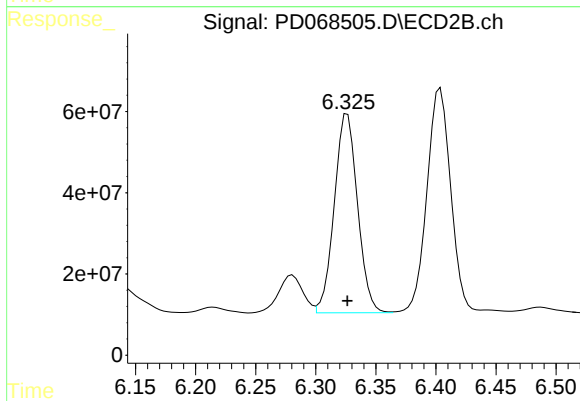

#25 Chlordane-3


R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 659899281
Conc: 500.00 ng/ml

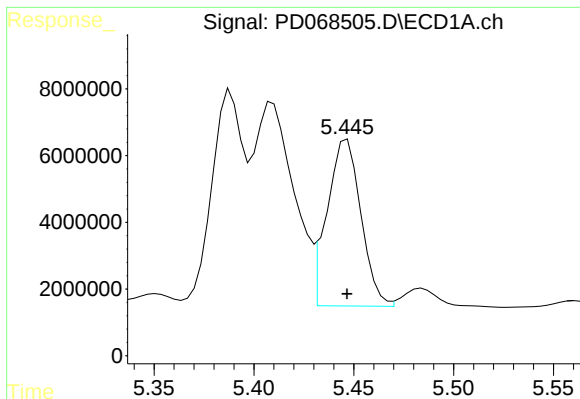

#26 Chlordane-4


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 58890589
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

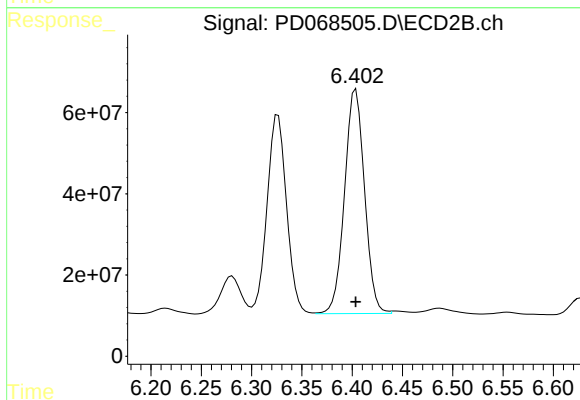


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 762120235
Conc: 500.00 ng/ml

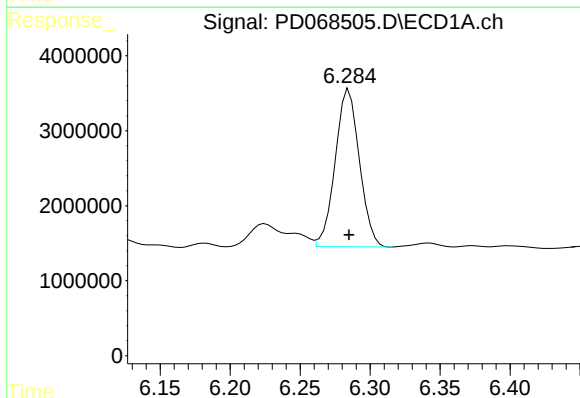


#27 Chlordane-5

R.T.: 6.285 min
Delta R.T.: 0.000 min
Response: 25315636
Conc: 500.00 ng/ml

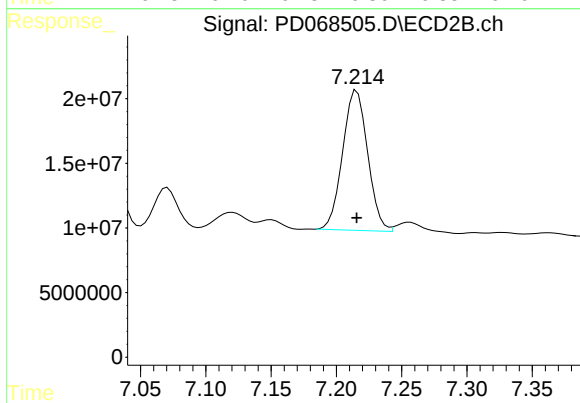

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 144727312
Conc: 500.00 ng/ml

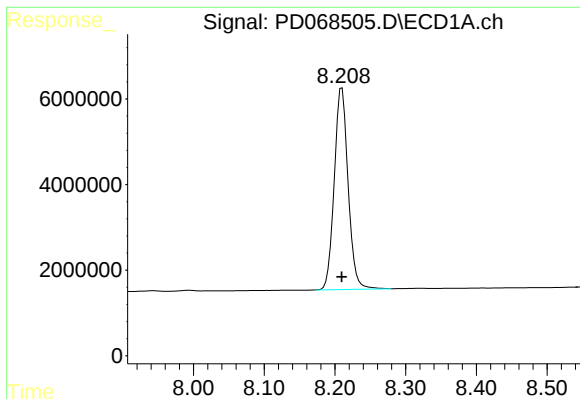

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 64078254
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

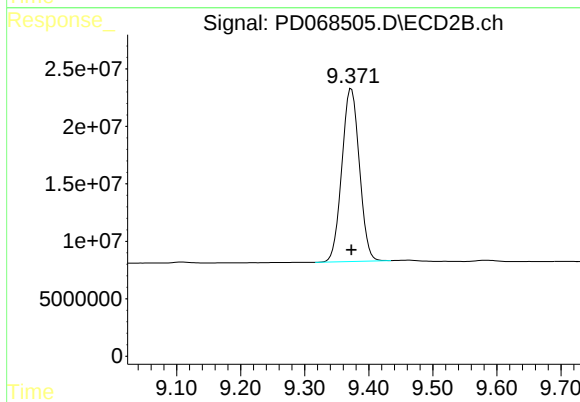

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 285708369
Conc: 50.00 ng/ml