

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
 Data File : PD068503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 21:11
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:48:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 02:46:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	150.4E6	906.7E6	100.717	97.303
28)	SA Decachlor...	8.210	9.373	122.6E6	526.4E6	97.793	95.900
Target Compounds							
23)	Chlordane-1	4.319	5.198	42657710	367.3E6	996.124	966.574
24)	Chlordane-2	4.820	5.671	47383796	343.6E6	972.808	955.056
25)	Chlordane-3	5.389	6.327	144.2E6	1263.2E6	1014.451	978.086
26)	Chlordane-4	5.447	6.404	119.2E6	1452.9E6	1005.957	976.037
27)	Chlordane-5	6.285	7.215	50251312	271.5E6	996.234	968.031



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 21:11
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:48:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 02:46:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

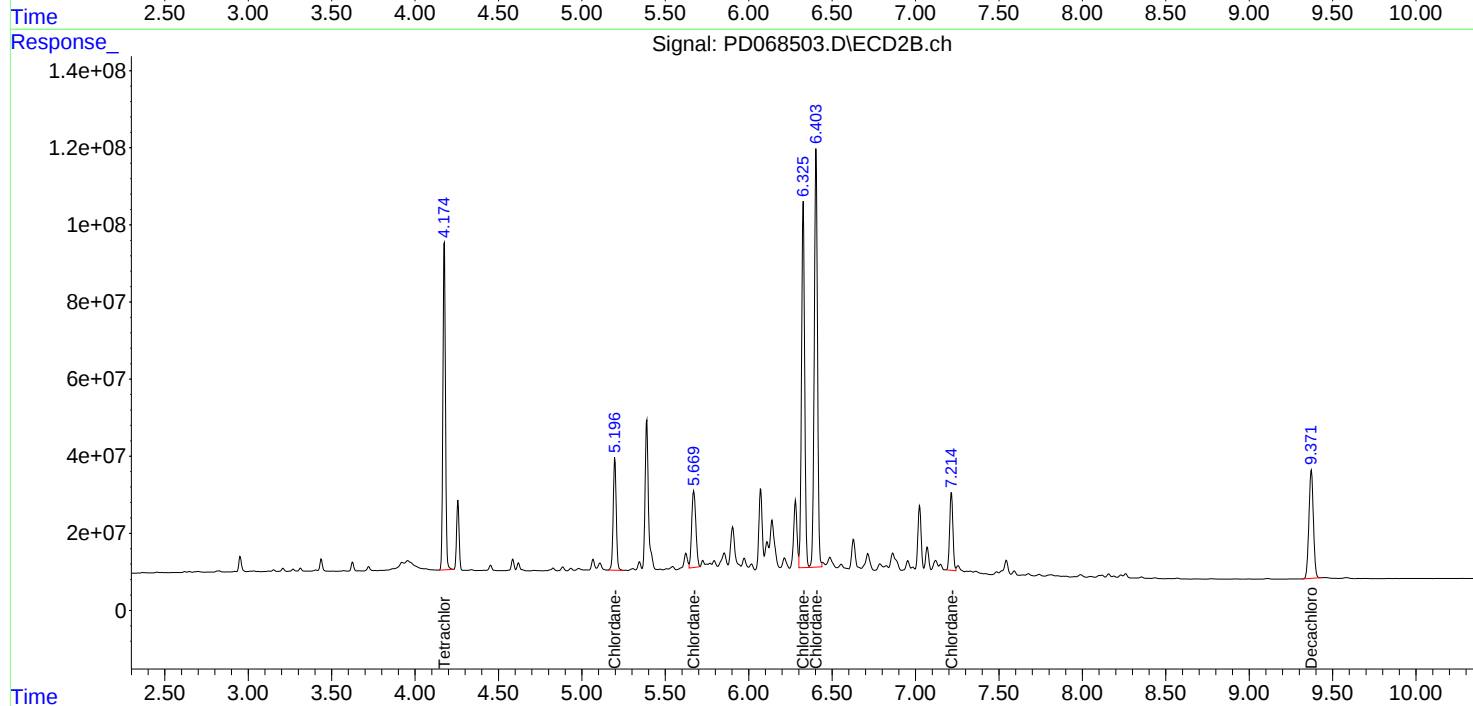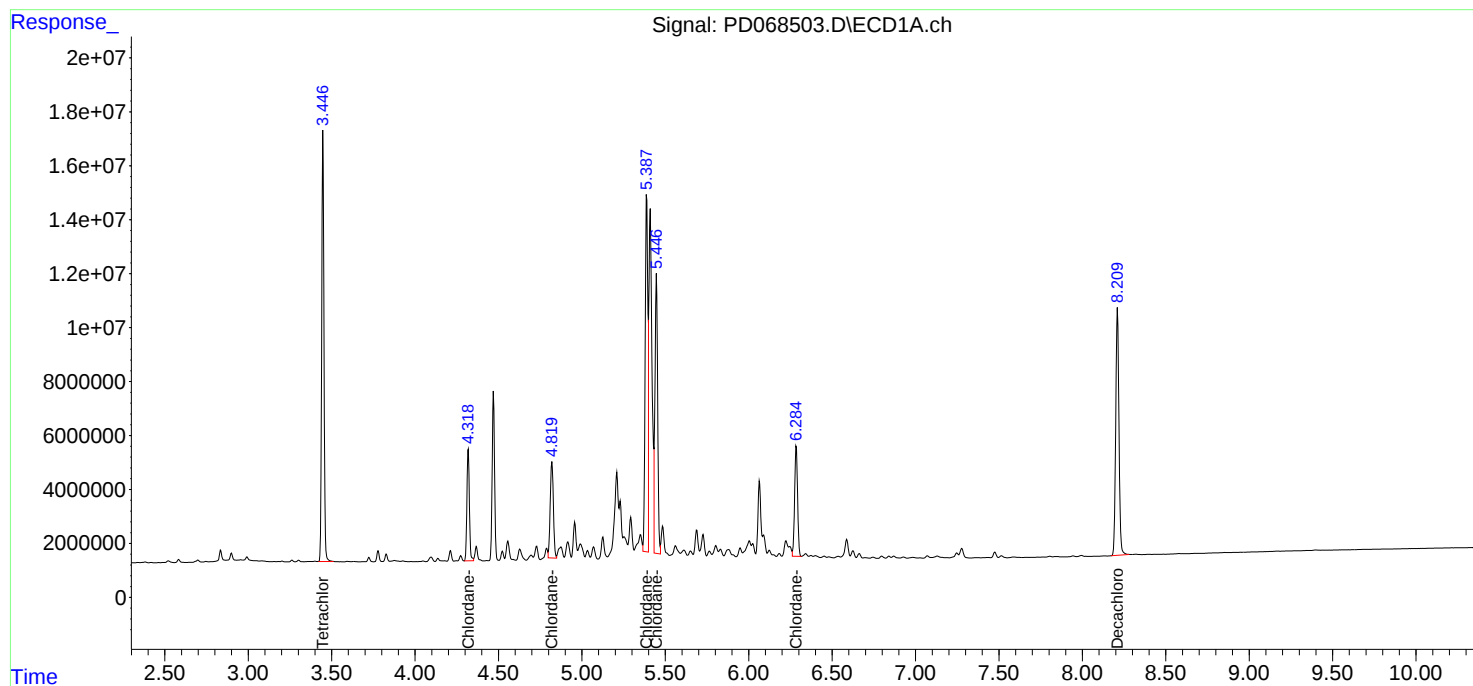


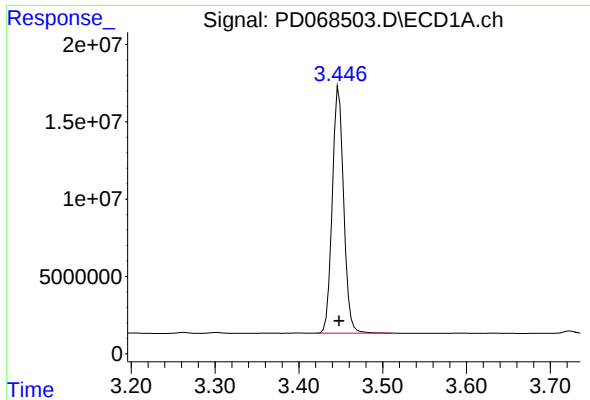

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 150398419
Conc: 100.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

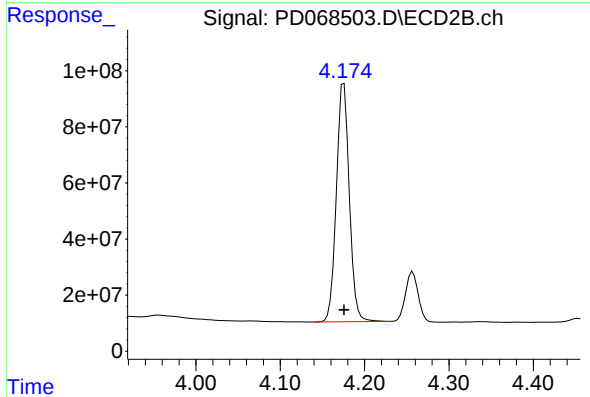


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 906690333
Conc: 97.30 ng/ml

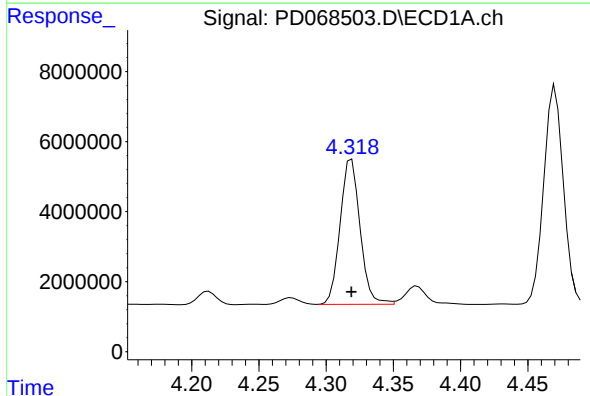


#23 Chlordane-1

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 42657710
Conc: 996.12 ng/ml

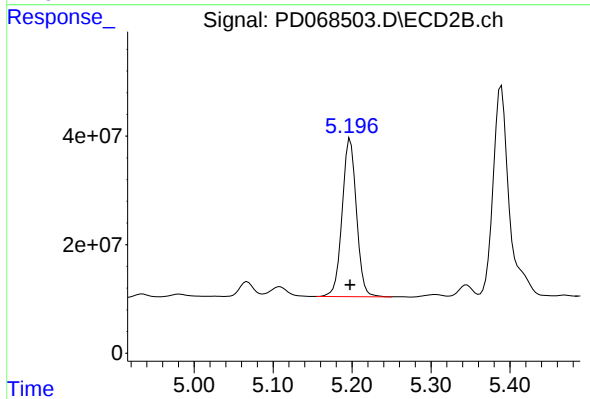

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 367268391
Conc: 966.57 ng/ml

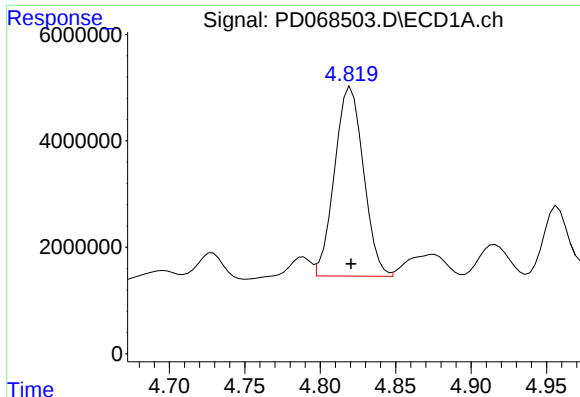

#24 Chlordane-2


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 47383796
Conc: 972.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

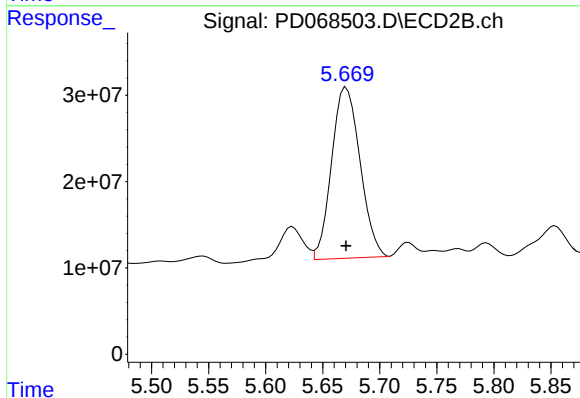


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 343563686
Conc: 955.06 ng/ml

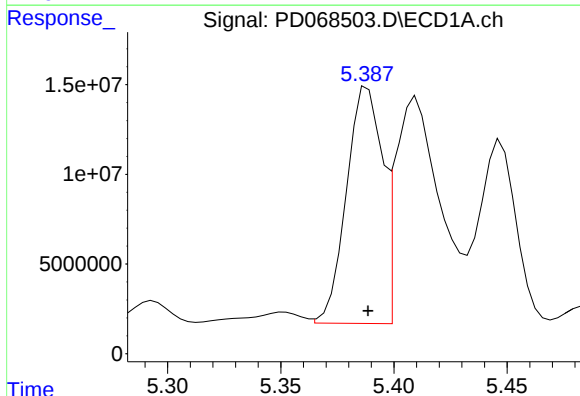


#25 Chlordane-3

R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 144195117
Conc: 1014.45 ng/ml

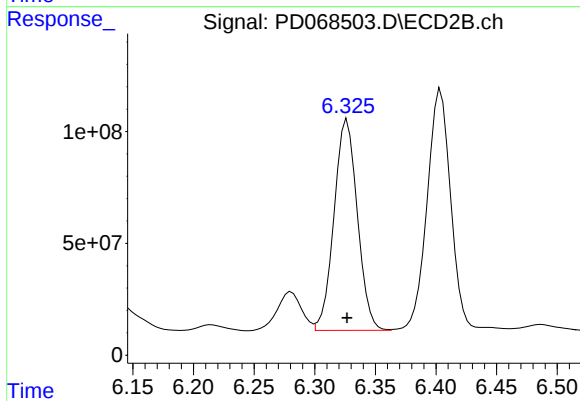

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 1263194134
Conc: 978.09 ng/ml

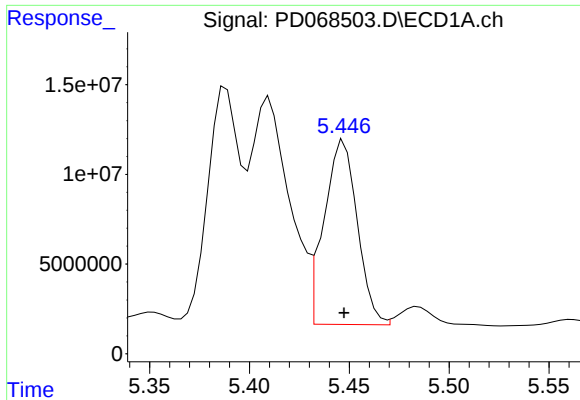

#26 Chlordane-4


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 119192902
Conc: 1005.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

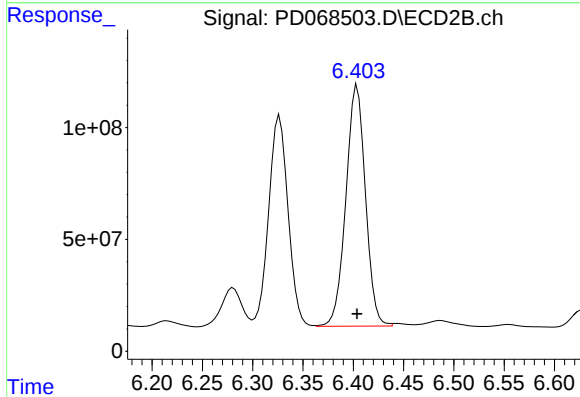


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 1452899355
Conc: 976.04 ng/ml

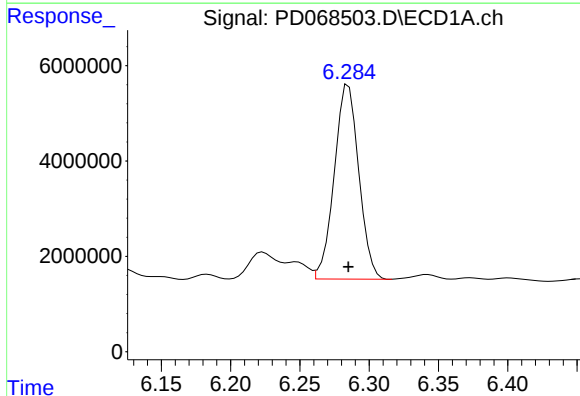


#27 Chlordane-5

R.T.: 6.285 min
Delta R.T.: 0.000 min
Response: 50251312
Conc: 996.23 ng/ml

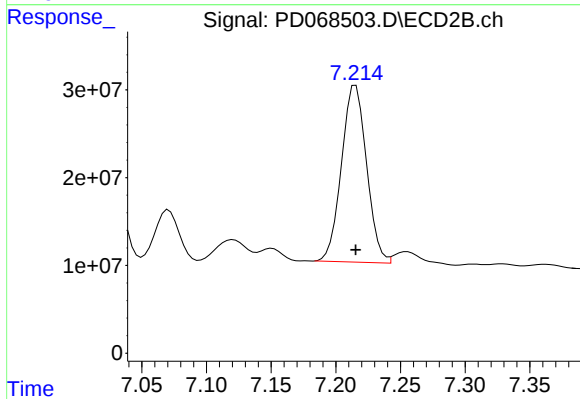

#27 Chlordane-5


R.T.: 7.215 min
Delta R.T.: 0.000 min
Response: 271520923
Conc: 968.03 ng/ml

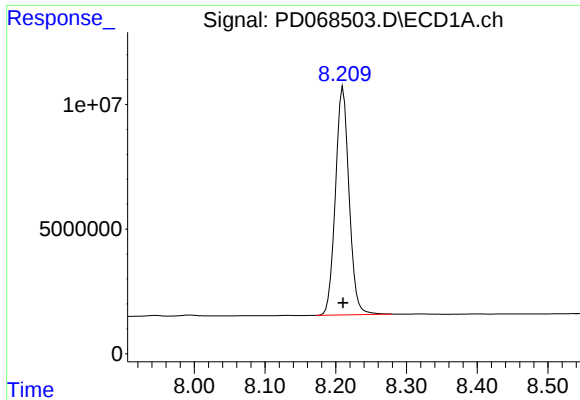

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 122621323
Conc: 97.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

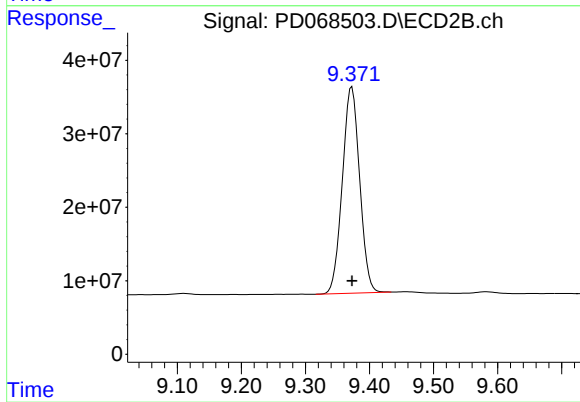

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 526409741
Conc: 95.90 ng/ml