

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
 Data File : PD068504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 21:25
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:50:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 02:46:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	110.7E6	688.3E6	74.441	74.239
28)	SA Decachlor...	8.211	9.373	92643935	403.3E6	74.253	73.980
Target Compounds							
23)	Chlordane-1	4.319	5.198	31588227	279.3E6	741.711	739.921
24)	Chlordane-2	4.821	5.671	35861030	266.0E6	740.771	742.900
25)	Chlordane-3	5.389	6.326	103.4E6	955.5E6	734.635	743.201
26)	Chlordane-4	5.447	6.404	88161989	1101.6E6	746.032	743.313
27)	Chlordane-5	6.285	7.216	37456437	207.6E6	745.034	743.305



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 21:25
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:50:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 02:46:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

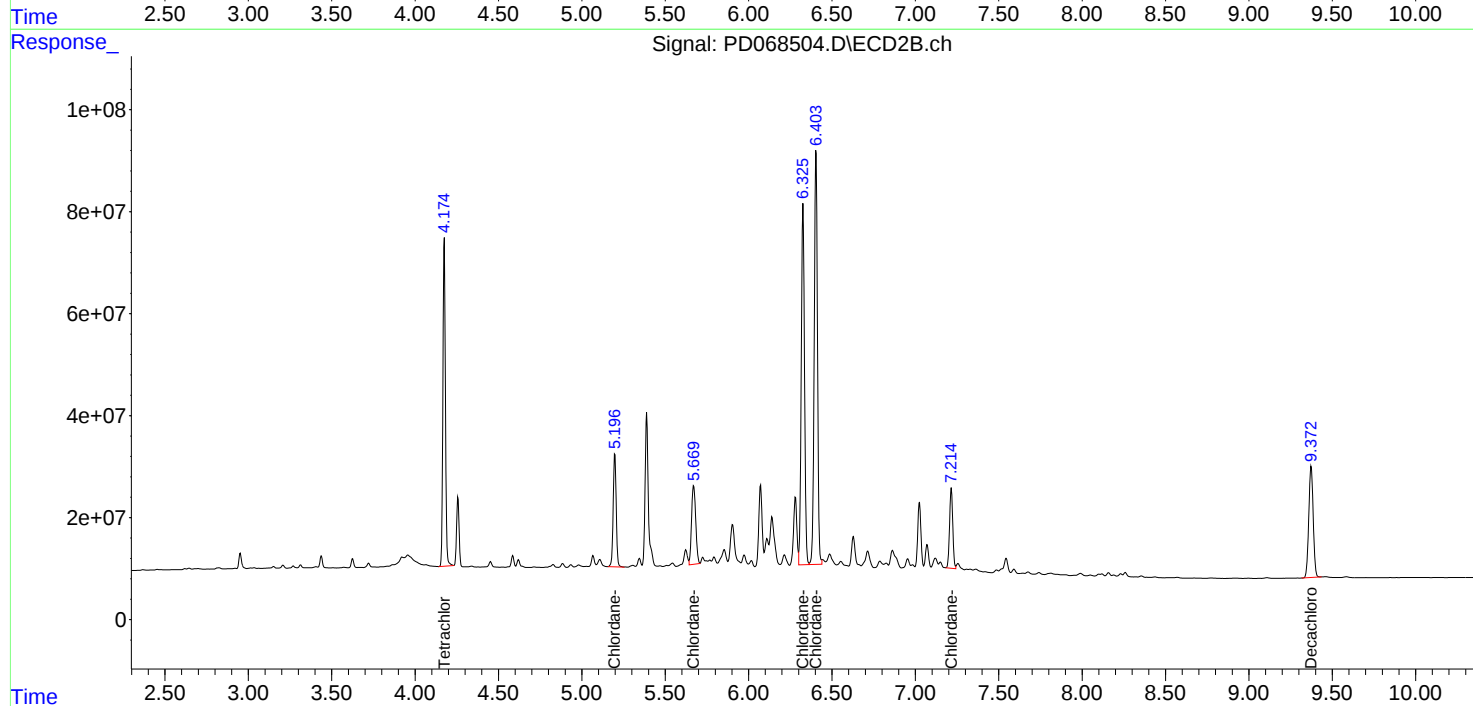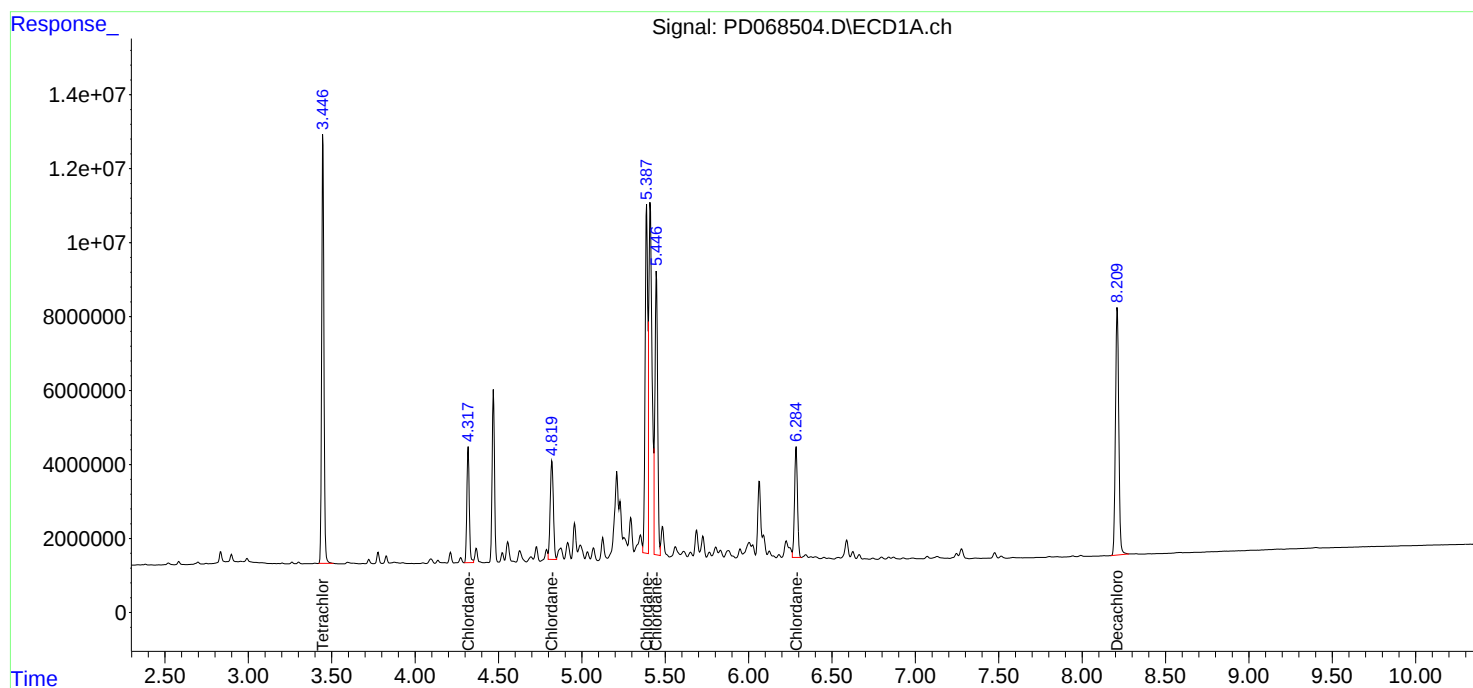


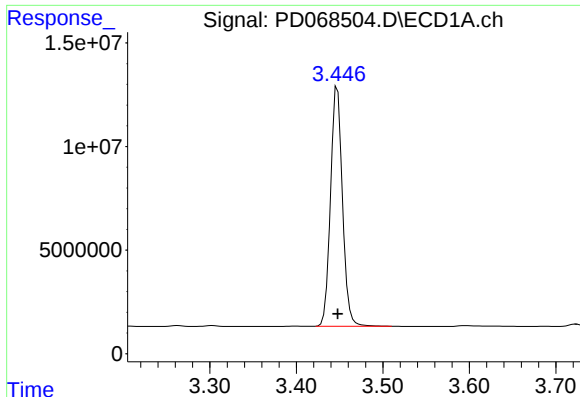

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 110748037
Conc: 74.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

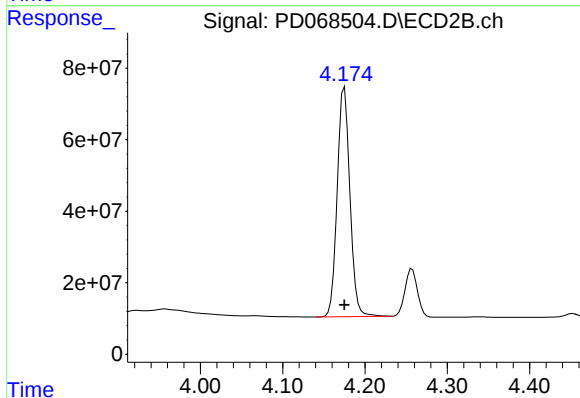


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 688290496
Conc: 74.24 ng/ml

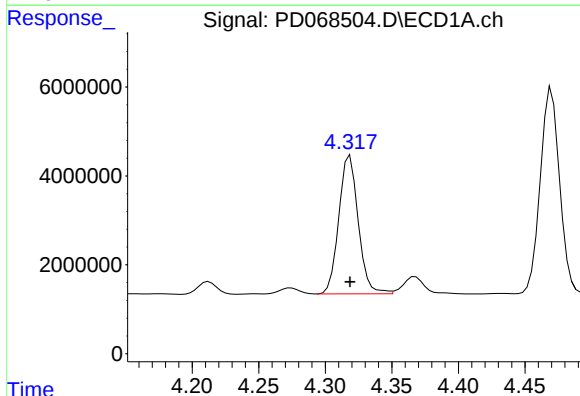


#23 Chlordane-1

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 31588227
Conc: 741.71 ng/ml

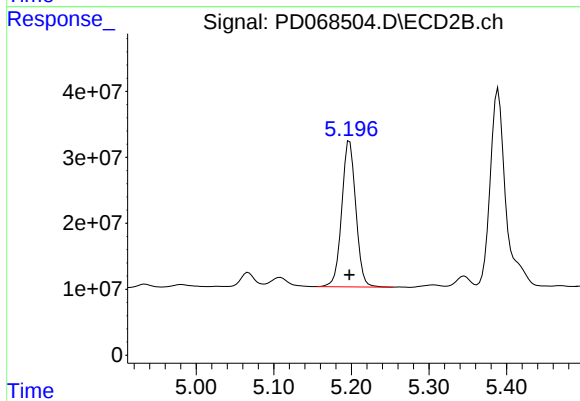

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 279270822
Conc: 739.92 ng/ml

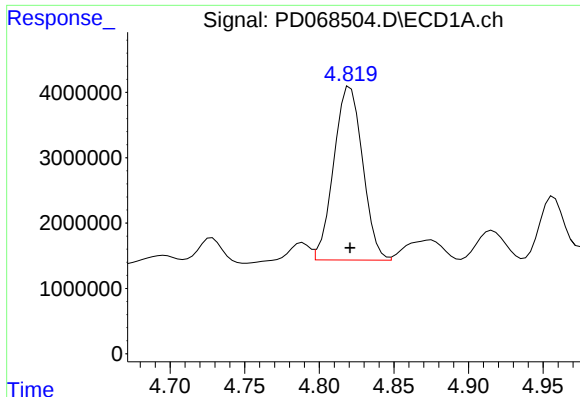

#24 Chlordane-2


R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 35861030
Conc: 740.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

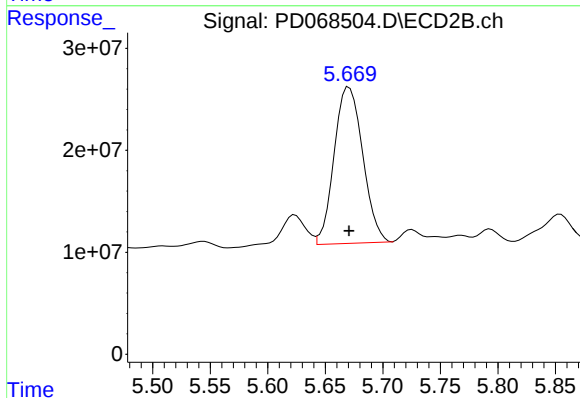


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 265985608
Conc: 742.90 ng/ml

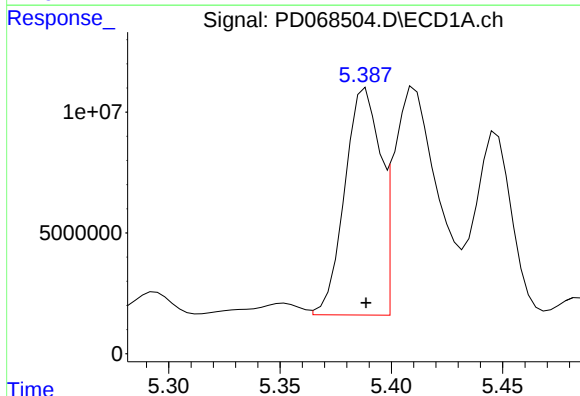


#25 Chlordane-3

R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 103362999
Conc: 734.63 ng/ml

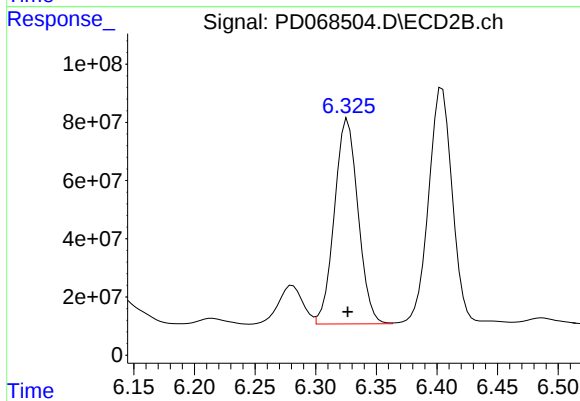

#25 Chlordane-3


R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 955510677
Conc: 743.20 ng/ml

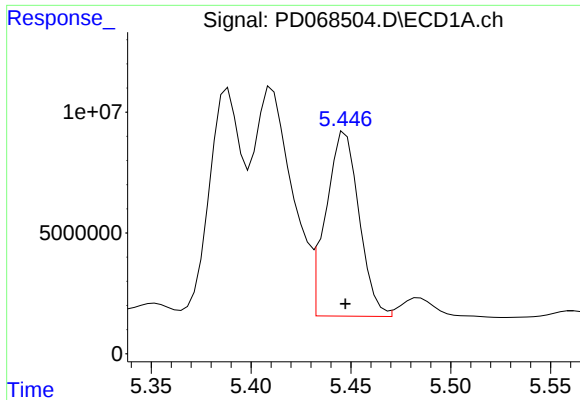

#26 Chlordane-4


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 88161989
Conc: 746.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

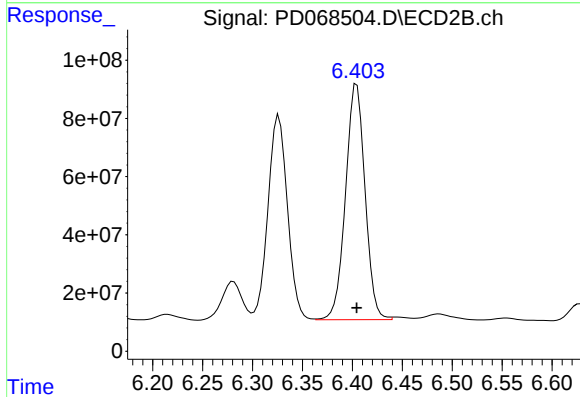


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 1101562488
Conc: 743.31 ng/ml

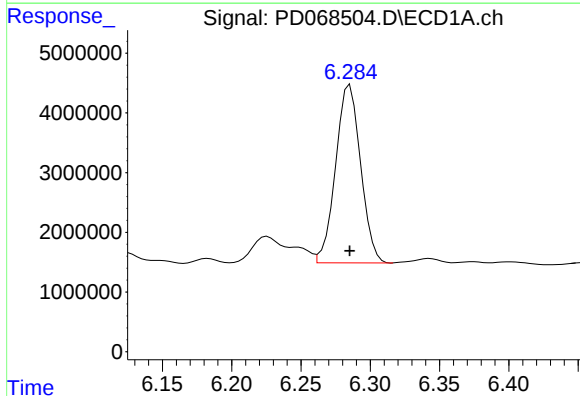


#27 Chlordane-5

R.T.: 6.285 min
Delta R.T.: 0.000 min
Response: 37456437
Conc: 745.03 ng/ml

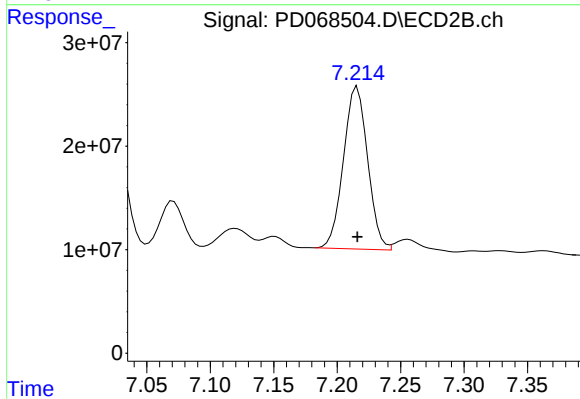

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 207561621
Conc: 743.31 ng/ml

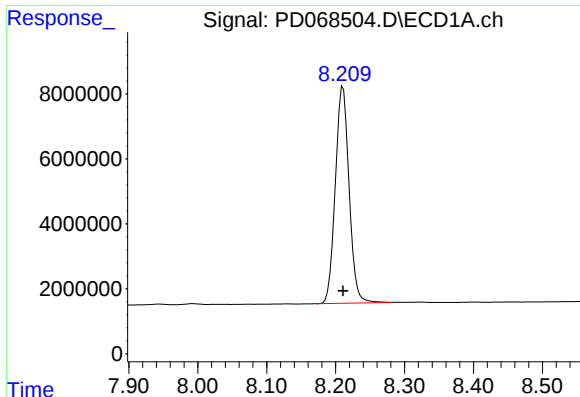

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 92643935
Conc: 74.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

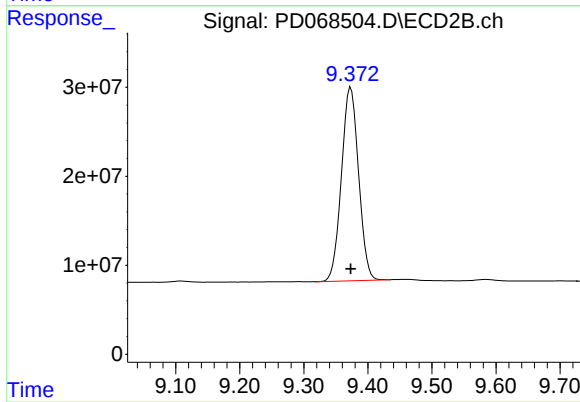

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 403343722
Conc: 73.98 ng/ml