

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
 Data File : PD068506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 21:53
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:52:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 02:46:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	35706502	246.3E6	24.243	26.156
28)	SA Decachlor...	8.210	9.373	32645929	148.9E6	25.864	26.688
Target Compounds							
23)	Chlordane-1	4.319	5.198	10701533	101.5E6	250.958	263.907
24)	Chlordane-2	4.821	5.671	12959619	98813667	263.046	268.997
25)	Chlordane-3	5.389	6.327	34168111	338.4E6	244.594	259.802
26)	Chlordane-4	5.447	6.404	29105611	392.5E6	247.210	260.980
27)	Chlordane-5	6.286	7.216	12707898	75590546	252.071	265.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 21:53
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:52:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 02:46:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

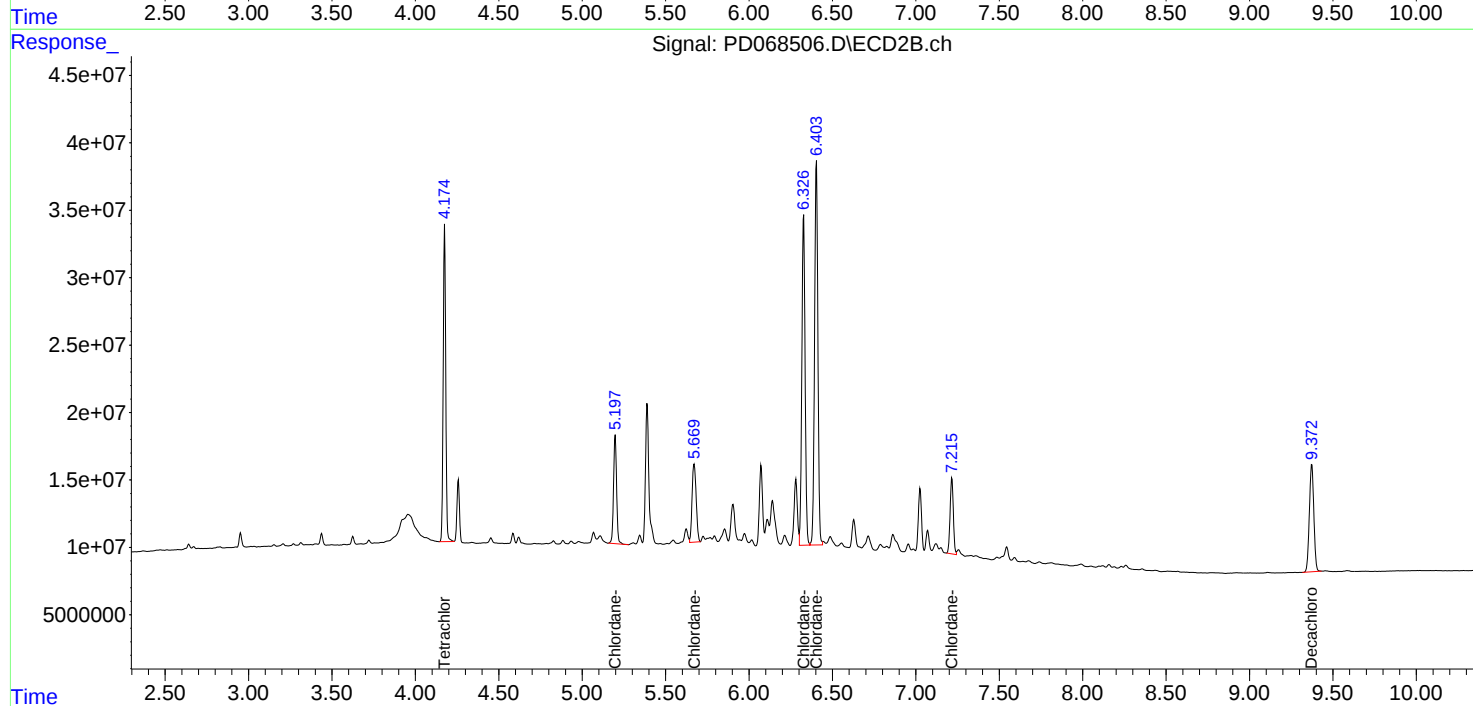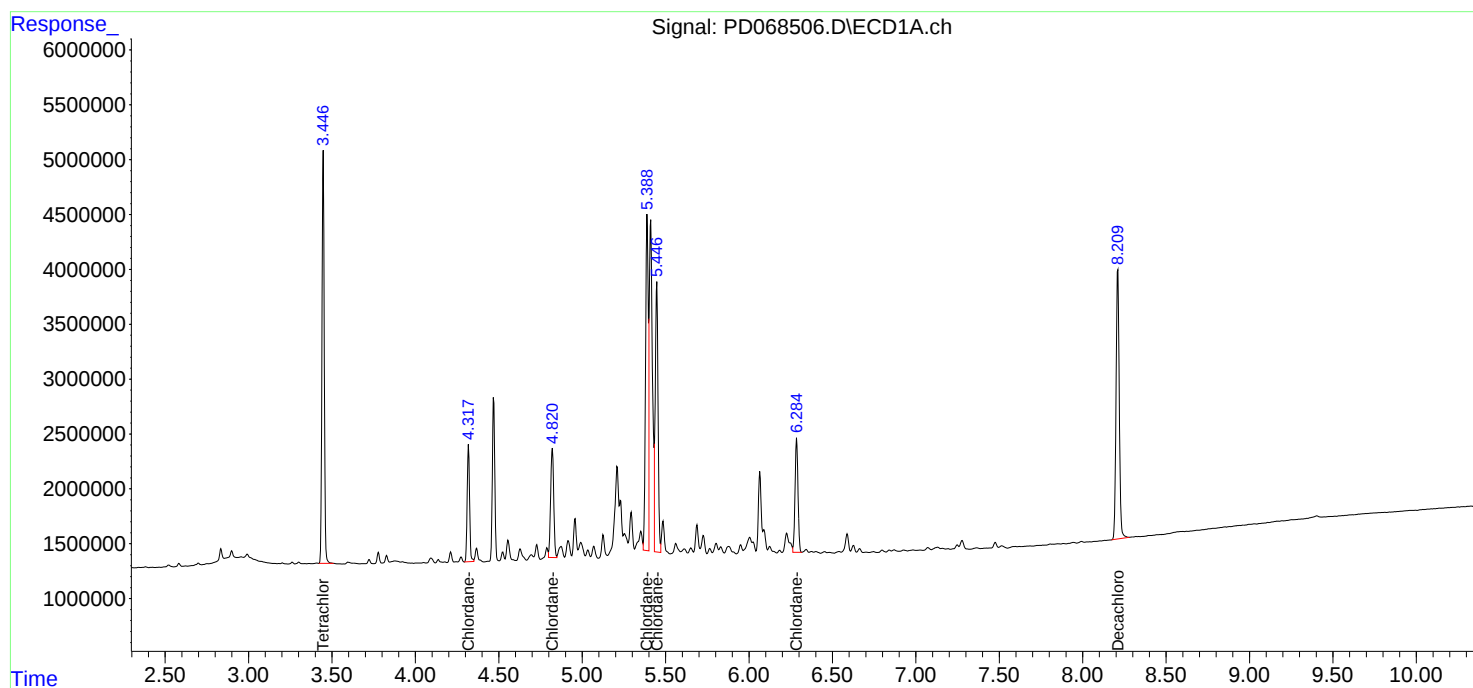


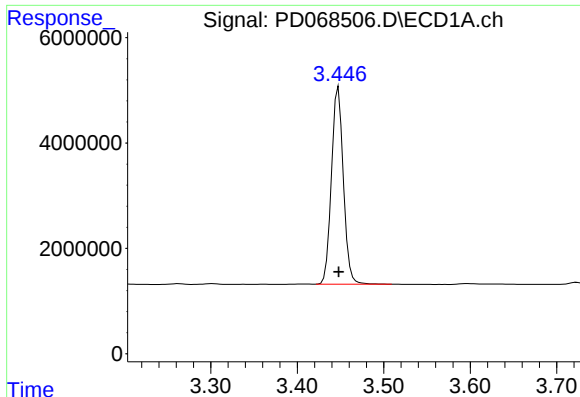

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 35706502
Conc: 24.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

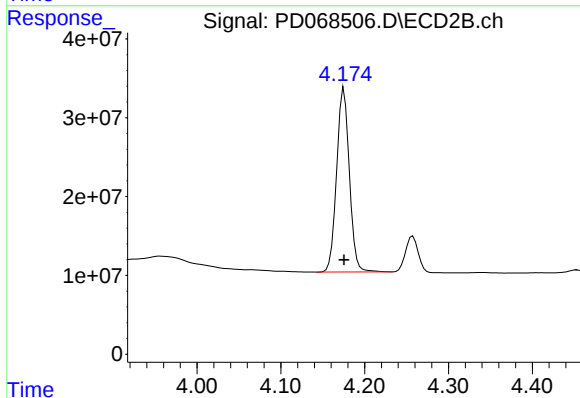


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 246298347
Conc: 26.16 ng/ml

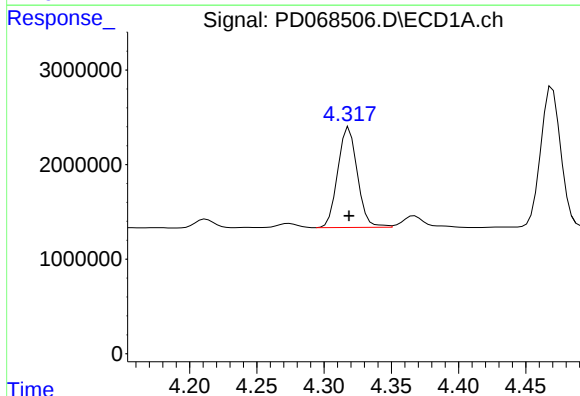


#23 Chlordane-1

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 10701533
Conc: 250.96 ng/ml

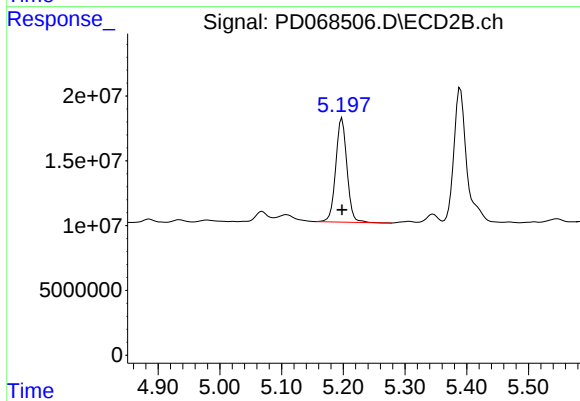

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 101489316
Conc: 263.91 ng/ml

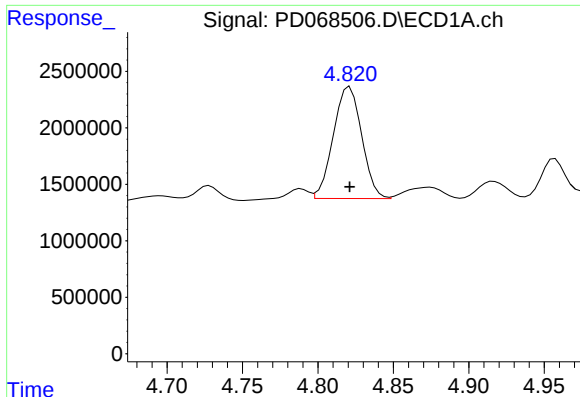

#24 Chlordane-2


R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 12959619
Conc: 263.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

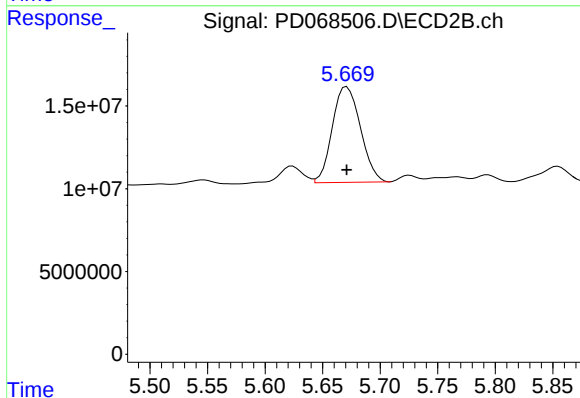


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 98813667
Conc: 269.00 ng/ml

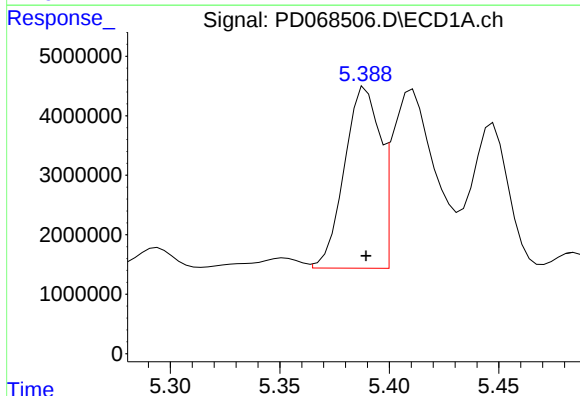


#25 Chlordane-3

R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 34168111
Conc: 244.59 ng/ml

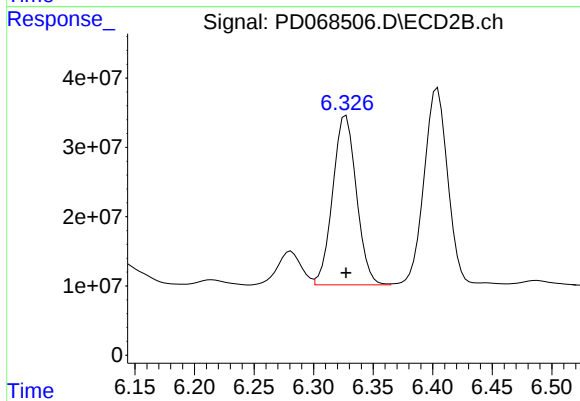

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 338442790
Conc: 259.80 ng/ml

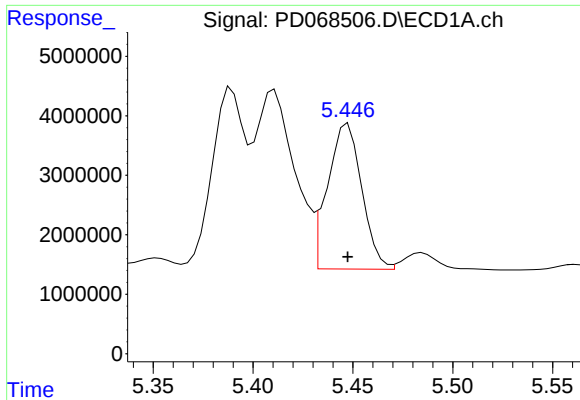

#26 Chlordane-4


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 29105611
Conc: 247.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

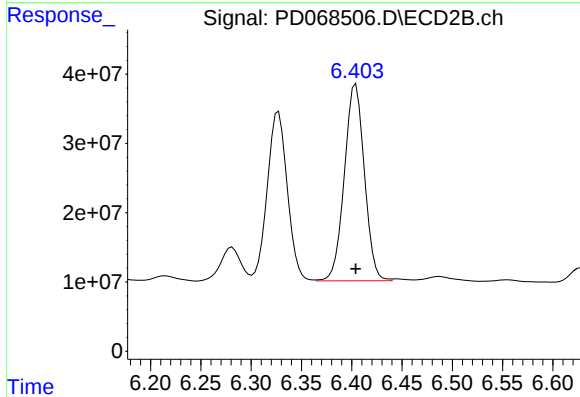


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 392508620
Conc: 260.98 ng/ml

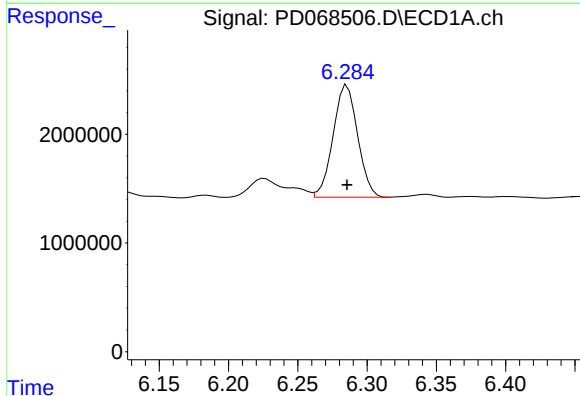


#27 Chlordane-5

R.T.: 6.286 min
Delta R.T.: 0.000 min
Response: 12707898
Conc: 252.07 ng/ml

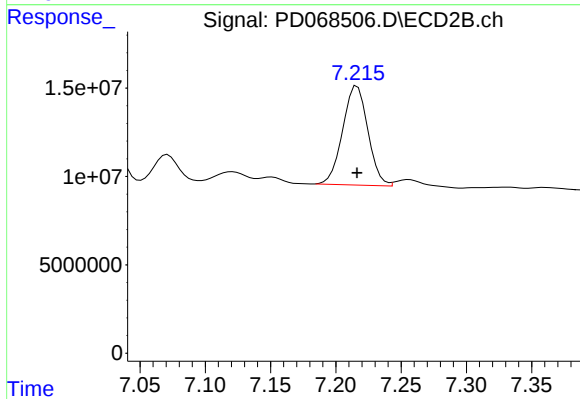

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 75590546
Conc: 265.21 ng/ml

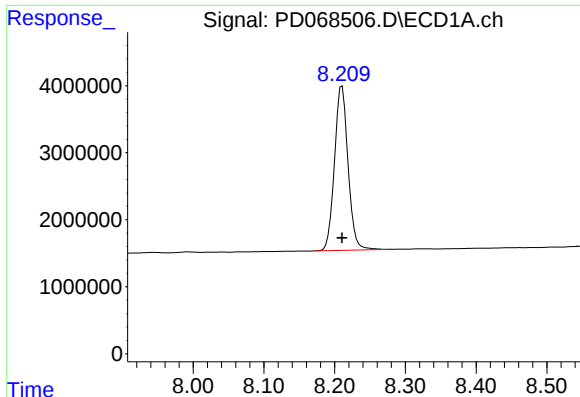

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 32645929
Conc: 25.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

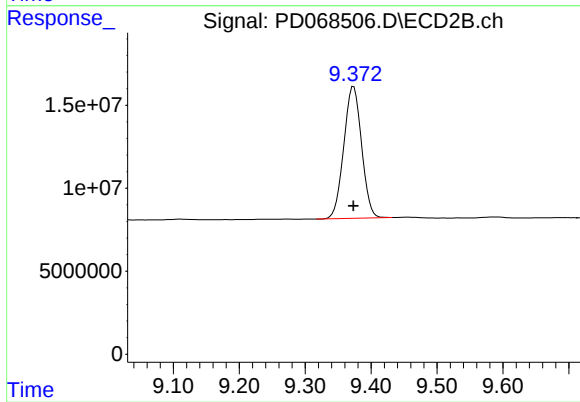

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 148856715
Conc: 26.69 ng/ml