

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
 Data File : PD068514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 23:45
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:57:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 02:56:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.176	72044845	470.0E6	49.183	48.286
28)	SA Decachlor...	8.211	9.374	64402589	289.7E6	49.685	50.230
Target Compounds							
23)	Chlordane-1	4.320	5.198	21505512	196.8E6	506.772	498.753
24)	Chlordane-2	4.822	5.672	25315544	190.9E6	504.446	499.236
25)	Chlordane-3	5.390	6.327	72464027	674.5E6	519.706	502.014
26)	Chlordane-4	5.449	6.405	60020372	778.5E6	507.140	500.796
27)	Chlordane-5	6.287	7.217	25821856	149.3E6	516.854	511.834



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 23:45
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:57:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 02:56:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

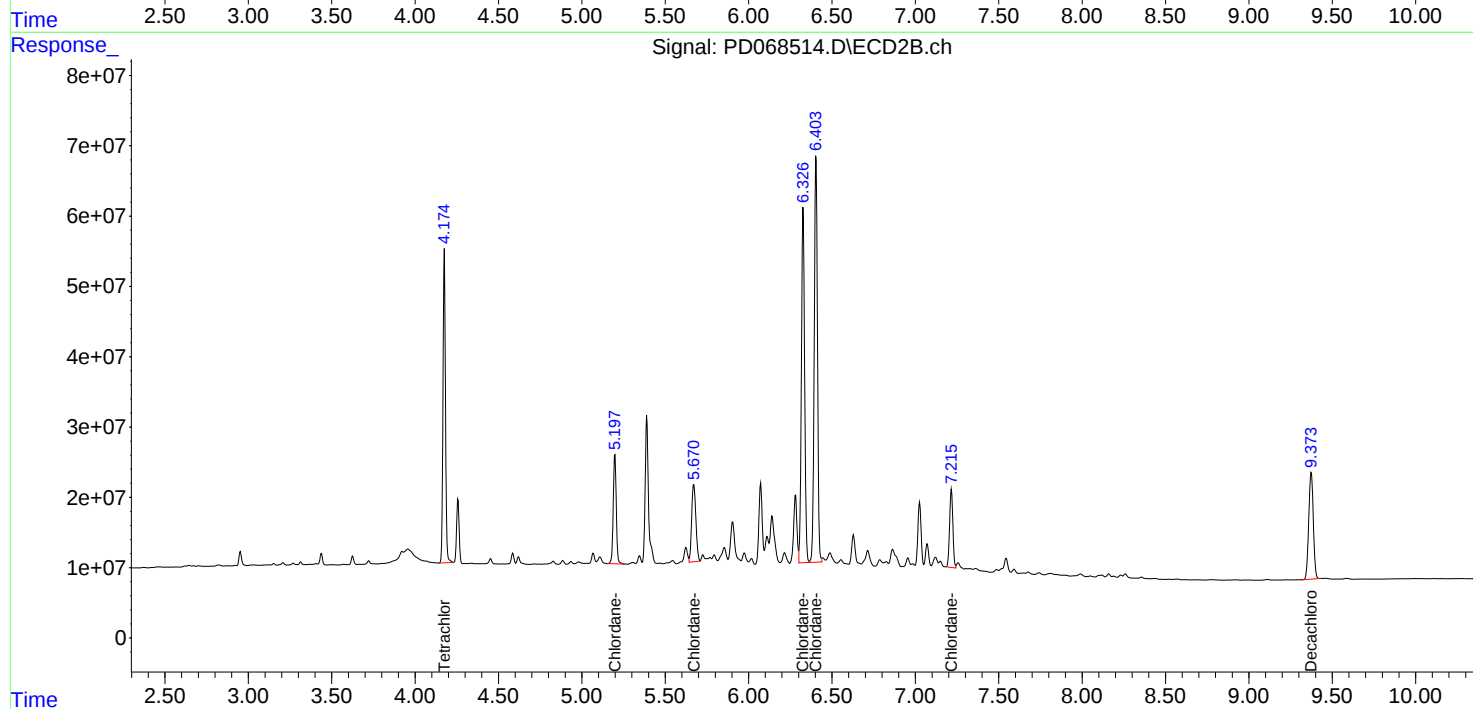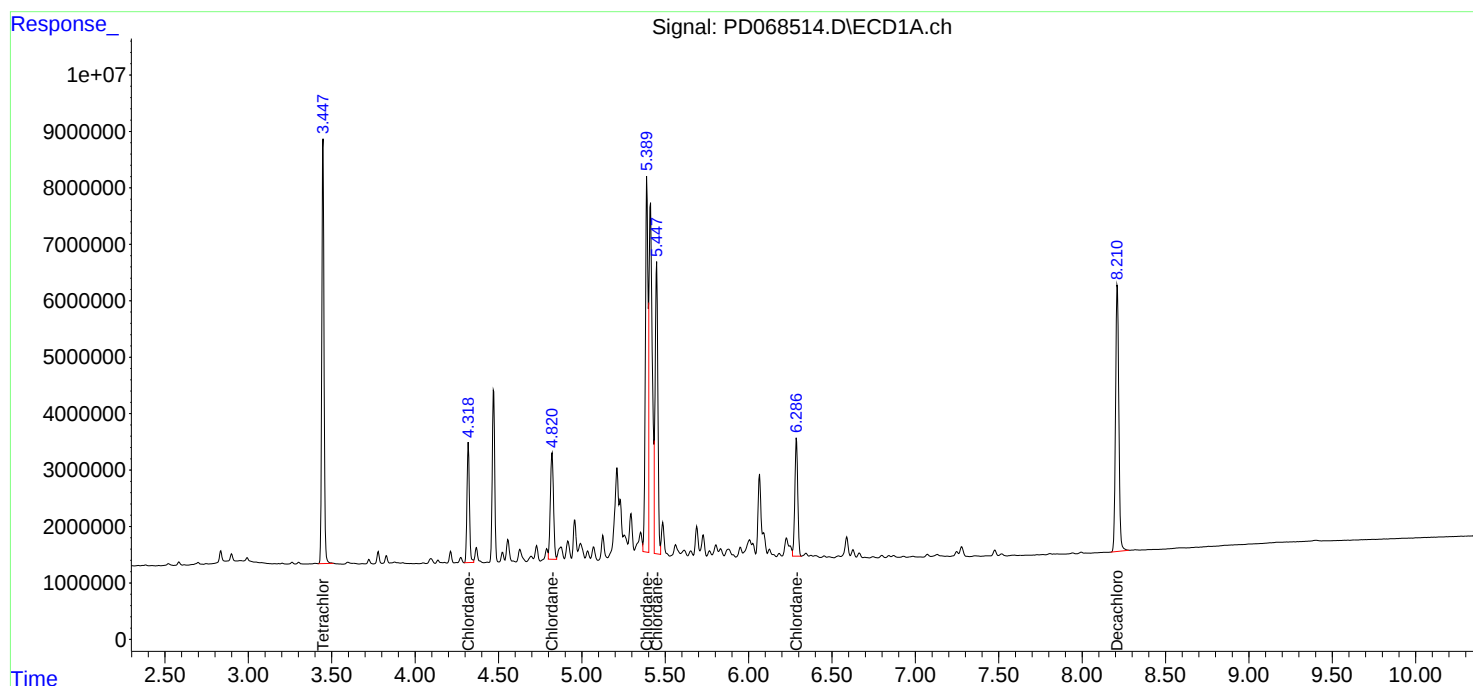


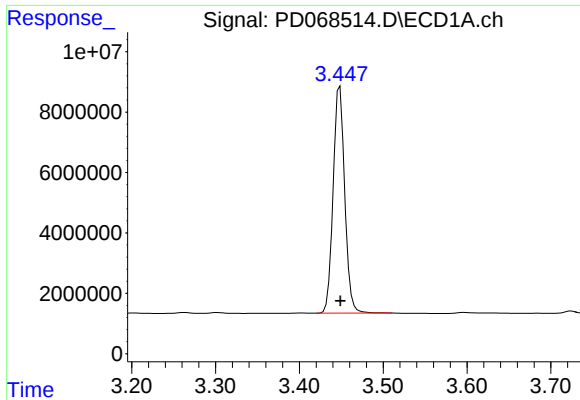

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 72044845
Conc: 49.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031222CHLOR

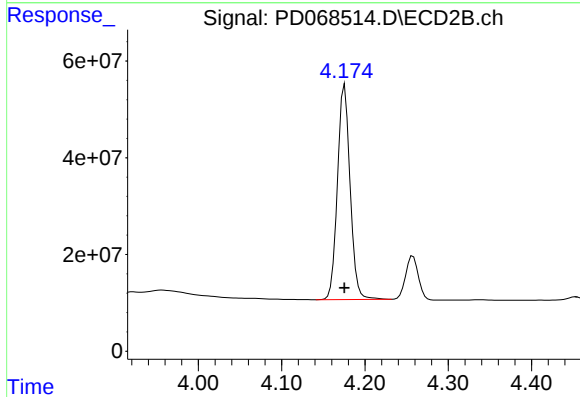


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 470012080
Conc: 48.29 ng/ml

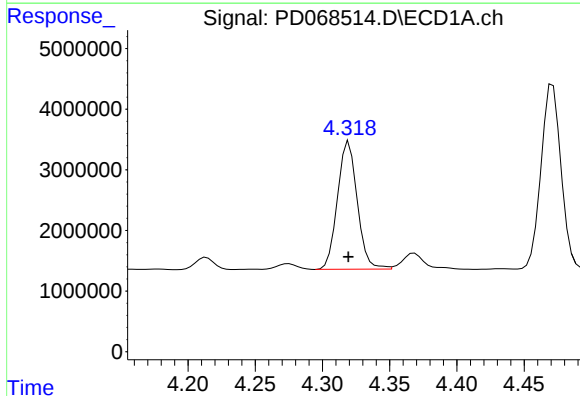


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 21505512
Conc: 506.77 ng/ml

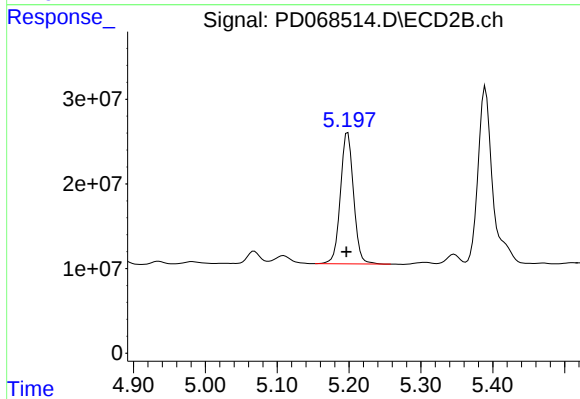

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.002 min
Response: 196774368
Conc: 498.75 ng/ml

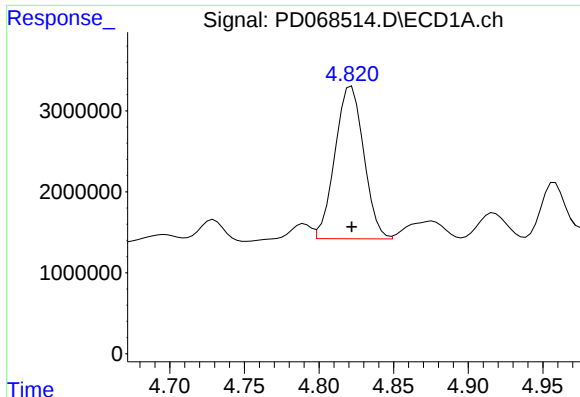

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 25315544
Conc: 504.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031222CHLOR

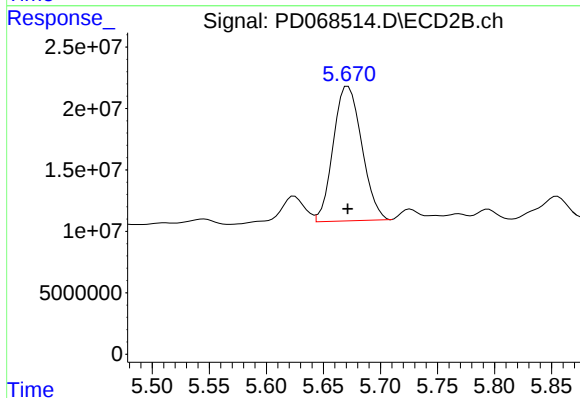


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 190852064
Conc: 499.24 ng/ml

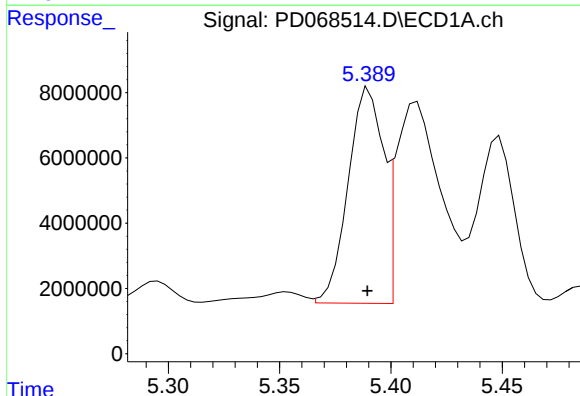


#25 Chlordane-3

R.T.: 5.390 min
Delta R.T.: 0.001 min
Response: 72464027
Conc: 519.71 ng/ml

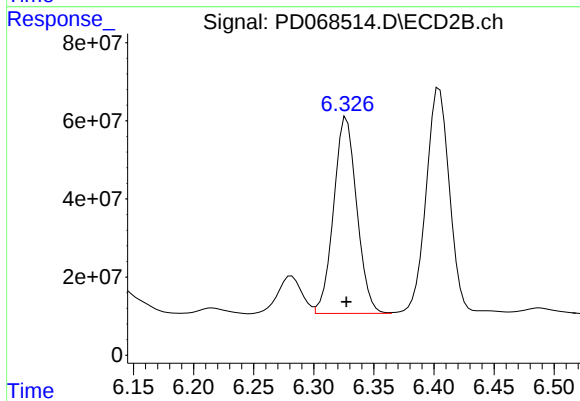

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 674496791
Conc: 502.01 ng/ml

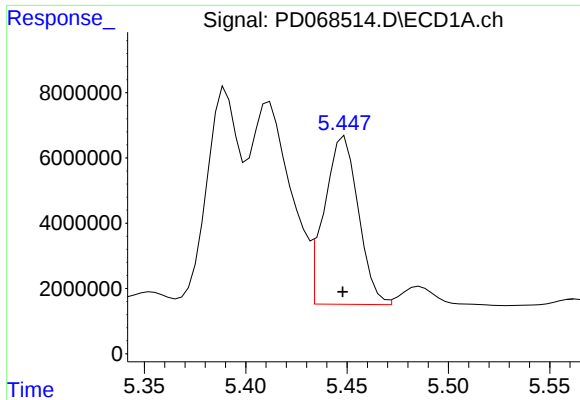

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 60020372
Conc: 507.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031222CHLOR

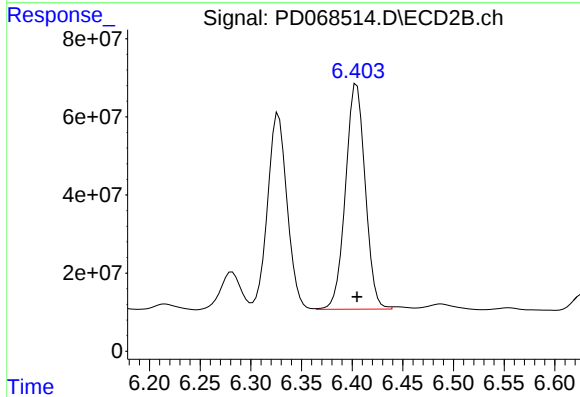


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 778530473
Conc: 500.80 ng/ml

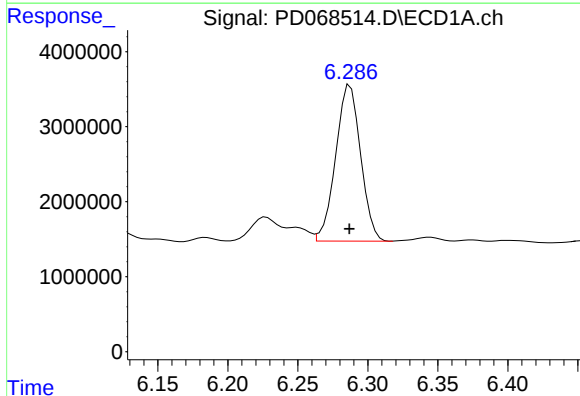


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 25821856
Conc: 516.85 ng/ml

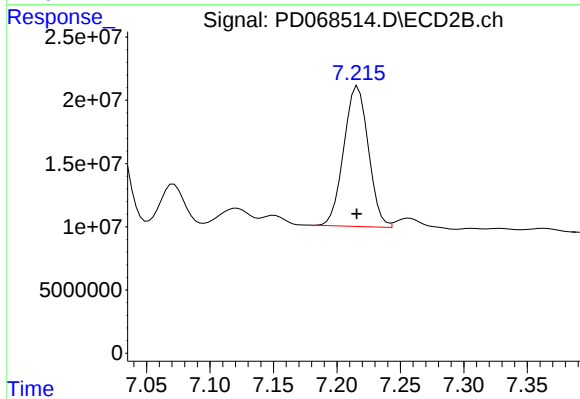

#27 Chlordane-5


R.T.: 7.217 min
Delta R.T.: 0.001 min
Response: 149347415
Conc: 511.83 ng/ml

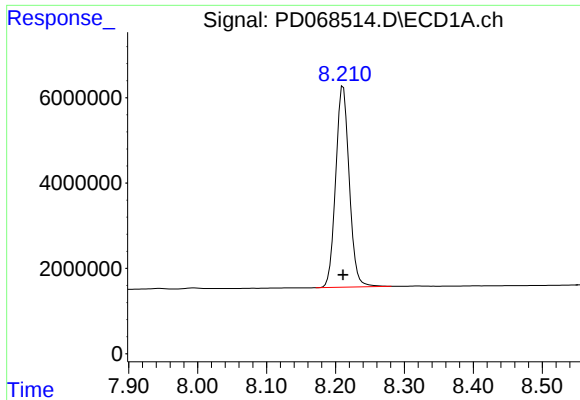

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 64402589
Conc: 49.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031222CHLOR

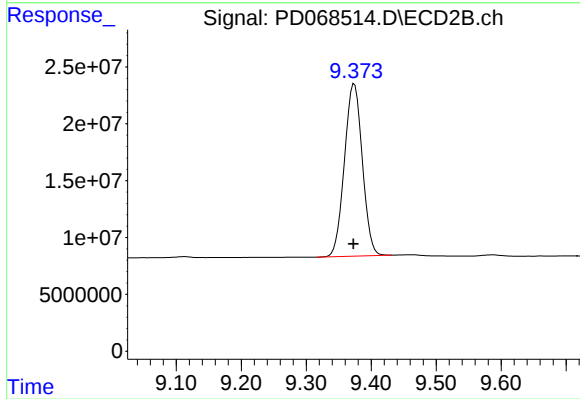

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.001 min
Response: 289696238
Conc: 50.23 ng/ml