

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
 Data File : PD082106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 18:42
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 03:53:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 12 03:53:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.789	112.4E6	-96649292	75.469	N.D. #
28)	SA Decachlor...	9.113	7.927	151.3E6	120.4E6	75.459	43.137 #
Target Compounds							
23)	Chlordane-1	4.730	3.787	58454865	77080200	748.375	748.411
24)	Chlordane-2	5.261	4.363	60302362	86909801	749.850	753.769
25)	Chlordane-3	5.974	4.993	245.1E6	249.9E6	750.007	751.774
26)	Chlordane-4	6.056	5.057	290.4E6	236.2E6	750.692	758.272
27)	Chlordane-5	6.908	5.952	51985065	89381425	752.434	749.026



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
Data File : PD082106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 18:42
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:53:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
Quant Title : GC Extractables
QLast Update : Tue Mar 12 03:53:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

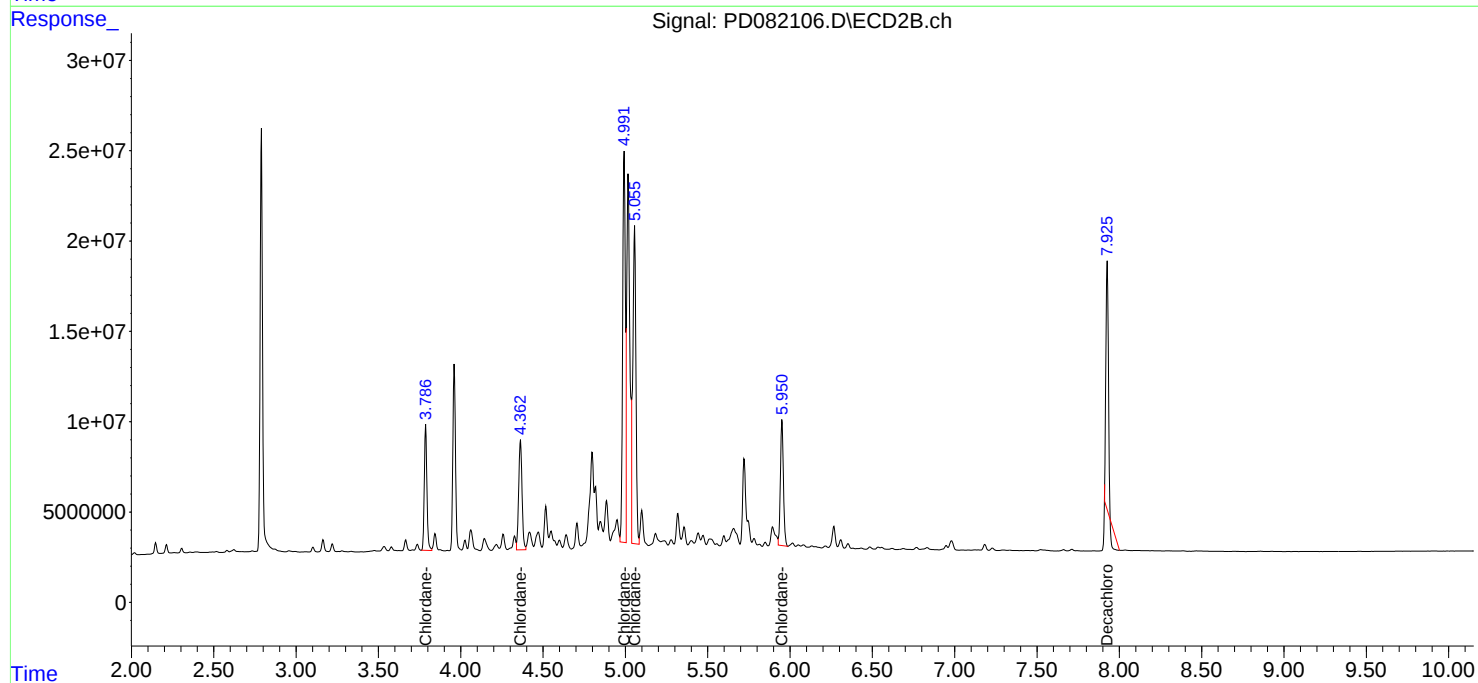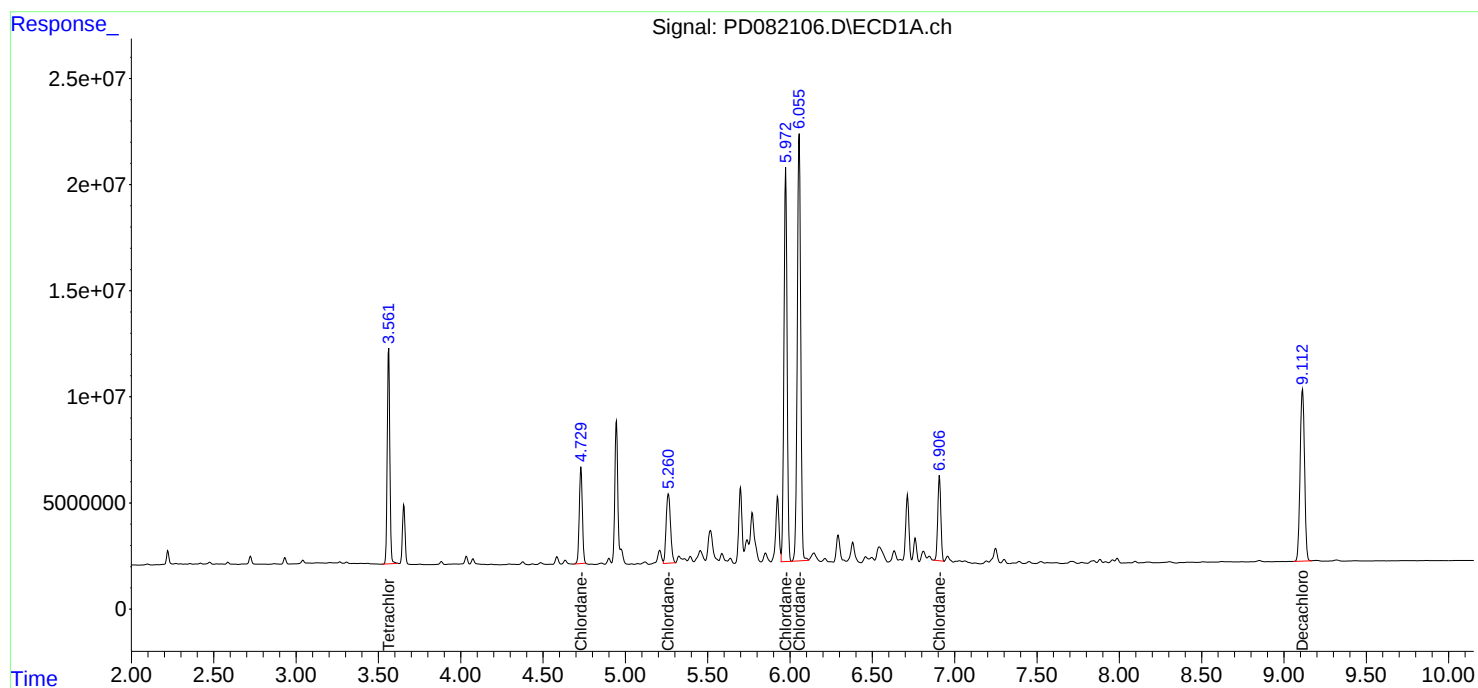


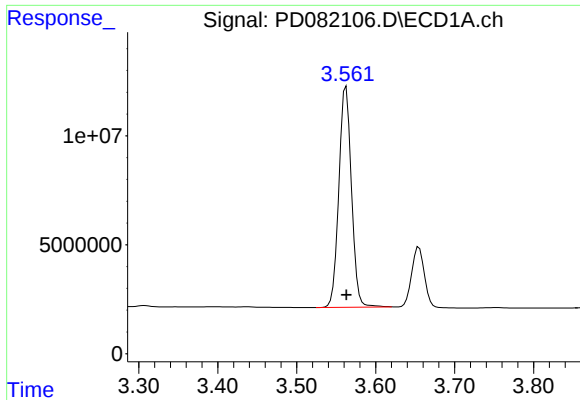

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 112377597
Conc: 75.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

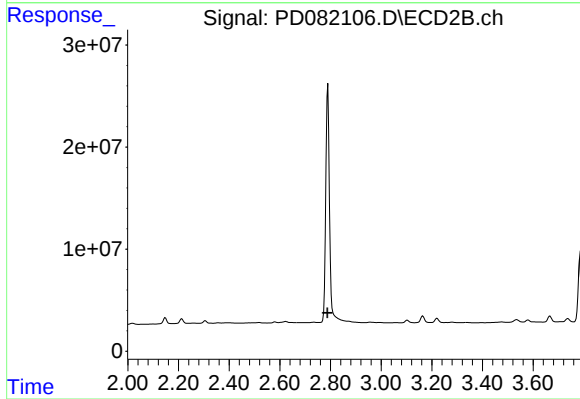


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.001 min
Response: -96649292
Conc: N.D.

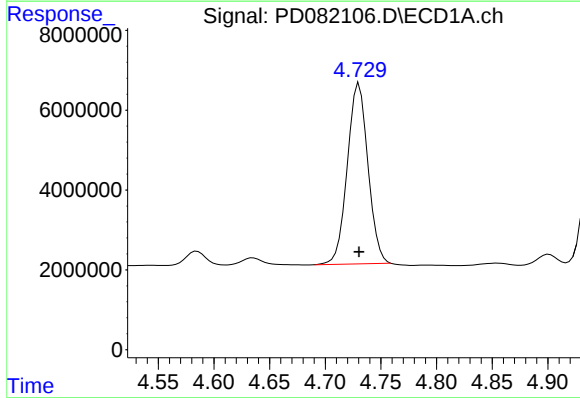


#23 Chlordane-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 58454865
Conc: 748.38 ng/ml

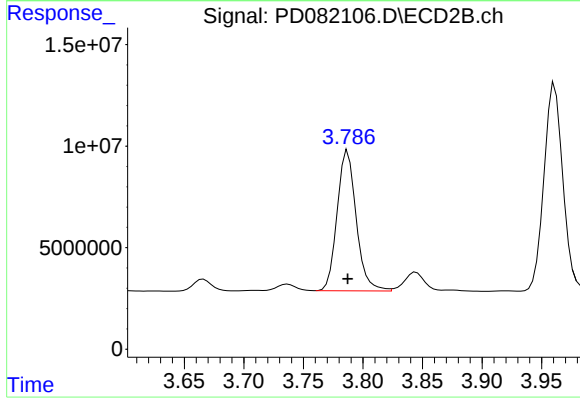

#23 Chlordane-1


R.T.: 3.787 min
Delta R.T.: 0.000 min
Response: 77080200
Conc: 748.41 ng/ml

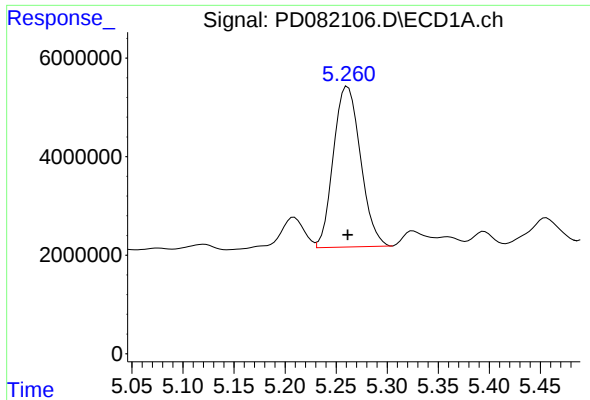

#24 Chlordane-2


R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 60302362
Conc: 749.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

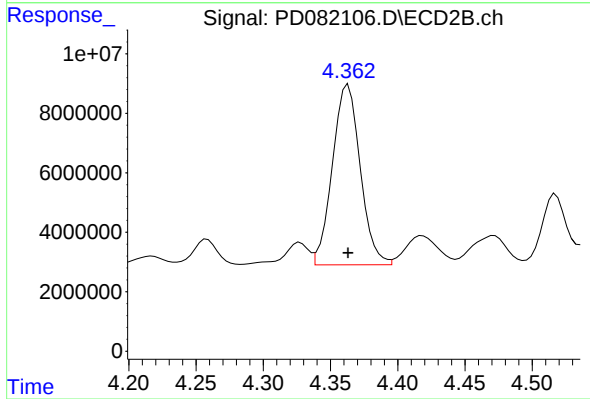


#24 Chlordane-2

R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 86909801
Conc: 753.77 ng/ml

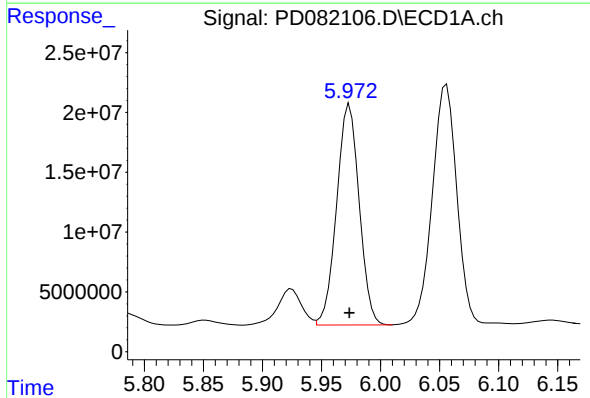


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 245147408
Conc: 750.01 ng/ml

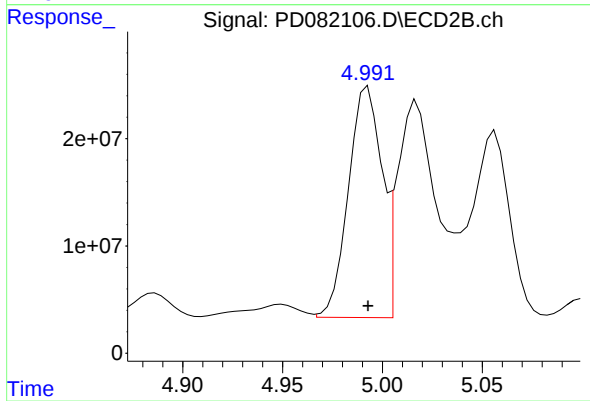

#25 Chlordane-3


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 249865994
Conc: 751.77 ng/ml

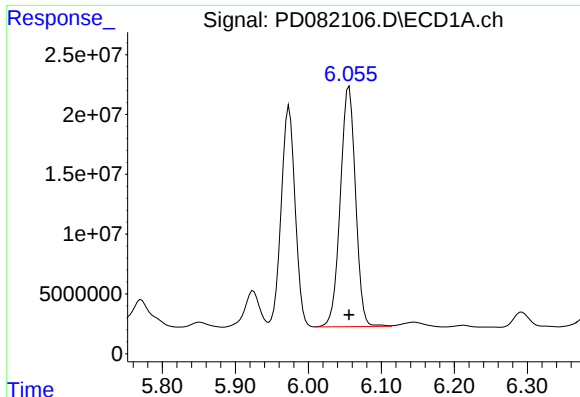

#26 Chlordane-4


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 290368087
Conc: 750.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

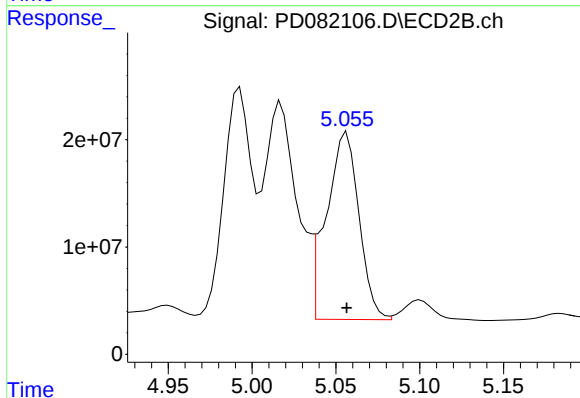


#26 Chlordane-4

R.T.: 5.057 min
Delta R.T.: 0.000 min
Response: 236181933
Conc: 758.27 ng/ml

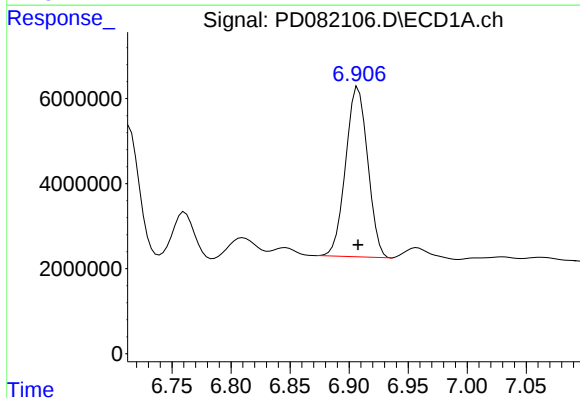


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 51985065
Conc: 752.43 ng/ml

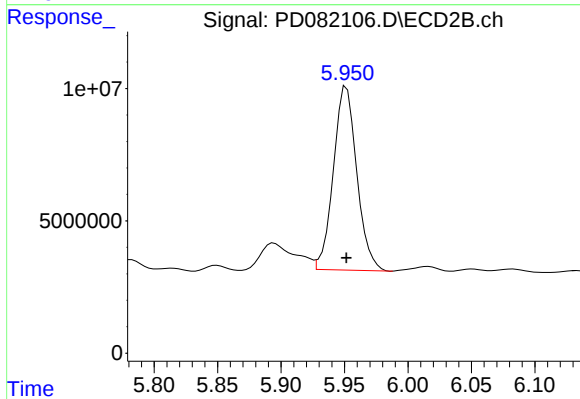

#27 Chlordane-5


R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 89381425
Conc: 749.03 ng/ml

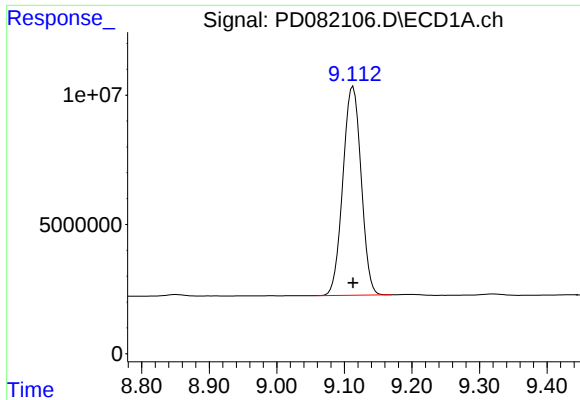

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 151302406
Conc: 75.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

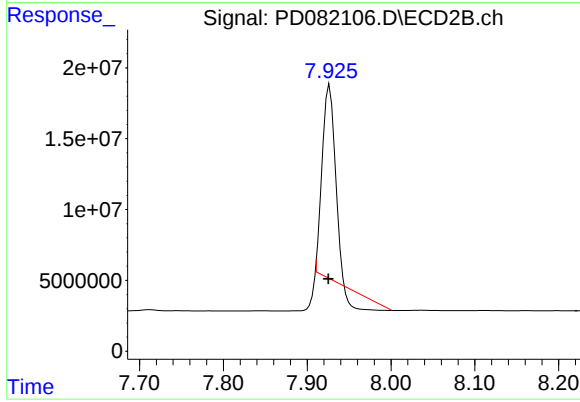

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.001 min
Response: 120381358
Conc: 43.14 ng/ml