

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
 Data File : PD082108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 19:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 03:55:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 12 03:55:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.790	33061635	-10488675	22.842	N.D. #
28) SA Decachlor...	9.112	7.927	52131148	40034801	25.742	14.272 #
Target Compounds						
23) Chlordane-1	4.731	3.787	17388673	25988269	228.887	251.746
24) Chlordane-2	5.261	4.363	20101574	30892577	249.970	263.212
25) Chlordane-3	5.974	4.993	76627041	81748570	238.141	246.956
26) Chlordane-4	6.056	5.057	92570608	77348994	241.906	248.747
27) Chlordane-5	6.908	5.952	16358271	29585917	239.945	248.447



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
Data File : PD082108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 19:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:55:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
Quant Title : GC Extractables
QLast Update : Tue Mar 12 03:55:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

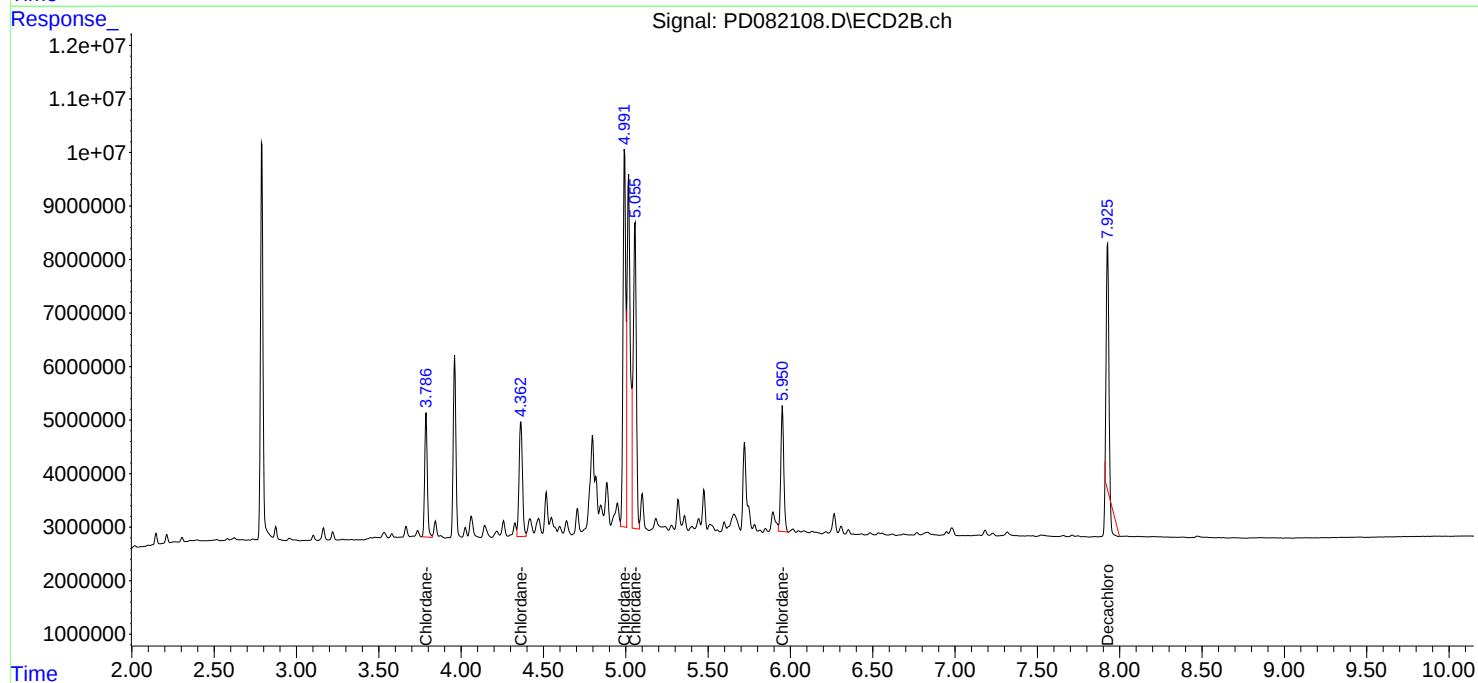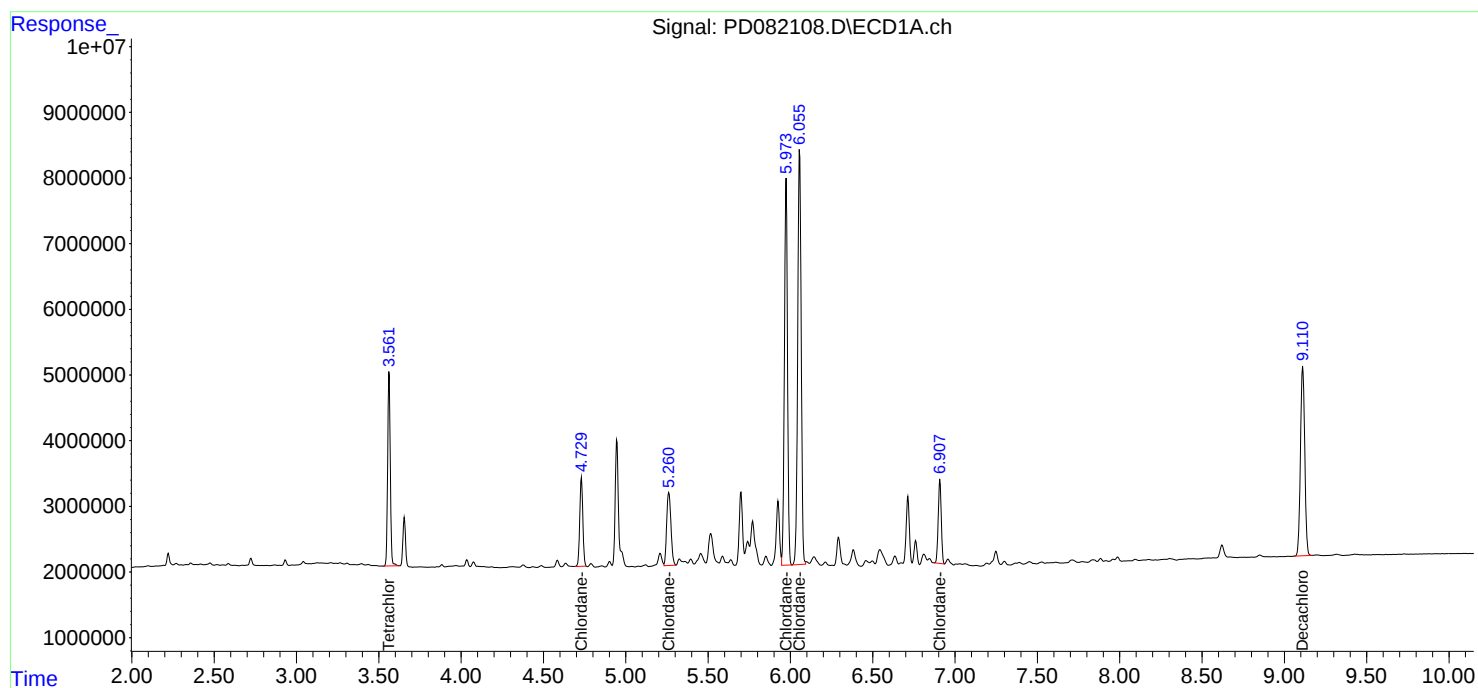


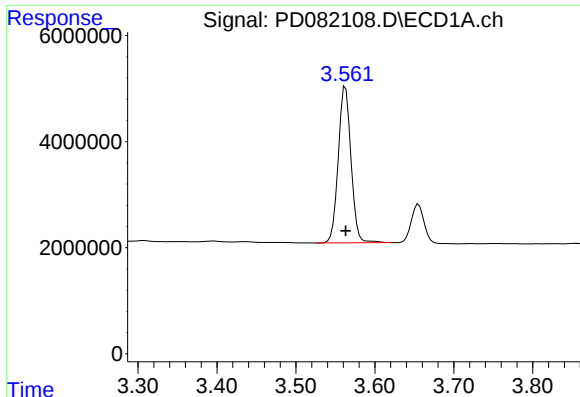

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 33061635
Conc: 22.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

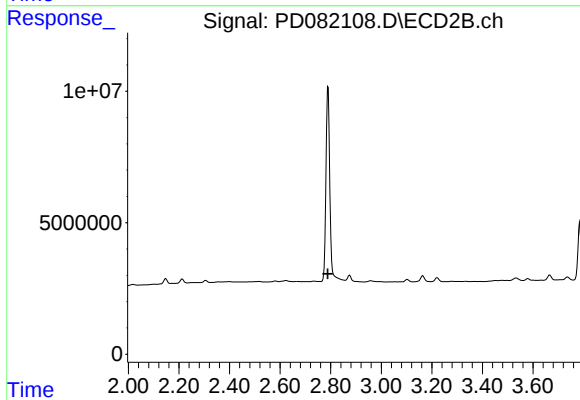


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.001 min
Response: -10488675
Conc: N.D.

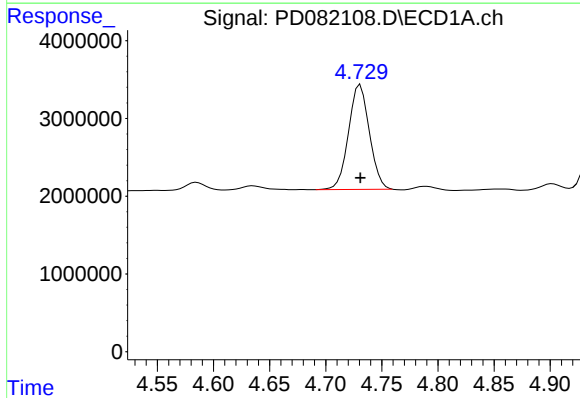


#23 Chlordane-1

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 17388673
Conc: 228.89 ng/ml

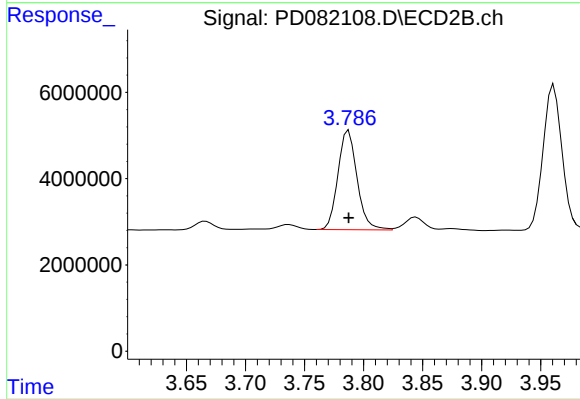

#23 Chlordane-1


R.T.: 3.787 min
Delta R.T.: 0.000 min
Response: 25988269
Conc: 251.75 ng/ml

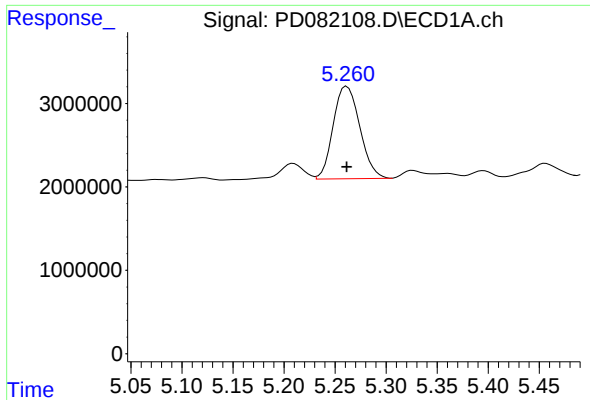

#24 Chlordane-2


R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 20101574
Conc: 249.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

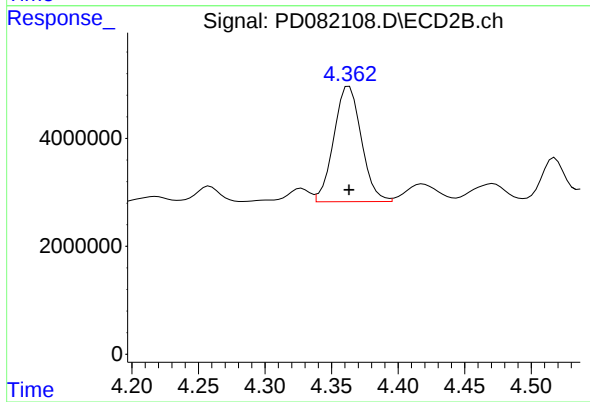


#24 Chlordane-2

R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 30892577
Conc: 263.21 ng/ml

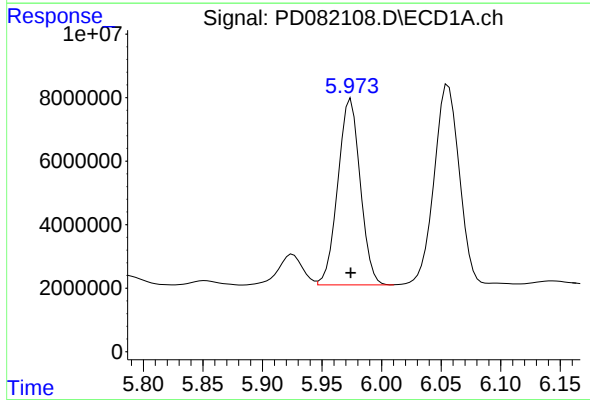


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 76627041
Conc: 238.14 ng/ml

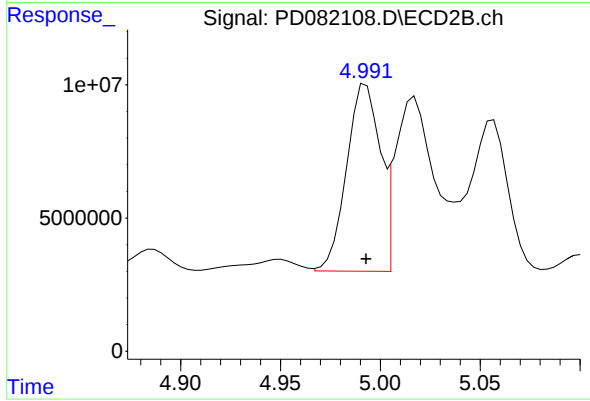

#25 Chlordane-3


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 81748570
Conc: 246.96 ng/ml

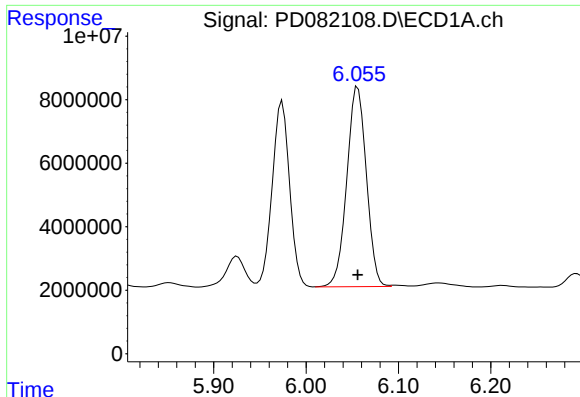

#26 Chlordane-4


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 92570608
Conc: 241.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

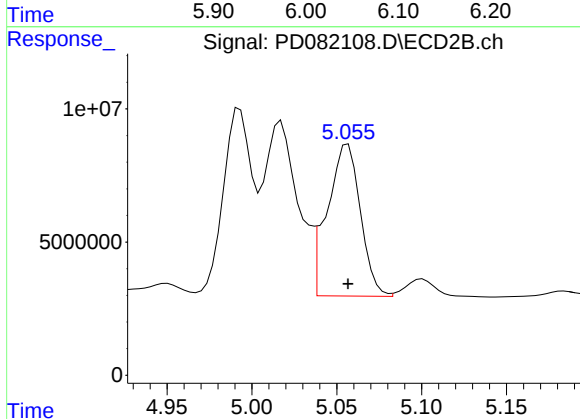


#26 Chlordane-4

R.T.: 5.057 min
Delta R.T.: 0.000 min
Response: 77348994
Conc: 248.75 ng/ml

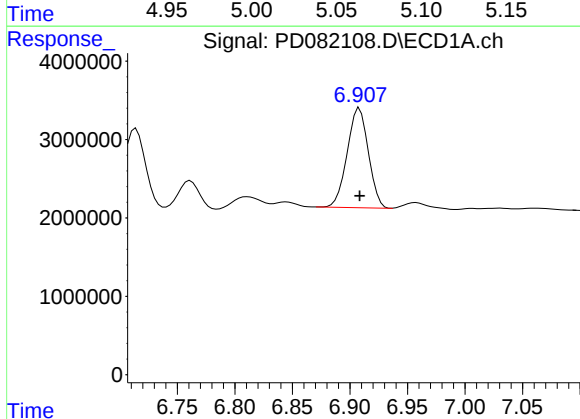


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 16358271
Conc: 239.94 ng/ml

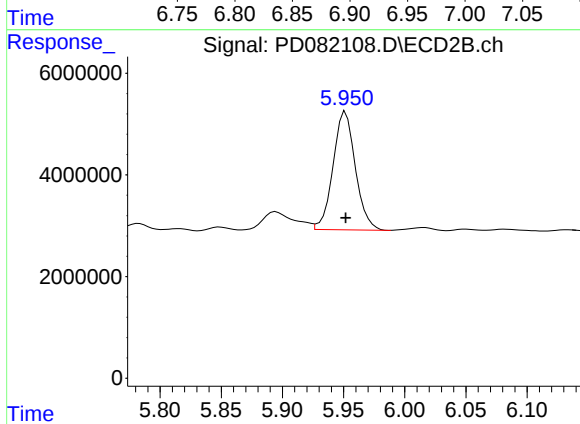

#27 Chlordane-5


R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 29585917
Conc: 248.45 ng/ml

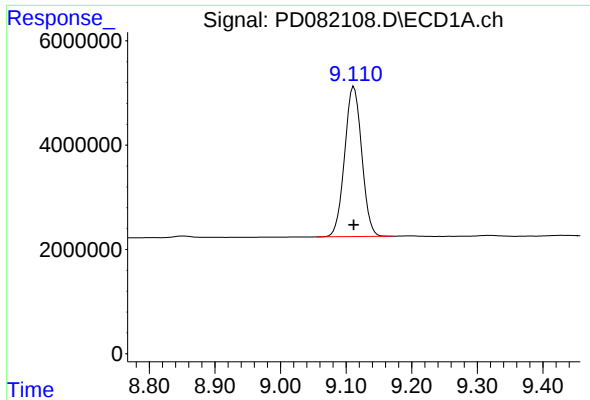

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 52131148
Conc: 25.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

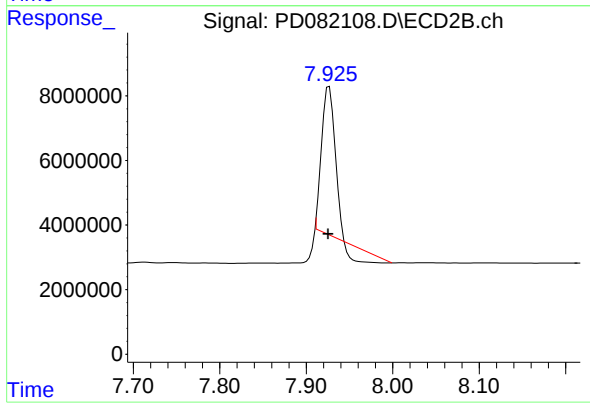

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.001 min
Response: 40034801
Conc: 14.27 ng/ml