

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
 Data File : PD082107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 18:56
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 02:45:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 12 02:44:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.813	73057369	154.3E6	50.000	50.000
28)	SA Decachlor...	9.113	7.950	97029331	135.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.730	3.810	37540084	50029090	500.000	500.000
24)	Chlordane-2	5.260	4.386	39383630	56317999	500.000	500.000
25)	Chlordane-3	5.973	5.016	154.1E6	158.9E6	500.000	500.000
26)	Chlordane-4	6.055	5.080	183.4E6	150.0E6	500.000	500.000
27)	Chlordane-5	6.907	5.974	33033348	57937761	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031224\
Data File : PD082107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 18:56
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 02:45:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031224.M
Quant Title : GC Extractables
QLast Update : Tue Mar 12 02:44:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

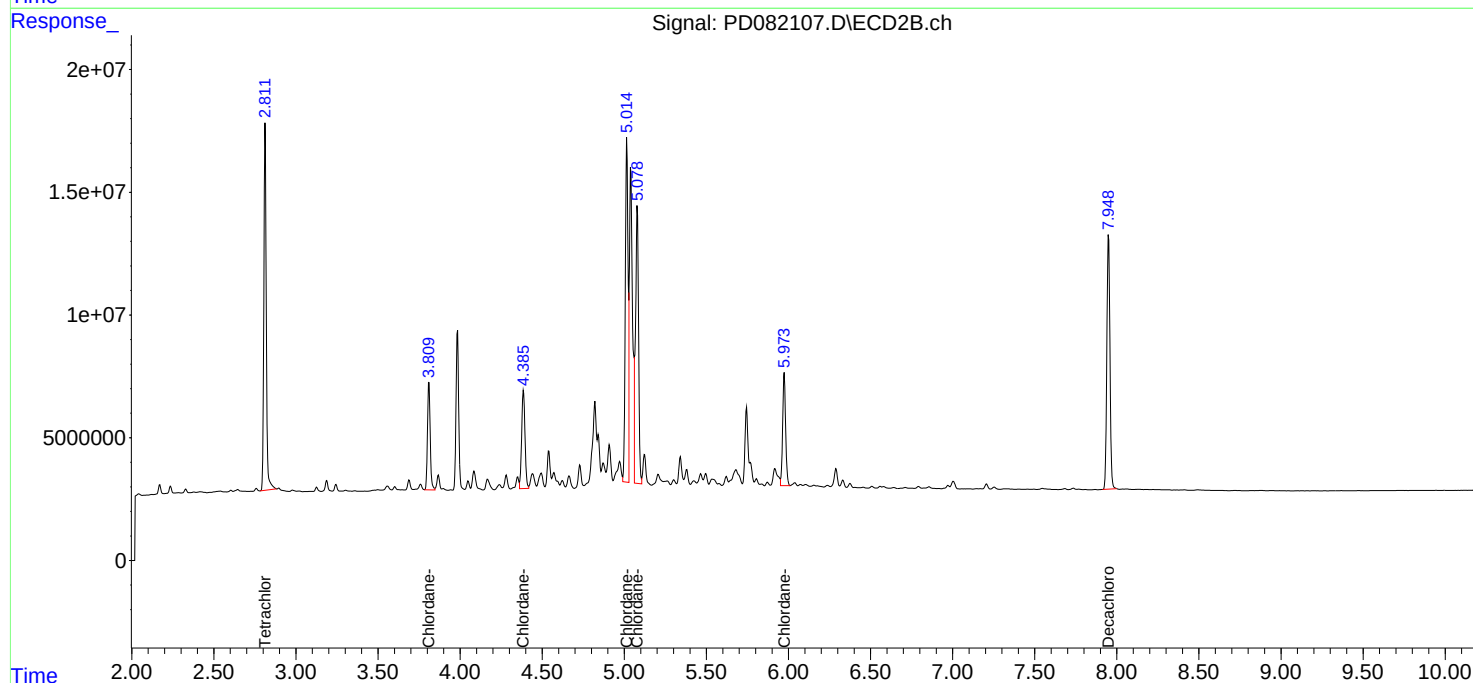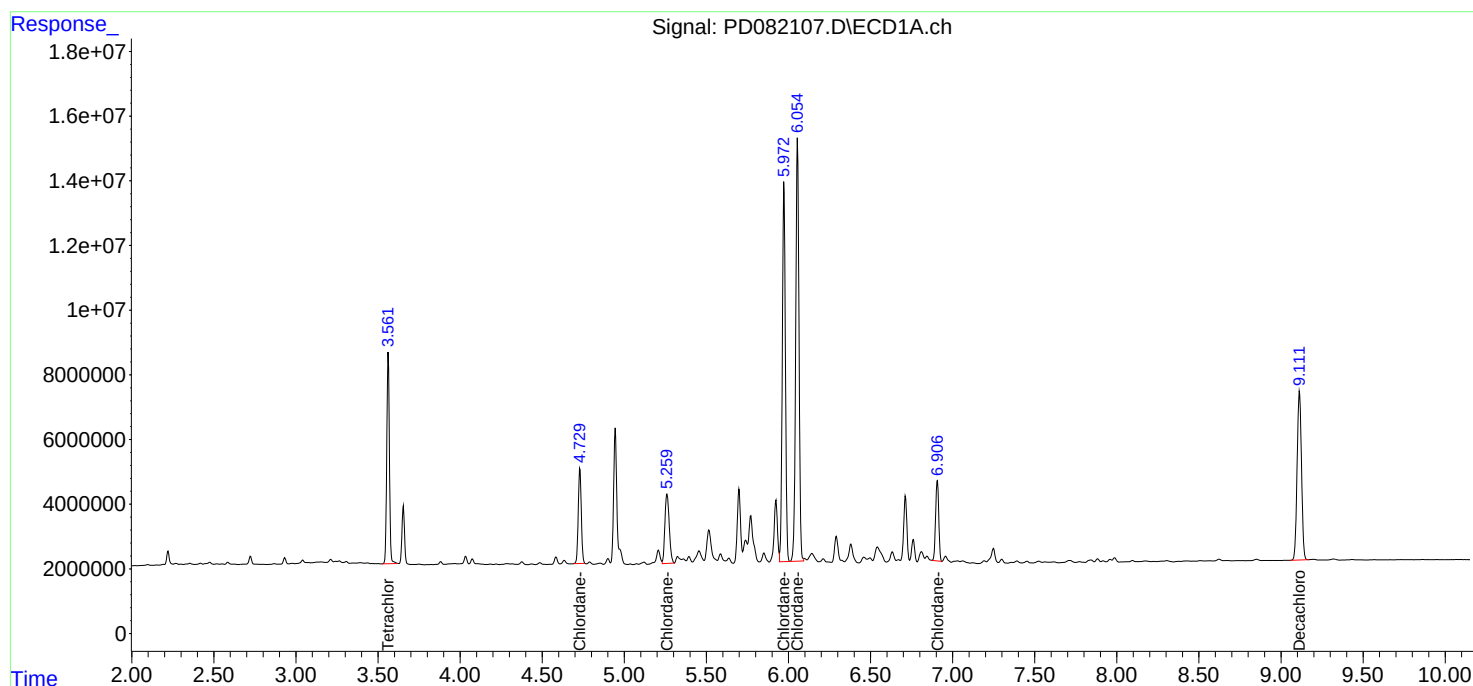


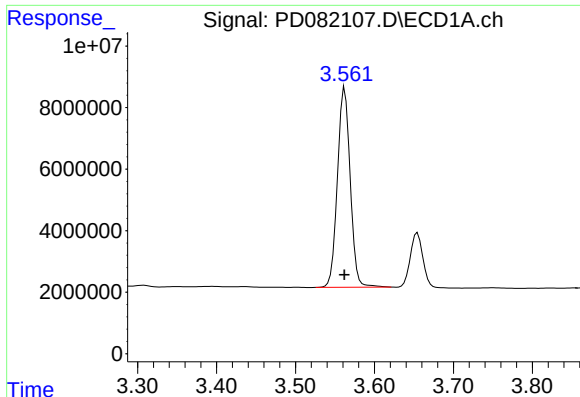

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 73057369
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

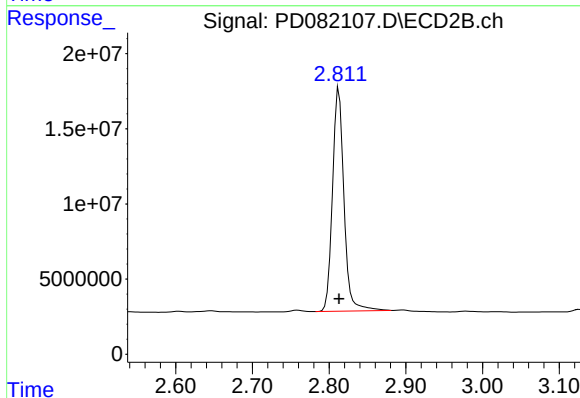


#1 Tetrachloro-m-xylene

R.T.: 2.813 min
Delta R.T.: 0.000 min
Response: 154331852
Conc: 50.00 ng/ml

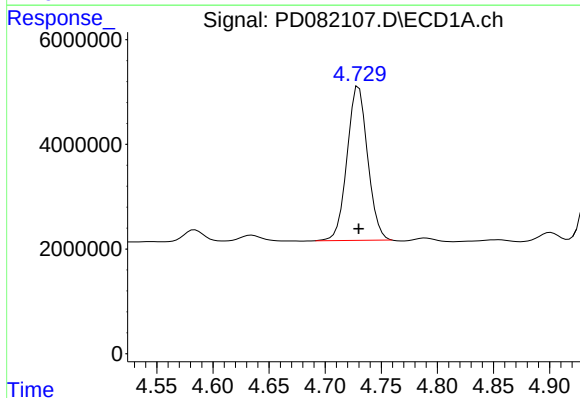


#23 Chlordane-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 37540084
Conc: 500.00 ng/ml

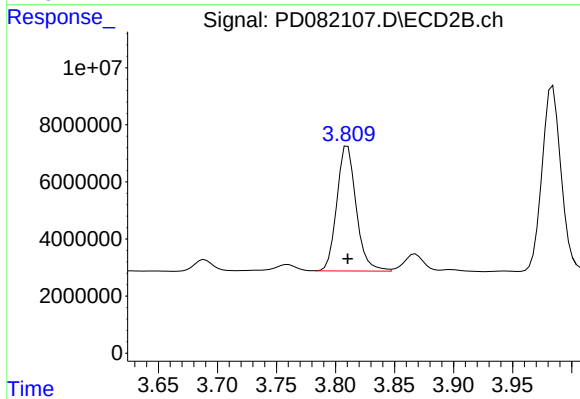

#23 Chlordane-1


R.T.: 3.810 min
Delta R.T.: 0.000 min
Response: 50029090
Conc: 500.00 ng/ml

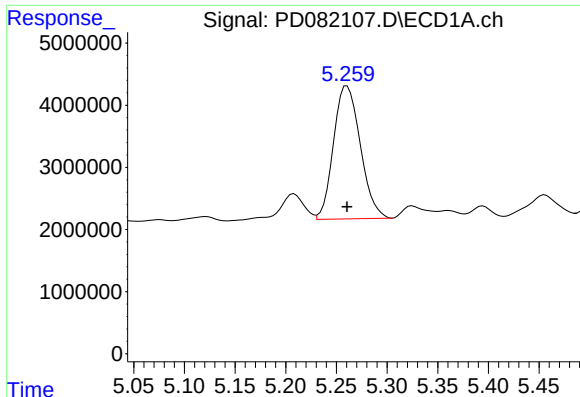

#24 Chlordane-2


R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 39383630
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

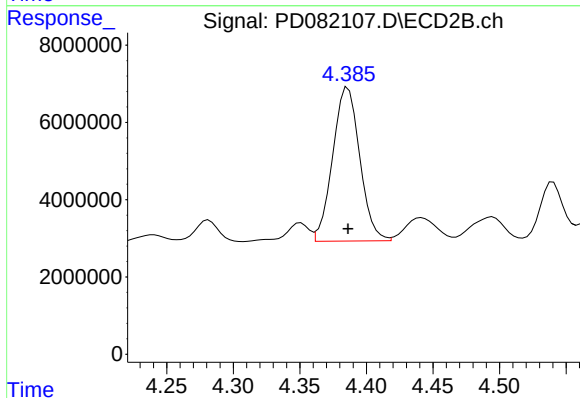


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 56317999
Conc: 500.00 ng/ml

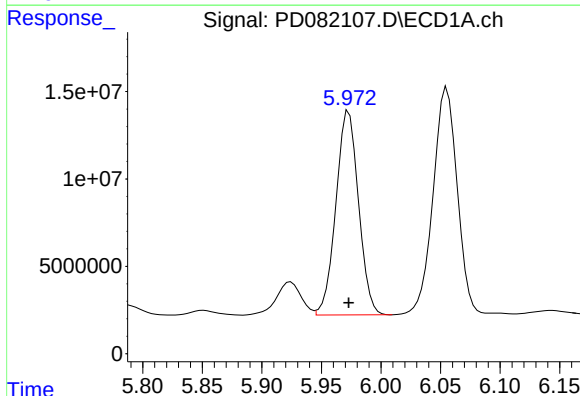


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 154144155
Conc: 500.00 ng/ml

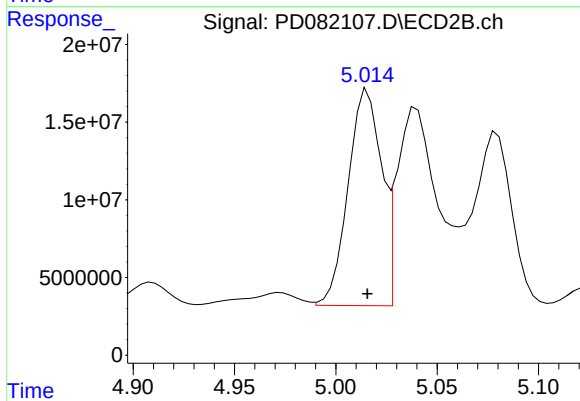

#25 Chlordane-3


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 158860527
Conc: 500.00 ng/ml

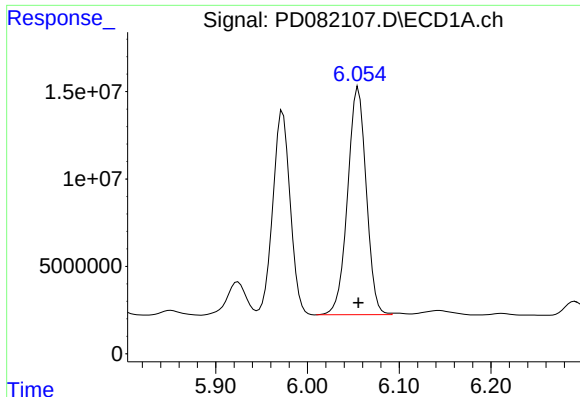

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 183381186
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

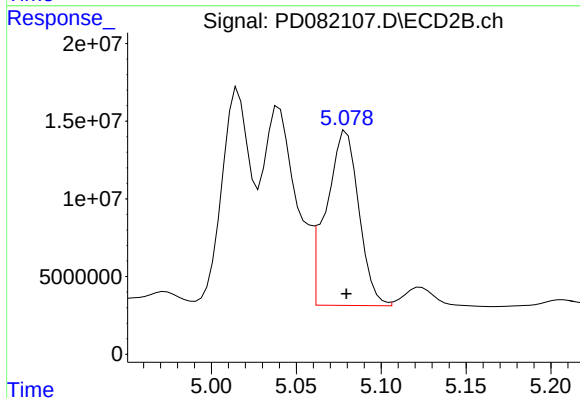


#26 Chlordane-4

R.T.: 5.080 min
Delta R.T.: 0.000 min
Response: 149977031
Conc: 500.00 ng/ml

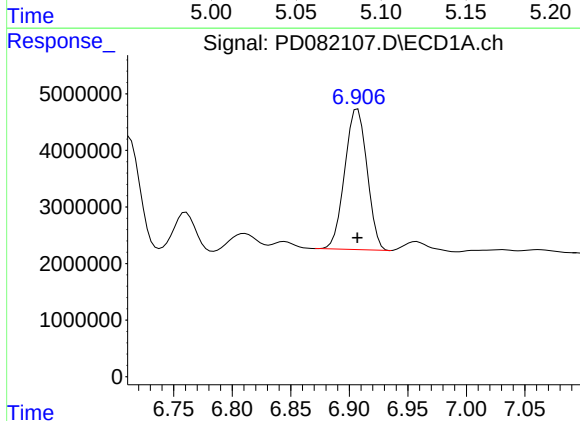


#27 Chlordane-5

R.T.: 6.907 min
Delta R.T.: 0.000 min
Response: 33033348
Conc: 500.00 ng/ml

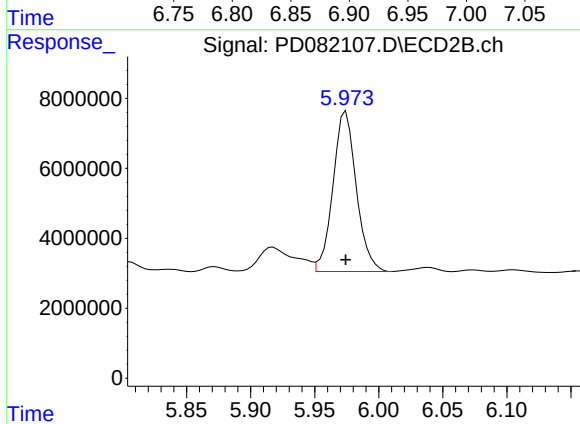

#27 Chlordane-5


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 57937761
Conc: 500.00 ng/ml

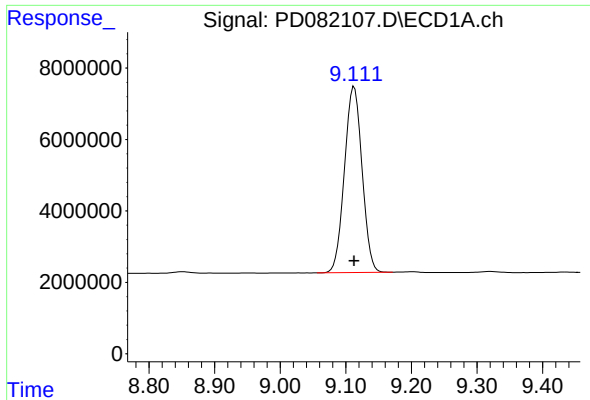

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 97029331
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

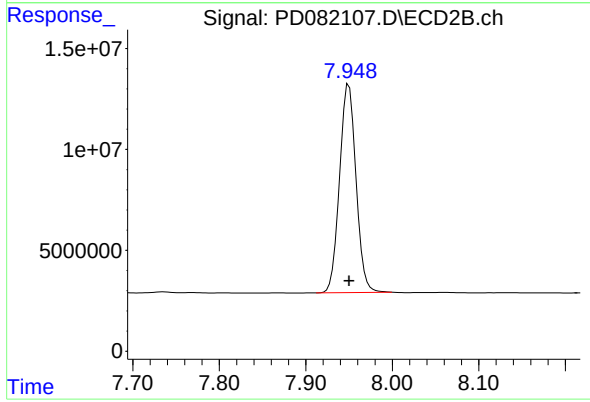

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 135861974
Conc: 50.00 ng/ml