

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031319\
 Data File : PD051807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2019 22:32
 Operator : AJ\SJ
 Sample : K1794-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5P5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:29:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	23885121	434.6E6	16.621	14.066
27)	SA Decachlor...	7.821	9.155	30072341	449.9E6	25.005	23.732
Target Compounds							
2)	A alpha-BHC	3.596f	4.475f	8908908	203.2E6	4.019	4.349
3)	MA gamma-BHC...	0.000	4.691f	0	149.9E6	N.D.	3.508
8)	B Heptachlo...	0.000	5.913	0	39706763	N.D.	1.109
9)	A Endosulfan I	0.000	6.232f	0	28458878	N.D.	0.858
10)	B trans-Chl...	0.000	6.232f	0	28458878	N.D.	0.788
11)	B cis-Chlor...	0.000	6.232	0	28458878	N.D.	0.822
12)	B 4,4'-DDE	0.000	6.372	0	8897567	N.D.	0.272
15)	B Endosulfa...	0.000	6.985	0	14369472	N.D.	0.523


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031319\
Data File : PD051807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2019 22:32
Operator : AJ\SJ
Sample : K1794-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5P5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:29:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

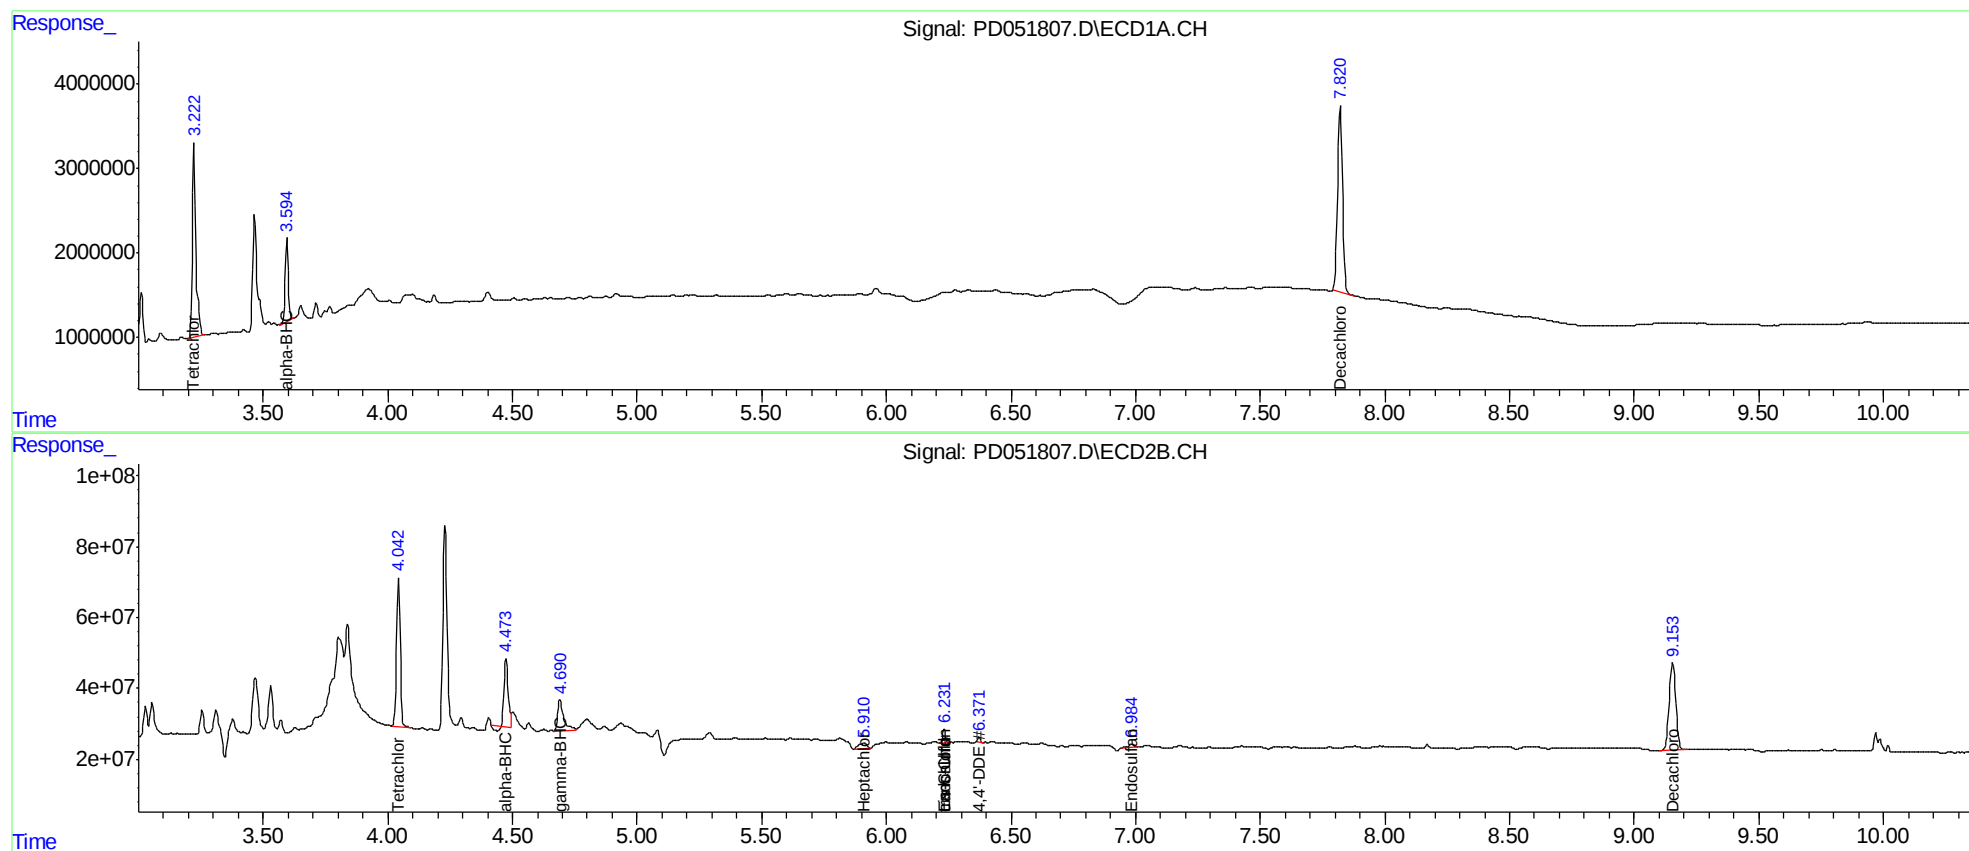


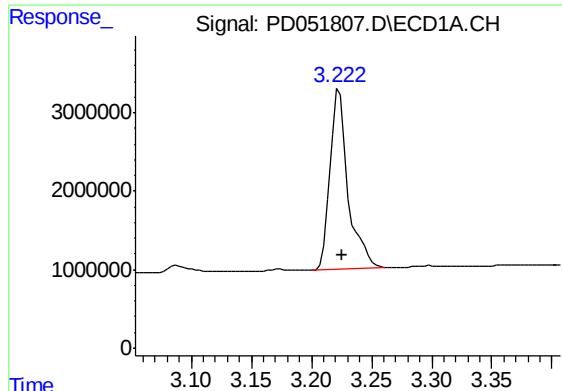

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.002 min
Response: 23885121
Conc: 16.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5P5

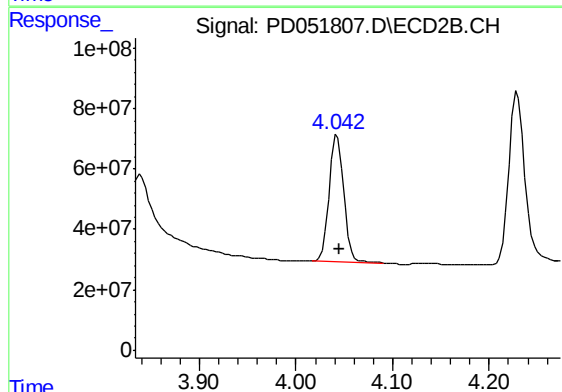


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 434578400
Conc: 14.07 ng/ml

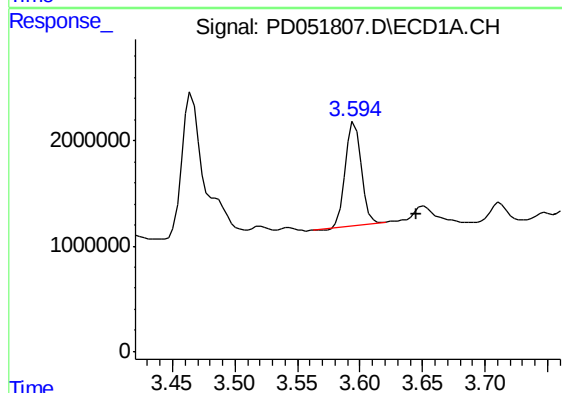


#2 alpha-BHC

R.T.: 3.596 min
Delta R.T.: -0.049 min
Response: 8908908
Conc: 4.02 ng/ml

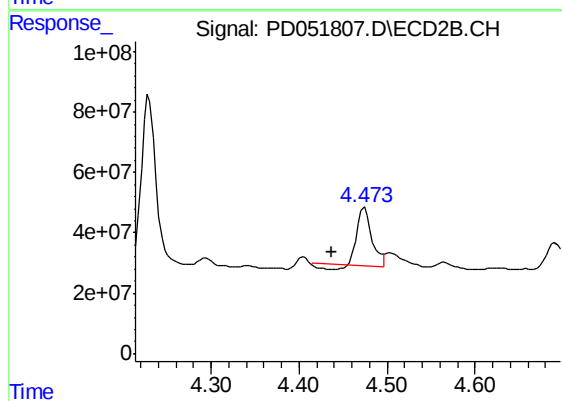

#2 alpha-BHC


R.T.: 4.475 min
Delta R.T.: 0.037 min
Response: 203177381
Conc: 4.35 ng/ml

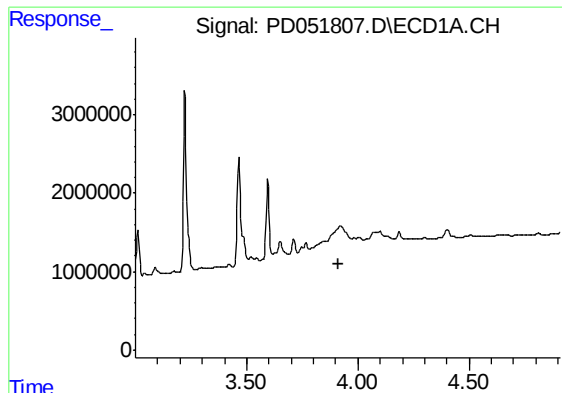

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.913 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5P5

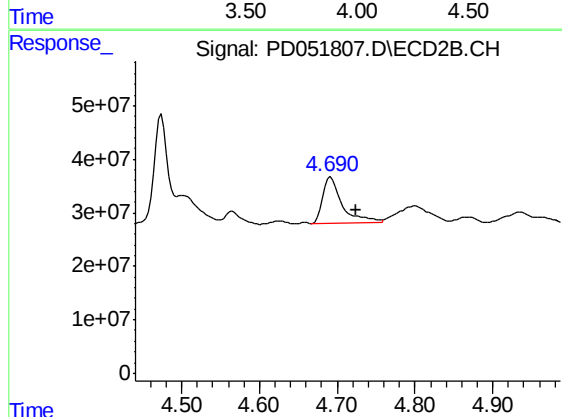


#3 gamma-BHC (Lindane)

R.T.: 4.691 min
Delta R.T.: -0.033 min
Response: 149864358
Conc: 3.51 ng/ml

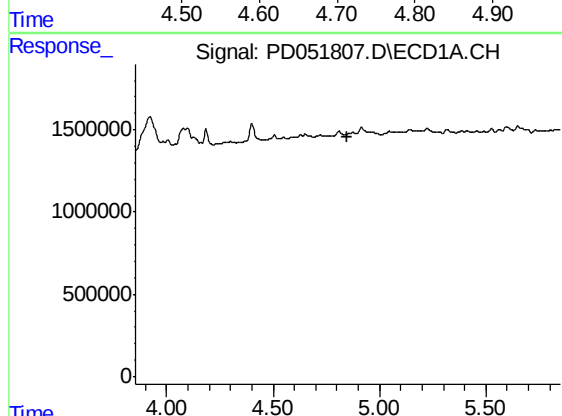


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

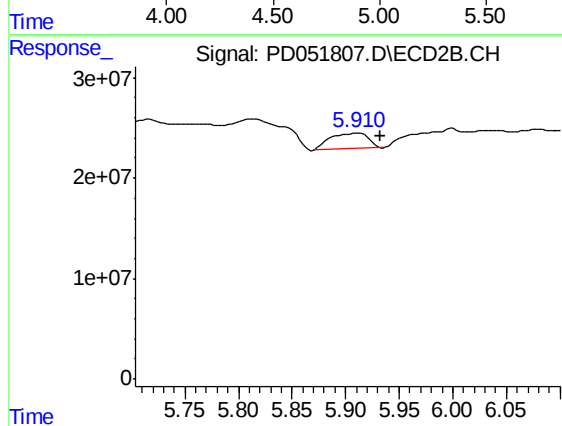

#8 Heptachlor epoxide


R.T.: 5.913 min
Delta R.T.: -0.020 min
Response: 39706763
Conc: 1.11 ng/ml

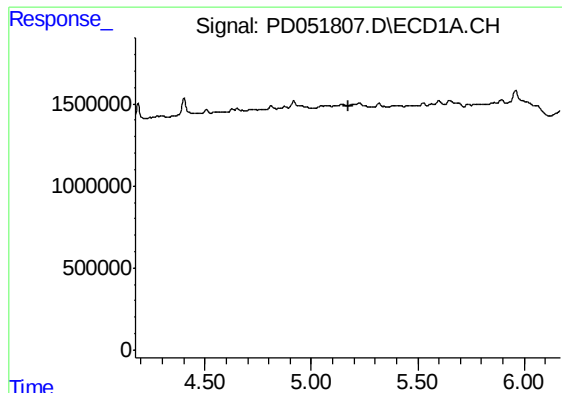

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5P5

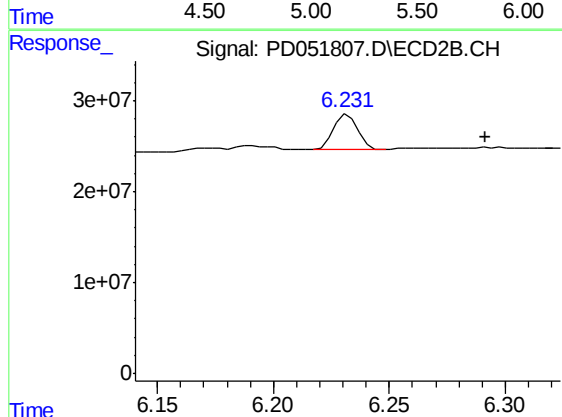


#9 Endosulfan I

R.T.: 6.232 min
Delta R.T.: -0.059 min
Response: 28458878
Conc: 0.86 ng/ml

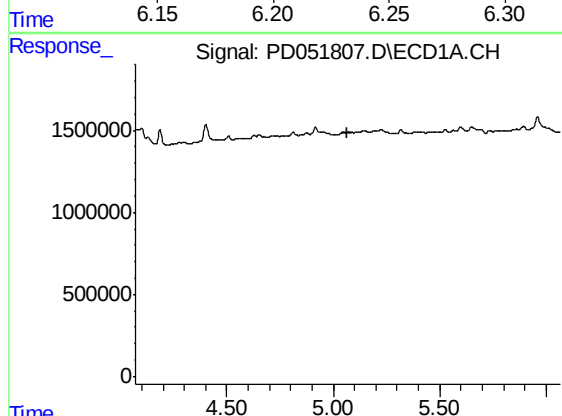


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

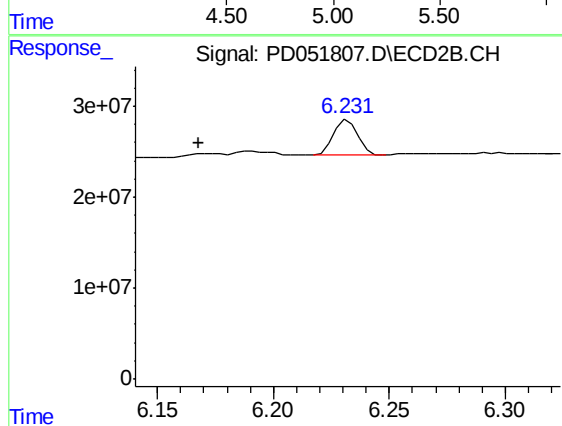

#10 trans-Chlordane


R.T.: 6.232 min
Delta R.T.: 0.064 min
Response: 28458878
Conc: 0.79 ng/ml

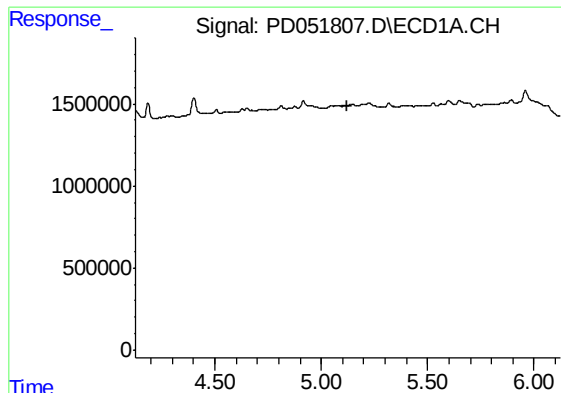

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5P5

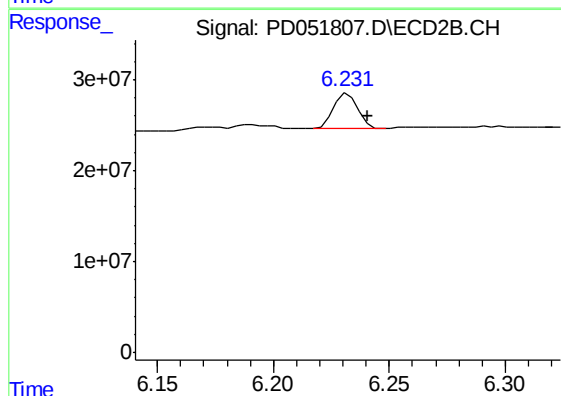


#11 cis-Chlordane

R.T.: 6.232 min
Delta R.T.: -0.008 min
Response: 28458878
Conc: 0.82 ng/ml

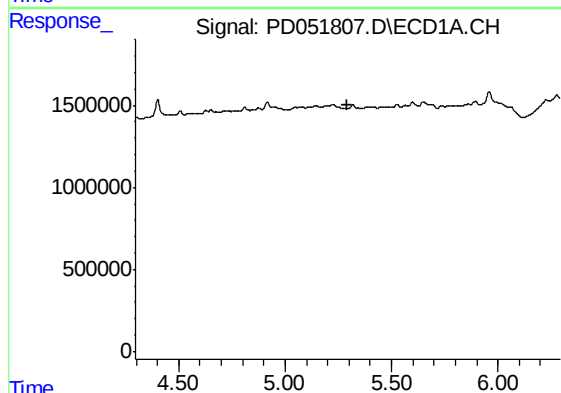


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

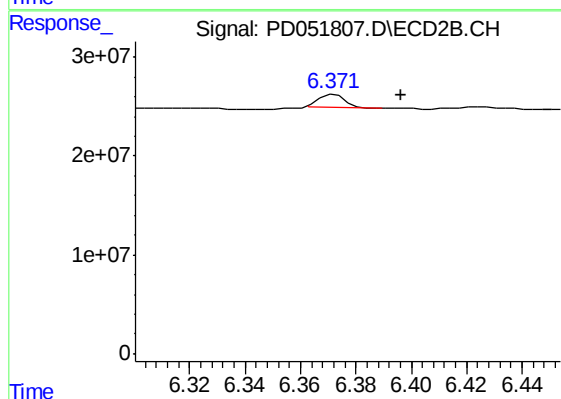

#12 4,4'-DDE


R.T.: 6.372 min
Delta R.T.: -0.024 min
Response: 8897567
Conc: 0.27 ng/ml

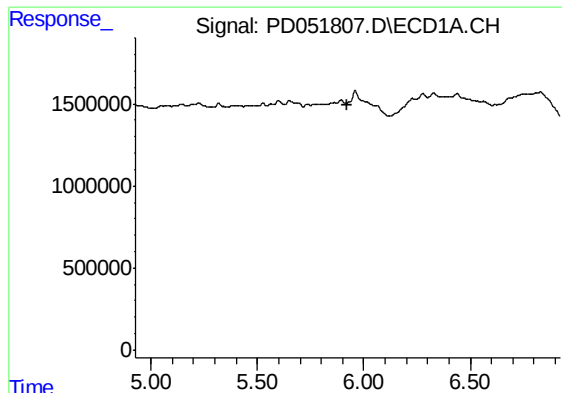

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5P5

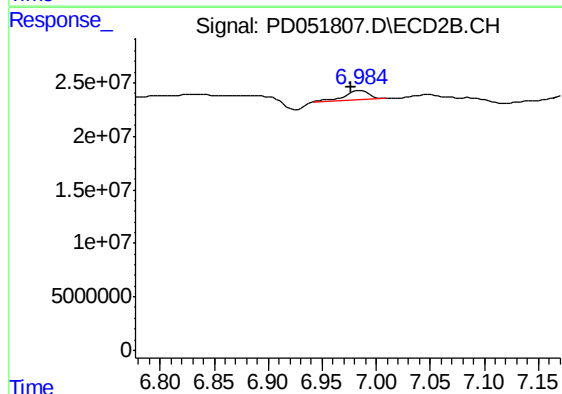


#15 Endosulfan II

R.T.: 6.985 min
Delta R.T.: 0.008 min
Response: 14369472
Conc: 0.52 ng/ml

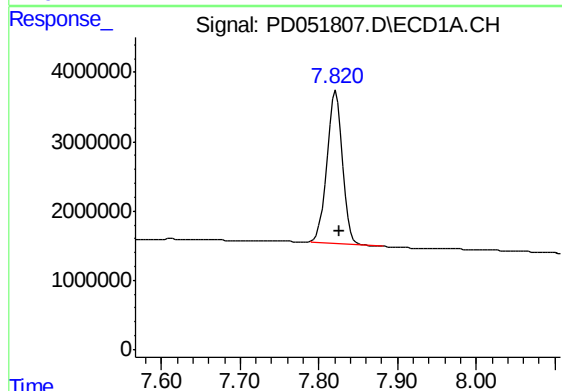

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: -0.005 min
Response: 30072341
Conc: 25.01 ng/ml

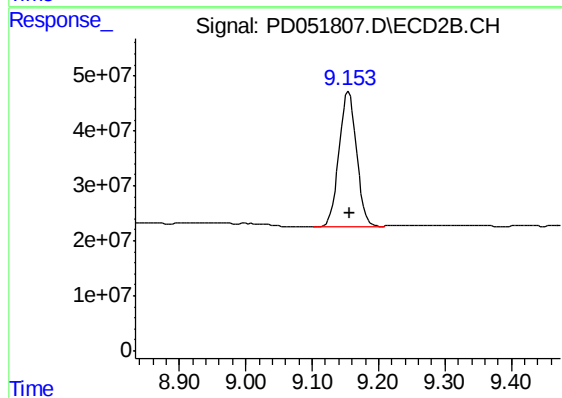

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 449905246
Conc: 23.73 ng/ml