

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
 Data File : PD068520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2022 01:10
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 05:28:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 05:20:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	13513189	113.7E6	10.229	10.895
27)	SA Decachlor...	8.212	9.374	28592307	132.8E6	21.365	22.157
Target Compounds							
22)	Toxaphene-1	5.707	6.610	9923192	44122581	992.590	1090.127
23)	Toxaphene-2	6.190	6.799	10896443	106.9E6	1025.736	1101.714
24)	Toxaphene-3	6.311	7.388	25120106	232.1E6	974.858	1079.159
25)	Toxaphene-4	6.558	7.478	26909886	139.0E6	962.519	1072.579
26)	Toxaphene-5	7.045	7.891	28579903	90427321	983.848	1072.760

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
Data File : PD068520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2022 01:10
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 05:28:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 05:20:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

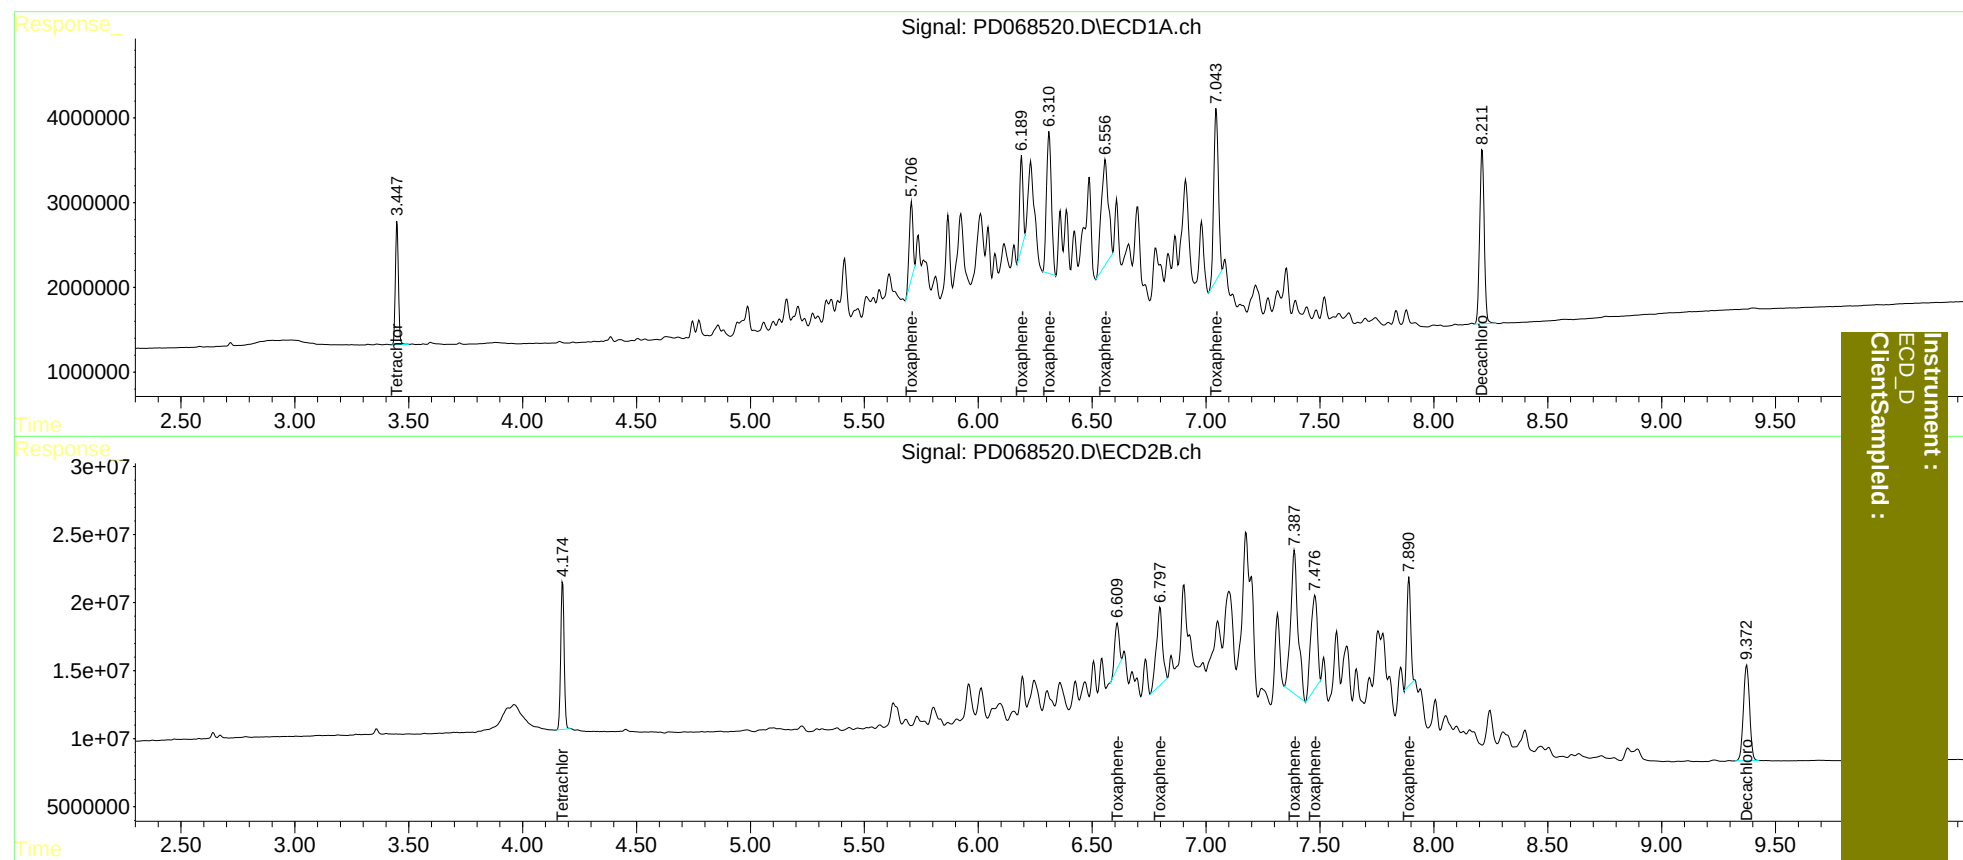

Instrument :
ECD_D
ClientSampled :
Instrument :
ECD_D
ClientSampled :