

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
 Data File : PD068523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2022 01:51
 Operator : AR\AJ
 Sample : TOXAPH501
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 05:25:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 05:20:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	105.7E6	777.4E6	80.229	76.669
27)	SA Decachlor...	8.211	9.374	204.1E6	863.5E6	155.083	148.712
Target Compounds							
22)	Toxaphene-1	5.708	6.610	82219111	300.3E6	8141.070	7706.796
23)	Toxaphene-2	6.191	6.799	85491945	733.3E6	8047.201	7762.736
24)	Toxaphene-3	6.312	7.389	216.3E6	1622.3E6	8302.247	7698.813
25)	Toxaphene-4	6.558	7.479	235.9E6	988.9E6	8304.048	7756.415
26)	Toxaphene-5	7.046	7.892	242.4E6	623.2E6	8312.524	7597.376

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
Data File : PD068523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2022 01:51
Operator : AR\AJ
Sample : TOXAPH501
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 05:25:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 05:20:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

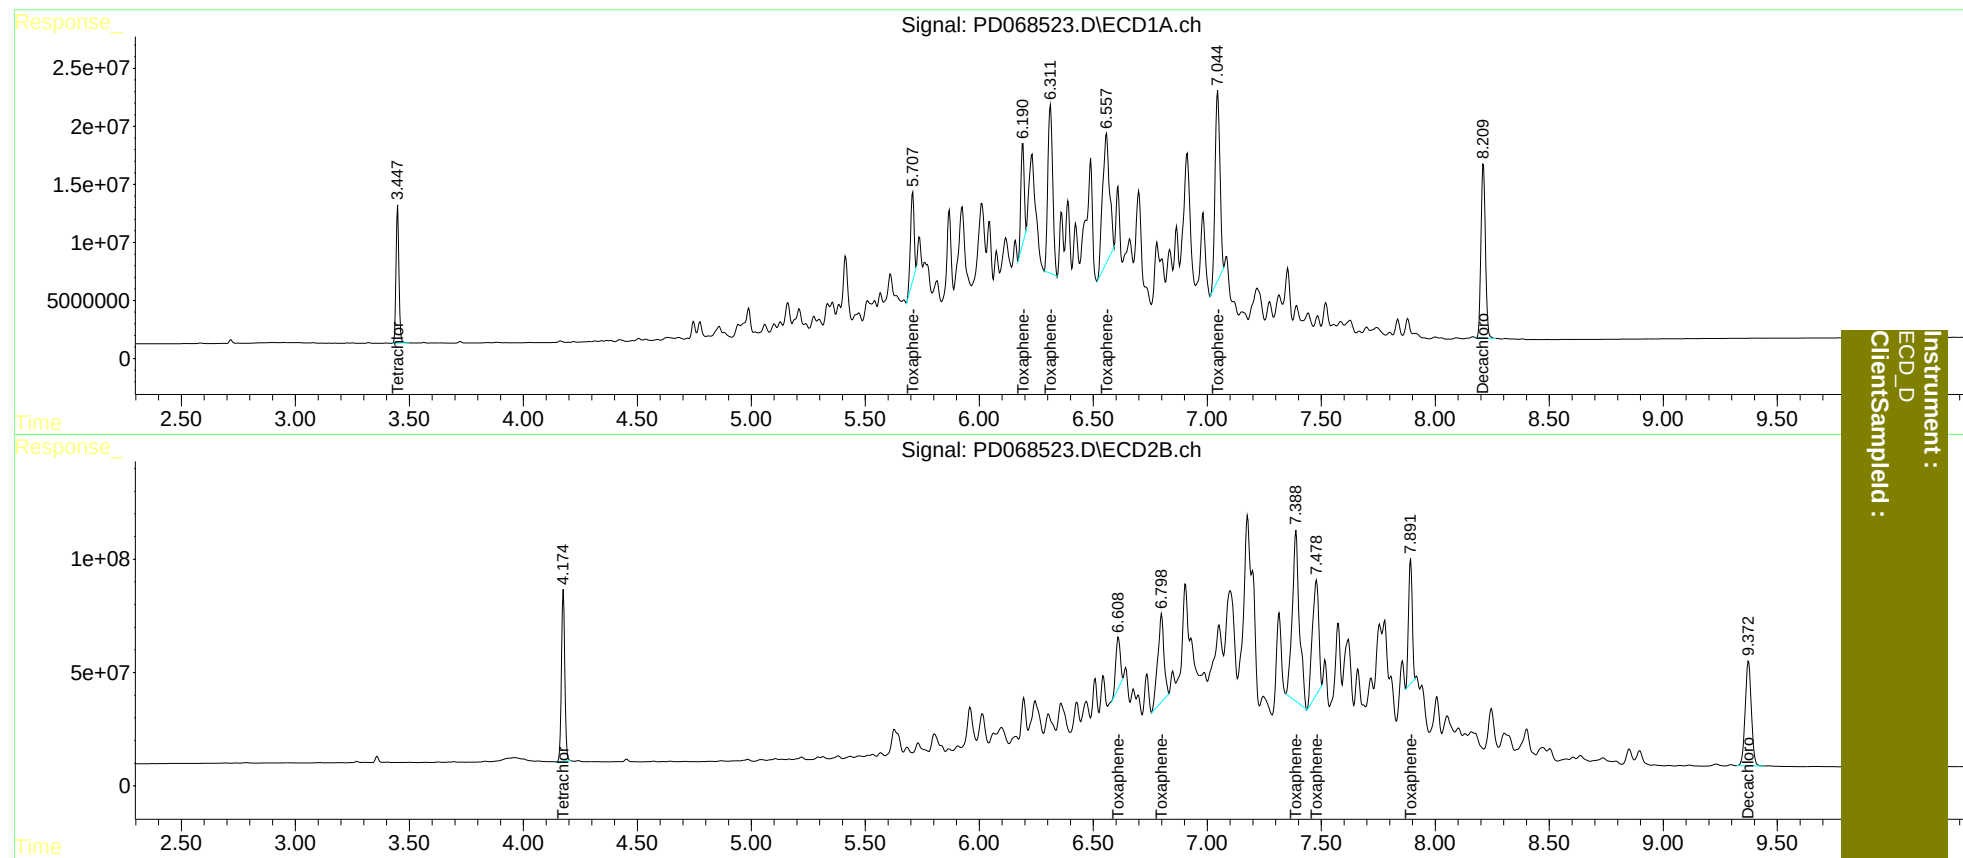

Instrument :
ECD_D
ClientSampled :