

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
 Data File : PD068530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2022 03:30
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 06:36:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 06:33:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	52187781	399.2E6	38.923	38.551
27)	SA Decachlor...	8.213	9.377	102.5E6	458.7E6	77.854	78.273
Target Compounds							
2)	A alpha-BHC	3.889	4.572	77003554	591.0E6	39.003	39.117
3)	MA gamma-BHC...	4.172	4.863	72049921	544.6E6	38.929	39.131
4)	MA Heptachlor	4.471	5.390	69272344	511.2E6	38.673	38.983
9)	A Endosulfan I	5.503	6.455	58801307	402.5E6	38.732	39.147
13)	MA Dieldrin	5.747	6.713	132.3E6	829.8E6	77.661	78.153
14)	MA Endrin	6.006	6.934	109.6E6	624.4E6	76.934	77.108
16)	A 4,4'-DDD	6.133	7.045	103.7E6	625.0E6	77.969	78.251
17)	MA 4,4'-DDT	6.373	7.348	105.7E6	589.8E6	77.370	77.688
20)	A Methoxychlor	6.926	7.801	269.7E6	1285.2E6	389.422	390.096

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031322\
Data File : PD068530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2022 03:30
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 06:36:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 06:33:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

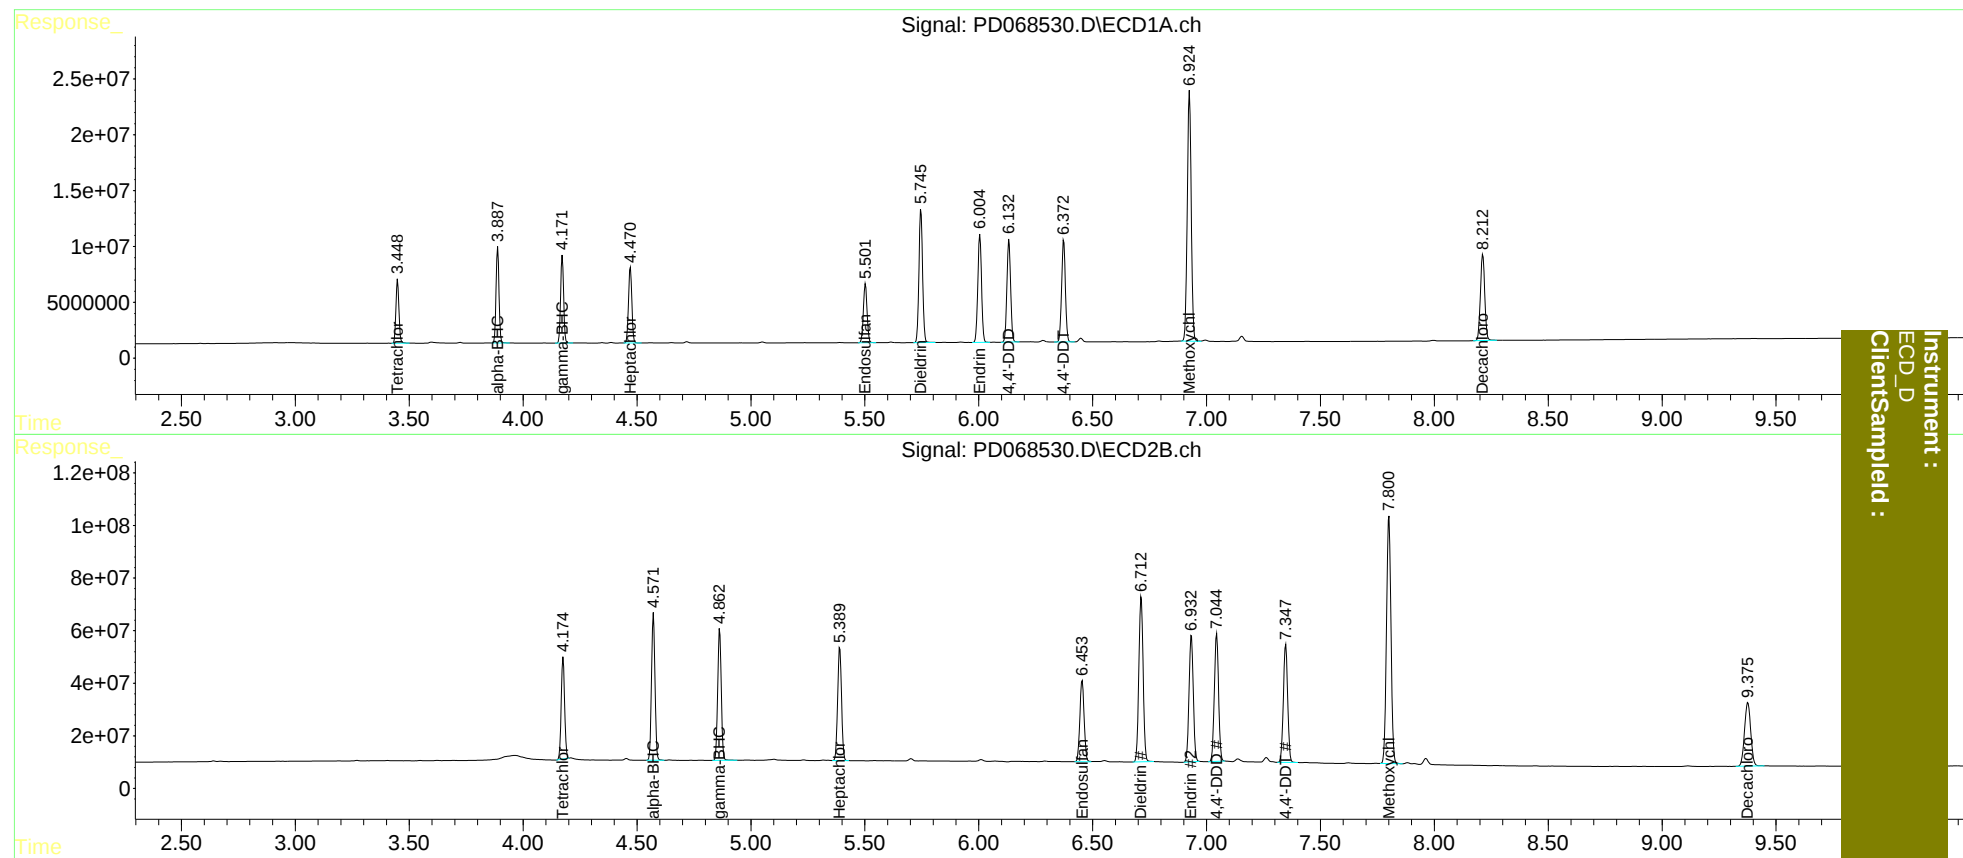

Instrument :
ECD_D
ClientSampled :
INDA401