

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
 Data File : PS018558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 04:44
 Operator : AJ\MA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 05:46:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 05:46:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.813	2023.5E6	589.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.032	2.534	2298.4E6	574.3E6	682.500	682.500
2) T	3,5-DICHL...	6.443	5.984	2595.5E6	813.3E6	697.500	697.500
3) T	4-Nitroph...	7.062	6.422	1098.4E6	307.1E6	682.500	682.500
5) T	DICAMBA	7.430	6.981	7400.6E6	2362.6E6	705.000	705.000
6) T	MCPD	7.603	7.081	589.7E6	194.4E6	70.500	70.500
7) T	MCPA	7.752	7.295	829.2E6	272.4E6	69.750	69.750
8) T	DICHLORPROP	8.125	7.604	1880.4E6	627.5E6	705.000	705.000
9) T	2,4-D	8.352	7.894	2297.4E6	740.2E6	705.000	705.000
10) T	Pentachlo...	8.665	8.326	25503.5E6	7643.3E6	712.500	712.500
11) T	2,4,5-TP ...	9.217	8.686	10903.5E6	3481.4E6	712.500	712.500
12) T	2,4,5-T	9.501	9.063	10818.7E6	3309.9E6	712.500	712.500
13) T	2,4-DB	10.053	9.569	2001.6E6	455.4E6	712.500	712.500
14) T	DINOSEB	11.219	9.899	7907.5E6	2426.1E6	705.000	705.000
15) T	Picloram	11.032	10.876	15518.3E6	4237.5E6	712.500	712.500
16) T	DCPA	11.487	10.833	13439.4E6	4193.2E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 04:44
Operator : AJ\MA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 05:46:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 05:46:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

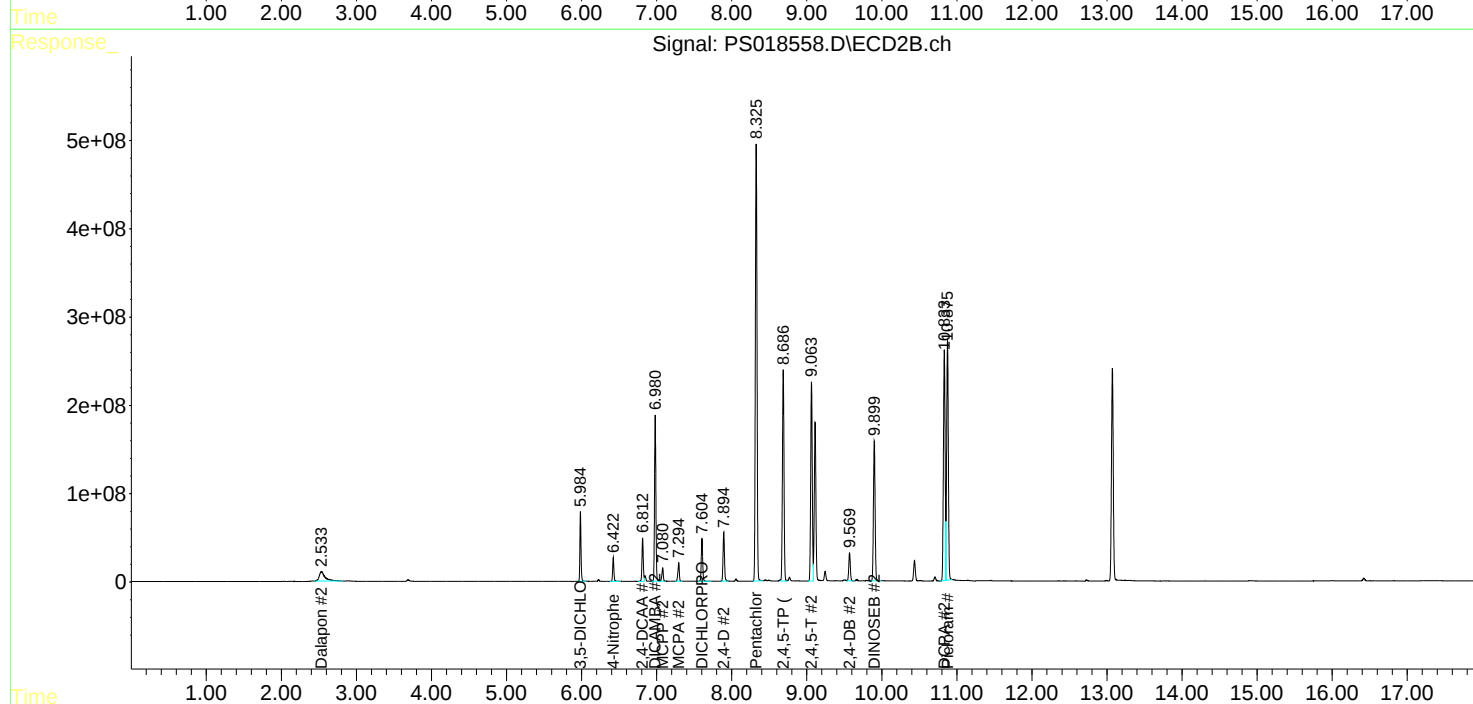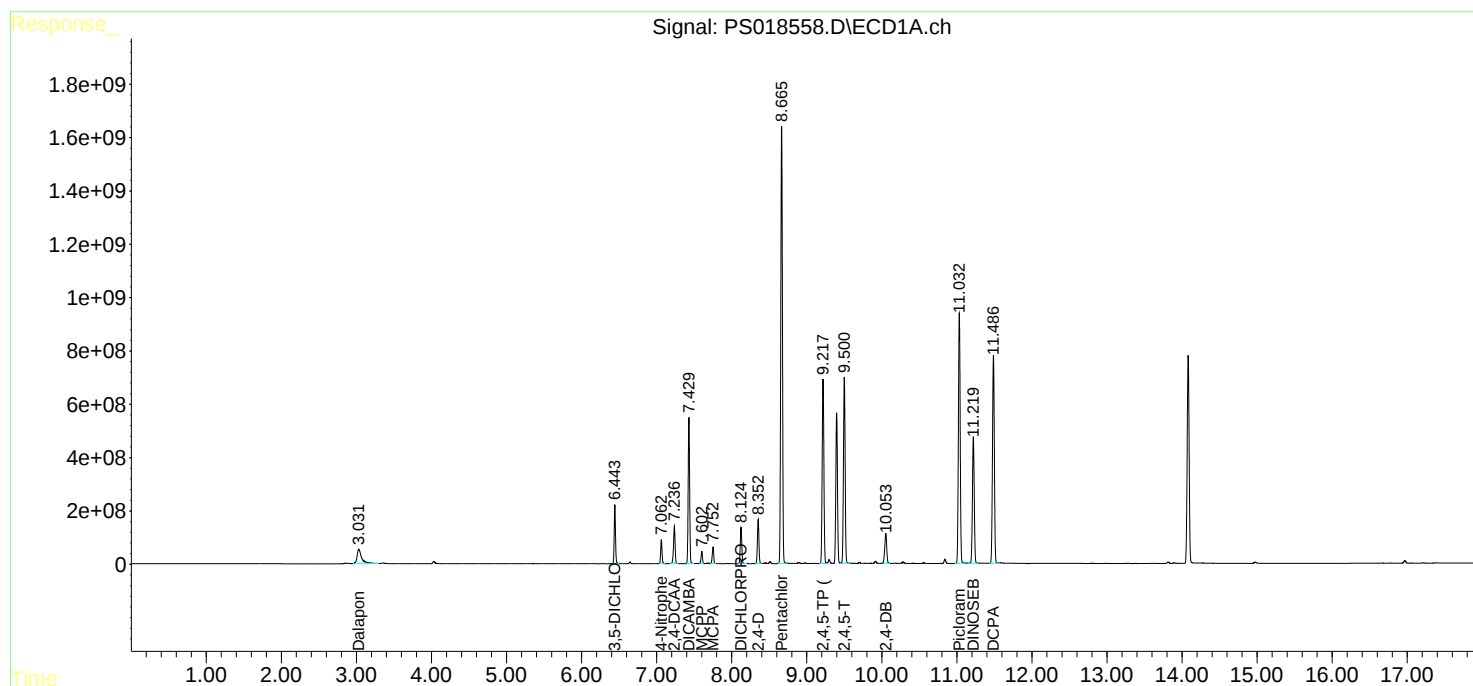


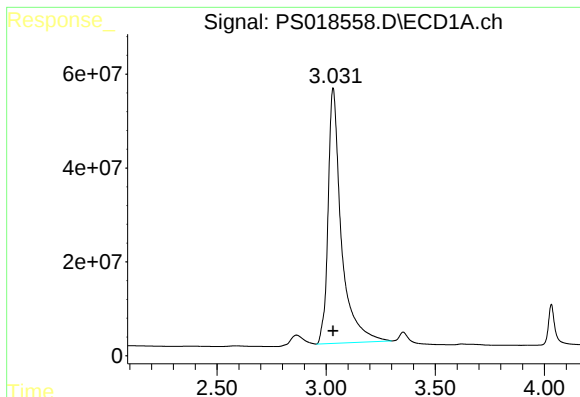

#1 Dalapon


R.T.: 3.032 min
Delta R.T.: 0.000 min
Response: 2298418081
Conc: 682.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

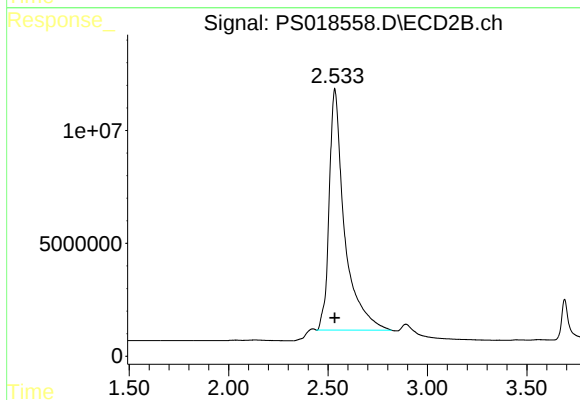


#1 Dalapon

R.T.: 2.534 min
Delta R.T.: 0.000 min
Response: 574269579
Conc: 682.50 ng/ml

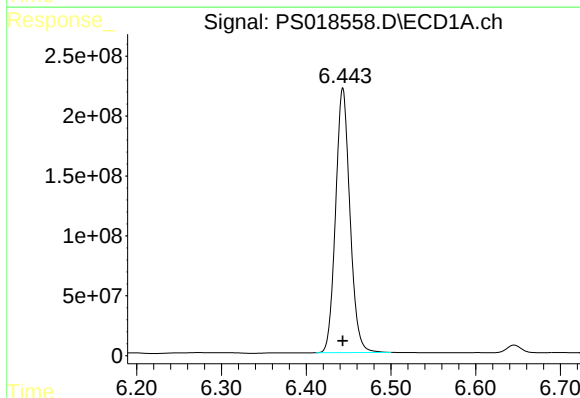


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 2595515363
Conc: 697.50 ng/ml

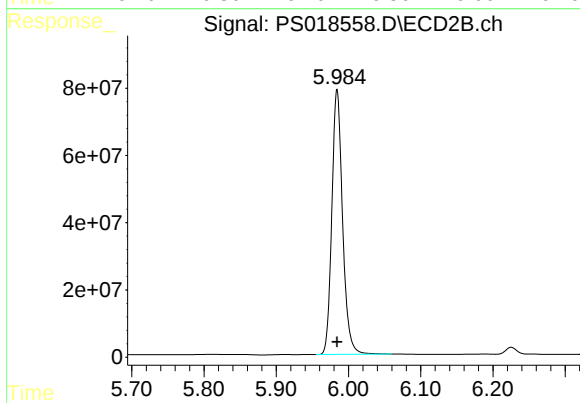

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 813342372
Conc: 697.50 ng/ml

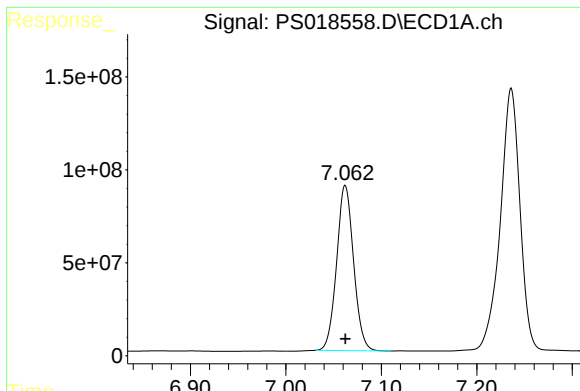

#3 4-Nitrophenol


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 1098428382
Conc: 682.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

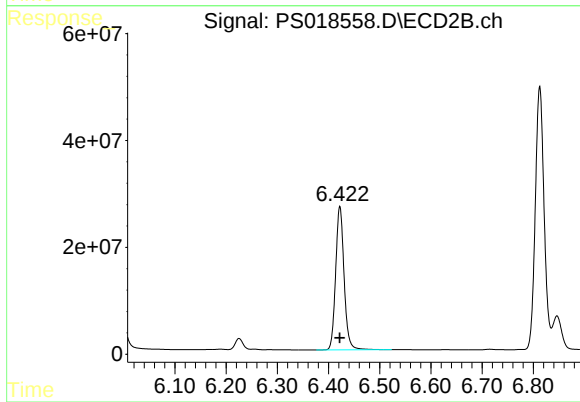


#3 4-Nitrophenol

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 307133170
Conc: 682.50 ng/ml

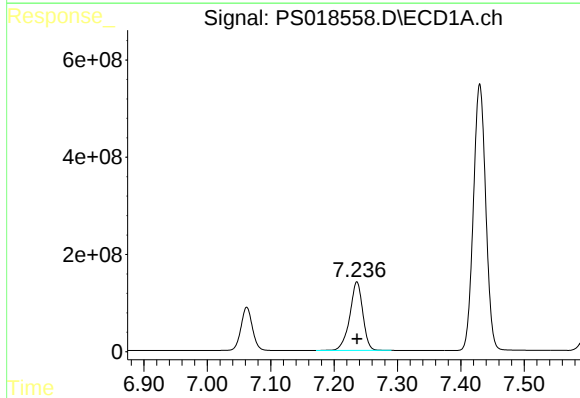


#4 2,4-DCAA

R.T.: 7.236 min
Delta R.T.: 0.000 min
Response: 2023527917
Conc: 750.00 ng/ml

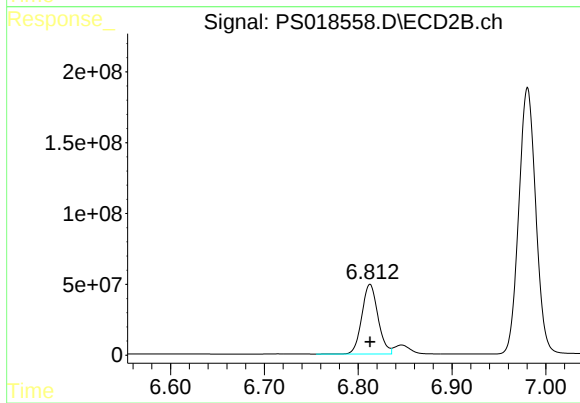

#4 2,4-DCAA


R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 589240715
Conc: 750.00 ng/ml

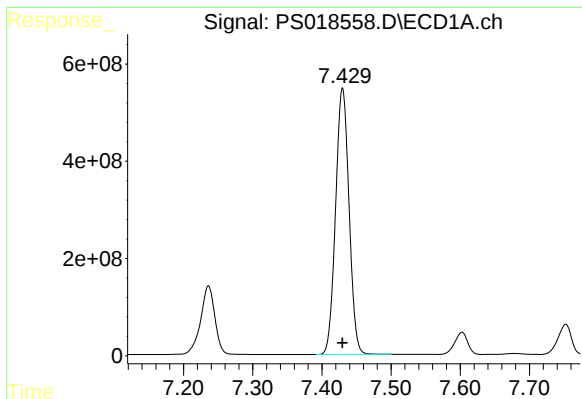

#5 DICAMBA


R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 7400560289
Conc: 705.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

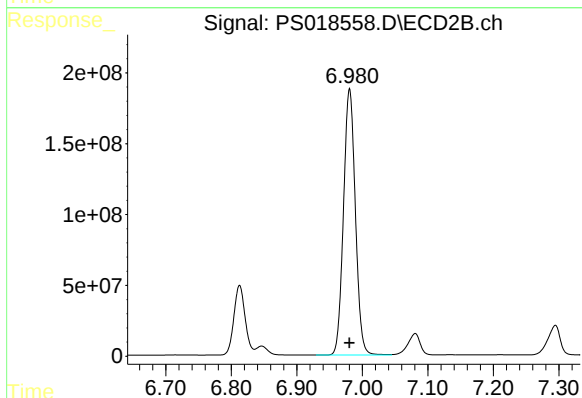


#5 DICAMBA

R.T.: 6.981 min
Delta R.T.: 0.000 min
Response: 2362628272
Conc: 705.00 ng/ml

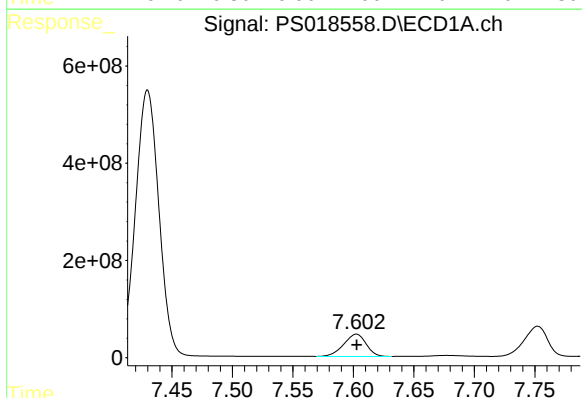


#6 MCP

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 589685625
Conc: 70.50 ug/ml

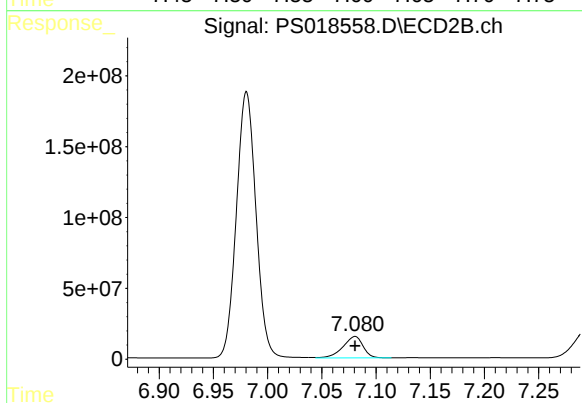

#6 MCP


R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 194354979
Conc: 70.50 ug/ml

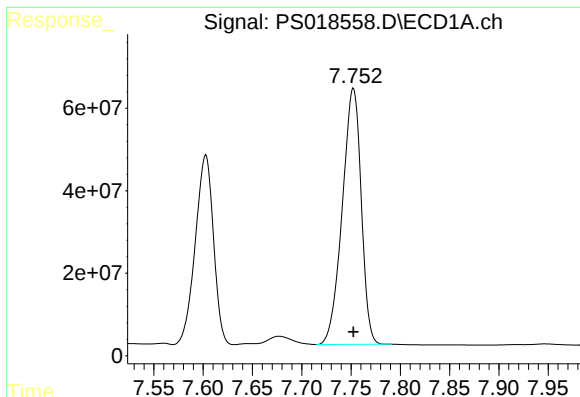

#7 MCPA


R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 829224616
Conc: 69.75 ug/ml

Instrument :
ECD_D
ClientSampleId :

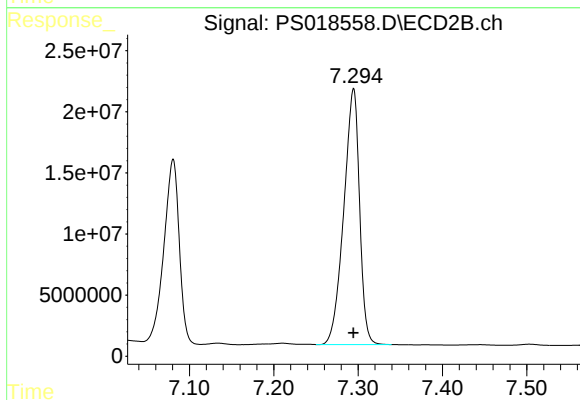


#7 MCPA

R.T.: 7.295 min
Delta R.T.: 0.000 min
Response: 272365372
Conc: 69.75 ug/ml

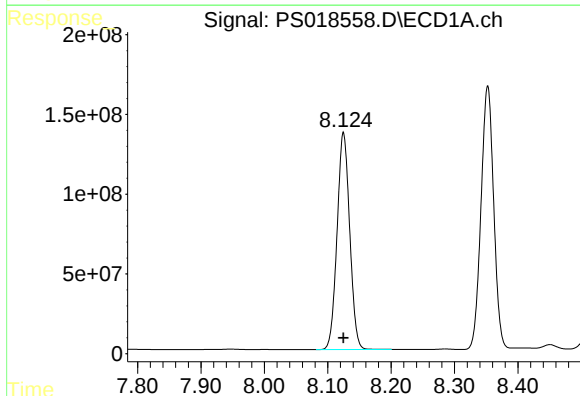


#8 DICHLORPROP

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 1880444760
Conc: 705.00 ng/ml

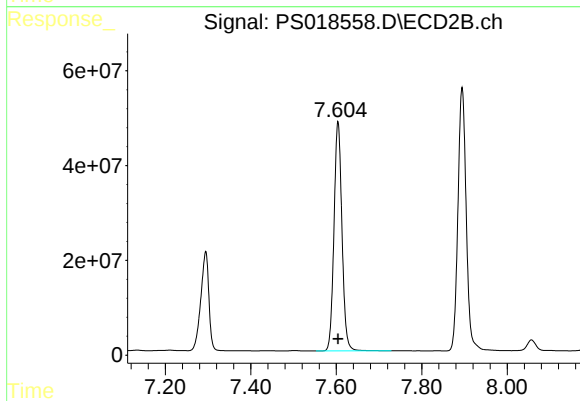

#8 DICHLORPROP


R.T.: 7.604 min
Delta R.T.: 0.000 min
Response: 627518433
Conc: 705.00 ng/ml

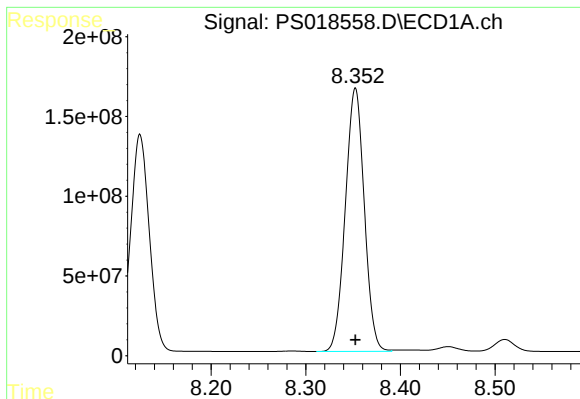

#9 2,4-D


R.T.: 8.352 min
Delta R.T.: 0.000 min
Response: 2297437912
Conc: 705.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

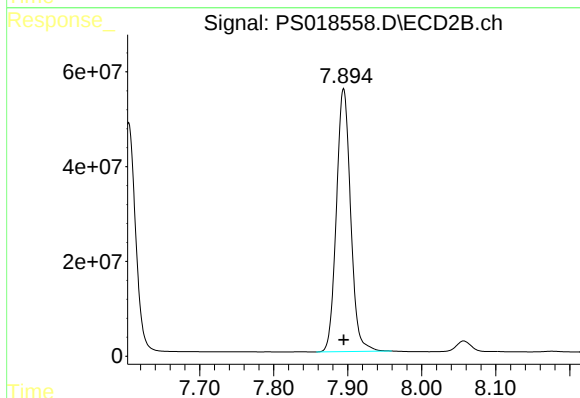


#9 2,4-D

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 740172904
Conc: 705.00 ng/ml

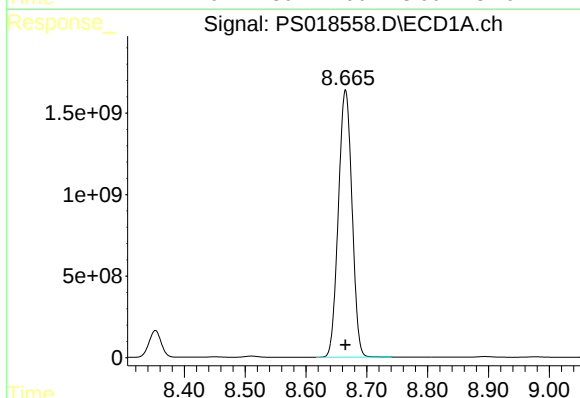


#10 Pentachlorophenol

R.T.: 8.665 min
Delta R.T.: 0.000 min
Response: 25503483792
Conc: 712.50 ng/ml

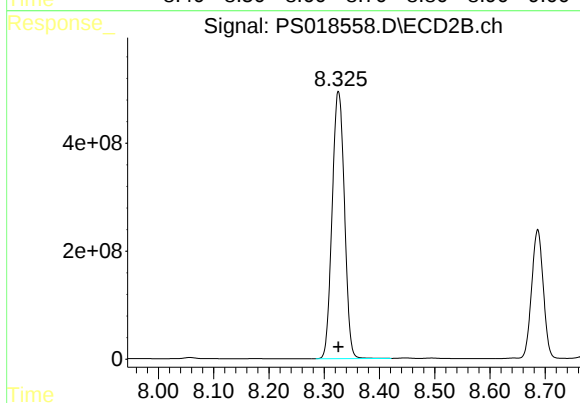

#10 Pentachlorophenol


R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 7643347225
Conc: 712.50 ng/ml

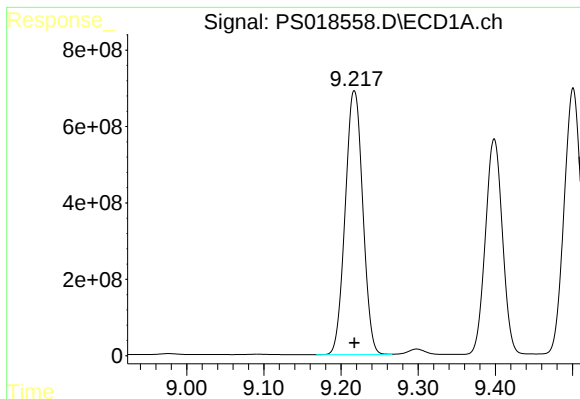

#11 2,4,5-TP (SILVEX)


R.T.: 9.217 min
Delta R.T.: 0.000 min
Response: 10903496806
Conc: 712.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

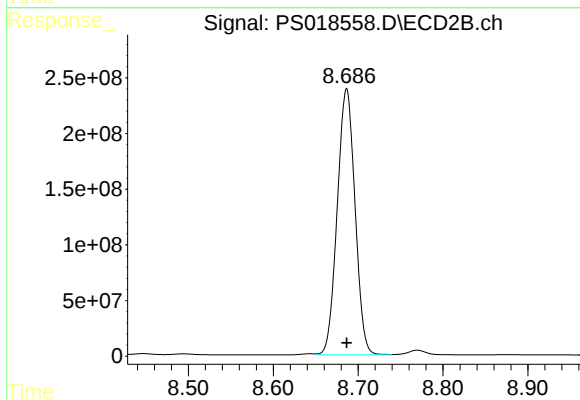


#11 2,4,5-TP (SILVEX)

R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 3481373351
Conc: 712.50 ng/ml

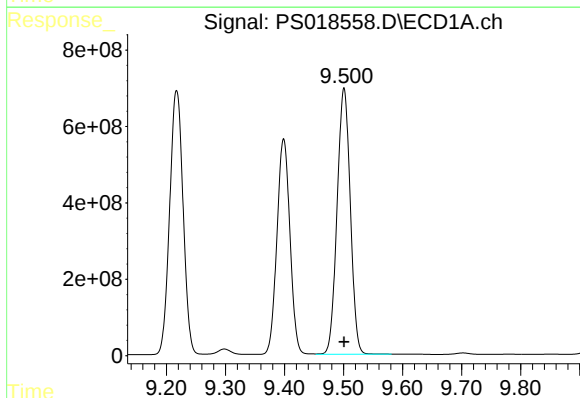


#12 2,4,5-T

R.T.: 9.501 min
Delta R.T.: 0.000 min
Response: 10818659162
Conc: 712.50 ng/ml

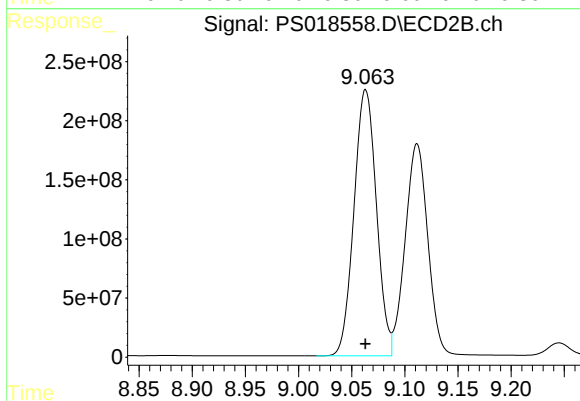

#12 2,4,5-T


R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 3309859680
Conc: 712.50 ng/ml

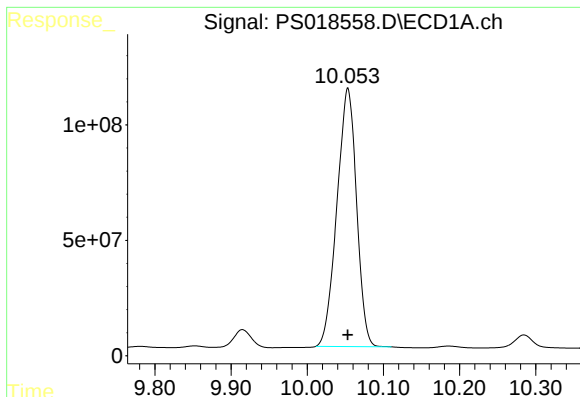

#13 2,4-DB


R.T.: 10.053 min
Delta R.T.: 0.000 min
Response: 2001616839
Conc: 712.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

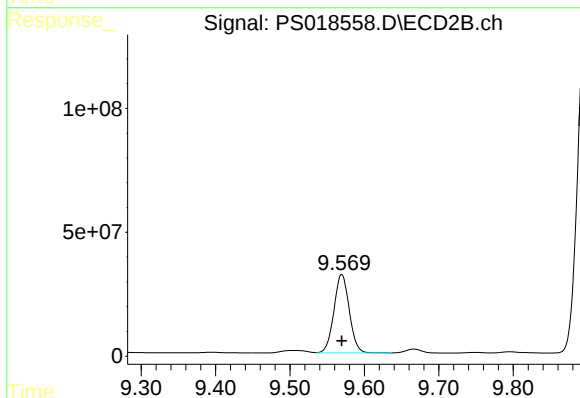


#13 2,4-DB

R.T.: 9.569 min
Delta R.T.: 0.000 min
Response: 455427759
Conc: 712.50 ng/ml

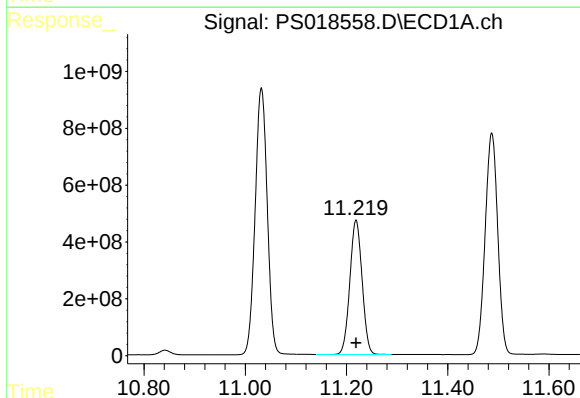


#14 DINOSEB

R.T.: 11.219 min
Delta R.T.: 0.000 min
Response: 7907481583
Conc: 705.00 ng/ml

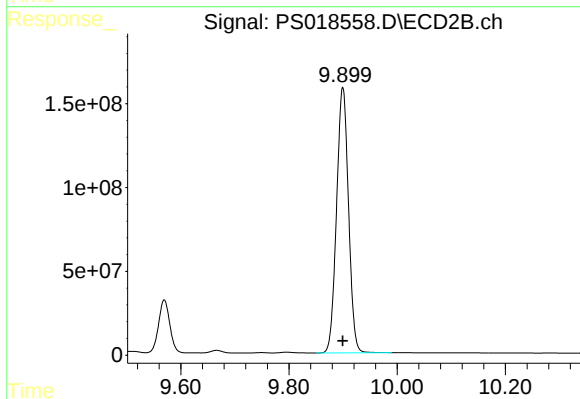

#14 DINOSEB


R.T.: 9.899 min
Delta R.T.: 0.000 min
Response: 2426128658
Conc: 705.00 ng/ml

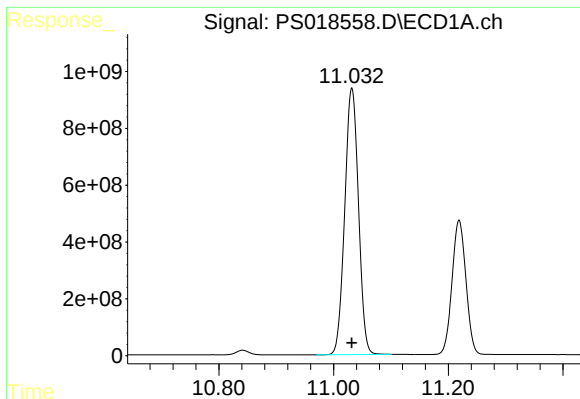

#15 Picloram


R.T.: 11.032 min
Delta R.T.: 0.000 min
Response: 15518261657
Conc: 712.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

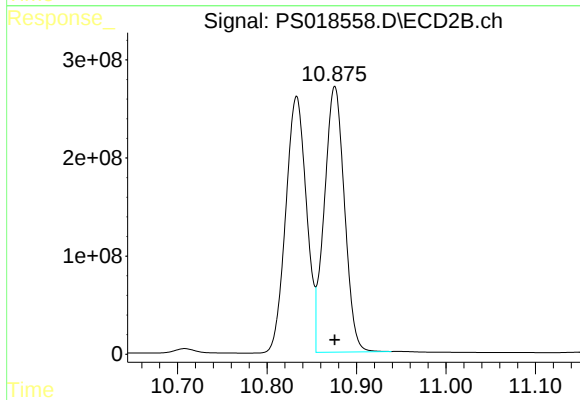


#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 4237484822
Conc: 712.50 ng/ml

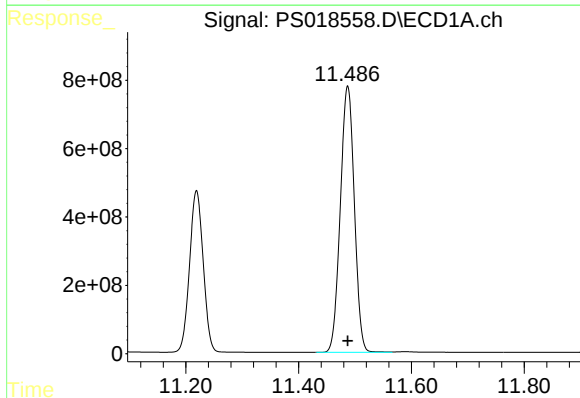

#16 DCPA

R.T.: 11.487 min
Delta R.T.: 0.000 min
Response: 13439367522
Conc: 720.00 ng/ml

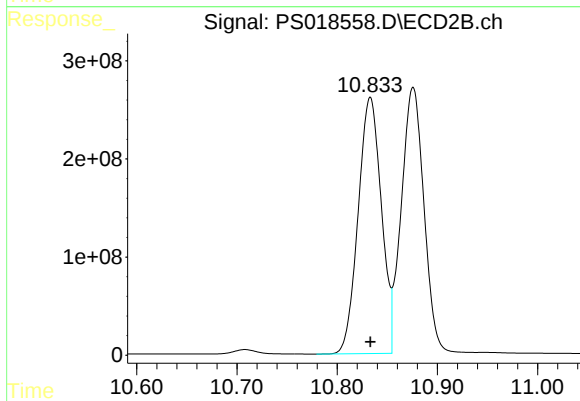

#16 DCPA

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 4193195808
Conc: 720.00 ng/ml