

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 13:43
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:35:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 01:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.792	13108081	6487926	5.360	5.253
27)	SA Decachlor...	9.097	7.945	32139409	13804009	11.910	11.704
Target Compounds							
2)	A alpha-BHC	4.007	3.295	18516485	8613687	4.813	4.885
3)	MA gamma-BHC...	4.340	3.625	17937510	8394801	4.908	4.942
4)	MA Heptachlor	4.933	3.967	19141346	8388856	5.110	5.119
9)	A Endosulfan I	6.090	5.121	15845765	7221366	5.378	5.181
13)	MA Dieldrin	6.367	5.387	31414896	15598363	10.005	10.047
14)	MA Endrin	6.597	5.662	26120520	13561134	9.972	10.073
16)	A 4,4'-DDD	6.730	5.811	23528862	11728868	10.047	9.941
17)	MA 4,4'-DDT	7.044	6.063	25194606	12402797	10.183	9.942
20)	A Methoxychlor	7.521	6.639	71529581	33707625	52.729	54.439


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 13:43
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:35:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 01:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

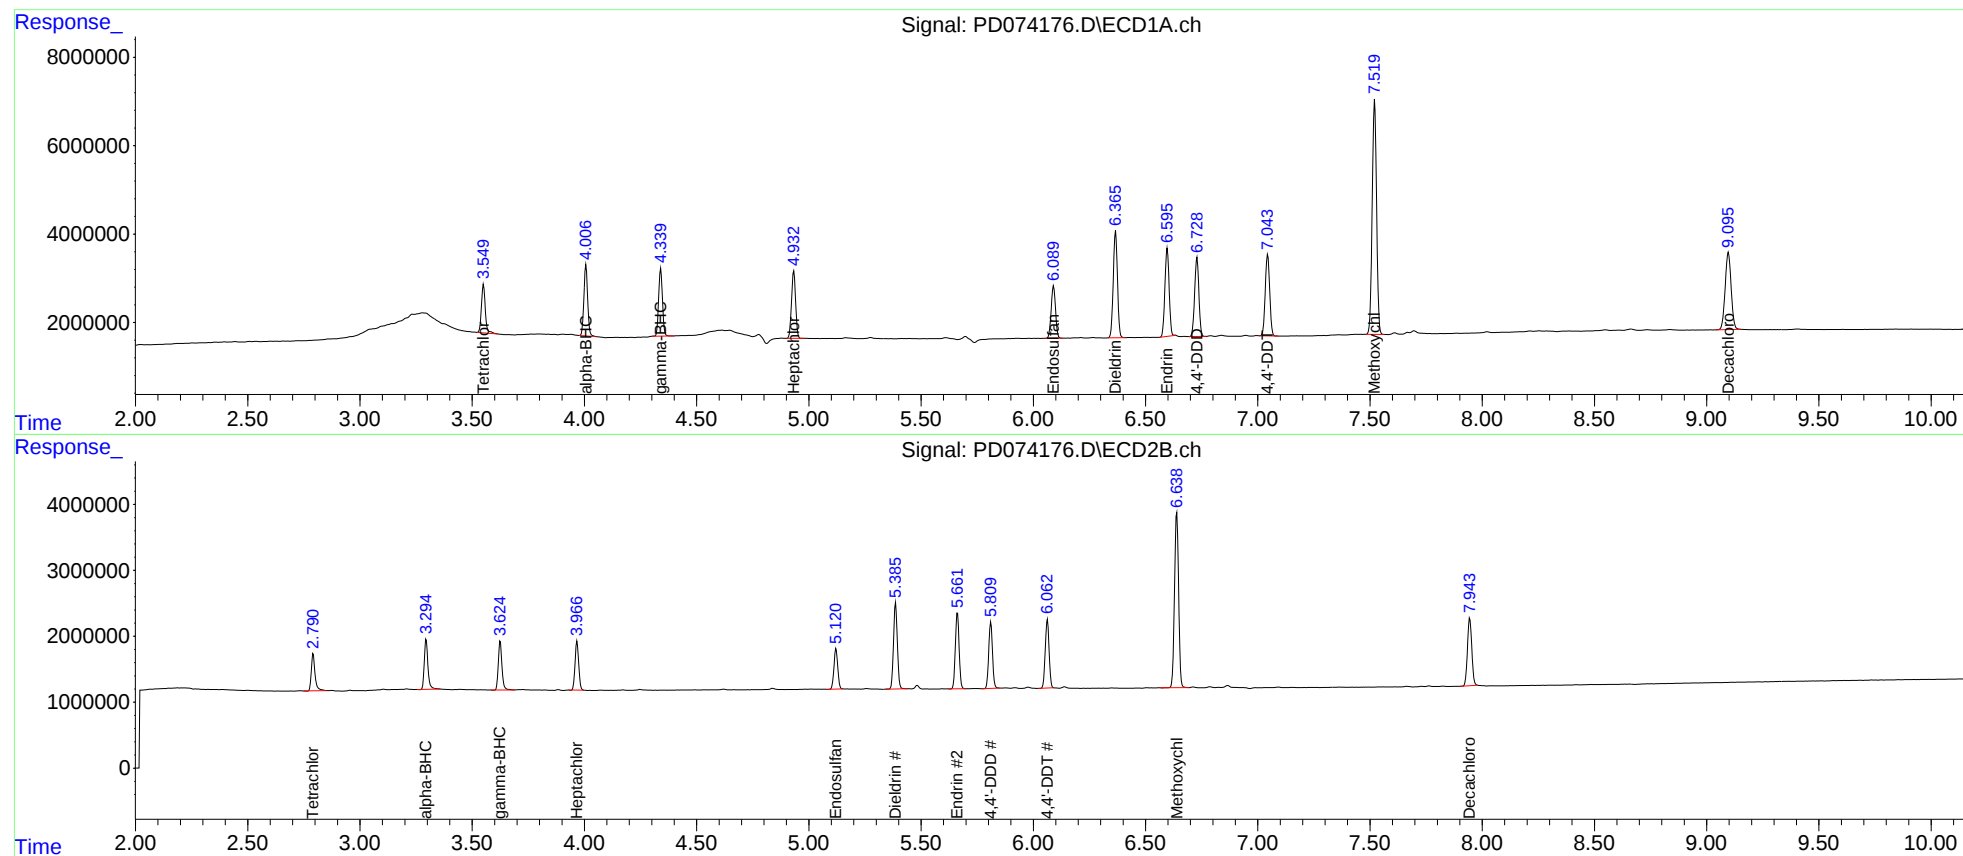

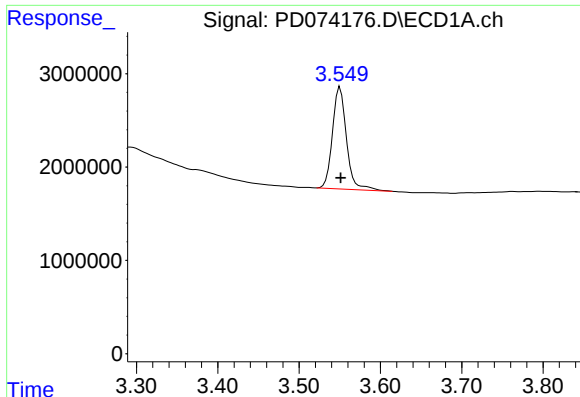


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 13108081
Conc: 5.36 ng/ml

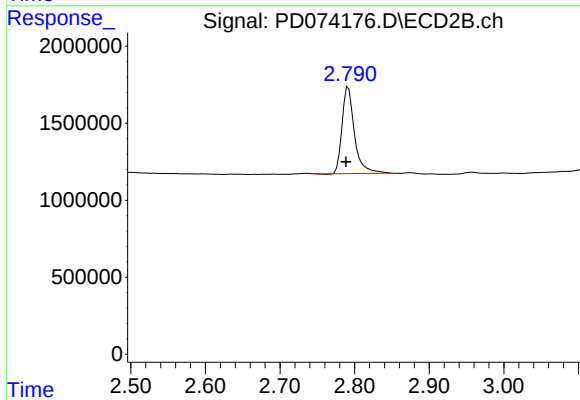


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: 0.003 min
Response: 6487926
Conc: 5.25 ng/ml

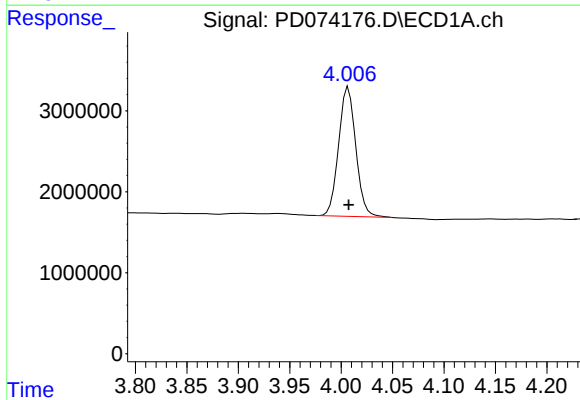


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 18516485
Conc: 4.81 ng/ml

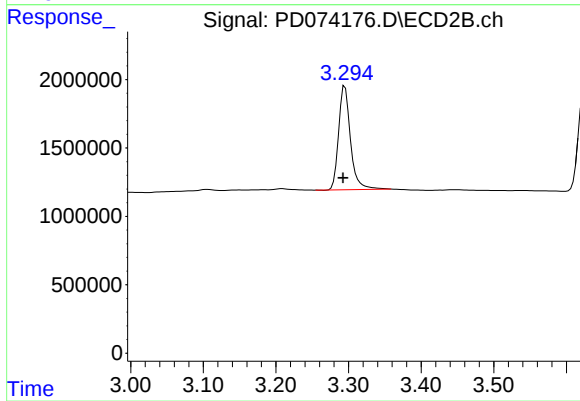


#2 alpha-BHC

R.T.: 3.295 min
Delta R.T.: 0.003 min
Response: 8613687
Conc: 4.88 ng/ml

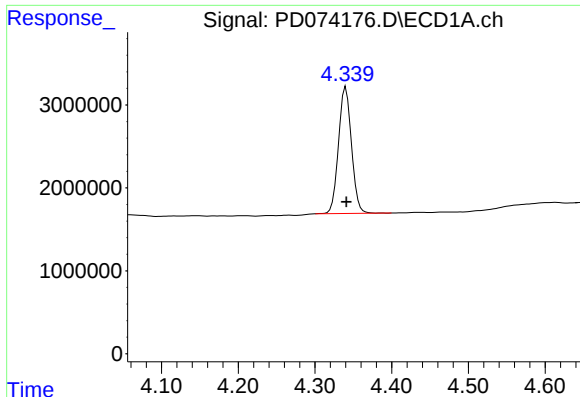


#3 gamma-BHC (Lindane)

R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 17937510
Conc: 4.91 ng/ml

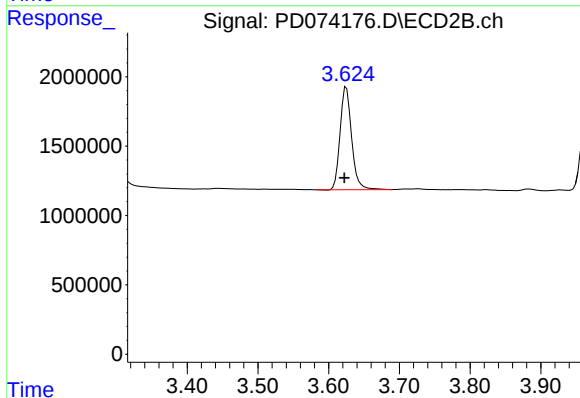


#3 gamma-BHC (Lindane)

R.T.: 3.625 min
Delta R.T.: 0.003 min
Response: 8394801
Conc: 4.94 ng/ml

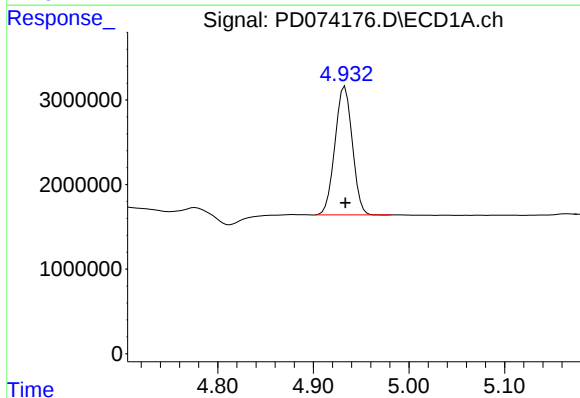


#4 Heptachlor

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 19141346
Conc: 5.11 ng/ml

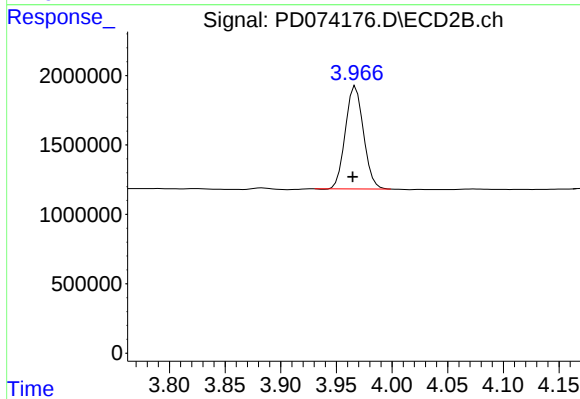


#4 Heptachlor

R.T.: 3.967 min
Delta R.T.: 0.003 min
Response: 8388856
Conc: 5.12 ng/ml

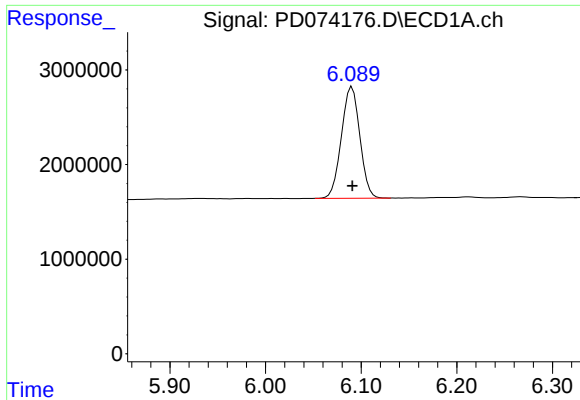


#9 Endosulfan I

R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 15845765
Conc: 5.38 ng/ml

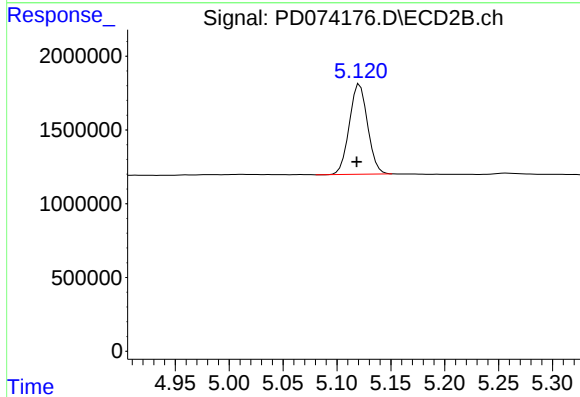


#9 Endosulfan I

R.T.: 5.121 min
Delta R.T.: 0.003 min
Response: 7221366
Conc: 5.18 ng/ml

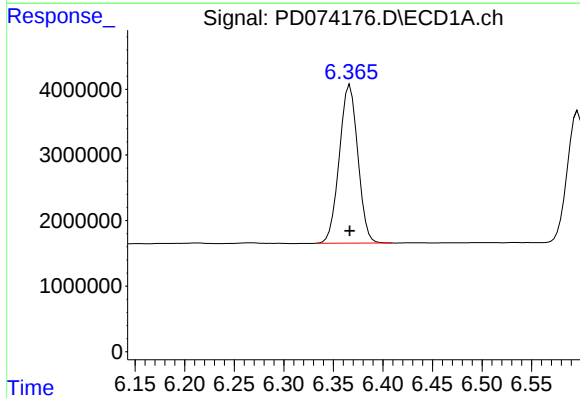


#13 Dieldrin

R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 31414896
Conc: 10.00 ng/ml

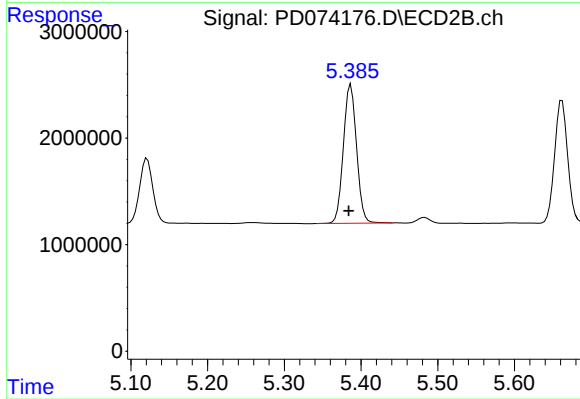


#13 Dieldrin

R.T.: 5.387 min
Delta R.T.: 0.003 min
Response: 15598363
Conc: 10.05 ng/ml

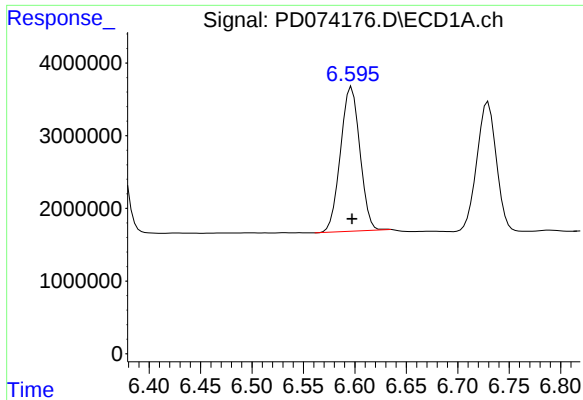


#14 Endrin

R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 26120520
Conc: 9.97 ng/ml

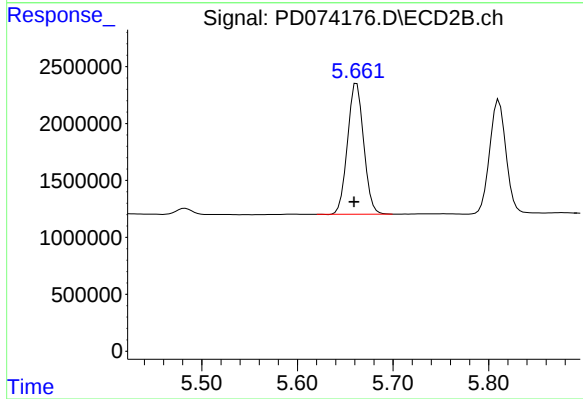


#14 Endrin

R.T.: 5.662 min
Delta R.T.: 0.003 min
Response: 13561134
Conc: 10.07 ng/ml

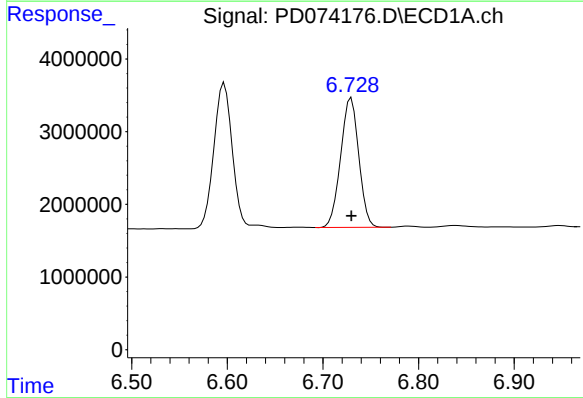


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 23528862
Conc: 10.05 ng/ml

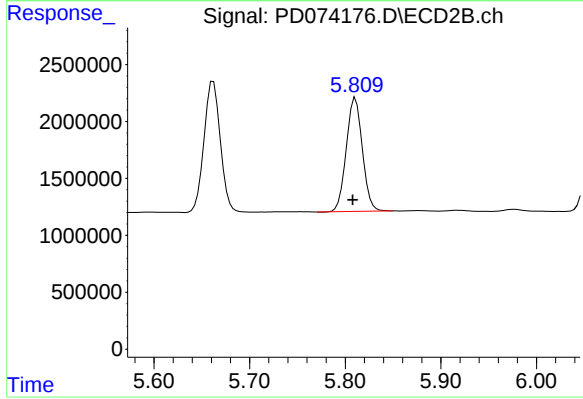


#16 4,4'-DDD

R.T.: 5.811 min
Delta R.T.: 0.003 min
Response: 11728868
Conc: 9.94 ng/ml

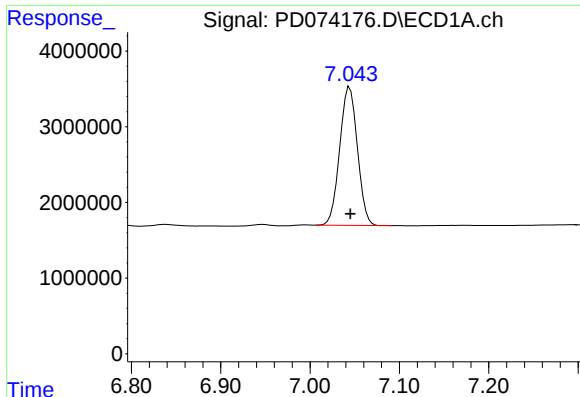


#17 4,4'-DDT

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 25194606
Conc: 10.18 ng/ml

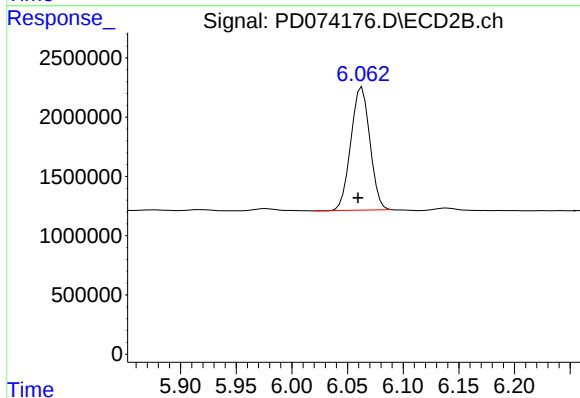


#17 4,4'-DDT

R.T.: 6.063 min
Delta R.T.: 0.003 min
Response: 12402797
Conc: 9.94 ng/ml

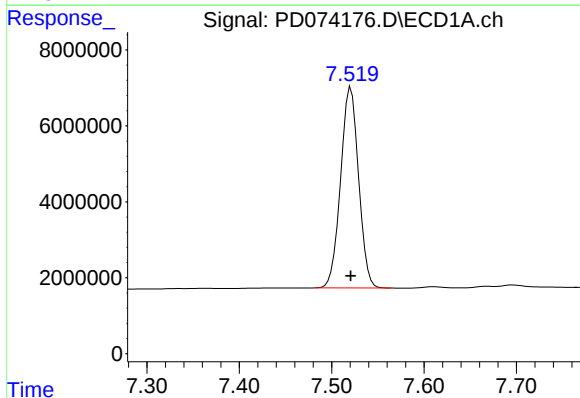


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 71529581
Conc: 52.73 ng/ml

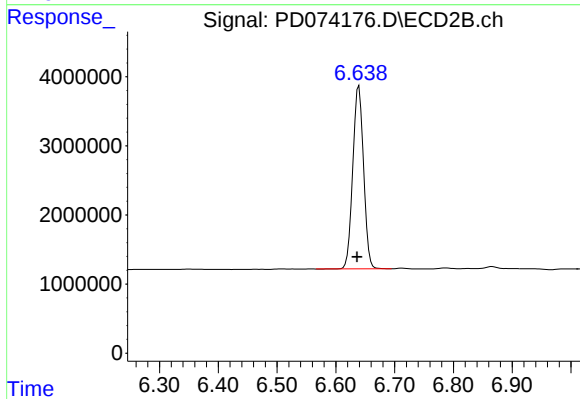


#20 Methoxychlor

R.T.: 6.639 min
Delta R.T.: 0.003 min
Response: 33707625
Conc: 54.44 ng/ml

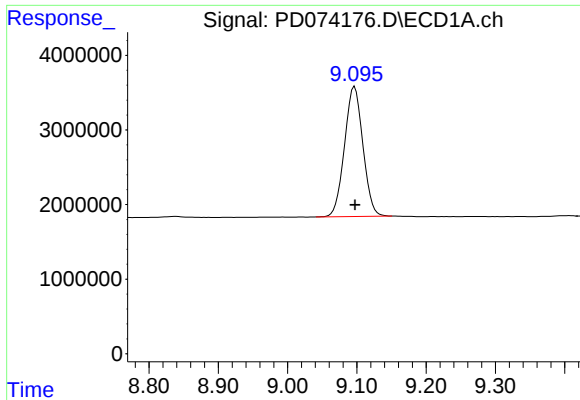

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 32139409
Conc: 11.91 ng/ml

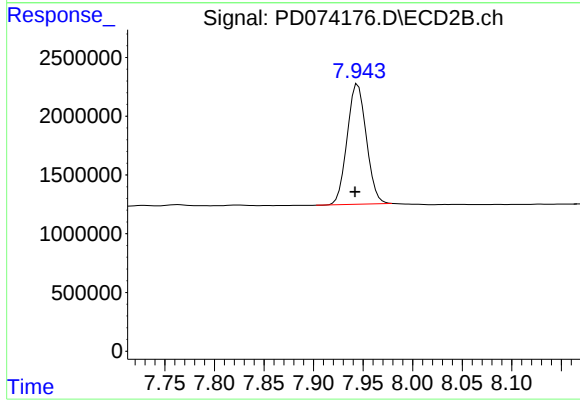

#27 Decachlorobiphenyl

R.T.: 7.945 min
Delta R.T.: 0.003 min
Response: 13804009
Conc: 11.70 ng/ml