

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 13:57
 Operator : AR\AJ
 Sample : INDB101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 23:23:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 13 23:20:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	13269299	6772430	5.472	5.427
27)	SA Decachlor...	9.098	7.925	33580383	14338670	12.298	11.886
Target Compounds							
5)	MB Aldrin	5.277	4.228	18557464	8778171	5.196	5.189
6)	B beta-BHC	4.535	3.901	9002245	4408799	5.346	5.474
7)	B delta-BHC	4.784	4.132	19857747	8868274	5.551	5.091
8)	B Heptachlo...	5.704	4.731	18206722	8313018	5.677	5.324
10)	B trans-Chl...	5.960	4.982	16843119	8036799	5.394	5.284
11)	B cis-Chlor...	6.040	5.046	17442496	8283089	5.457	5.313
12)	B 4,4'-DDE	6.212	5.236	29336967	14412438	10.019	10.030
15)	B Endosulfa...	6.815	5.936	29187343	14017622	10.916	10.551
18)	B Endrin al...	6.946	6.116	24545026	11937365	11.235	11.015
19)	B Endosulfa...	7.181	6.339	27862949	13420327	11.048	10.830
21)	B Endrin ke...	7.668	6.845	31816318	16151252	11.100	10.706


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 13:57
Operator : AR\AJ
Sample : INDB101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 23:23:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 13 23:20:33 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

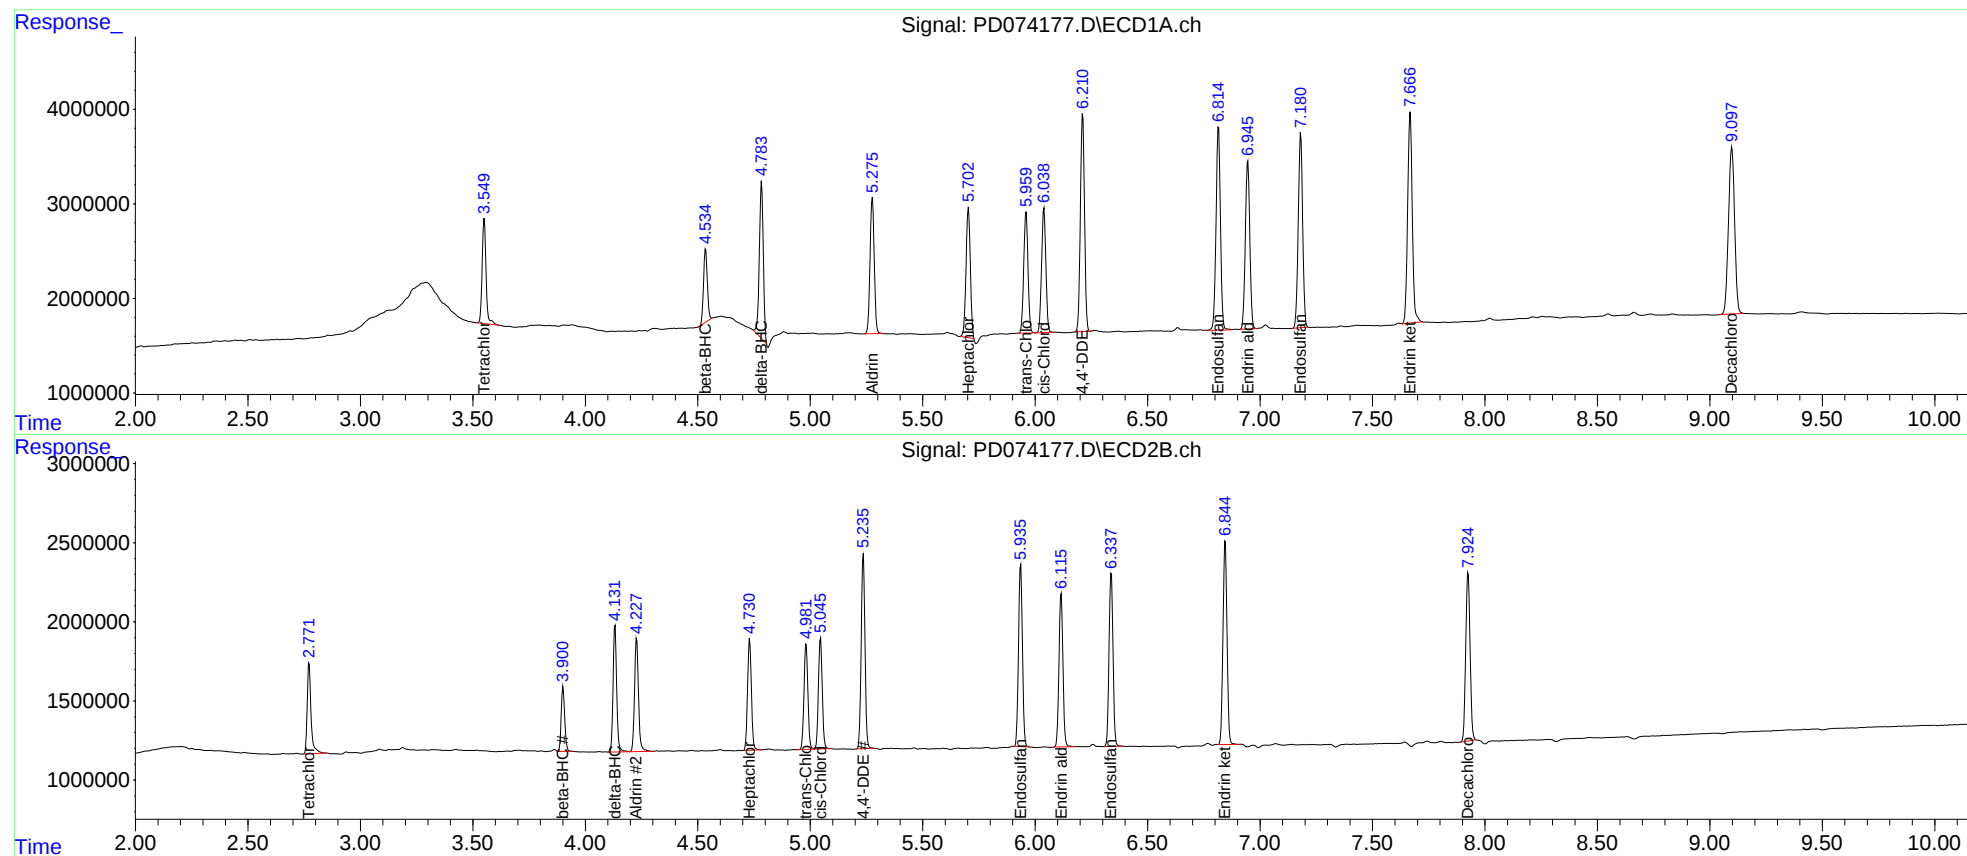

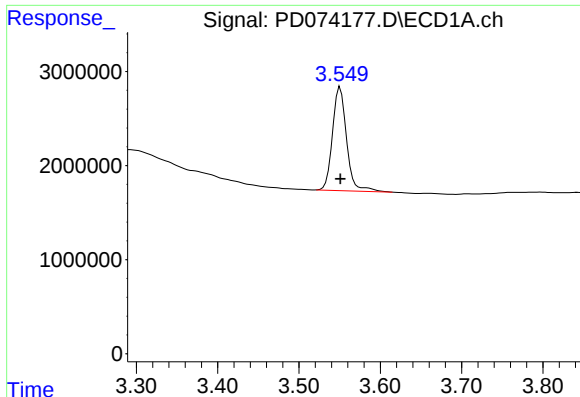


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 13269299
Conc: 5.47 ng/ml

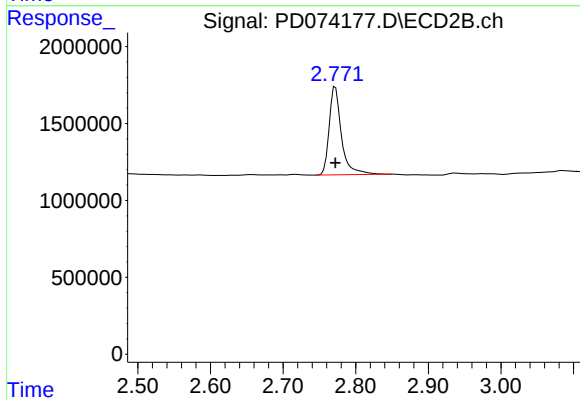


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 6772430
Conc: 5.43 ng/ml

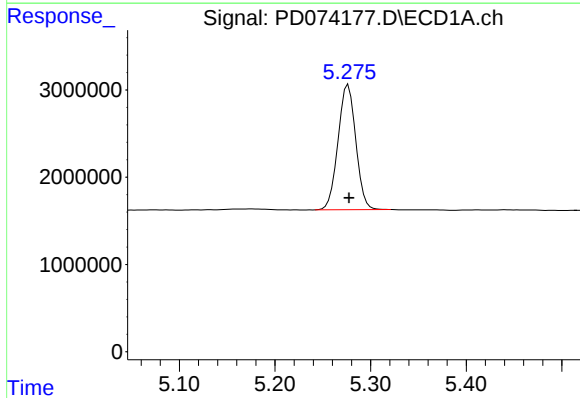


#5 Aldrin

R.T.: 5.277 min
Delta R.T.: -0.001 min
Response: 18557464
Conc: 5.20 ng/ml

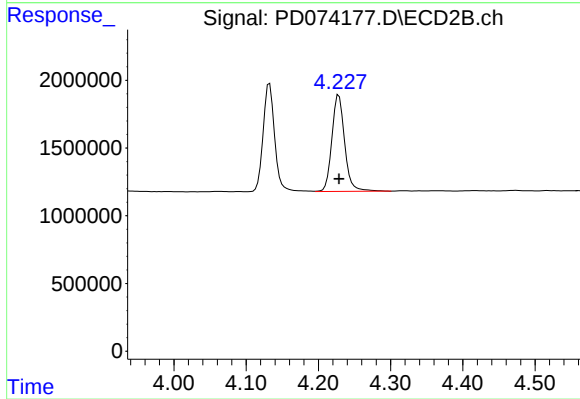


#5 Aldrin

R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 8778171
Conc: 5.19 ng/ml

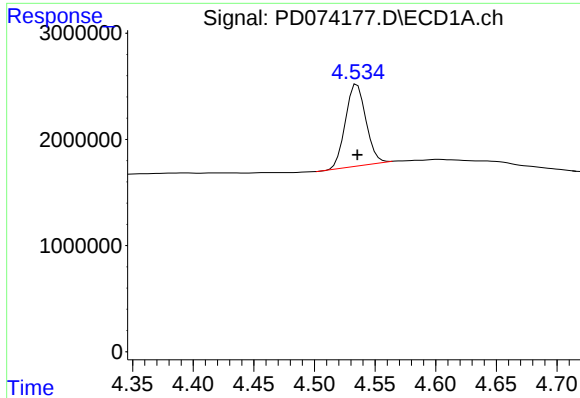


#6 beta-BHC

R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 9002245
Conc: 5.35 ng/ml

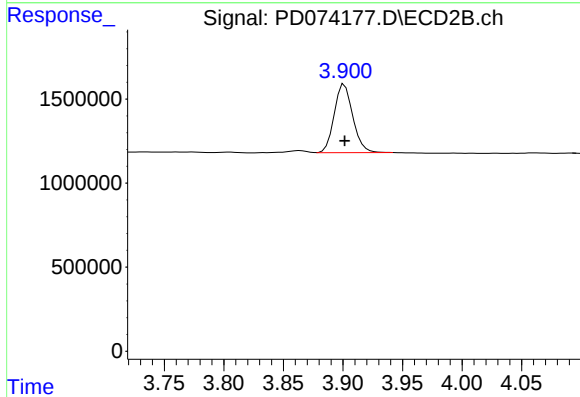


#6 beta-BHC

R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 4408799
Conc: 5.47 ng/ml

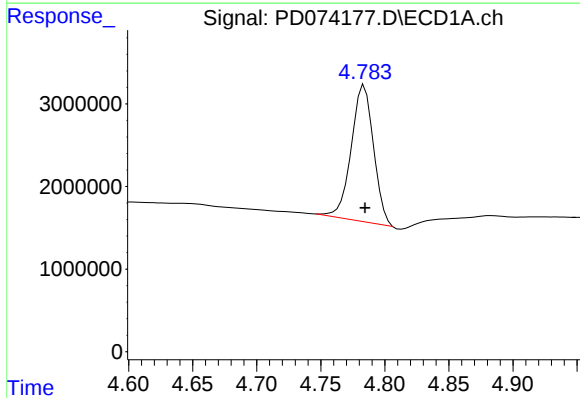


#7 delta-BHC

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 19857747
Conc: 5.55 ng/ml

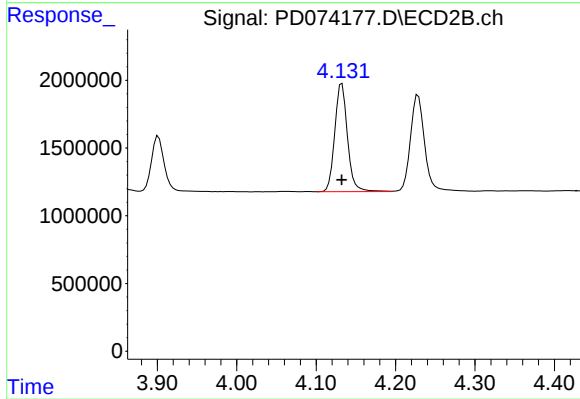


#7 delta-BHC

R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 8868274
Conc: 5.09 ng/ml

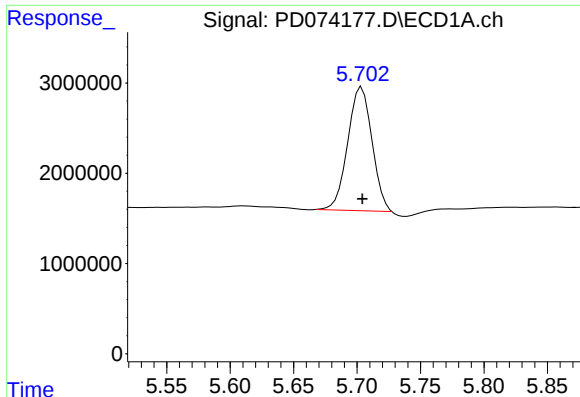


#8 Heptachlor epoxide

R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 18206722
Conc: 5.68 ng/ml

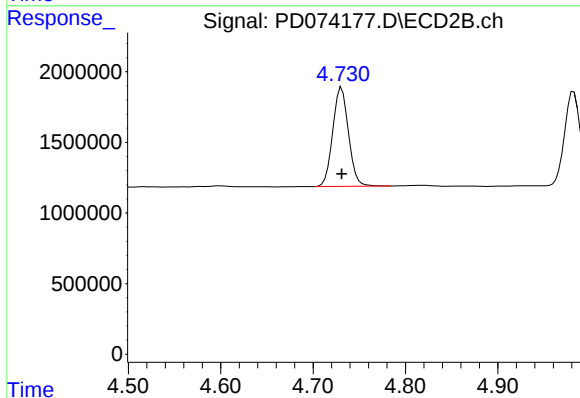


#8 Heptachlor epoxide

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 8313018
Conc: 5.32 ng/ml

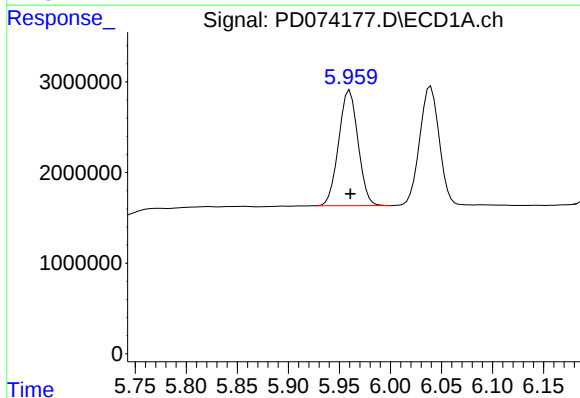


#10 trans-Chlordane

R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 16843119
Conc: 5.39 ng/ml

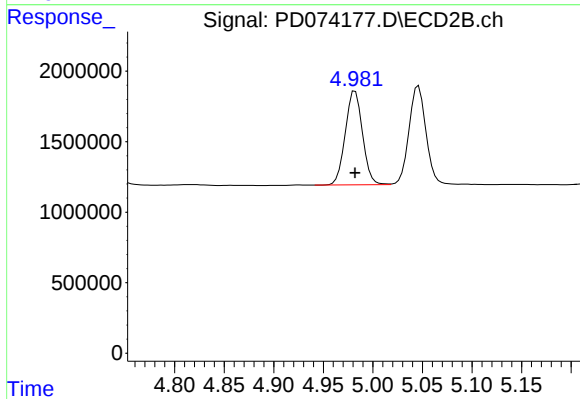


#10 trans-Chlordane

R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 8036799
Conc: 5.28 ng/ml

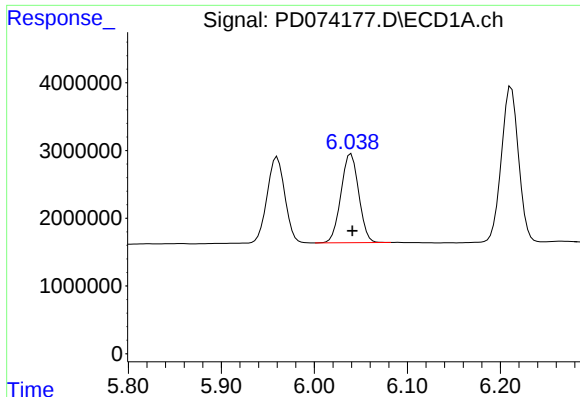


#11 cis-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.001 min
Response: 17442496
Conc: 5.46 ng/ml

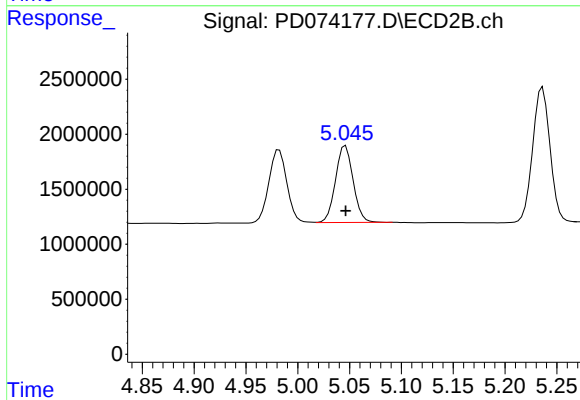


#11 cis-Chlordane

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 8283089
Conc: 5.31 ng/ml

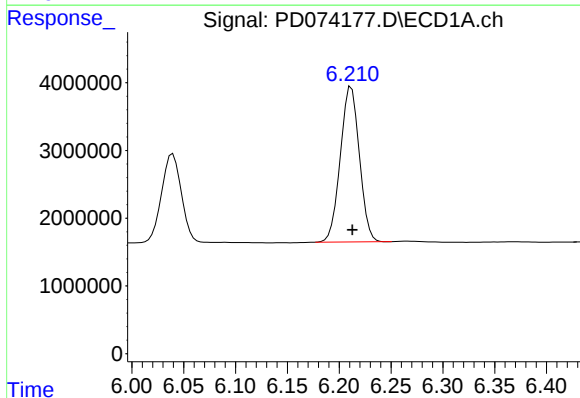


#12 4,4'-DDE

R.T.: 6.212 min
Delta R.T.: -0.001 min
Response: 29336967
Conc: 10.02 ng/ml

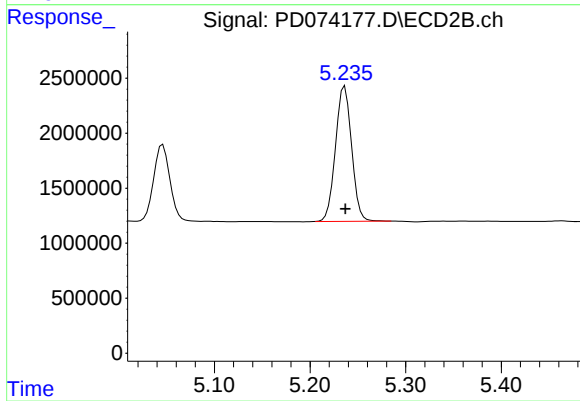


#12 4,4'-DDE

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 14412438
Conc: 10.03 ng/ml

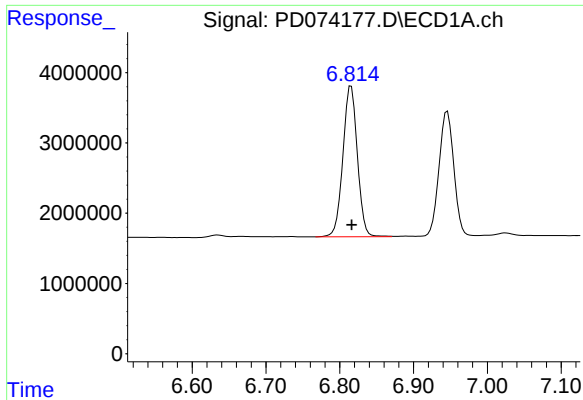


#15 Endosulfan II

R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 29187343
Conc: 10.92 ng/ml

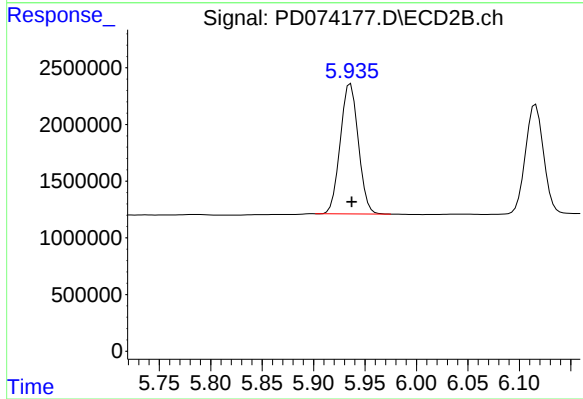


#15 Endosulfan II

R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 14017622
Conc: 10.55 ng/ml

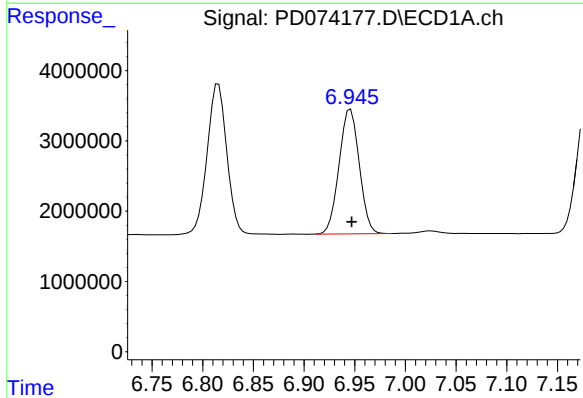


#18 Endrin aldehyde

R.T.: 6.946 min
Delta R.T.: -0.001 min
Response: 24545026
Conc: 11.24 ng/ml

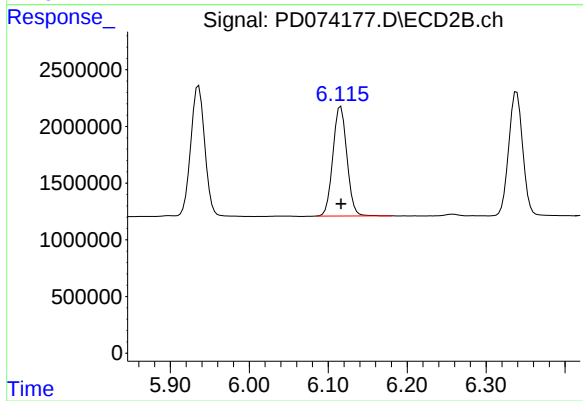


#18 Endrin aldehyde

R.T.: 6.116 min
Delta R.T.: 0.000 min
Response: 11937365
Conc: 11.02 ng/ml

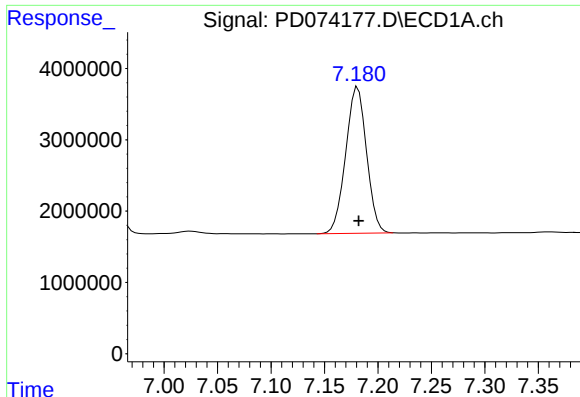


#19 Endosulfan Sulfate

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 27862949
Conc: 11.05 ng/ml

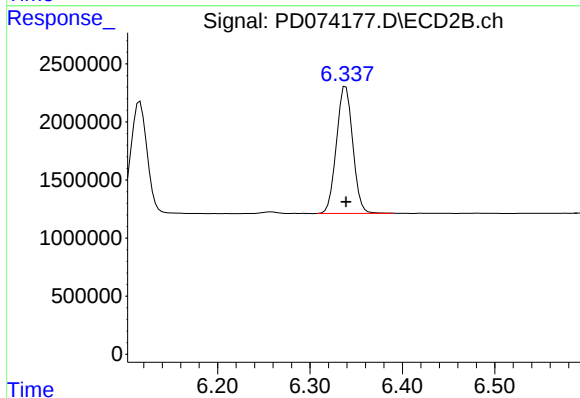


#19 Endosulfan Sulfate

R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 13420327
Conc: 10.83 ng/ml

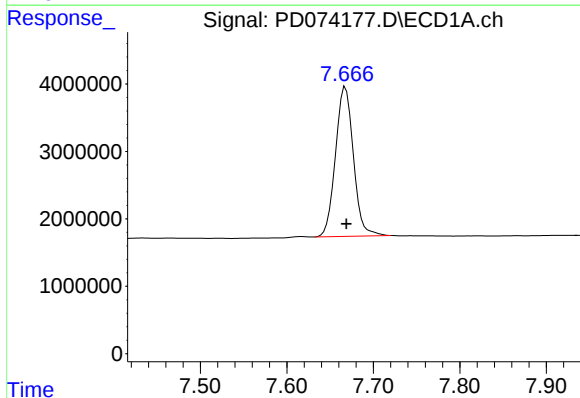


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 31816318
Conc: 11.10 ng/ml

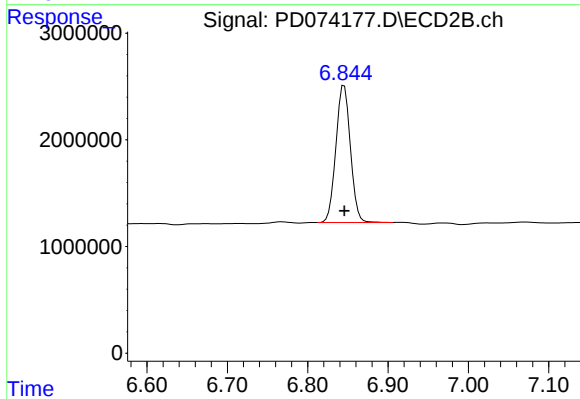


#21 Endrin ketone

R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 16151252
Conc: 10.71 ng/ml

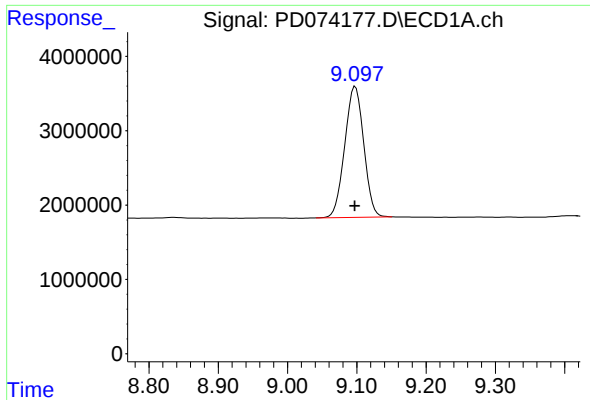

#27 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 33580383
Conc: 12.30 ng/ml

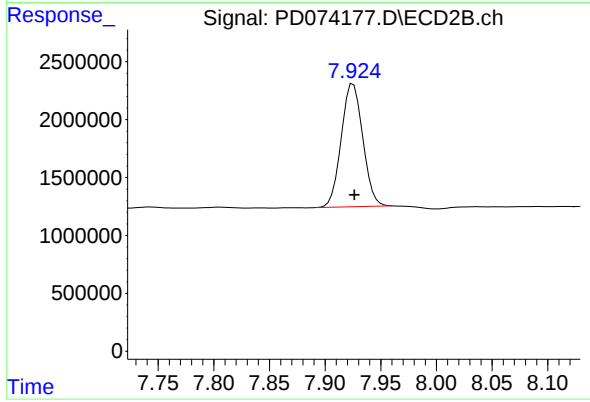

#27 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.001 min
Response: 14338670
Conc: 11.89 ng/ml