

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 14:10
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:35:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 01:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.772	25500016	13017548	10.428	10.539
27)	SA Decachlor...	9.097	7.925	58233005	24679495	21.579	20.924
Target Compounds							
2)	A alpha-BHC	4.007	3.275	37360304	17455575	9.711	9.899
3)	MA gamma-BHC...	4.340	3.605	35816272	16944916	9.800	9.976
4)	MA Heptachlor	4.933	3.947	36571790	13423412	9.764	8.191
9)	A Endosulfan I	6.090	5.101	29737974	13411094	10.092	9.621
13)	MA Dieldrin	6.366	5.367	61267076	30234507	19.512	19.473
14)	MA Endrin	6.597	5.642	51365420	25743062	19.610	19.121
16)	A 4,4'-DDD	6.729	5.791	46091986	21499132	19.681	18.221
17)	MA 4,4'-DDT	7.045	6.042	49118461	23350381	19.852	18.718
20)	A Methoxychlor	7.521	6.619	138.0E6	65001304	101.710	104.979


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 14:10
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:35:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 01:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

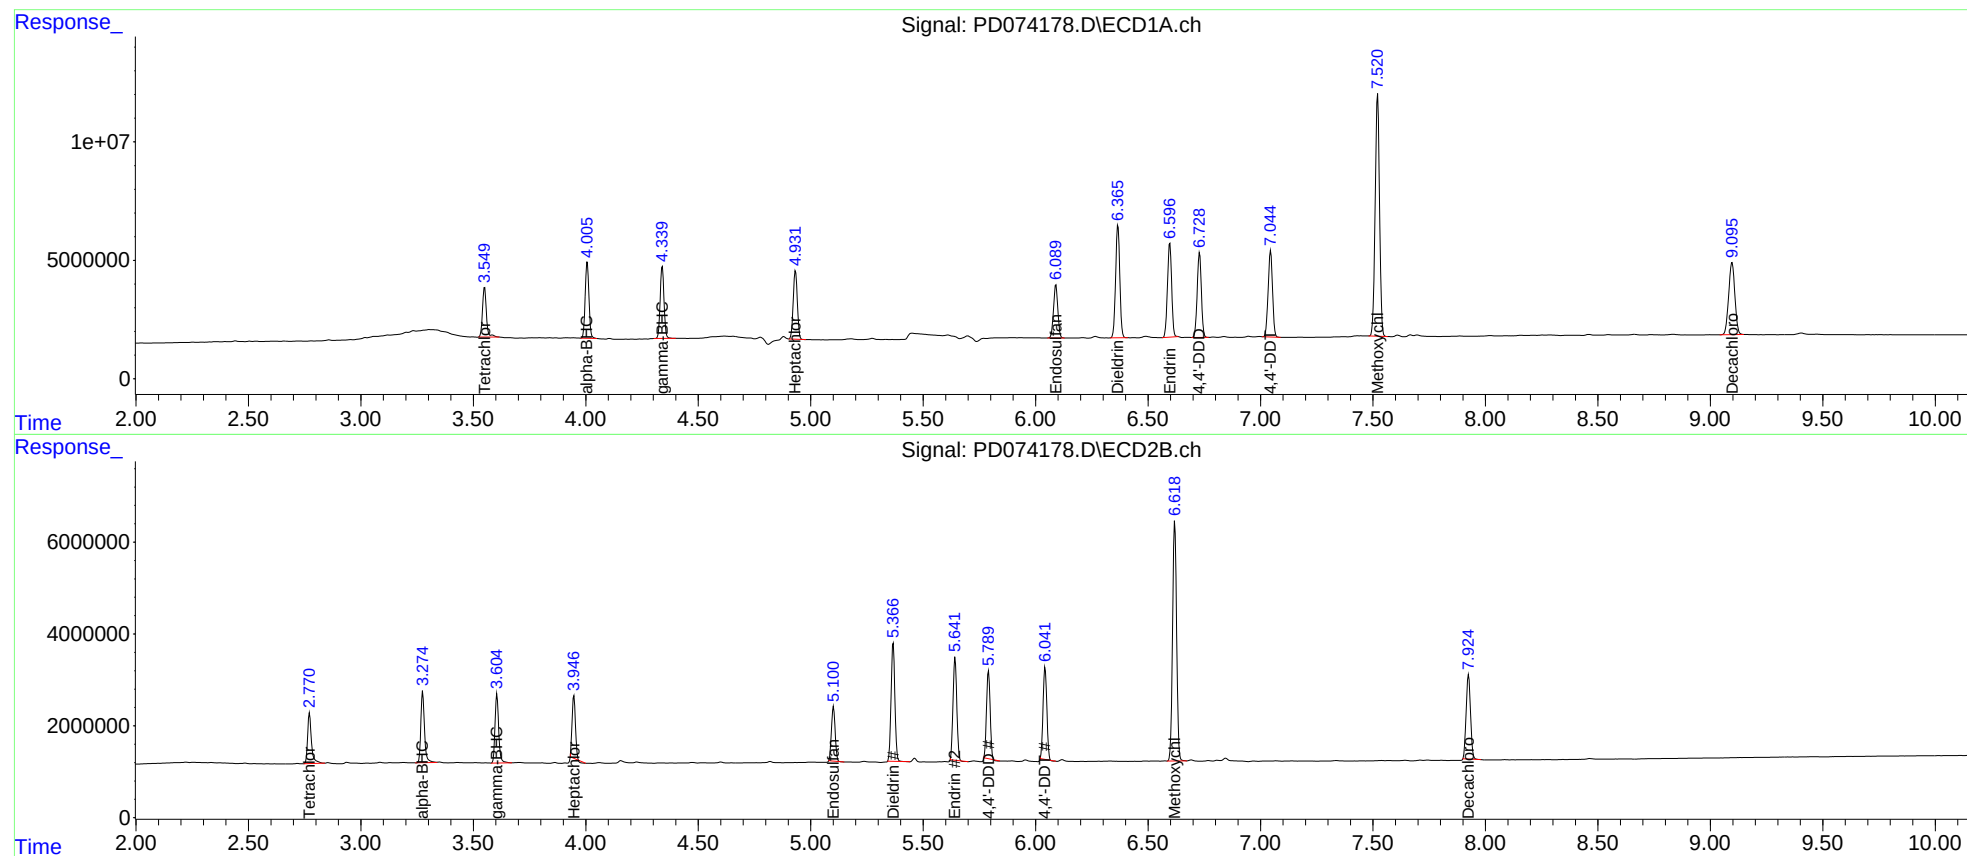

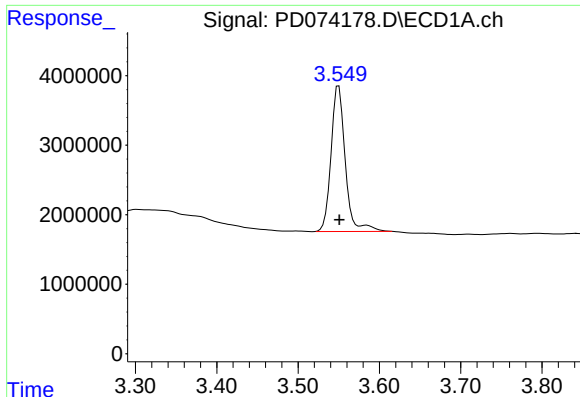


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 25500016
Conc: 10.43 ng/ml

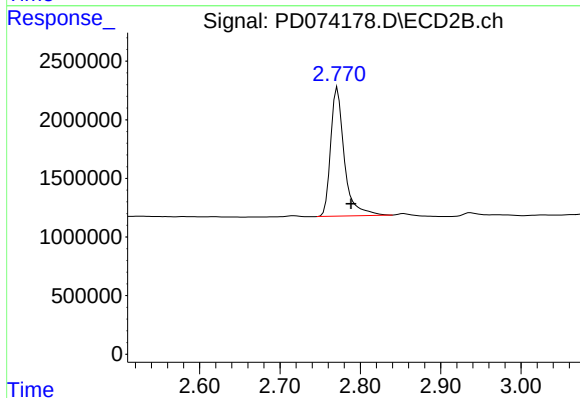


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.017 min
Response: 13017548
Conc: 10.54 ng/ml

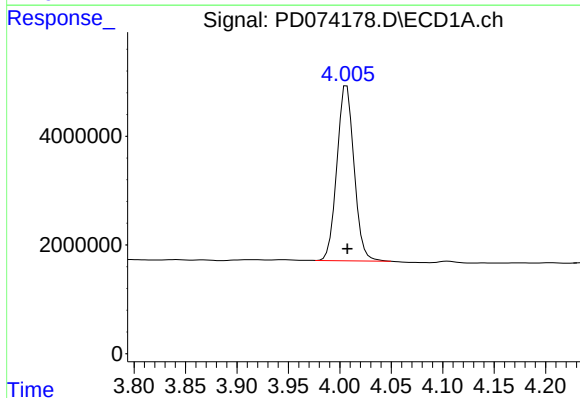


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 37360304
Conc: 9.71 ng/ml

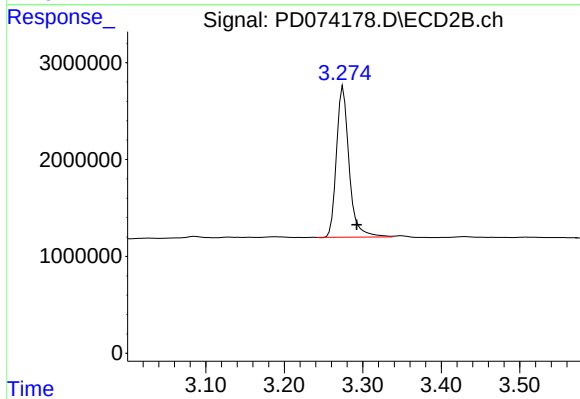


#2 alpha-BHC

R.T.: 3.275 min
Delta R.T.: -0.017 min
Response: 17455575
Conc: 9.90 ng/ml

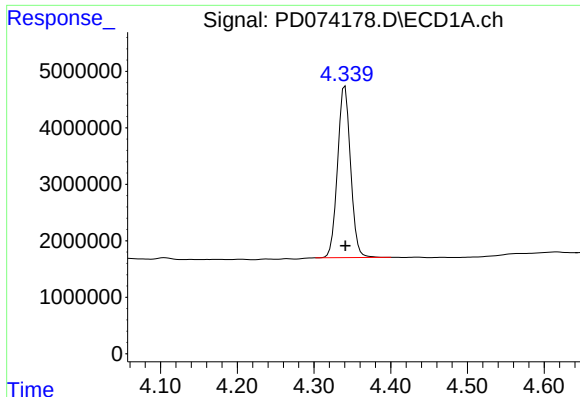


#3 gamma-BHC (Lindane)

R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 35816272
Conc: 9.80 ng/ml

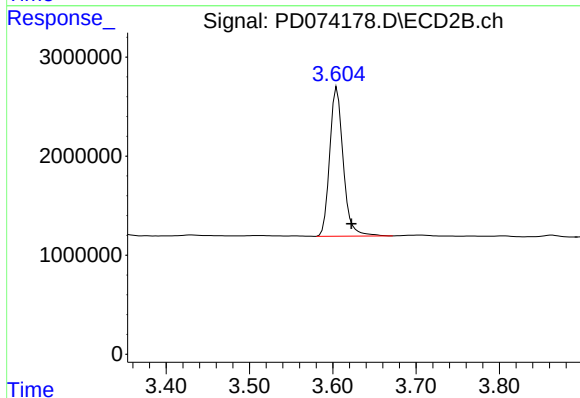


#3 gamma-BHC (Lindane)

R.T.: 3.605 min
Delta R.T.: -0.017 min
Response: 16944916
Conc: 9.98 ng/ml

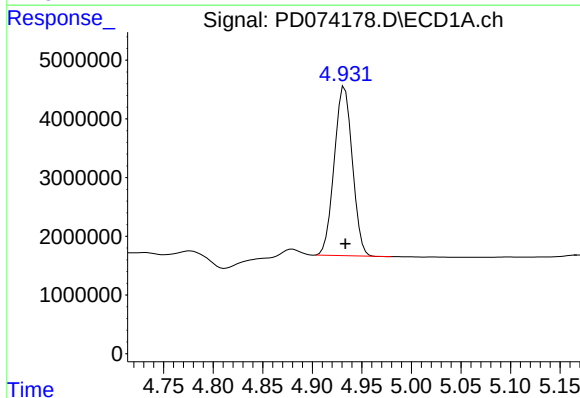


#4 Heptachlor

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 36571790
Conc: 9.76 ng/ml

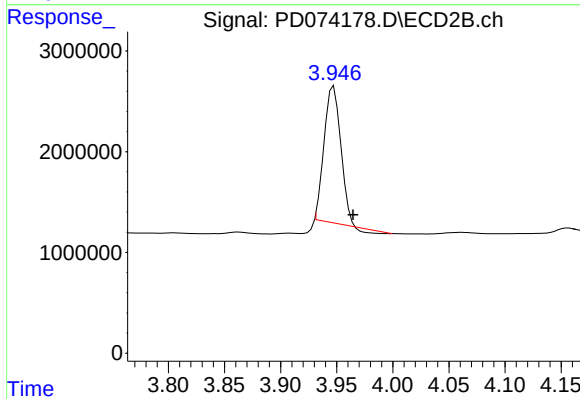


#4 Heptachlor

R.T.: 3.947 min
Delta R.T.: -0.017 min
Response: 13423412
Conc: 8.19 ng/ml

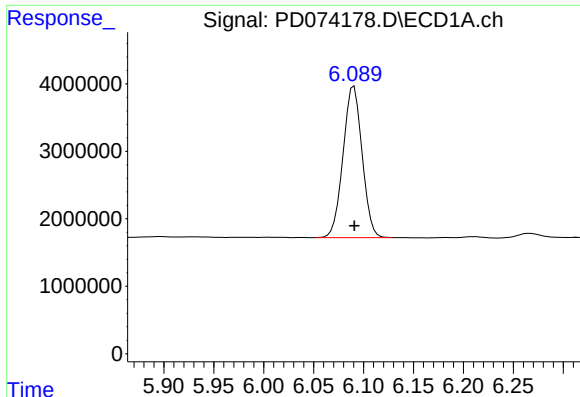


#9 Endosulfan I

R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 29737974
Conc: 10.09 ng/ml

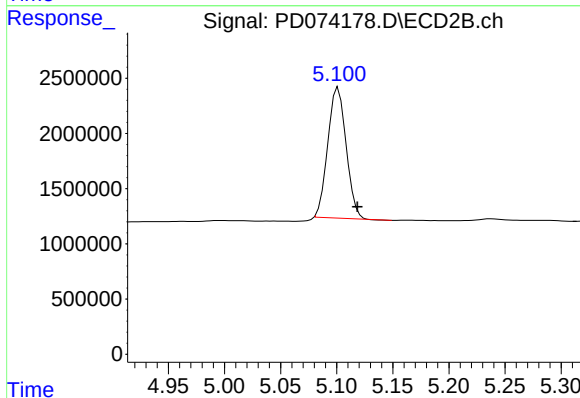


#9 Endosulfan I

R.T.: 5.101 min
Delta R.T.: -0.017 min
Response: 13411094
Conc: 9.62 ng/ml

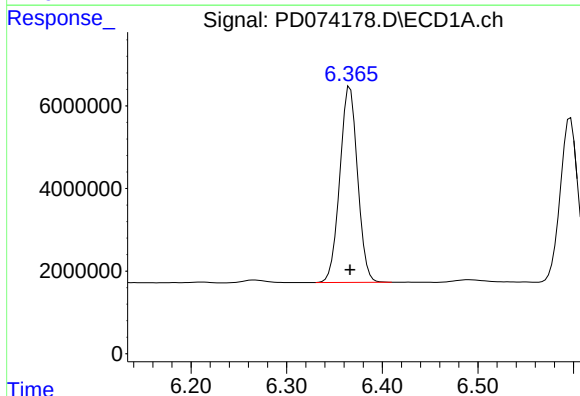


#13 Dieldrin

R.T.: 6.366 min
Delta R.T.: 0.000 min
Response: 61267076
Conc: 19.51 ng/ml

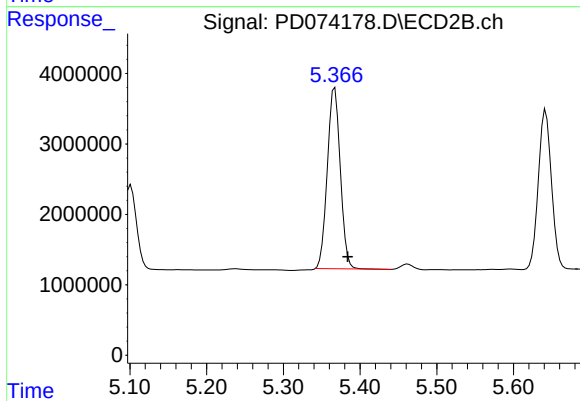


#13 Dieldrin

R.T.: 5.367 min
Delta R.T.: -0.017 min
Response: 30234507
Conc: 19.47 ng/ml

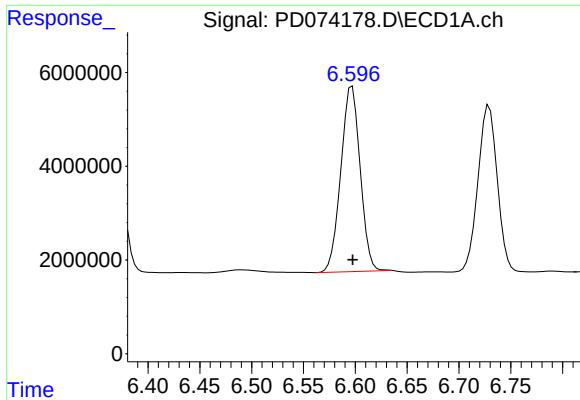


#14 Endrin

R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 51365420
Conc: 19.61 ng/ml

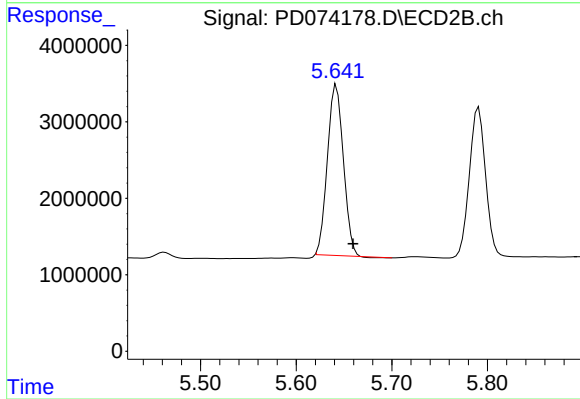


#14 Endrin

R.T.: 5.642 min
Delta R.T.: -0.017 min
Response: 25743062
Conc: 19.12 ng/ml

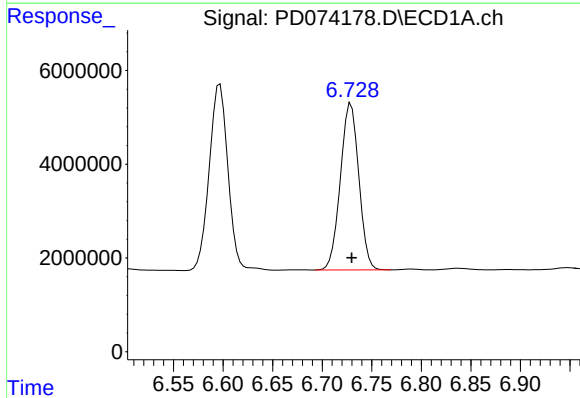


#16 4,4'-DDD

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 46091986
Conc: 19.68 ng/ml

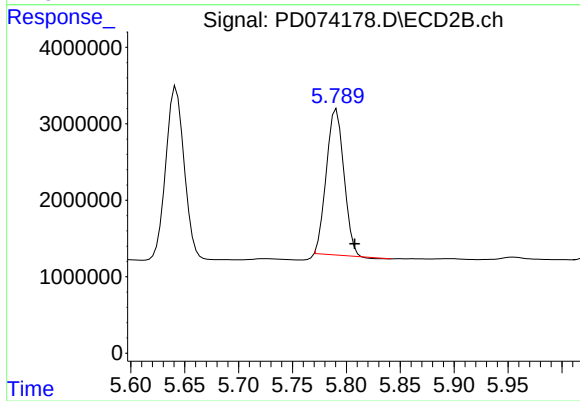


#16 4,4'-DDD

R.T.: 5.791 min
Delta R.T.: -0.017 min
Response: 21499132
Conc: 18.22 ng/ml

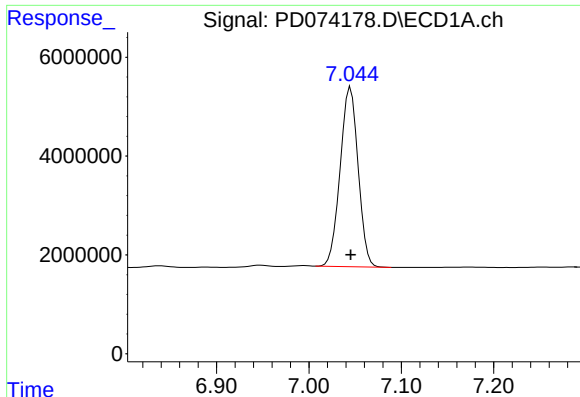


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 49118461
Conc: 19.85 ng/ml

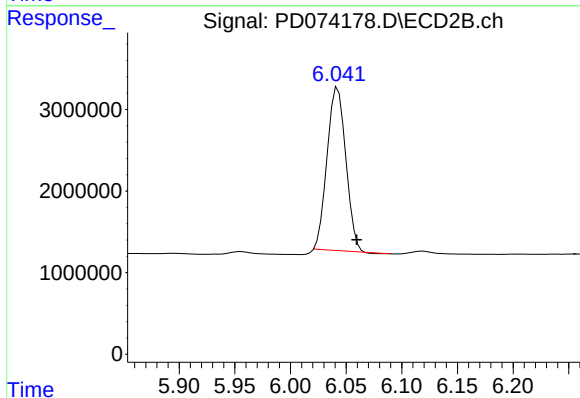


#17 4,4'-DDT

R.T.: 6.042 min
Delta R.T.: -0.017 min
Response: 23350381
Conc: 18.72 ng/ml

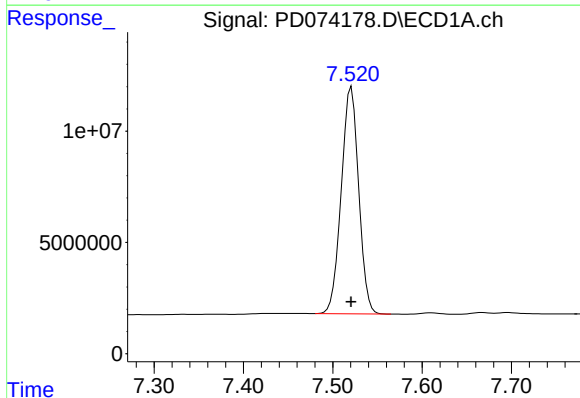


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 137973629
Conc: 101.71 ng/ml

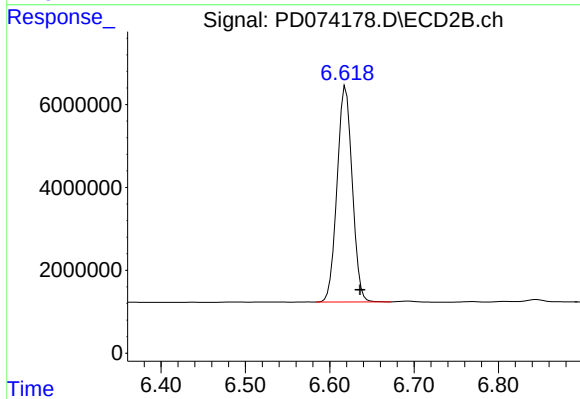

#20 Methoxychlor

R.T.: 6.619 min
Delta R.T.: -0.017 min
Response: 65001304
Conc: 104.98 ng/ml

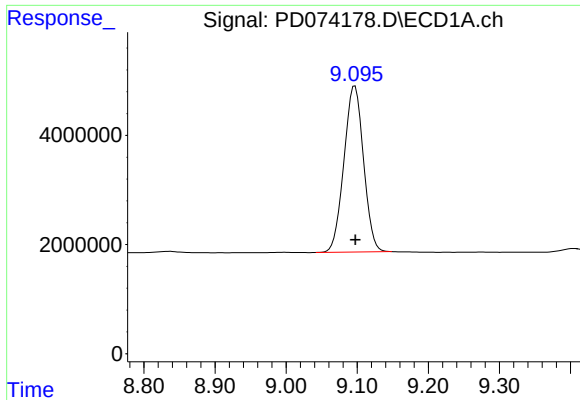


#27 Decachlorobiphenyl

R.T.: 9.097 min

Delta R.T.: 0.000 min

Response: 58233005

Conc: 21.58 ng/ml

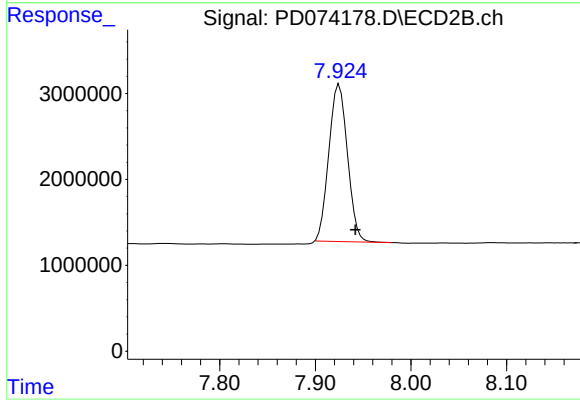

#27 Decachlorobiphenyl

R.T.: 7.925 min

Delta R.T.: -0.017 min

Response: 24679495

Conc: 20.92 ng/ml