

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 14:37
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:36:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 01:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.789	48907683	24702862	20.000	20.000
27)	SA Decachlor...	9.097	7.942	107.9E6	47178483	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.007	3.292	76948097	35267452	20.000	20.000
3)	MA gamma-BHC...	4.341	3.622	73095817	33971316	20.000	20.000
4)	MA Heptachlor	4.934	3.964	74915001	32776607	20.000	20.000
9)	A Endosulfan I	6.091	5.118	58933030	27877751	20.000	20.000
13)	MA Dieldrin	6.367	5.384	125.6E6	62104561	40.000	40.000
14)	MA Endrin	6.597	5.659	104.8E6	53853015	40.000	40.000
16)	A 4,4'-DDD	6.730	5.808	93677626	47195444	40.000	40.000
17)	MA 4,4'-DDT	7.045	6.059	98969923	49900506	40.000	40.000
20)	A Methoxychlor	7.521	6.636	271.3E6	123.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 14:37
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:36:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 01:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

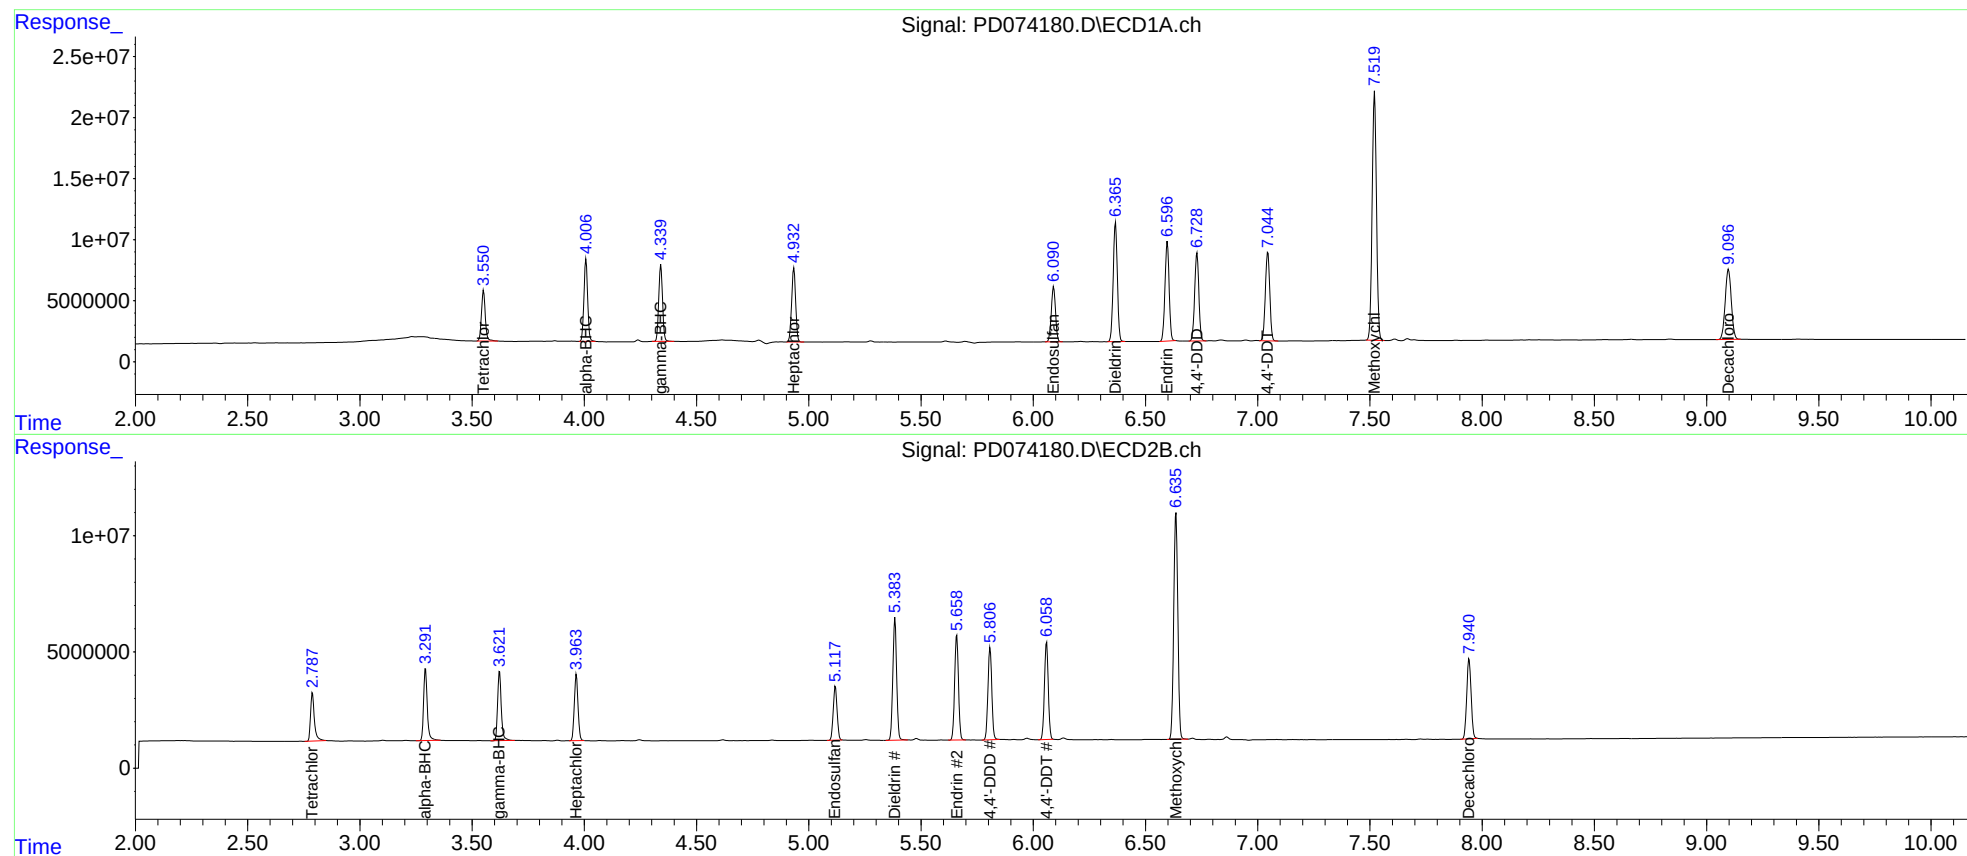

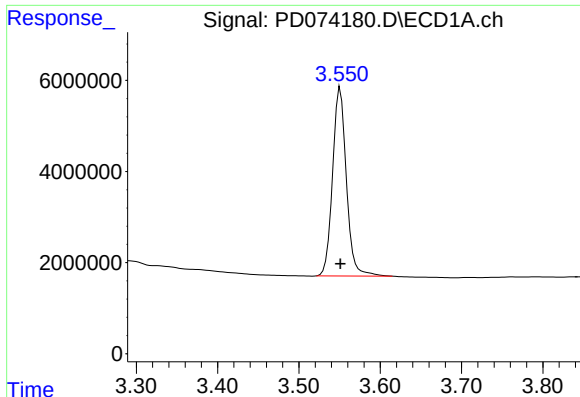


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 48907683
Conc: 20.00 ng/ml

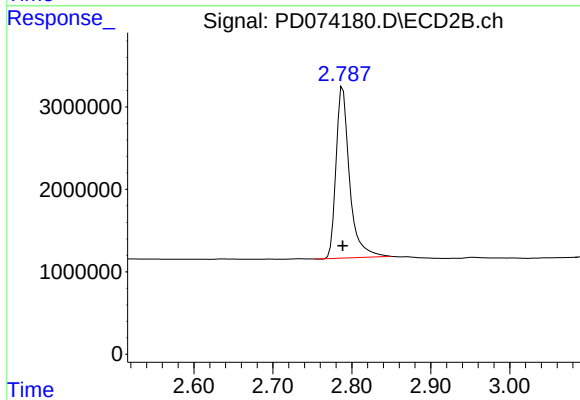


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 24702862
Conc: 20.00 ng/ml

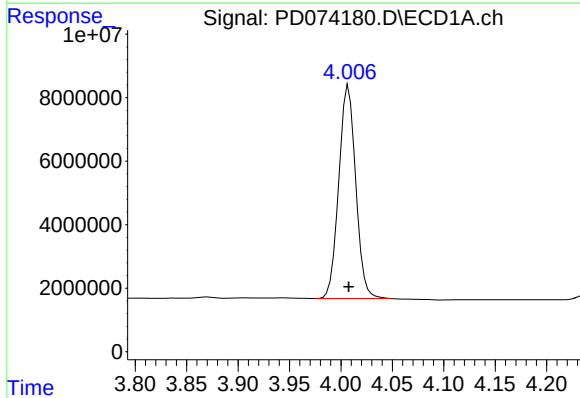


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 76948097
Conc: 20.00 ng/ml

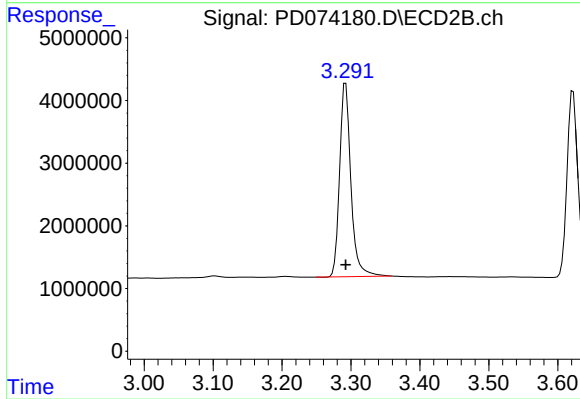


#2 alpha-BHC

R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 35267452
Conc: 20.00 ng/ml

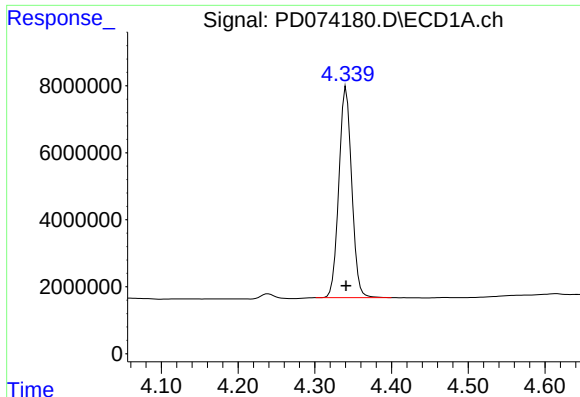


#3 gamma-BHC (Lindane)

R.T.: 4.341 min
Delta R.T.: 0.000 min
Response: 73095817
Conc: 20.00 ng/ml

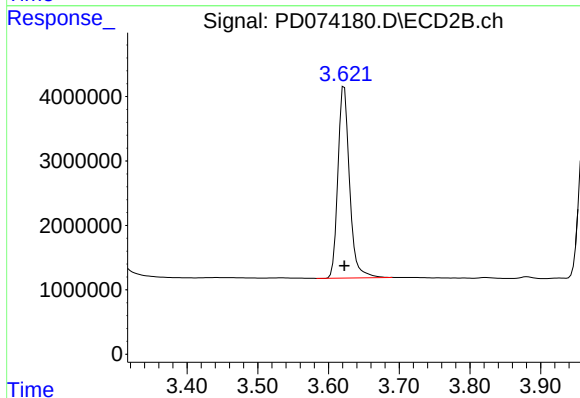


#3 gamma-BHC (Lindane)

R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 33971316
Conc: 20.00 ng/ml

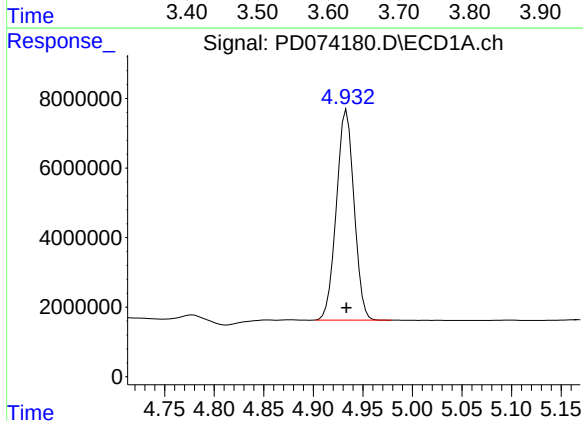


#4 Heptachlor

R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 74915001
Conc: 20.00 ng/ml

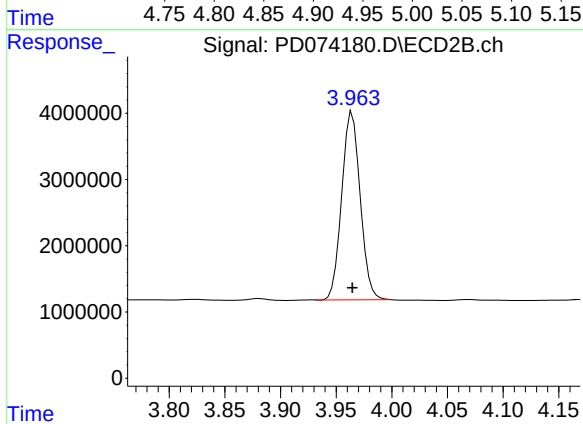


#4 Heptachlor

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 32776607
Conc: 20.00 ng/ml

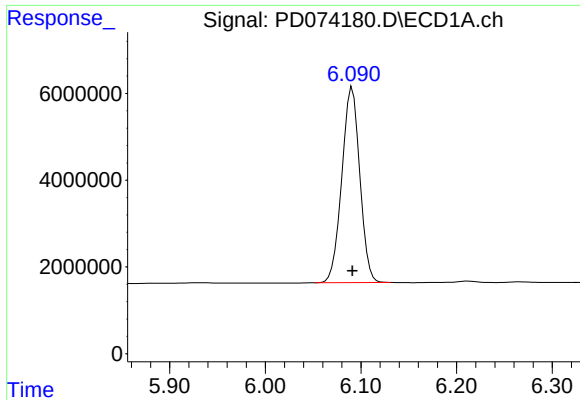


#9 Endosulfan I

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 58933030
Conc: 20.00 ng/ml

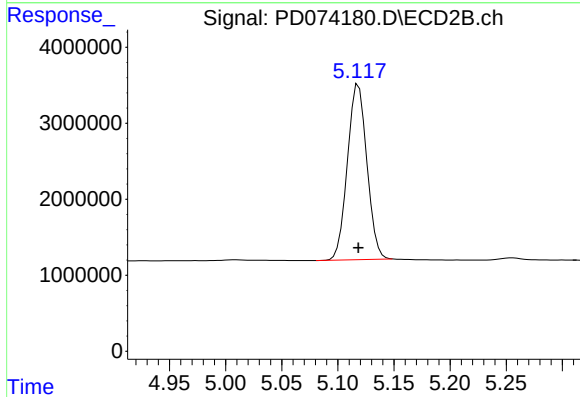


#9 Endosulfan I

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 27877751
Conc: 20.00 ng/ml

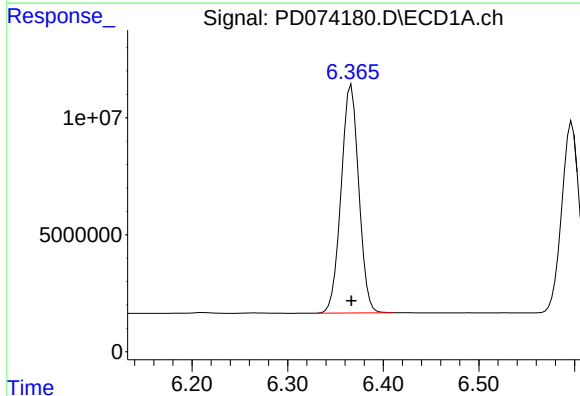


#13 Dieldrin

R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 125600534
Conc: 40.00 ng/ml

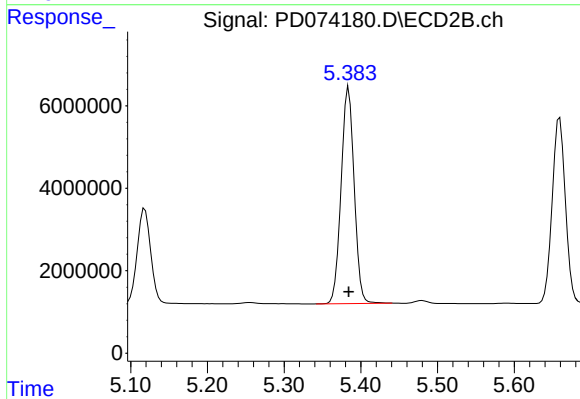


#13 Dieldrin

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 62104561
Conc: 40.00 ng/ml

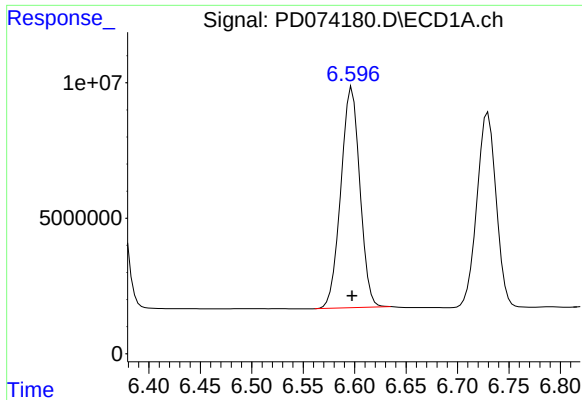


#14 Endrin

R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 104774080
Conc: 40.00 ng/ml

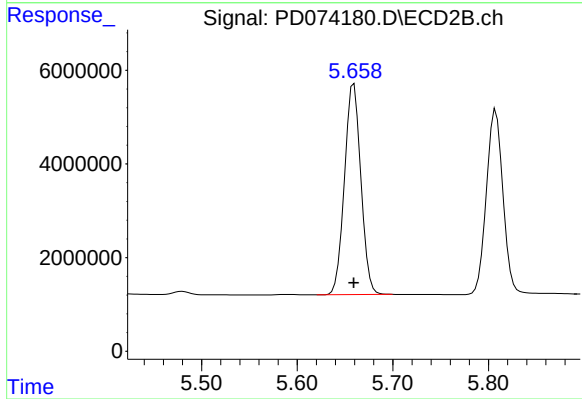


#14 Endrin

R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 53853015
Conc: 40.00 ng/ml

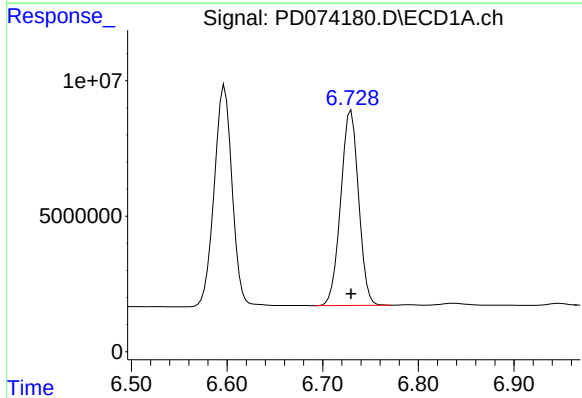


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 93677626
Conc: 40.00 ng/ml

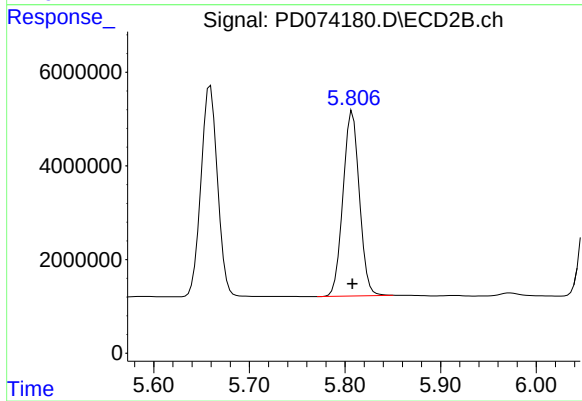


#16 4,4'-DDD

R.T.: 5.808 min
Delta R.T.: 0.000 min
Response: 47195444
Conc: 40.00 ng/ml

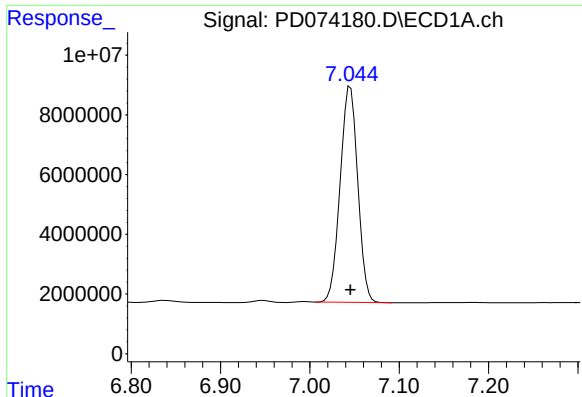


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 98969923
Conc: 40.00 ng/ml

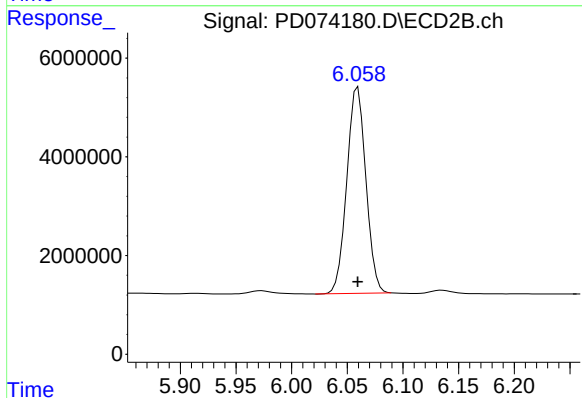


#17 4,4'-DDT

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 49900506
Conc: 40.00 ng/ml

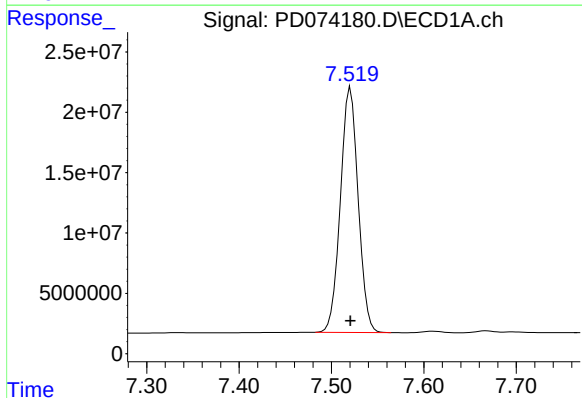


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 271308118
Conc: 200.00 ng/ml

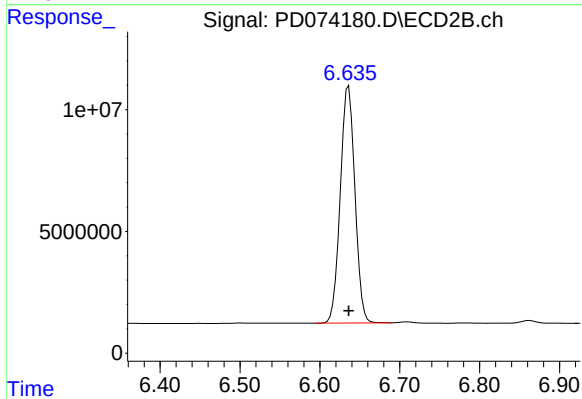


#20 Methoxychlor

R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 123836647
Conc: 200.00 ng/ml

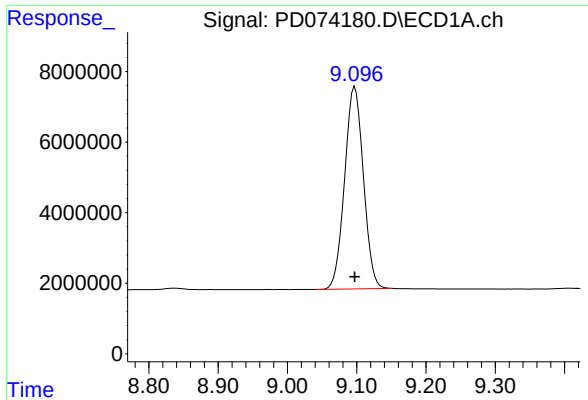

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 107944309
Conc: 40.00 ng/ml

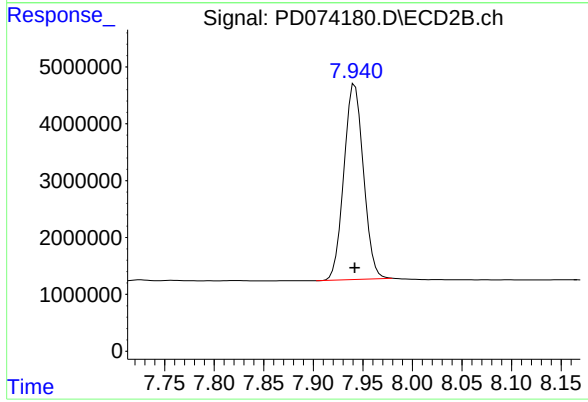

#27 Decachlorobiphenyl

R.T.: 7.942 min
Delta R.T.: 0.000 min
Response: 47178483
Conc: 40.00 ng/ml