

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 15:04
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:36:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 01:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	96772047	49774772	39.573	40.299
27)	SA Decachlor...	9.097	7.925	199.7E6	86198336	73.989	73.083
Target Compounds							
2)	A alpha-BHC	4.008	3.276	161.6E6	73353481	42.011	41.598
3)	MA gamma-BHC...	4.341	3.606	150.8E6	69028424	41.265	40.639
4)	MA Heptachlor	4.934	3.948	152.7E6	50492573	40.765	30.810
9)	A Endosulfan I	6.091	5.102	116.6E6	51376319	39.565	36.858
13)	MA Dieldrin	6.367	5.368	257.1E6	125.1E6	81.892	80.593
14)	MA Endrin	6.598	5.643	212.8E6	101.3E6	81.242	75.272
16)	A 4,4'-DDD	6.730	5.792	190.4E6	85687860	81.319	72.624
17)	MA 4,4'-DDT	7.046	6.043	201.3E6	93968498	81.343	75.325
20)	A Methoxychlor	7.521	6.619	538.0E6	234.4E6	396.618	378.497


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 15:04
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:36:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 01:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

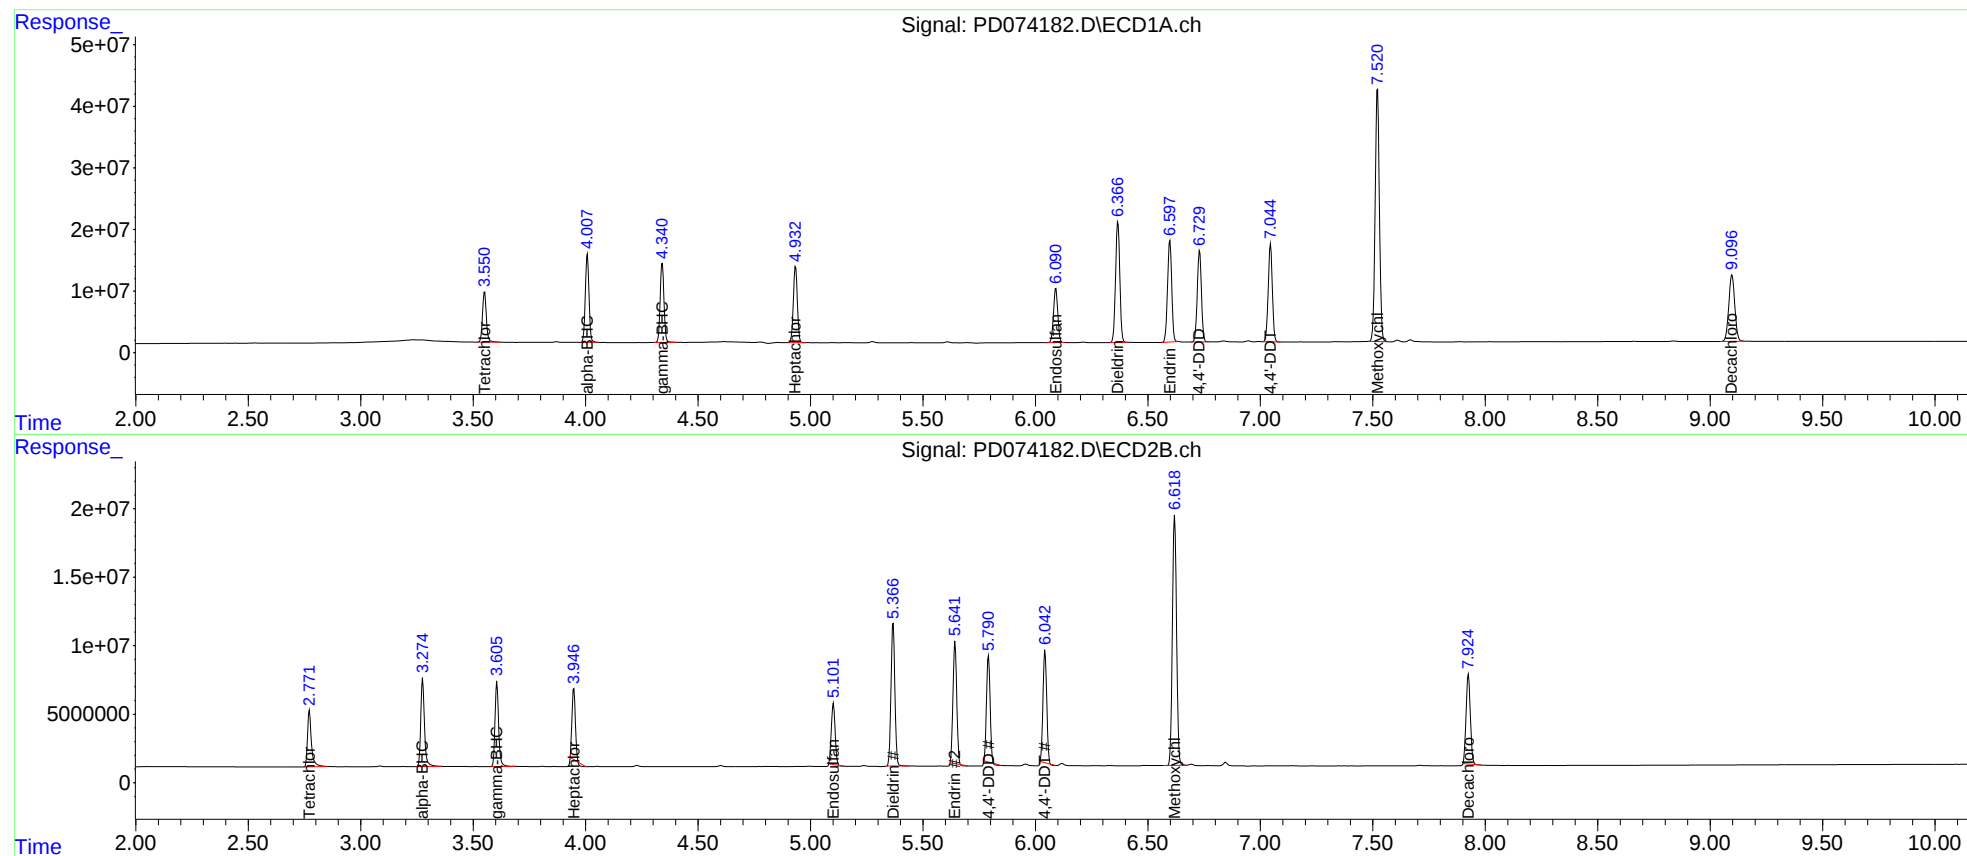

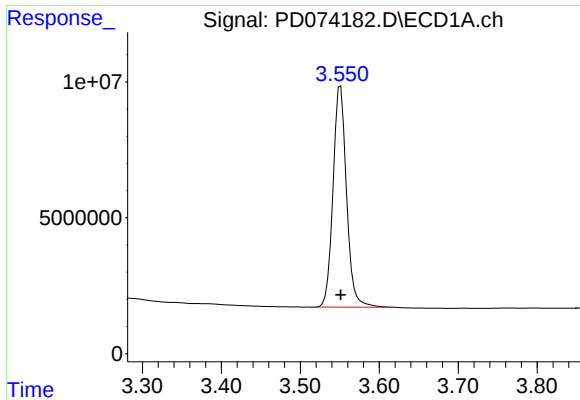


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 96772047
Conc: 39.57 ng/ml

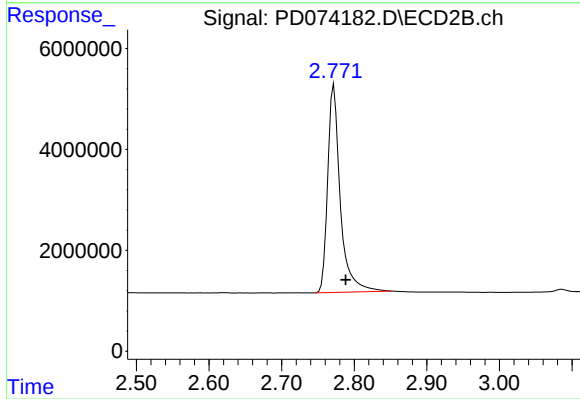


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.017 min
Response: 49774772
Conc: 40.30 ng/ml

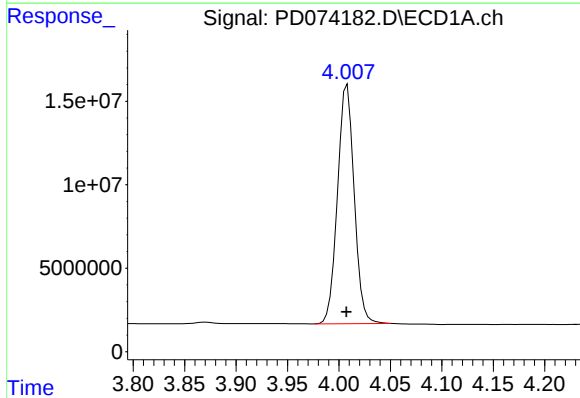


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 161631905
Conc: 42.01 ng/ml

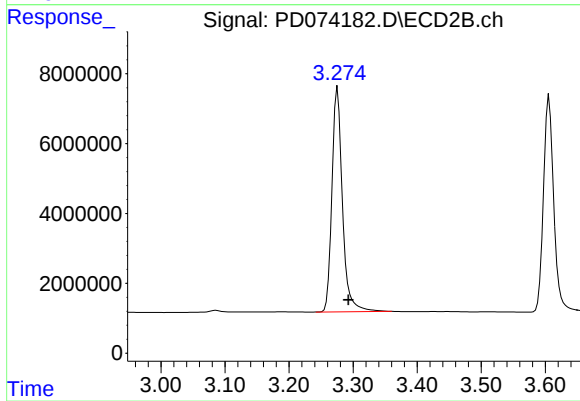


#2 alpha-BHC

R.T.: 3.276 min
Delta R.T.: -0.017 min
Response: 73353481
Conc: 41.60 ng/ml

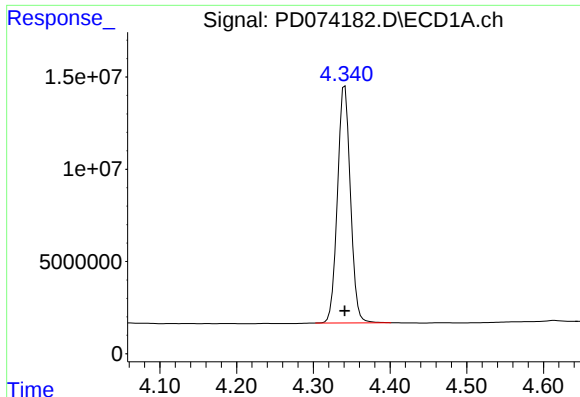


#3 gamma-BHC (Lindane)

R.T.: 4.341 min
Delta R.T.: 0.000 min
Response: 150816573
Conc: 41.27 ng/ml

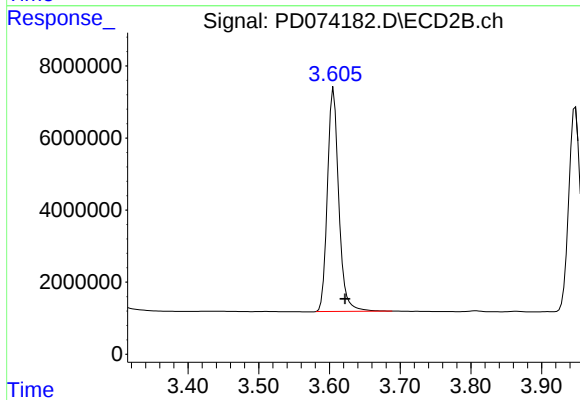


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: -0.016 min
Response: 69028424
Conc: 40.64 ng/ml

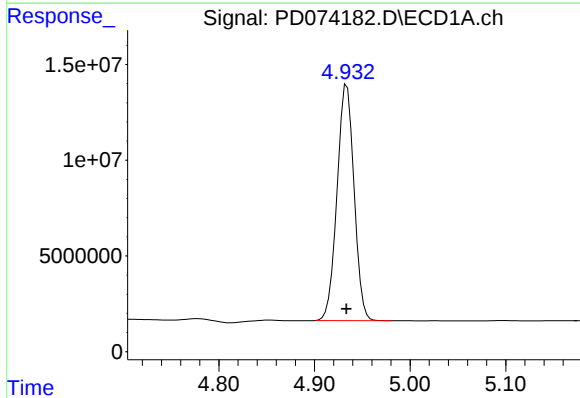


#4 Heptachlor

R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 152696536
Conc: 40.77 ng/ml

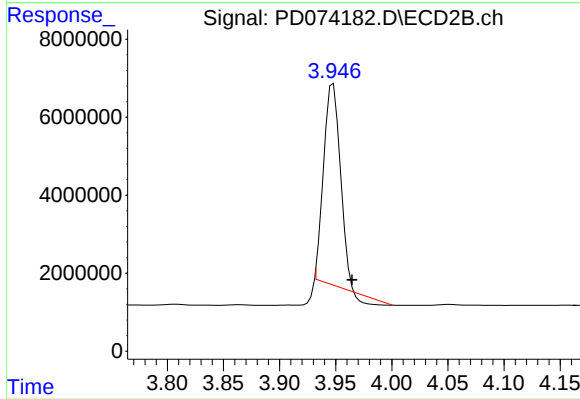


#4 Heptachlor

R.T.: 3.948 min
Delta R.T.: -0.017 min
Response: 50492573
Conc: 30.81 ng/ml

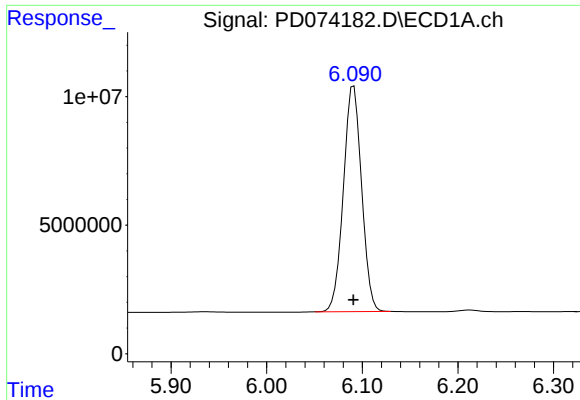


#9 Endosulfan I

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 116584701
Conc: 39.57 ng/ml

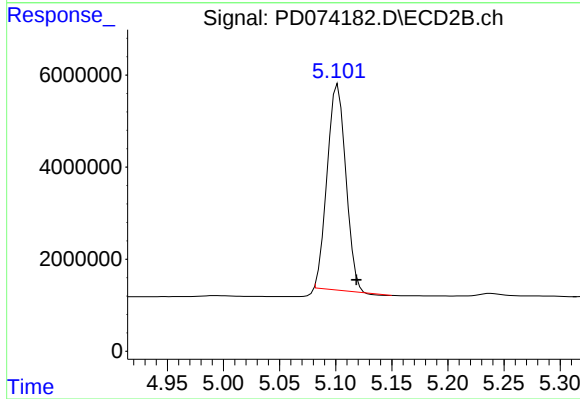


#9 Endosulfan I

R.T.: 5.102 min
Delta R.T.: -0.016 min
Response: 51376319
Conc: 36.86 ng/ml

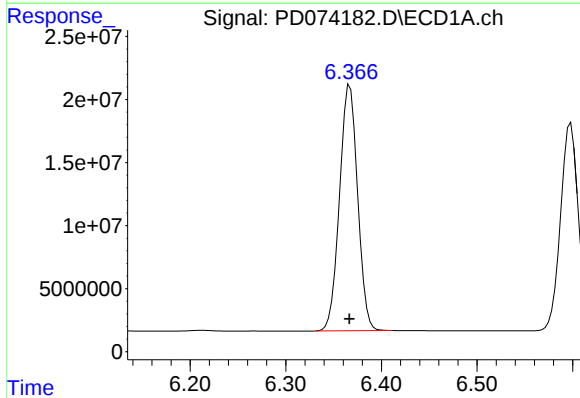


#13 Dieldrin

R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 257142567
Conc: 81.89 ng/ml

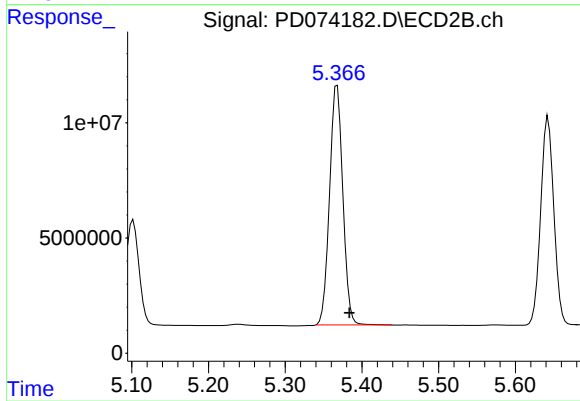


#13 Dieldrin

R.T.: 5.368 min
Delta R.T.: -0.016 min
Response: 125129383
Conc: 80.59 ng/ml

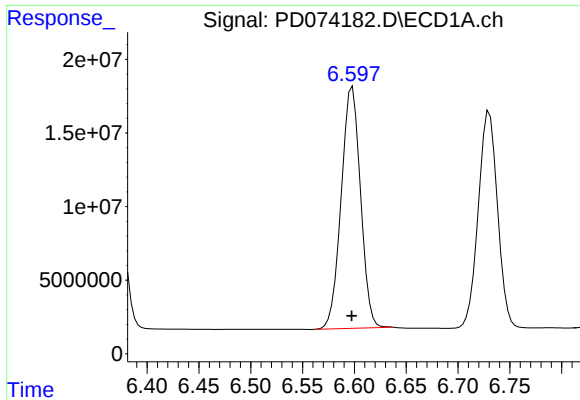


#14 Endrin

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 212801366
Conc: 81.24 ng/ml

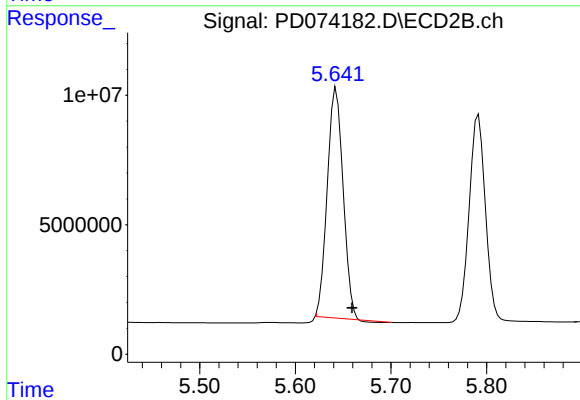


#14 Endrin

R.T.: 5.643 min
Delta R.T.: -0.016 min
Response: 101340798
Conc: 75.27 ng/ml

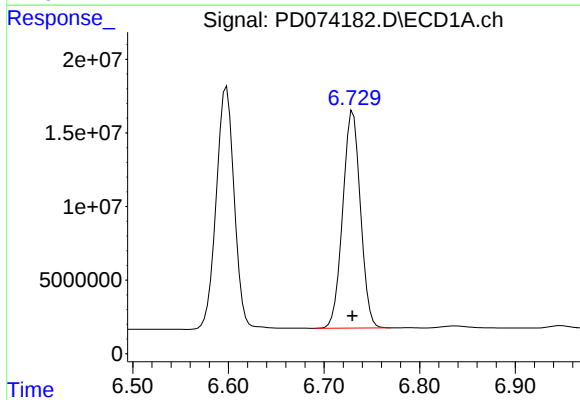


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 190443401
Conc: 81.32 ng/ml

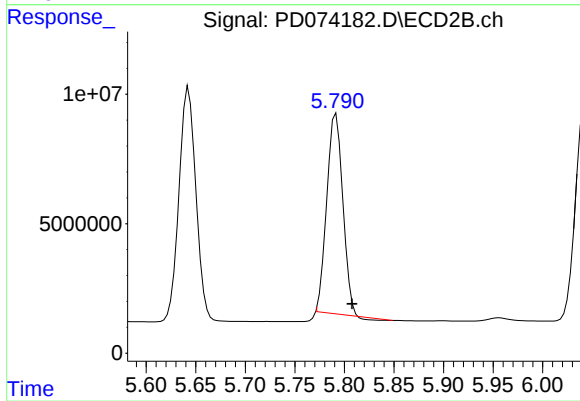


#16 4,4'-DDD

R.T.: 5.792 min
Delta R.T.: -0.016 min
Response: 85687860
Conc: 72.62 ng/ml

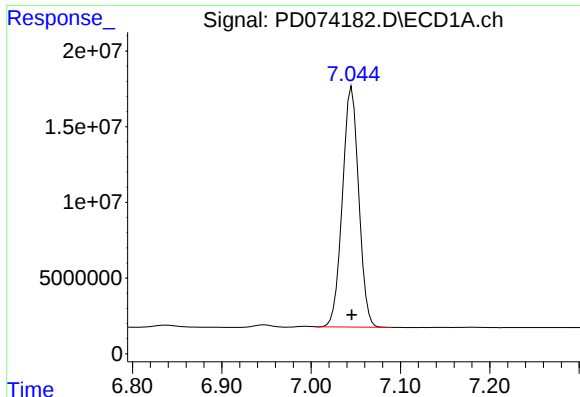


#17 4,4'-DDT

R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 201262641
Conc: 81.34 ng/ml

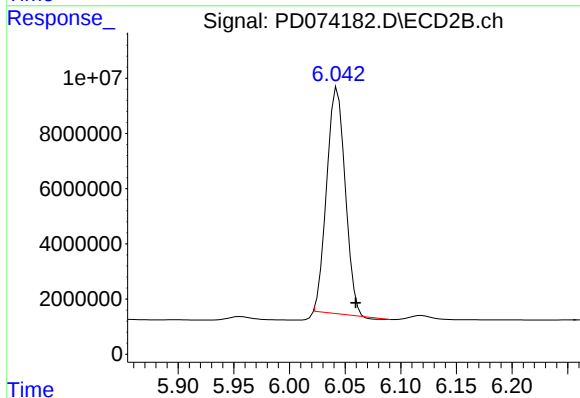


#17 4,4'-DDT

R.T.: 6.043 min
Delta R.T.: -0.016 min
Response: 93968498
Conc: 75.32 ng/ml

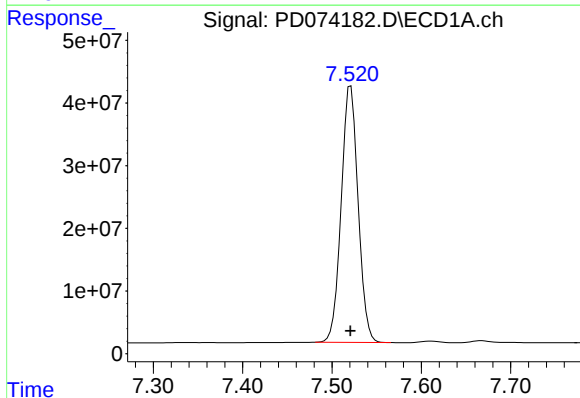


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 538028137
Conc: 396.62 ng/ml

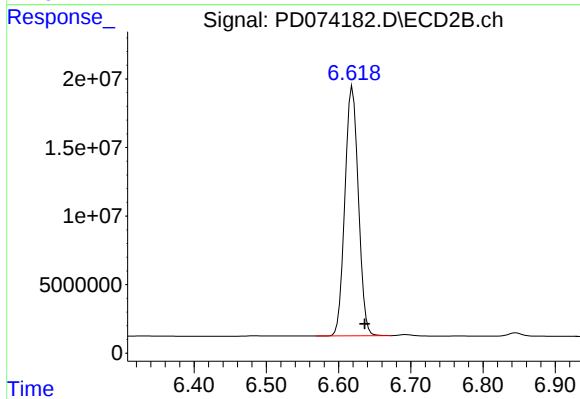


#20 Methoxychlor

R.T.: 6.619 min
Delta R.T.: -0.017 min
Response: 234358728
Conc: 378.50 ng/ml

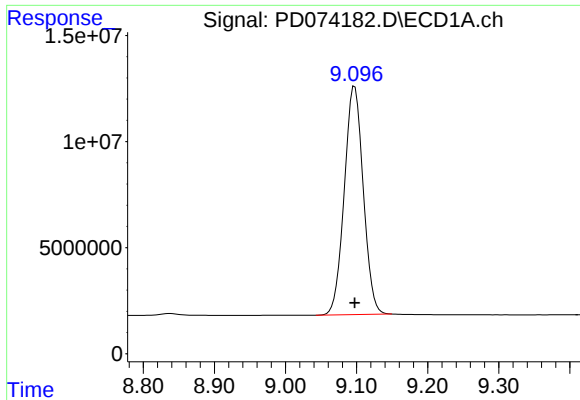

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 199666094
Conc: 73.99 ng/ml

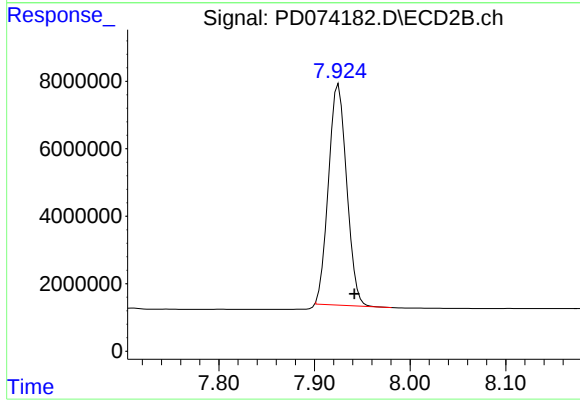

#27 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.017 min
Response: 86198336
Conc: 73.08 ng/ml