

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 15:18
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 23:24:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 13 23:20:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	96988994	49705258	39.998	39.830
27)	SA Decachlor...	9.097	7.926	208.7E6	92150552	76.433	76.389
Target Compounds							
5)	MB Aldrin	5.277	4.229	147.9E6	68494377	41.406	40.491
6)	B beta-BHC	4.536	3.902	65386229	31162771	38.831	38.695
7)	B delta-BHC	4.785	4.133	150.2E6	71703752	41.981	41.162
8)	B Heptachlo...	5.704	4.731	128.6E6	62558722	40.091	40.065
10)	B trans-Chl...	5.961	4.982	127.6E6	61327075	40.859	40.318
11)	B cis-Chlor...	6.040	5.047	129.2E6	62406178	40.433	40.029
12)	B 4,4'-DDE	6.213	5.237	247.9E6	118.9E6	84.657	82.755
15)	B Endosulfa...	6.817	5.936	219.7E6	107.2E6	82.184	80.671
18)	B Endrin al...	6.947	6.116	176.1E6	85806767	80.602	79.179
19)	B Endosulfa...	7.181	6.340	205.7E6	99102165	81.551	79.971
21)	B Endrin ke...	7.669	6.846	234.0E6	120.2E6	81.630	79.658


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 15:18
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 23:24:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 13 23:20:33 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

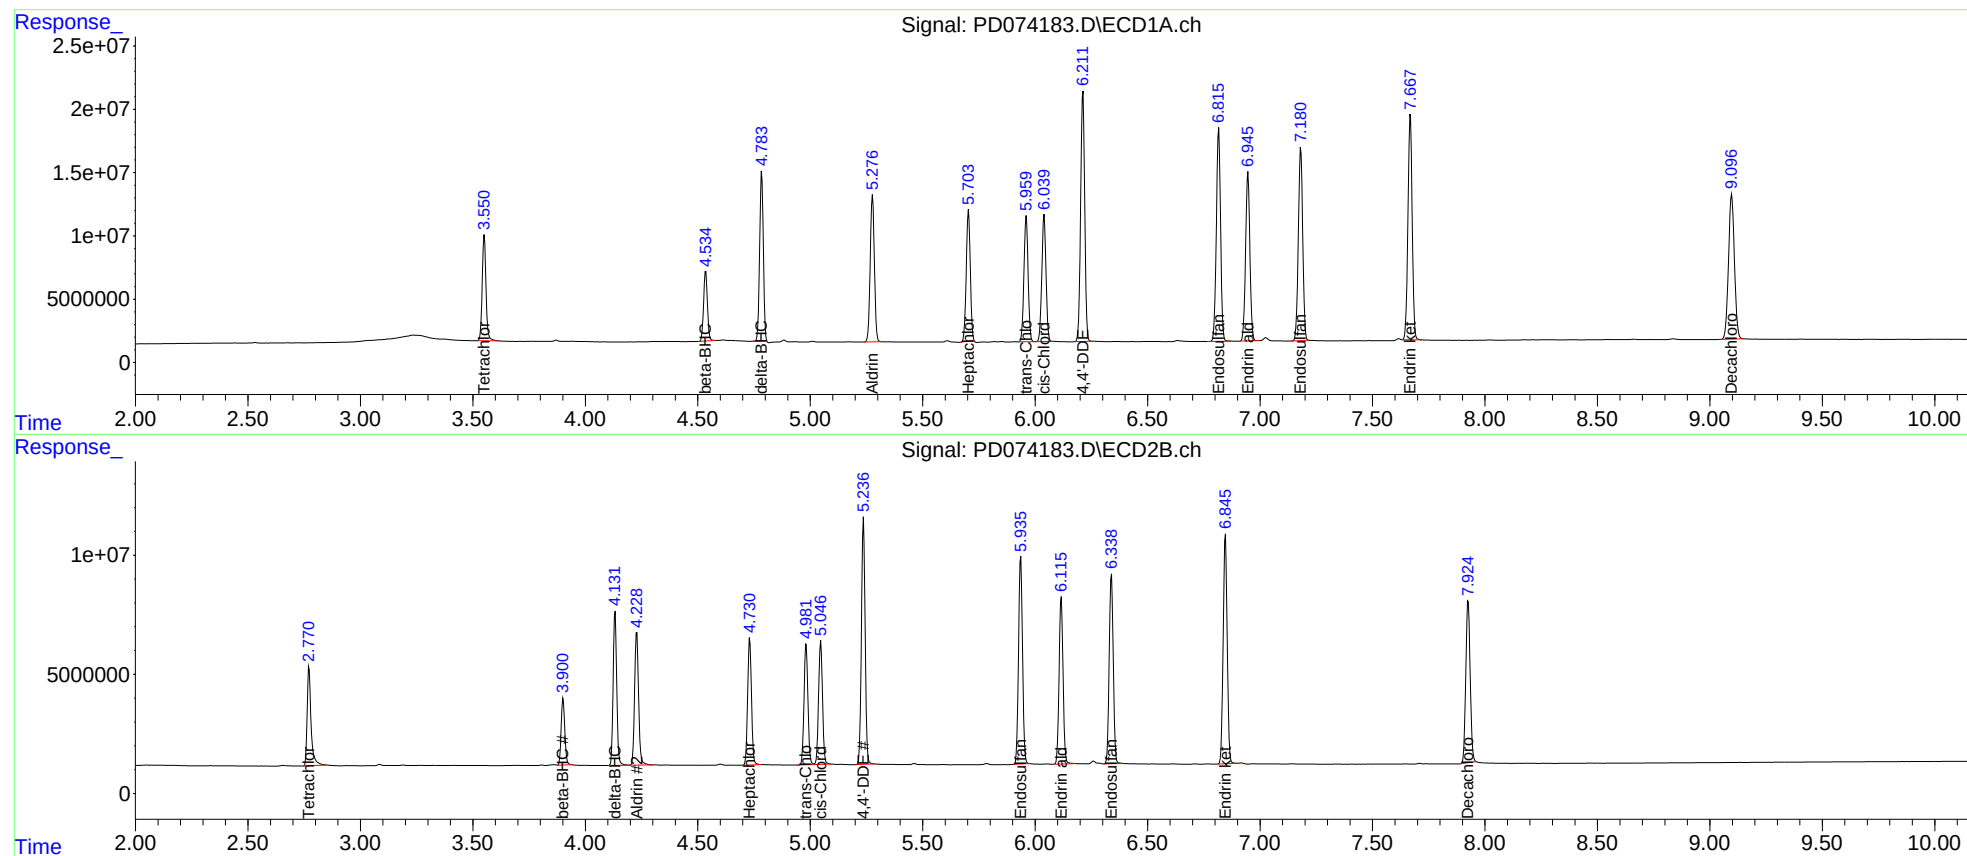

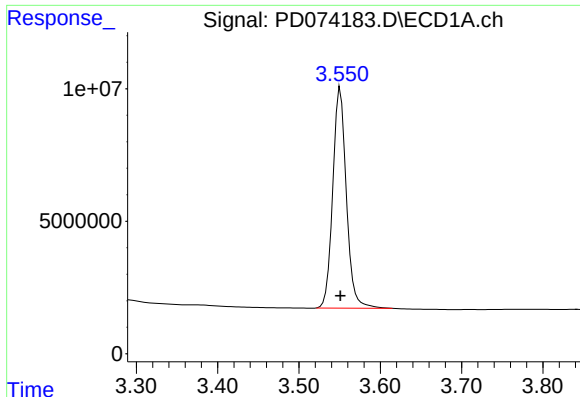


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 96988994
Conc: 40.00 ng/ml

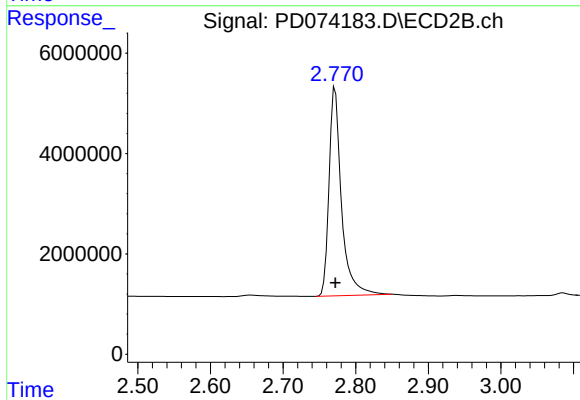


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 49705258
Conc: 39.83 ng/ml

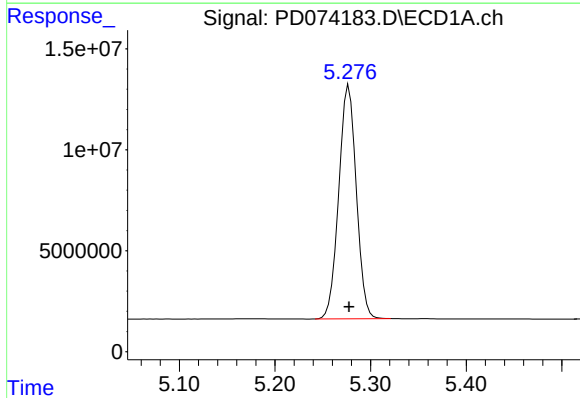


#5 Aldrin

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 147867849
Conc: 41.41 ng/ml

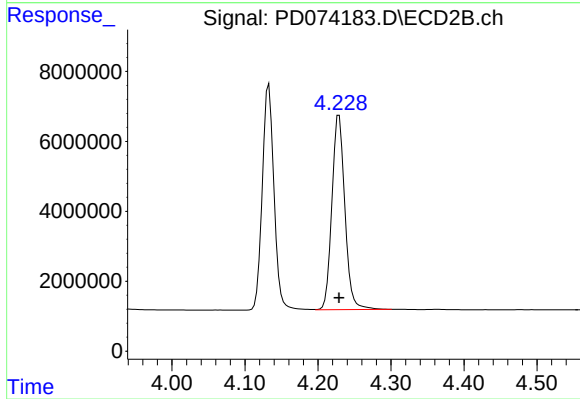


#5 Aldrin

R.T.: 4.229 min
Delta R.T.: 0.000 min
Response: 68494377
Conc: 40.49 ng/ml

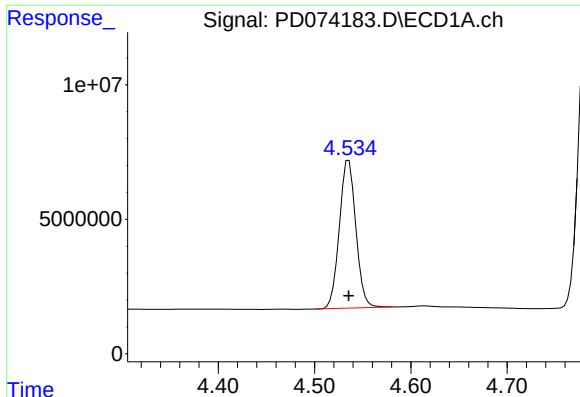


#6 beta-BHC

R.T.: 4.536 min
Delta R.T.: 0.000 min
Response: 65386229
Conc: 38.83 ng/ml

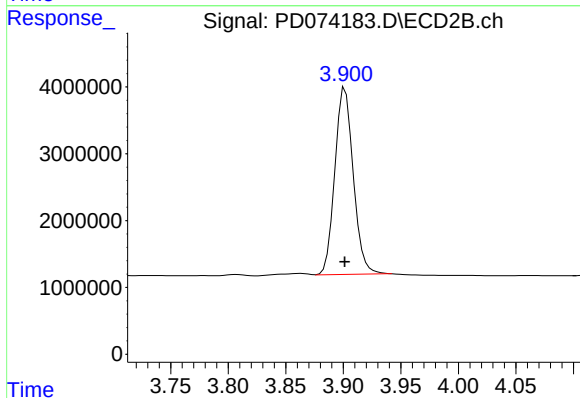


#6 beta-BHC

R.T.: 3.902 min
Delta R.T.: 0.000 min
Response: 31162771
Conc: 38.69 ng/ml

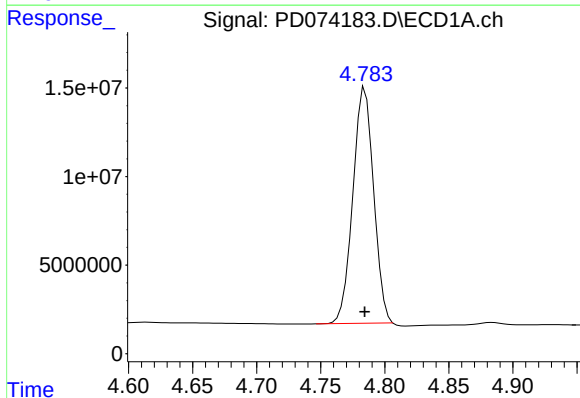


#7 delta-BHC

R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 150181967
Conc: 41.98 ng/ml

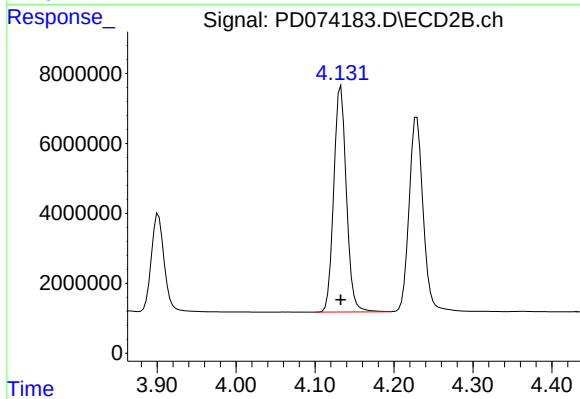


#7 delta-BHC

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 71703752
Conc: 41.16 ng/ml

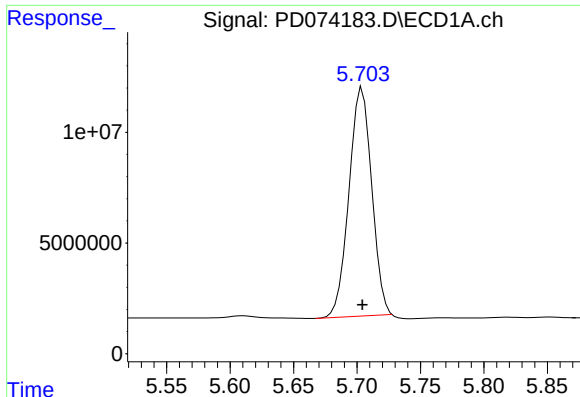


#8 Heptachlor epoxide

R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 128582629
Conc: 40.09 ng/ml

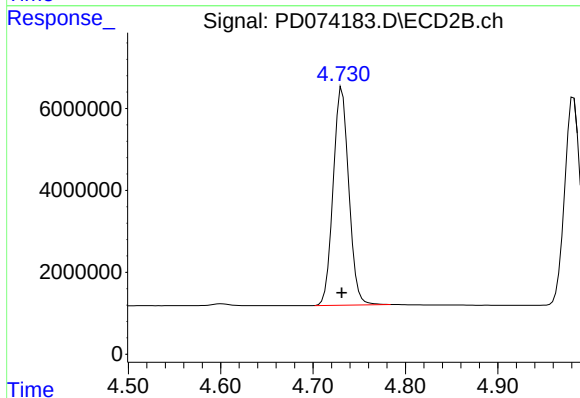


#8 Heptachlor epoxide

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 62558722
Conc: 40.07 ng/ml

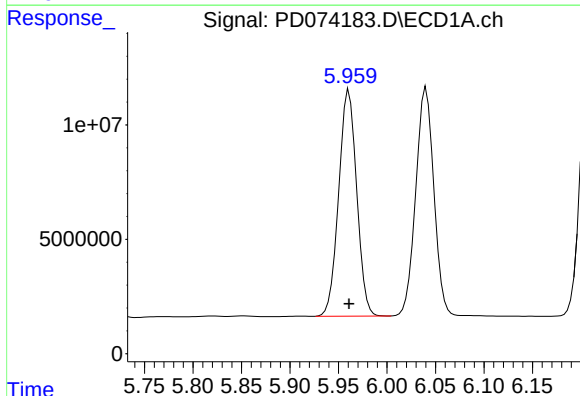


#10 trans-Chlordane

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 127586023
Conc: 40.86 ng/ml

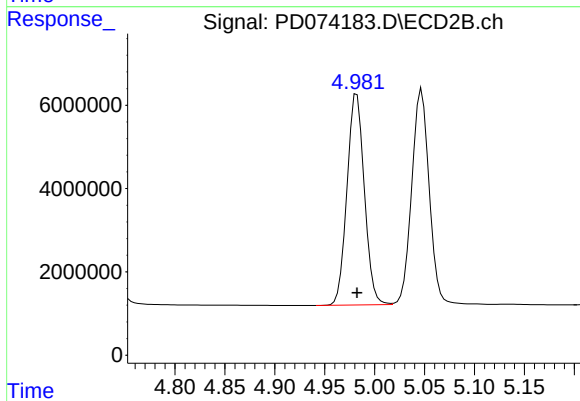


#10 trans-Chlordane

R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 61327075
Conc: 40.32 ng/ml

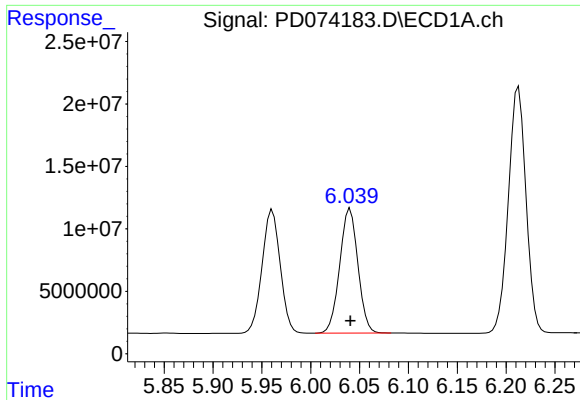


#11 cis-Chlordane

R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 129241127
Conc: 40.43 ng/ml

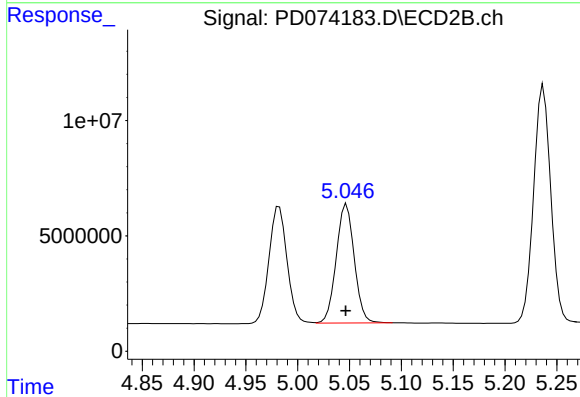


#11 cis-Chlordane

R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 62406178
Conc: 40.03 ng/ml

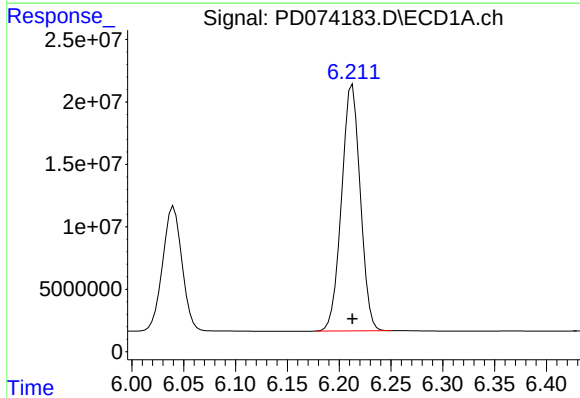


#12 4,4'-DDE

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 247879850
Conc: 84.66 ng/ml

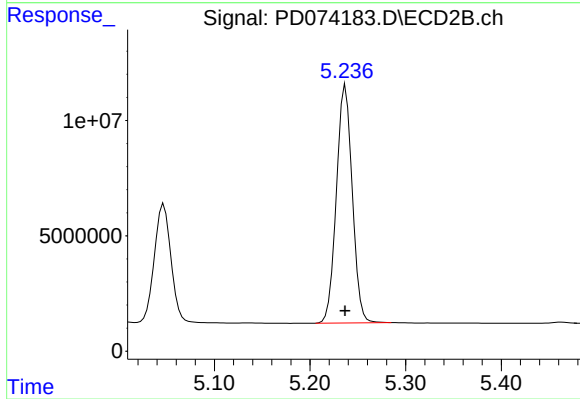


#12 4,4'-DDE

R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 118912111
Conc: 82.75 ng/ml

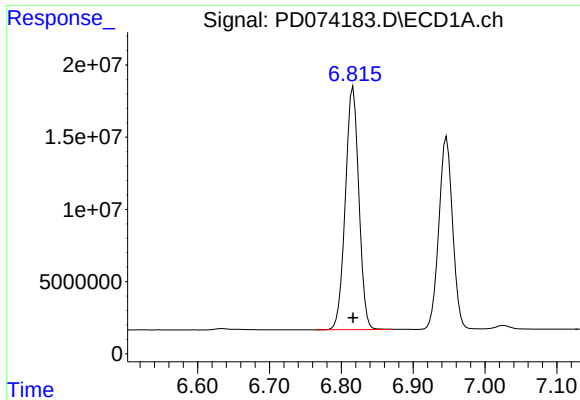


#15 Endosulfan II

R.T.: 6.817 min
Delta R.T.: 0.000 min
Response: 219737879
Conc: 82.18 ng/ml

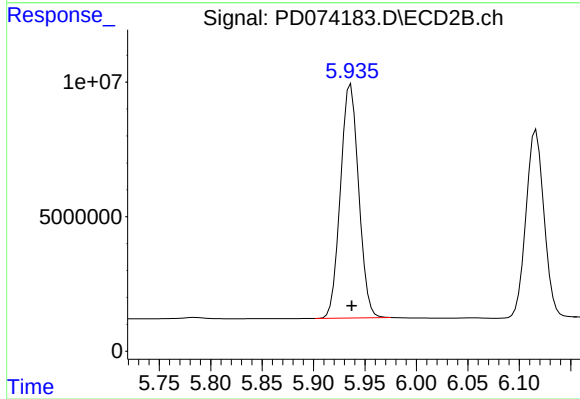


#15 Endosulfan II

R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 107177211
Conc: 80.67 ng/ml

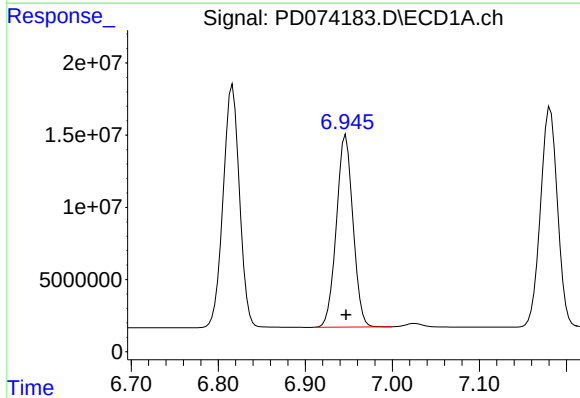


#18 Endrin aldehyde

R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 176083660
Conc: 80.60 ng/ml

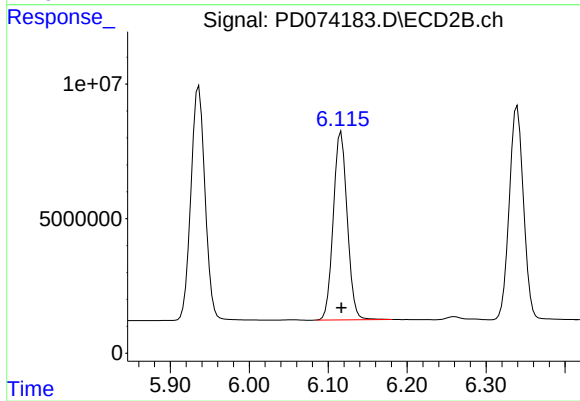


#18 Endrin aldehyde

R.T.: 6.116 min
Delta R.T.: 0.000 min
Response: 85806767
Conc: 79.18 ng/ml

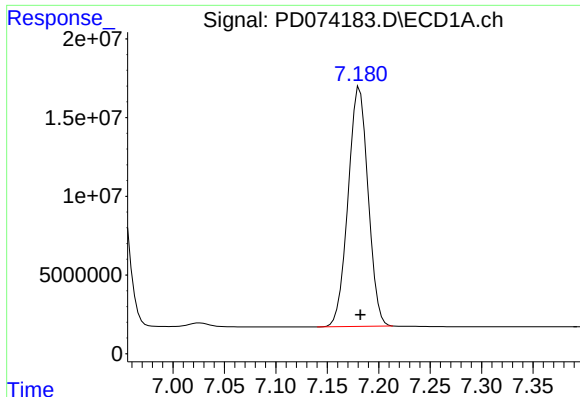


#19 Endosulfan Sulfate

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 205669995
Conc: 81.55 ng/ml

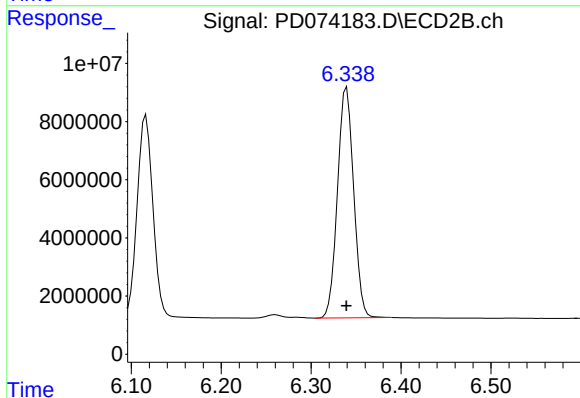


#19 Endosulfan Sulfate

R.T.: 6.340 min
Delta R.T.: 0.000 min
Response: 99102165
Conc: 79.97 ng/ml

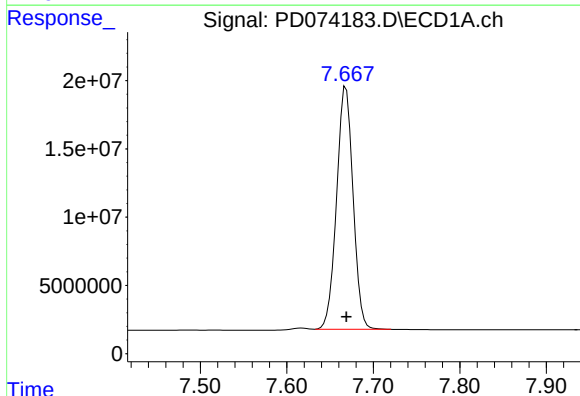


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 233970497
Conc: 81.63 ng/ml

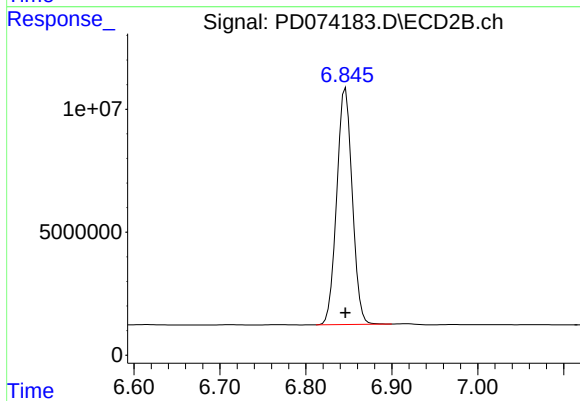

#21 Endrin ketone

R.T.: 6.846 min
Delta R.T.: 0.000 min
Response: 120173548
Conc: 79.66 ng/ml

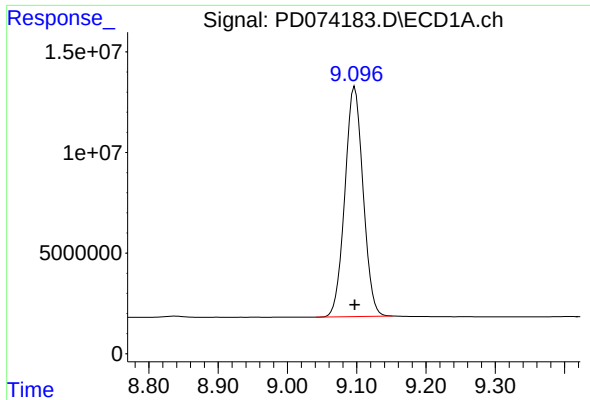


#27 Decachlorobiphenyl

R.T.: 9.097 min

Delta R.T.: 0.000 min

Response: 208697177

Conc: 76.43 ng/ml

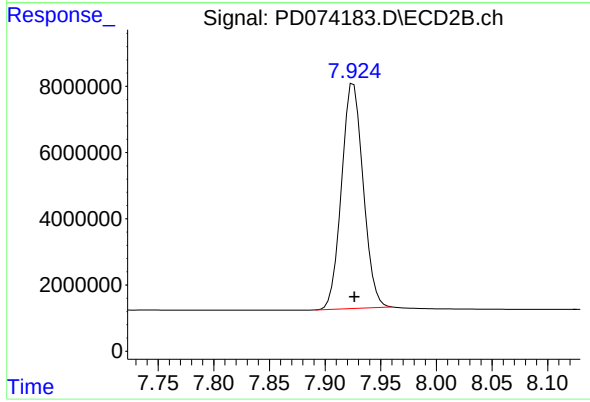

#27 Decachlorobiphenyl

R.T.: 7.926 min

Delta R.T.: 0.000 min

Response: 92150552

Conc: 76.39 ng/ml