

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 15:31
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:36:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 01:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	190.9E6	96933827	78.046	78.480
27)	SA Decachlor...	9.098	7.926	378.4E6	166.6E6	140.205	141.263
Target Compounds							
2)	A alpha-BHC	4.008	3.276	334.7E6	149.6E6	86.986	84.835
3)	MA gamma-BHC...	4.342	3.606	308.9E6	139.4E6	84.525	82.062
4)	MA Heptachlor	4.934	3.948	310.5E6	106.9E6	82.881	65.208
9)	A Endosulfan I	6.092	5.102	232.9E6	104.9E6	79.048	75.261
13)	MA Dieldrin	6.368	5.368	528.4E6	250.1E6	168.286	161.089
14)	MA Endrin	6.598	5.643	434.7E6	204.7E6	165.947	152.069
16)	A 4,4'-DDD	6.730	5.792	389.9E6	173.6E6	166.473	147.156
17)	MA 4,4'-DDT	7.046	6.043	413.1E6	191.4E6	166.942	153.414
20)	A Methoxychlor	7.521	6.620	1082.0E6	436.9E6	797.586	705.655


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 15:31
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:36:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 01:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

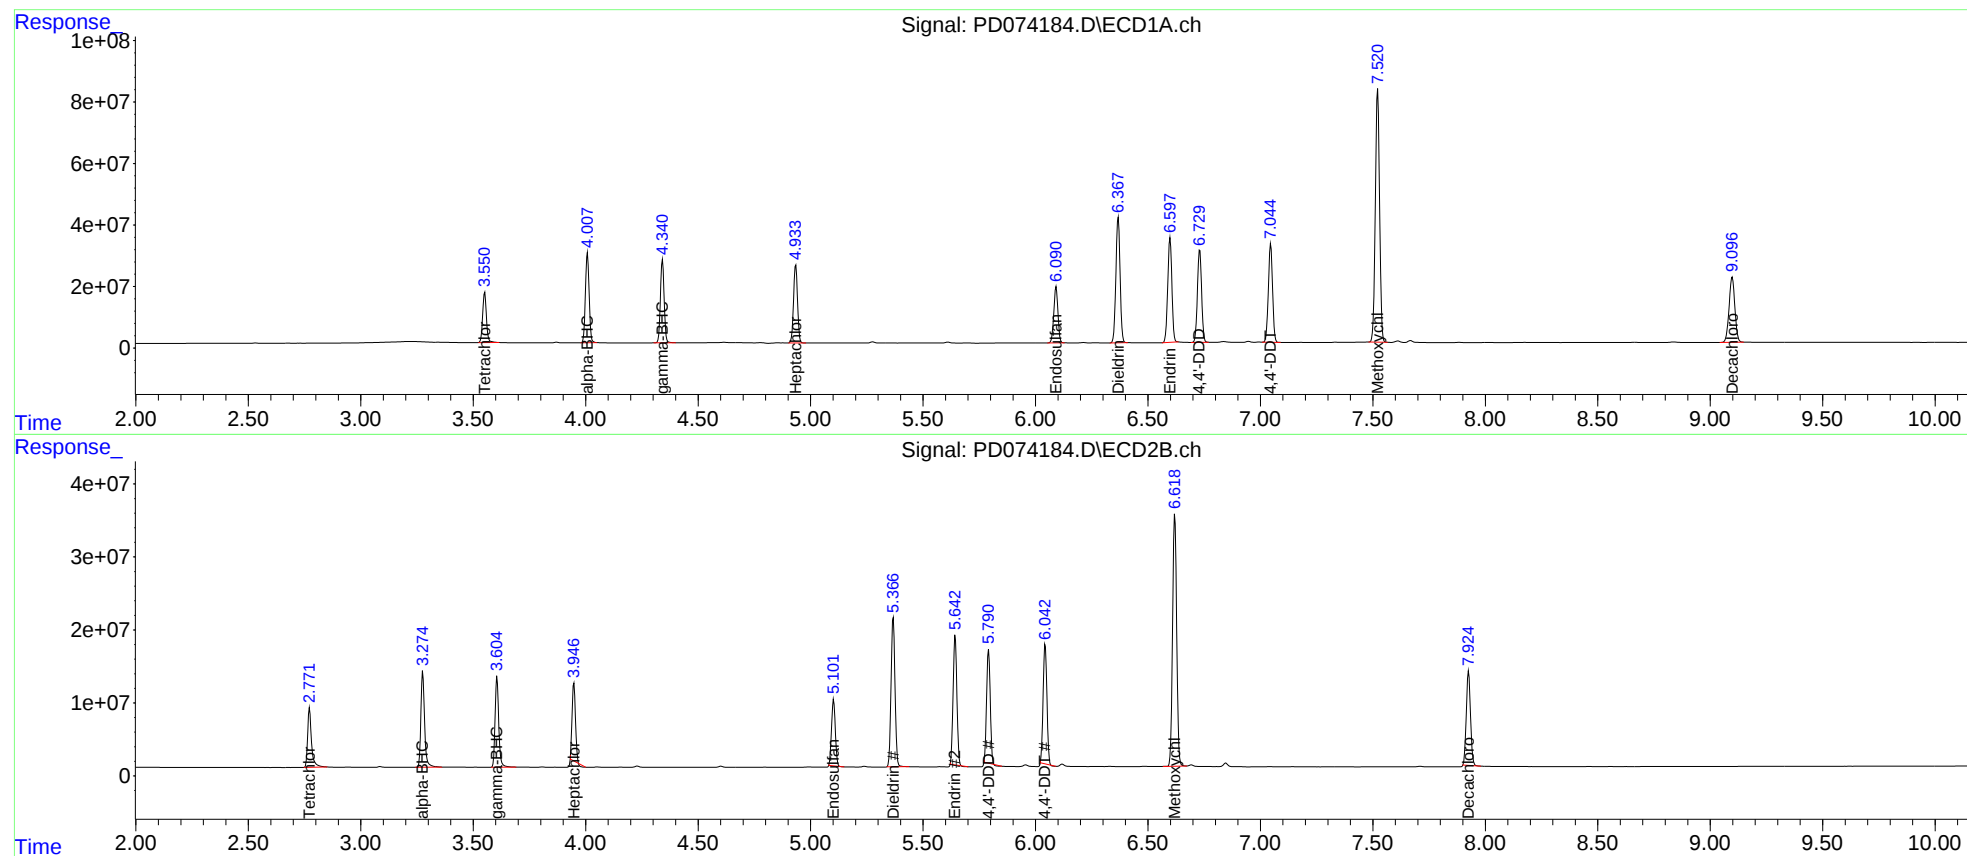

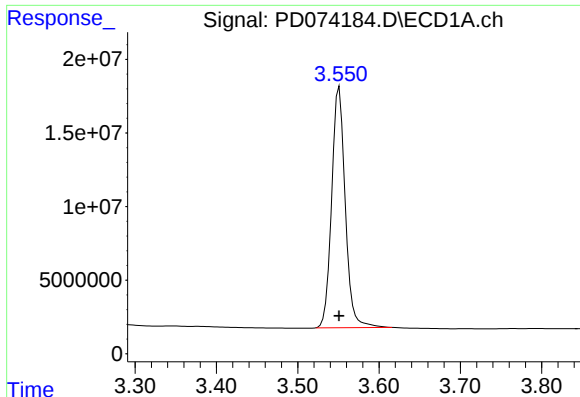


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 190852873
Conc: 78.05 ng/ml

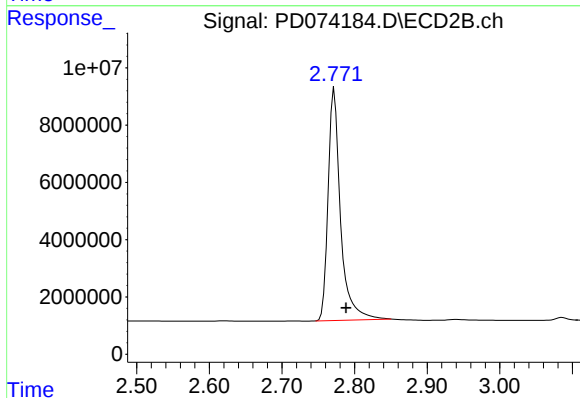


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.017 min
Response: 96933827
Conc: 78.48 ng/ml

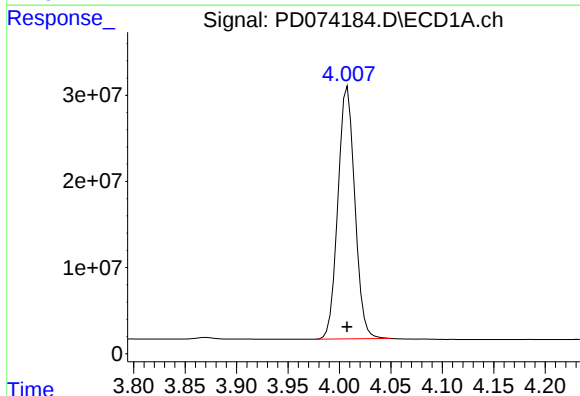


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 334669766
Conc: 86.99 ng/ml

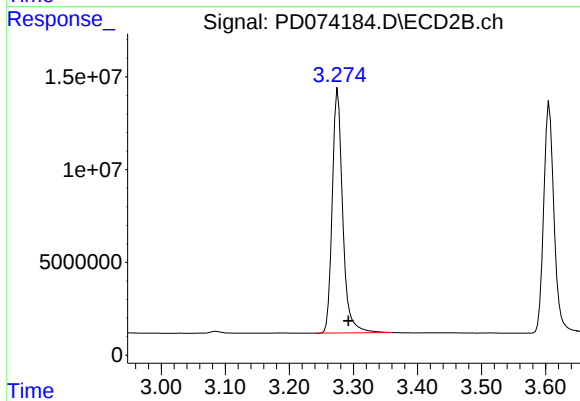


#2 alpha-BHC

R.T.: 3.276 min
Delta R.T.: -0.017 min
Response: 149594956
Conc: 84.83 ng/ml

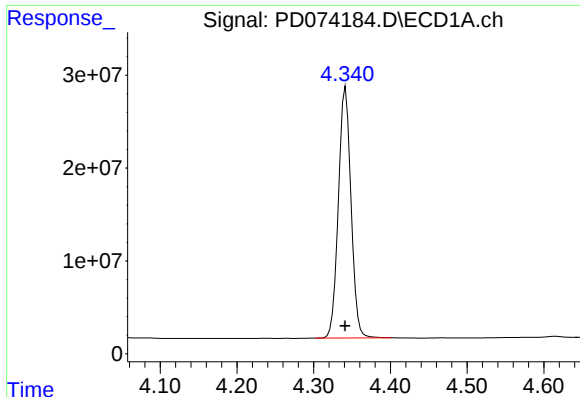


#3 gamma-BHC (Lindane)

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 308921850
Conc: 84.53 ng/ml

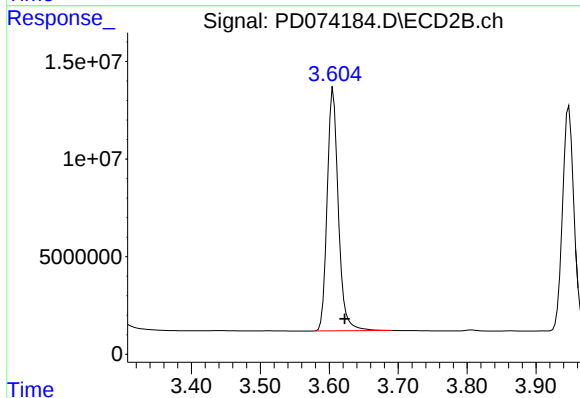


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: -0.016 min
Response: 139388340
Conc: 82.06 ng/ml

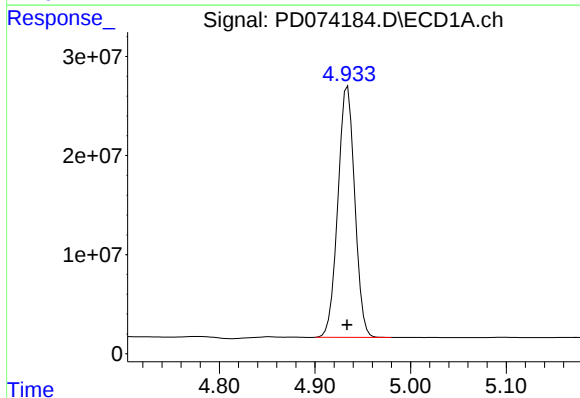


#4 Heptachlor

R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 310450312
Conc: 82.88 ng/ml

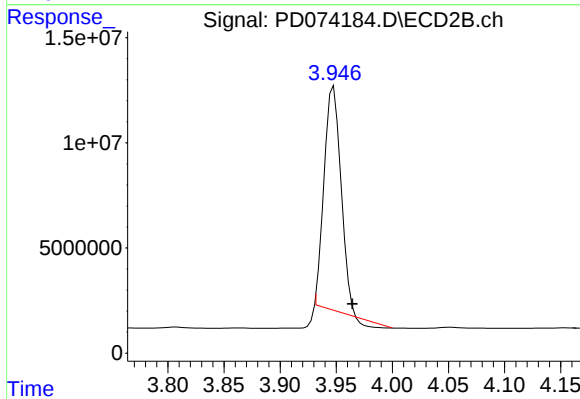


#4 Heptachlor

R.T.: 3.948 min
Delta R.T.: -0.017 min
Response: 106864869
Conc: 65.21 ng/ml

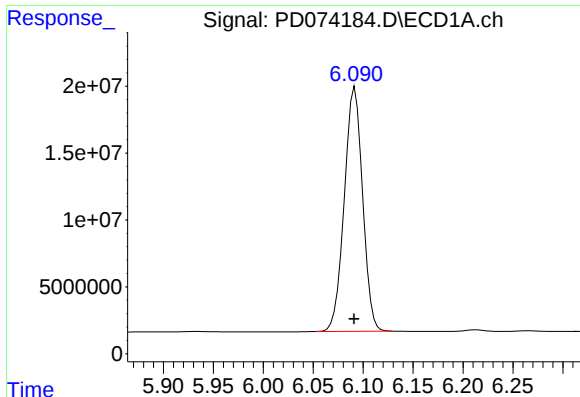


#9 Endosulfan I

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 232926878
Conc: 79.05 ng/ml

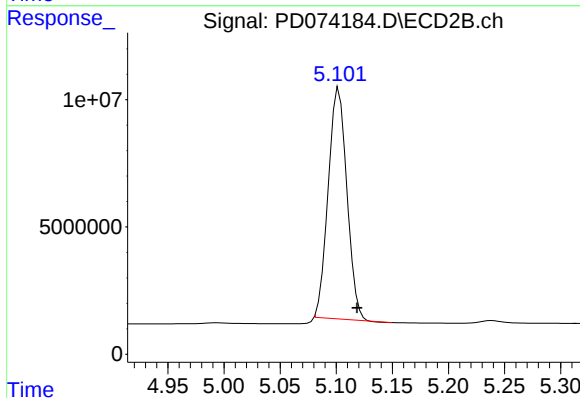


#9 Endosulfan I

R.T.: 5.102 min
Delta R.T.: -0.016 min
Response: 104905906
Conc: 75.26 ng/ml

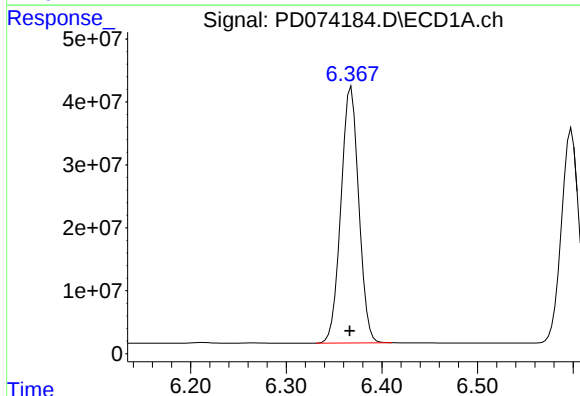


#13 Dieldrin

R.T.: 6.368 min
Delta R.T.: 0.001 min
Response: 528420827
Conc: 168.29 ng/ml

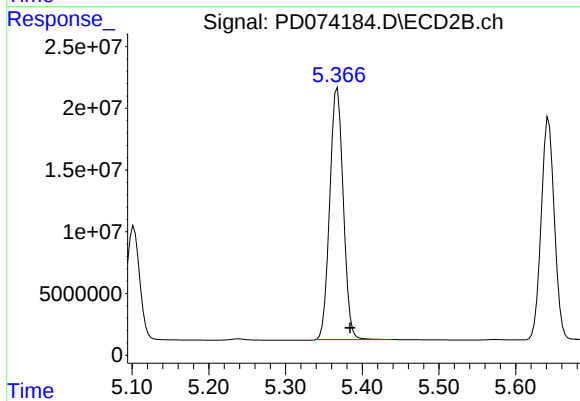


#13 Dieldrin

R.T.: 5.368 min
Delta R.T.: -0.016 min
Response: 250109213
Conc: 161.09 ng/ml

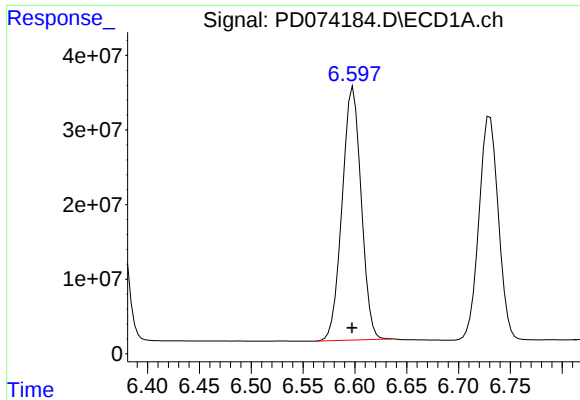


#14 Endrin

R.T.: 6.598 min
Delta R.T.: 0.001 min
Response: 434672679
Conc: 165.95 ng/ml

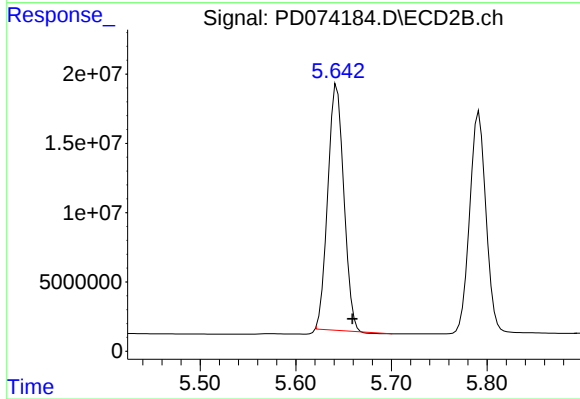


#14 Endrin

R.T.: 5.643 min
Delta R.T.: -0.016 min
Response: 204734464
Conc: 152.07 ng/ml

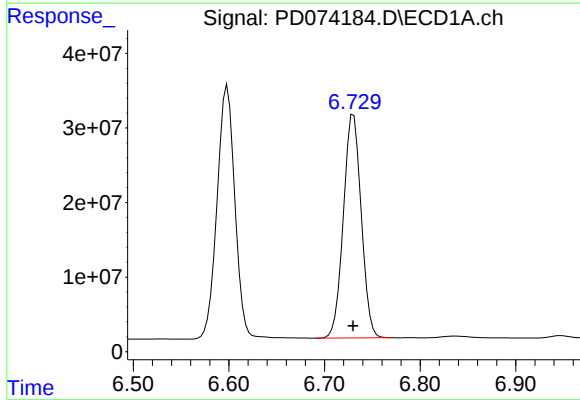


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 389869196
Conc: 166.47 ng/ml

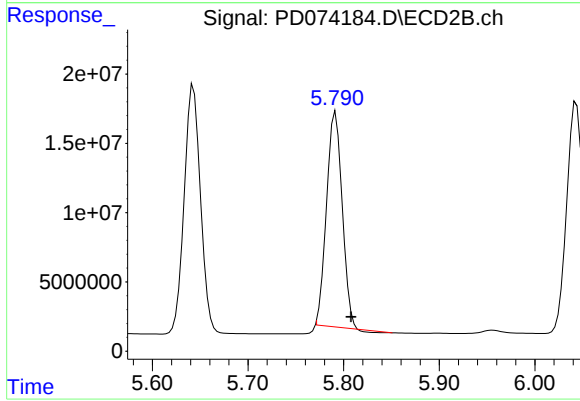


#16 4,4'-DDD

R.T.: 5.792 min
Delta R.T.: -0.016 min
Response: 173627539
Conc: 147.16 ng/ml

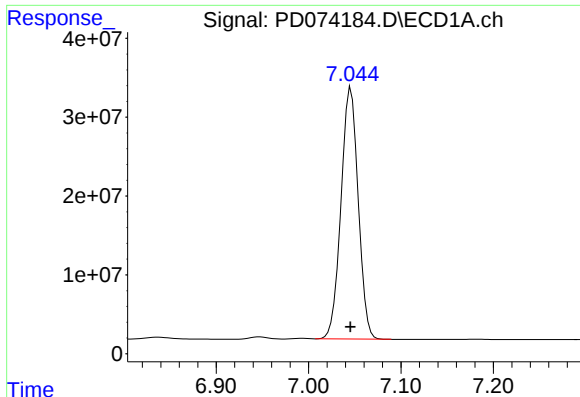


#17 4,4'-DDT

R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 413056069
Conc: 166.94 ng/ml

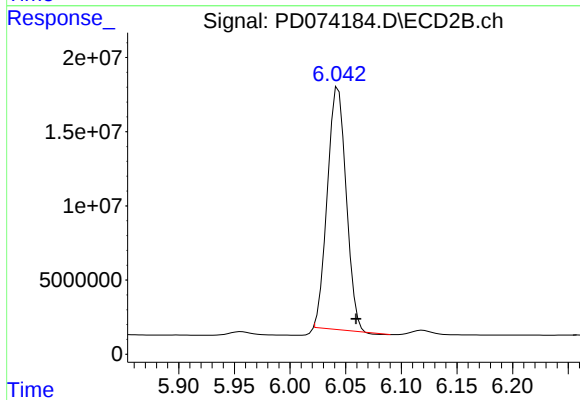


#17 4,4'-DDT

R.T.: 6.043 min
Delta R.T.: -0.016 min
Response: 191386179
Conc: 153.41 ng/ml

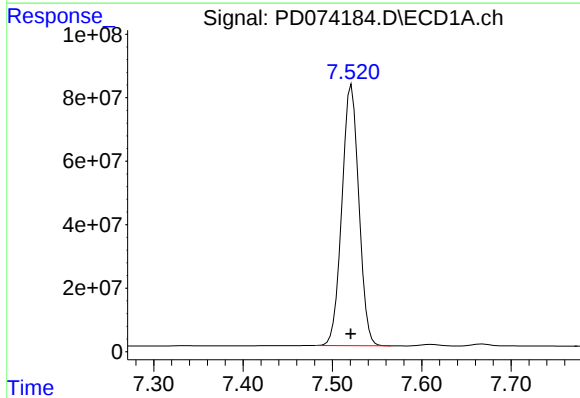


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 1081957855
Conc: 797.59 ng/ml

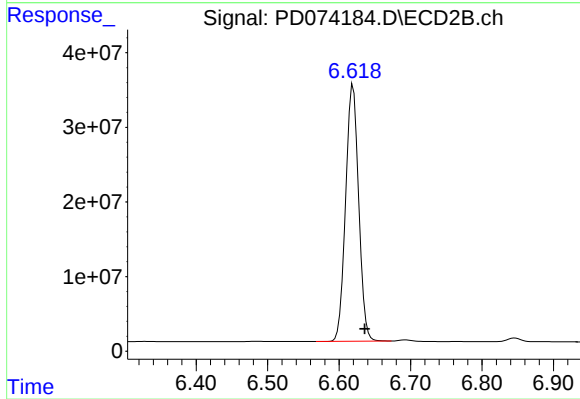


#20 Methoxychlor

R.T.: 6.620 min
Delta R.T.: -0.016 min
Response: 436929761
Conc: 705.66 ng/ml

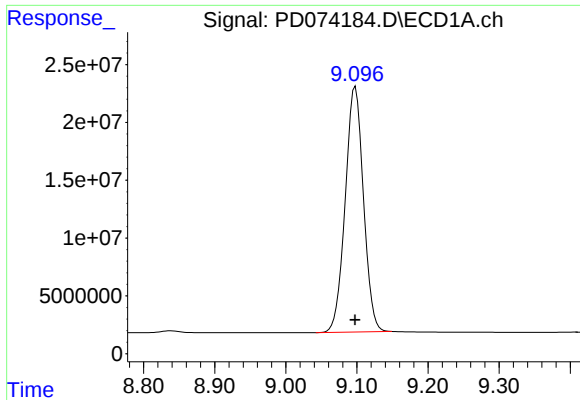

#27 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 378359640
Conc: 140.21 ng/ml

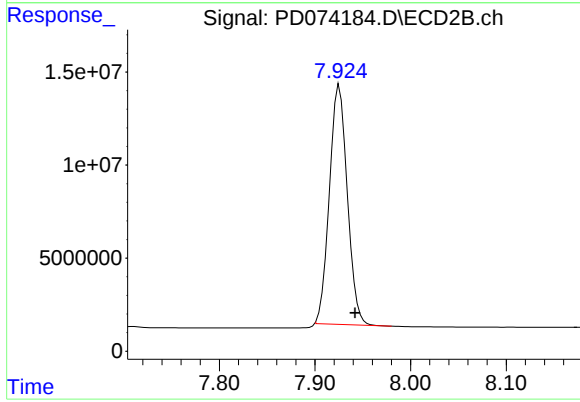

#27 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.016 min
Response: 166614712
Conc: 141.26 ng/ml