

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 12:09
 Operator : AR\AJ
 Sample : RESC353
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:35:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	48548064	25210024	19.541	20.038
27)	SA Decachlor...	9.098	7.926	109.7E6	48581565	40.092	40.573
Target Compounds							
2)	A alpha-BHC	4.007	3.275	36331298	17171300	9.311	9.609
3)	MA gamma-BHC...	4.341	3.605	34949396	16494584	9.468	9.657
4)	MA Heptachlor	4.934	3.948	36418760	16374611	9.620	9.876
5)	MB Aldrin	5.277	4.228	36330119	17405436	9.941	10.166
6)	B beta-BHC	4.535	3.901	17715079	8515162	10.479	10.510
7)	B delta-BHC	4.784	4.132	37160963	17234151	10.212	9.744
8)	B Heptachlo...	5.704	4.731	33113127	16001960	10.086	10.101
9)	A Endosulfan I	6.091	5.102	29662274	14281666	9.943	10.185
10)	B trans-Chl...	5.960	4.982	31944167	15760341	9.957	10.188
11)	B cis-Chlor...	6.041	5.046	33050274	16134324	10.086	10.200
12)	B 4,4'-DDE	6.212	5.237	58173676	28771642	19.421	19.808
13)	MA Dieldrin	6.367	5.367	60526713	30309037	19.079	19.550
14)	MA Endrin	6.597	5.643	50673766	26507023	19.229	19.704
15)	B Endosulfa...	6.816	5.937	55463180	27432567	20.094	20.404
16)	A 4,4'-DDD	6.730	5.791	45153063	22858210	19.106	19.414
17)	MA 4,4'-DDT	7.046	6.043	49067002	24482117	19.553	19.542
18)	B Endrin al...	6.946	6.116	46248359	23086338	20.533	21.001
19)	B Endosulfa...	7.181	6.339	52787383	25510704	20.267	20.266
20)	A Methoxychlor	7.521	6.620	136.3E6	62584448	99.295	101.750
21)	B Endrin ke...	7.668	6.846	60821045	31791060	20.514	20.893

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

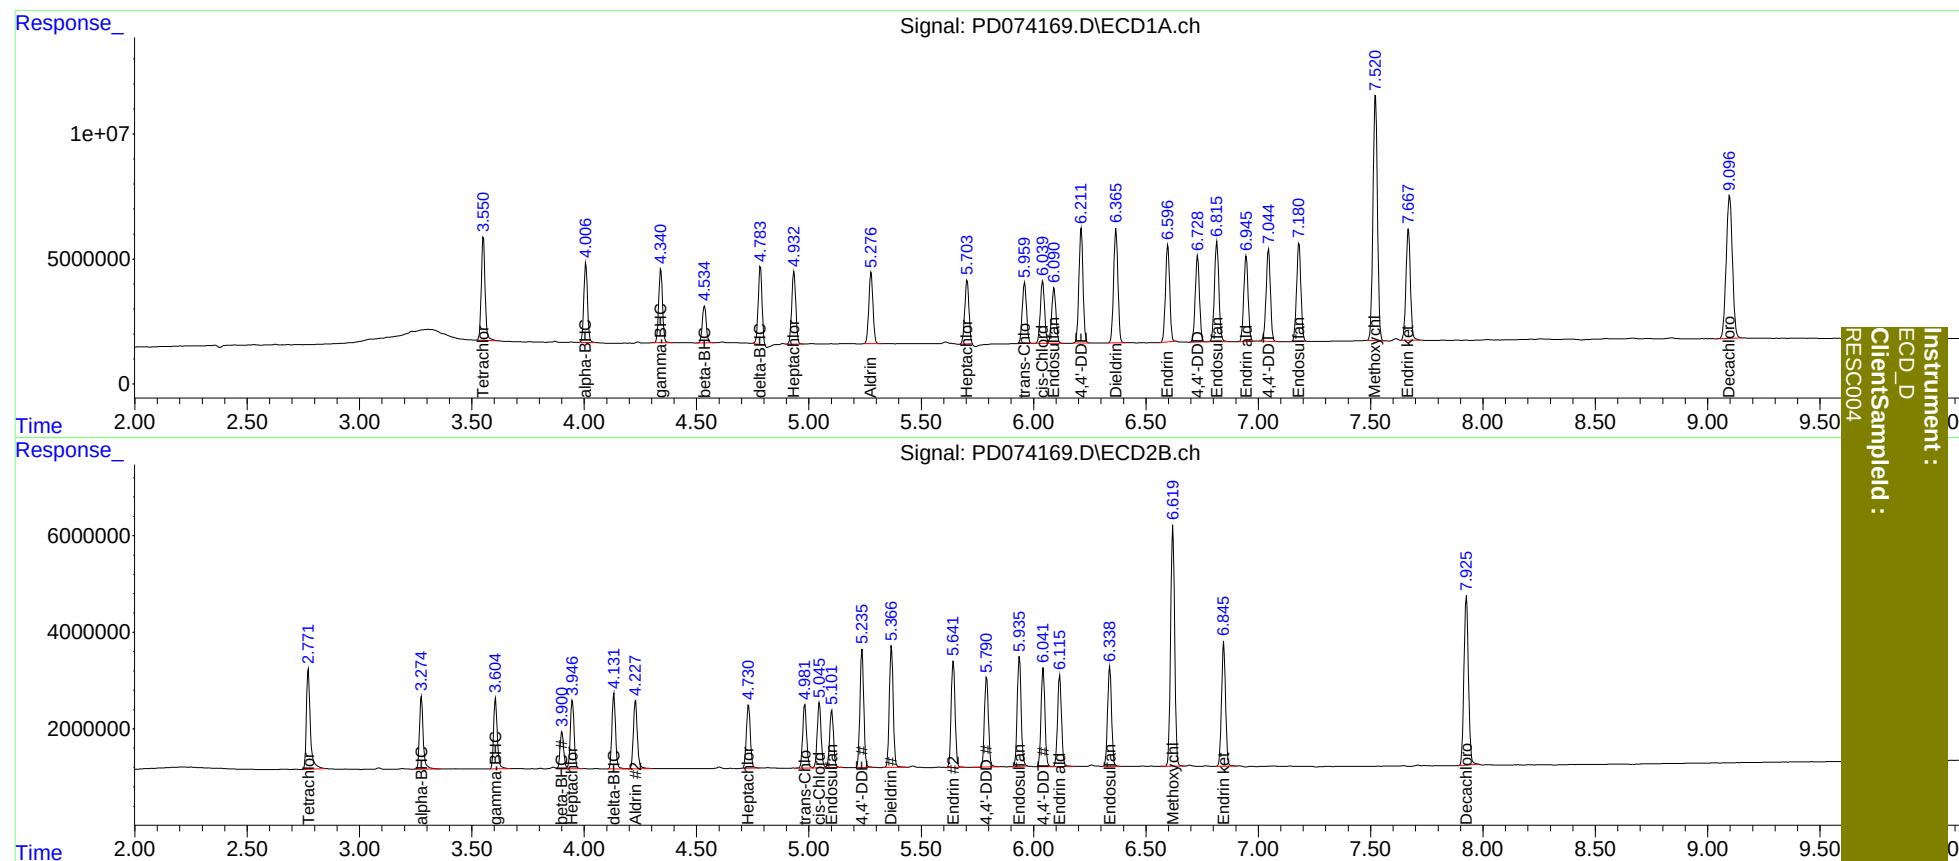

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Title : GC Extractables
Last Update : Tue Mar 14 03:05:06 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.551	4.007	100.00%
4.007	4.341	100.00%
4.341	4.535	100.00%
4.535	4.784	100.00%
4.784	4.934	100.00%
4.934	5.277	100.00%
5.277	5.704	100.00%
5.704	5.960	100.00%
5.960	6.041	100.00%
6.041	6.091	96.75%
6.091	6.212	100.00%
6.212	6.367	100.00%
6.367	6.597	100.00%
6.597	6.730	100.00%
6.730	6.816	100.00%
6.816	6.946	100.00%
6.946	7.046	100.00%
7.046	7.181	100.00%
7.181	7.521	100.00%
7.521	7.668	100.00%
7.668	9.098	100.00%

Signal #2


2.772	3.275	100.00%
3.275	3.605	100.00%
3.605	3.901	100.00%
3.901	3.948	95.28%
3.948	4.132	100.00%
4.132	4.228	99.82%
4.228	4.731	100.00%
4.731	4.982	100.00%
4.982	5.046	99.52%
5.046	5.102	99.25%
5.102	5.237	100.00%
5.237	5.367	100.00%
5.367	5.643	100.00%
5.643	5.791	100.00%
5.791	5.937	100.00%
5.937	6.043	100.00%
6.043	6.116	100.00%
6.116	6.339	100.00%
6.339	6.620	100.00%
6.620	6.846	100.00%
6.846	7.926	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

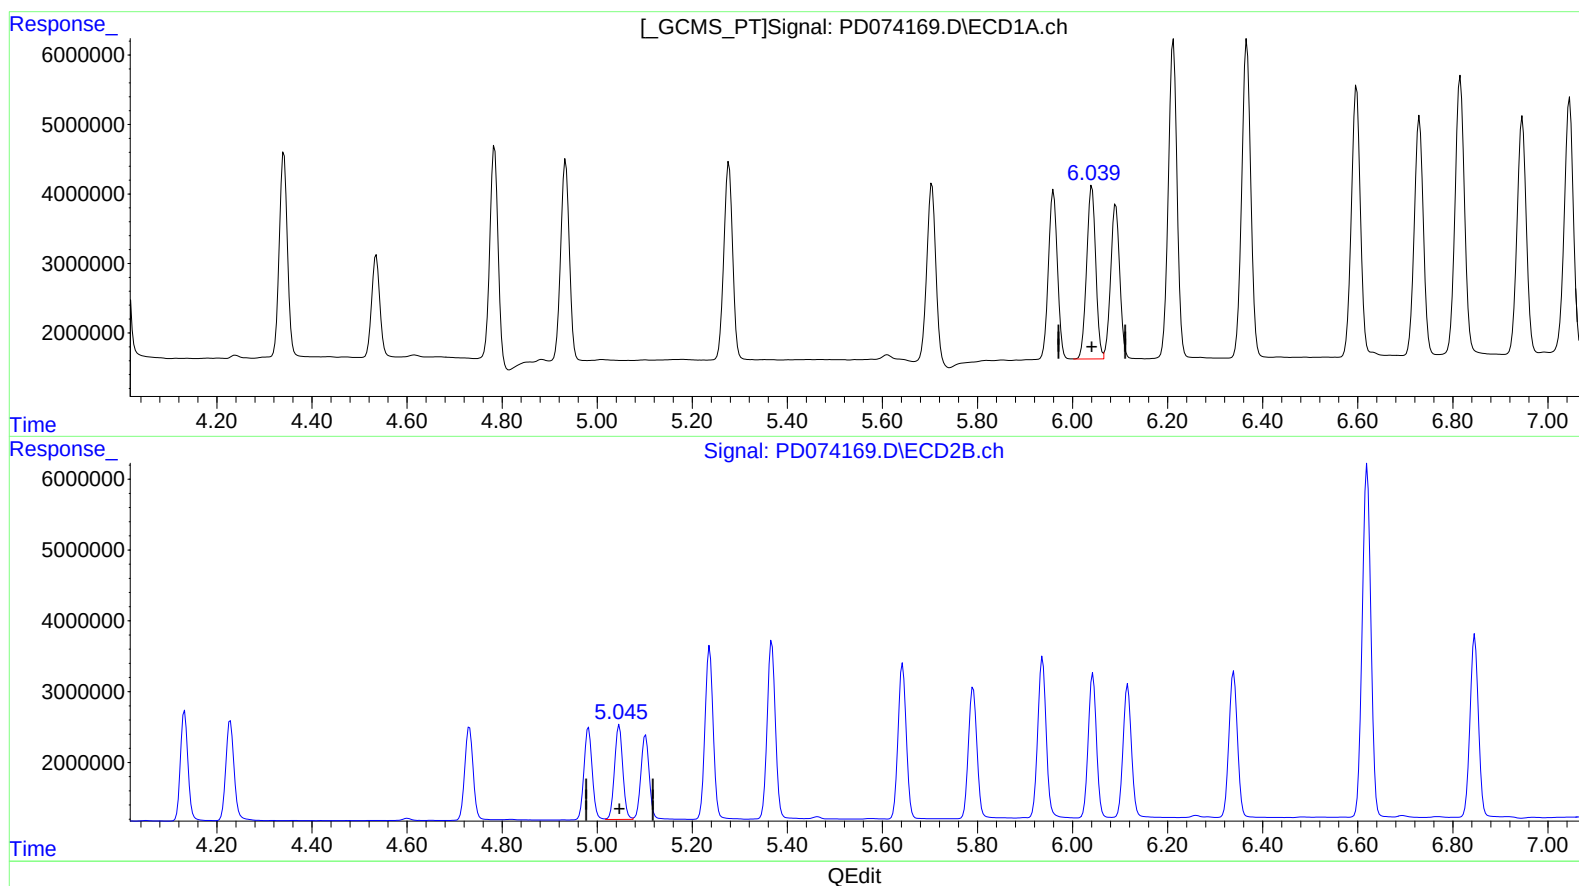

(11) cis-Chlordane (B)

6.041min 10.086 ng/ml

response 33050274

(11) cis-Chlordane #2 (B)

5.046min 10.200 ng/ml


response 16134324

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

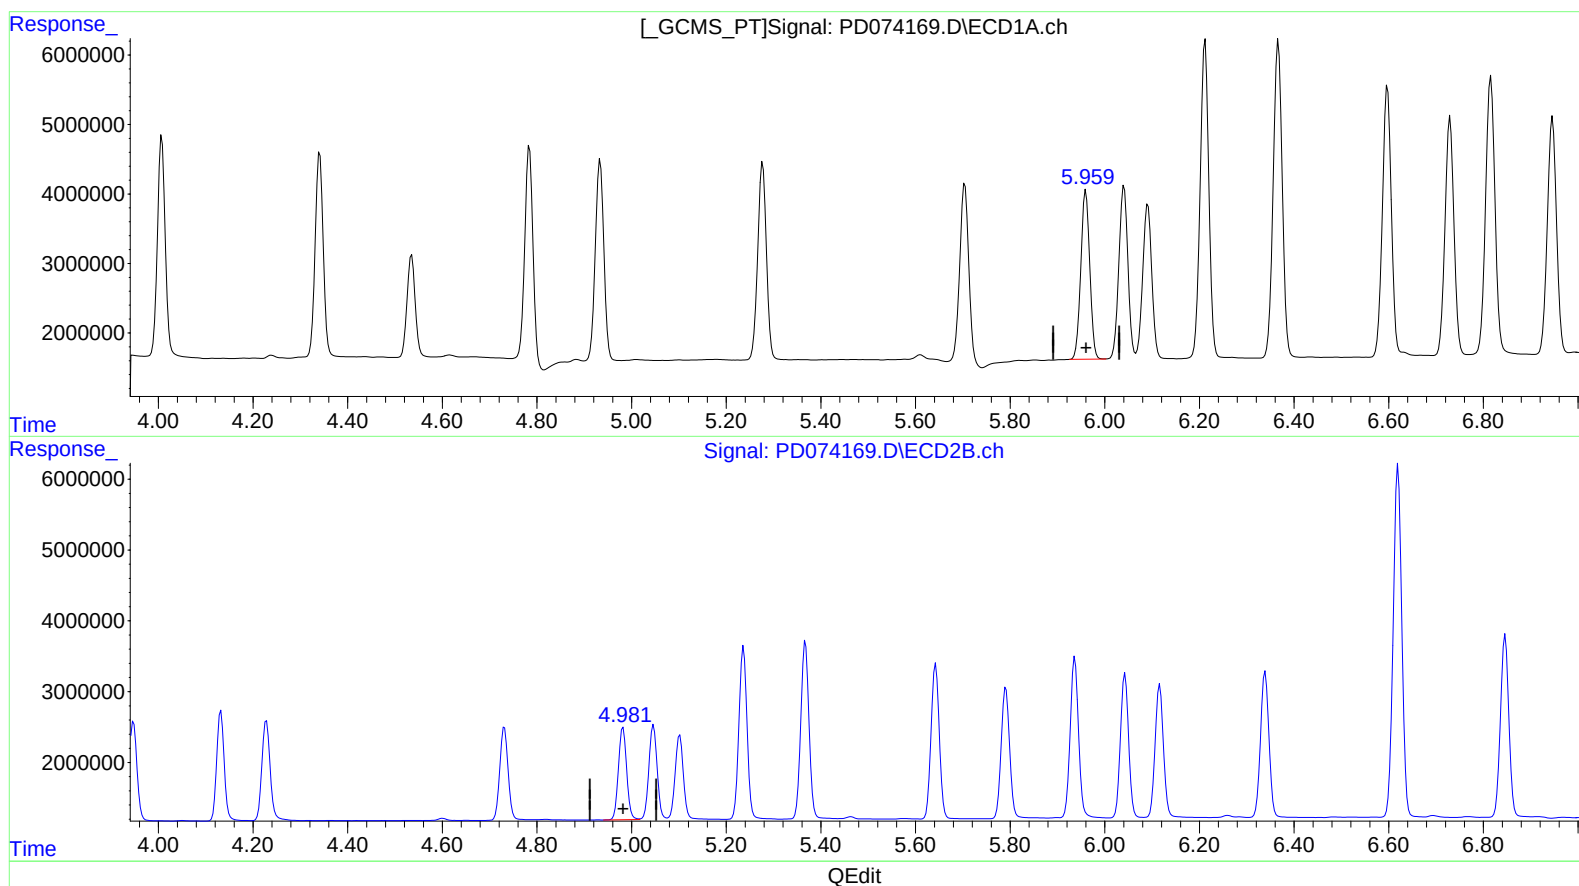

(10) trans-Chlordane (B)

5.960min 9.957 ng/ml

response 31944167

(10) trans-Chlordane #2 (B)

4.982min 10.188 ng/ml


response 15760341

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

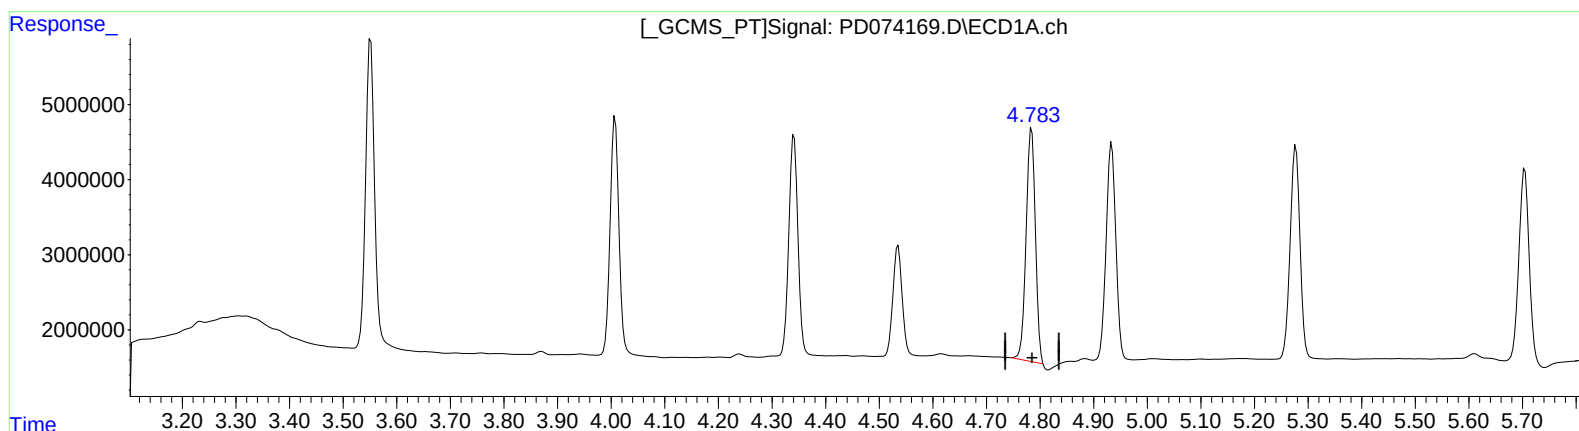

(7) delta-BHC (B)

4.784min 10.212 ng/ml

response 37160963

(7) delta-BHC #2 (B)

4.132min 9.744 ng/ml


response 17234151

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

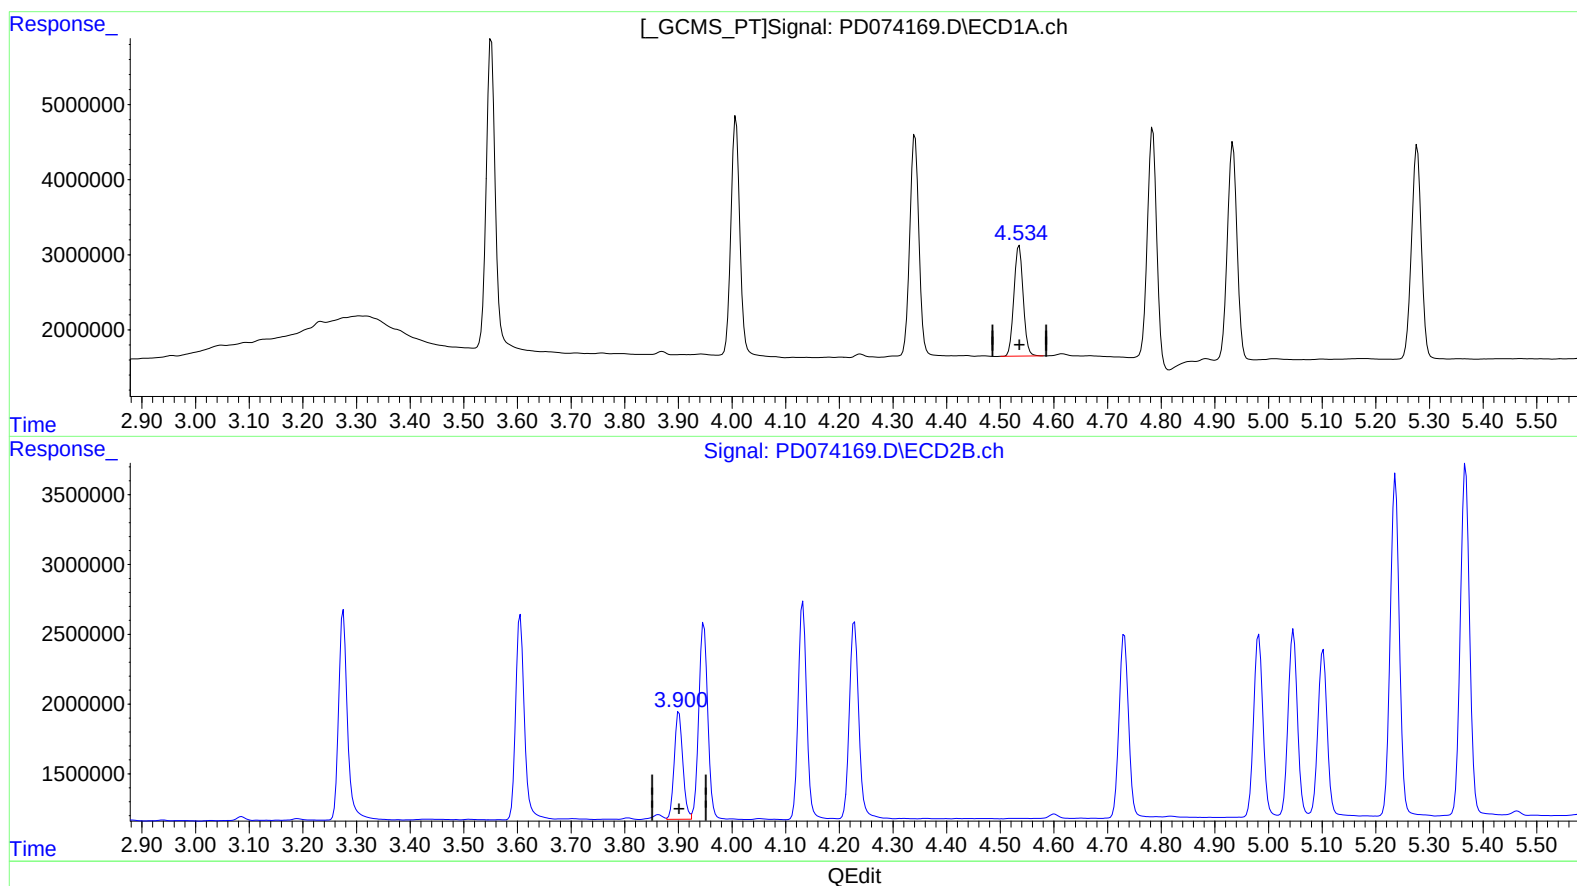

(6) beta-BHC (B)

4.535min 10.479 ng/ml

response 17715079

(6) beta-BHC #2 (B)

3.901min 10.510 ng/ml


response 8515162

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 12:09
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

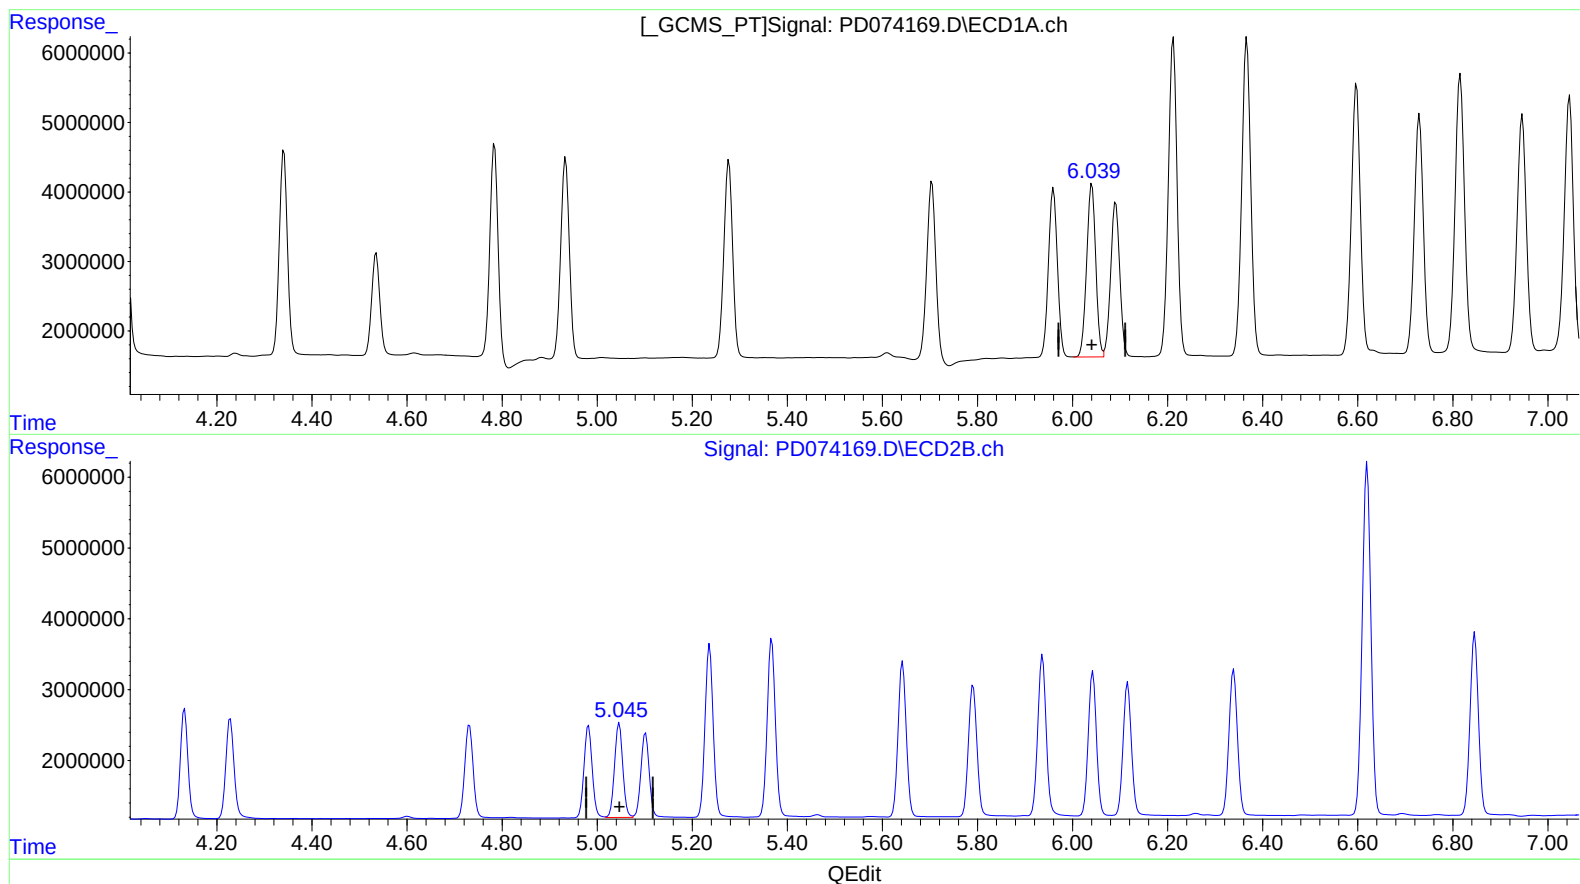

(11) cis-Chlordane (B)

6.041min 10.086 ng/ml

response 33050274

(11) cis-Chlordane #2 (B)

5.046min 10.200 ng/ml

response 16134324