

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
 Data File : PD074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 15:04
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4031

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/14/2023
 Supervised By :Ankita Jodhani 03/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 02:30:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 02:30:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.772	96772047	49774772	38.569	39.202
2) SA Decachlor...	9.097	7.924	199.7E6	89527589	70.553	72.389m
Target Compounds						
2) A alpha-BHC	4.008	3.276	161.6E6	73353481	42.181	41.528
3) MA gamma-BHC...	4.341	3.606	150.8E6	69028424	41.336	40.619
4) MA Heptachlor	4.934	3.946	152.7E6	66086854	40.588	39.787m
9) A Endosulfan I	6.091	5.101	116.6E6	55612675	38.848	39.878m
13) MA Dieldrin	6.367	5.368	257.1E6	125.1E6	81.898	80.881
14) MA Endrin	6.598	5.641	212.8E6	107.4E6	81.380	79.665m
16) A 4,4'-DDD	6.730	5.790	190.4E6	94938063	81.213	80.751m
17) MA 4,4'-DDT	7.046	6.042	201.3E6	101.0E6	80.784	80.967m
20) A Methoxychlor	7.521	6.619	538.0E6	234.4E6	390.446	370.638

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031323\
Data File : PD074182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 15:04
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 02:30:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 02:30:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

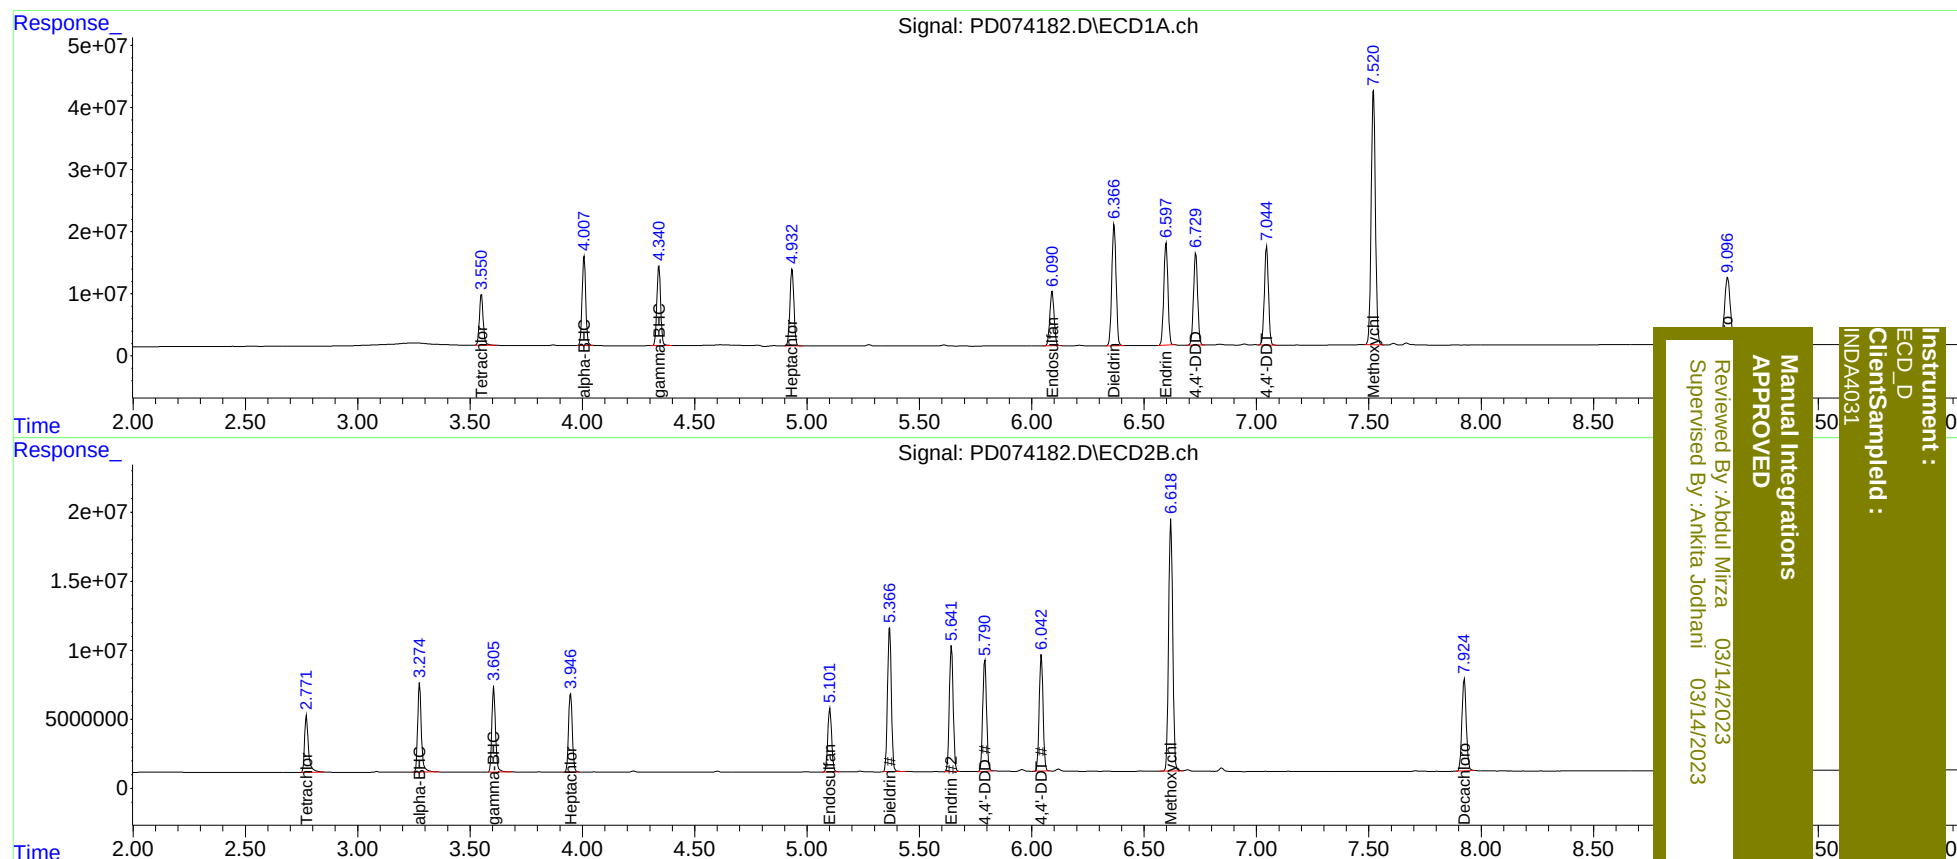

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/14/2023
Supervised By: Ankita Jodhani 03/14/2023

Instrument :
ECD_D
Client Sampled :
INDA4031