

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

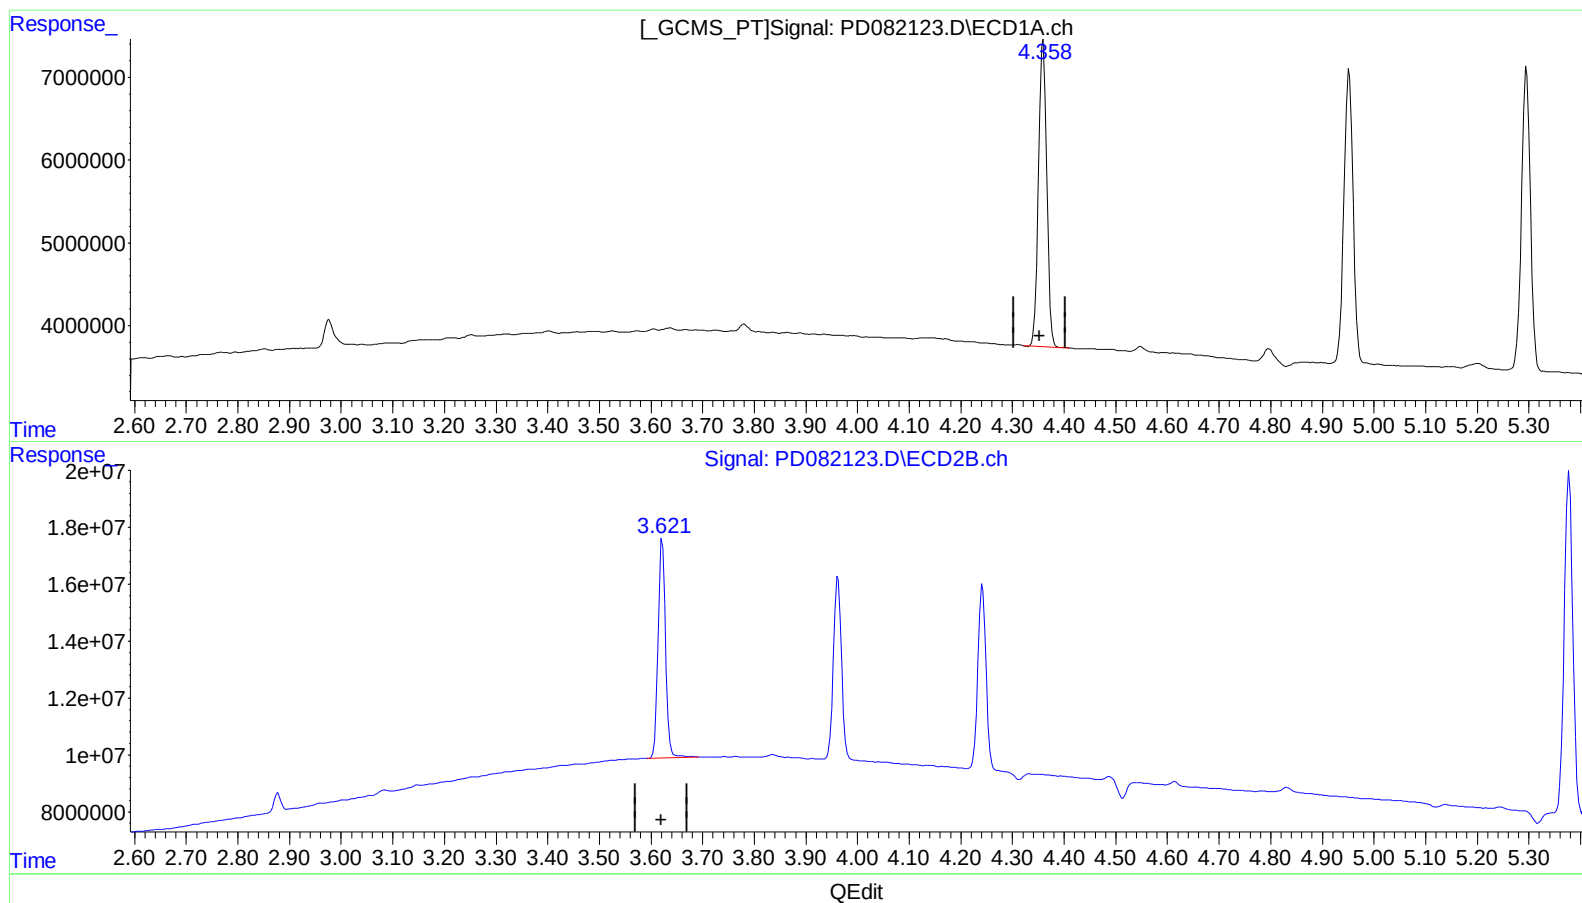

(3) gamma-BHC (Lindane) (MA)

4.360min 17.658 ng/ml

response 40908443

(3) gamma-BHC (Lindane) #2 (MA)

3.622min 20.654 ng/ml

response 77763624

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

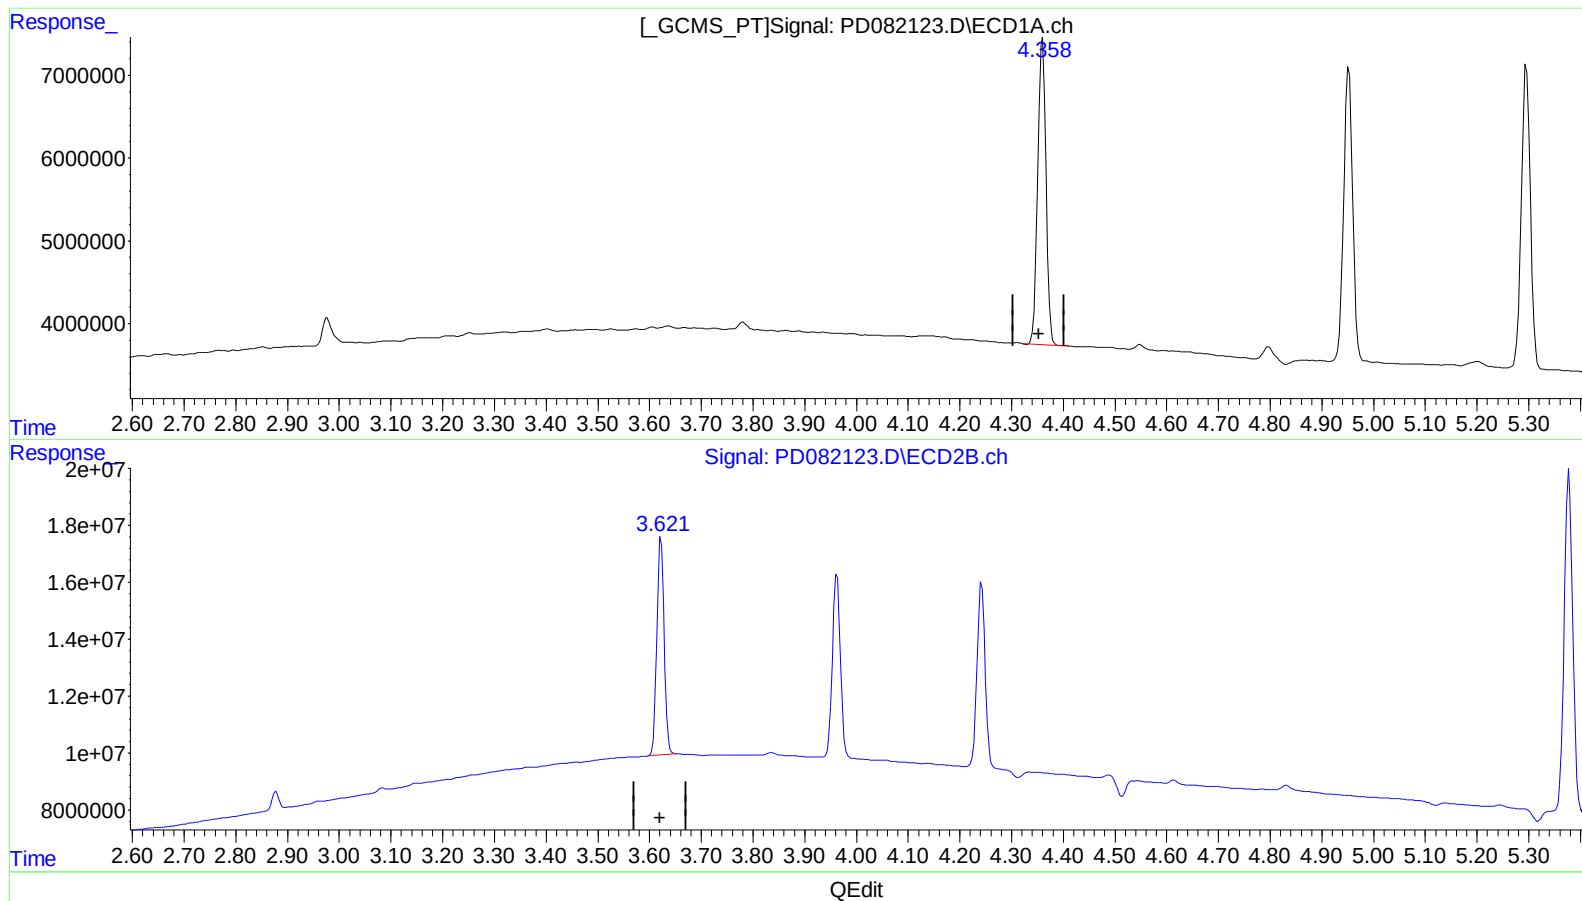

(3) gamma-BHC (Lindane) (MA)

4.360min 17.658 ng/ml

response 40908443

(3) gamma-BHC (Lindane) #2 (MA)

3.621min 20.150 ng/ml m

response 75865235

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

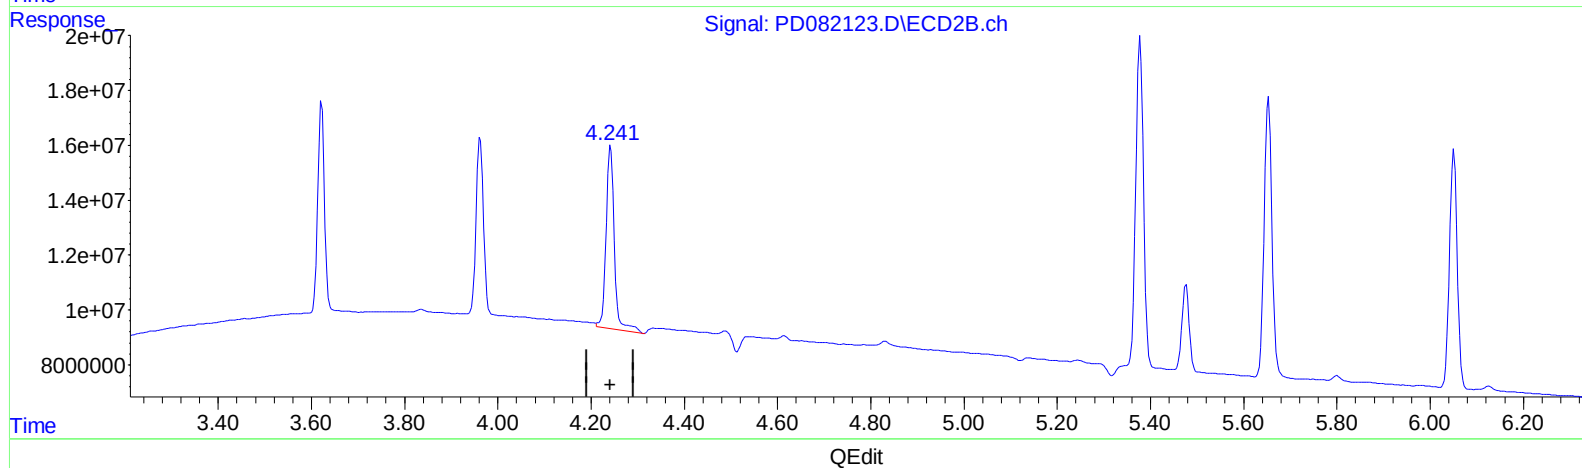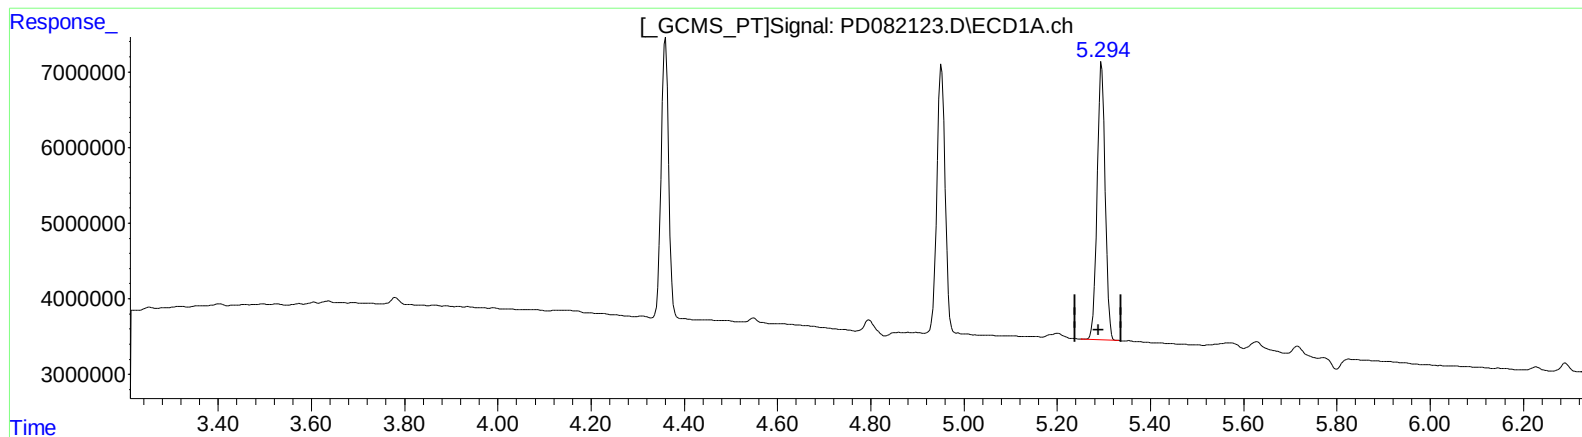

(5) Aldrin (MB)
5.296min 19.676 ng/ml
response 44184086

(5) Aldrin #2 (MB)
4.242min 23.993 ng/ml
response 81377271

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

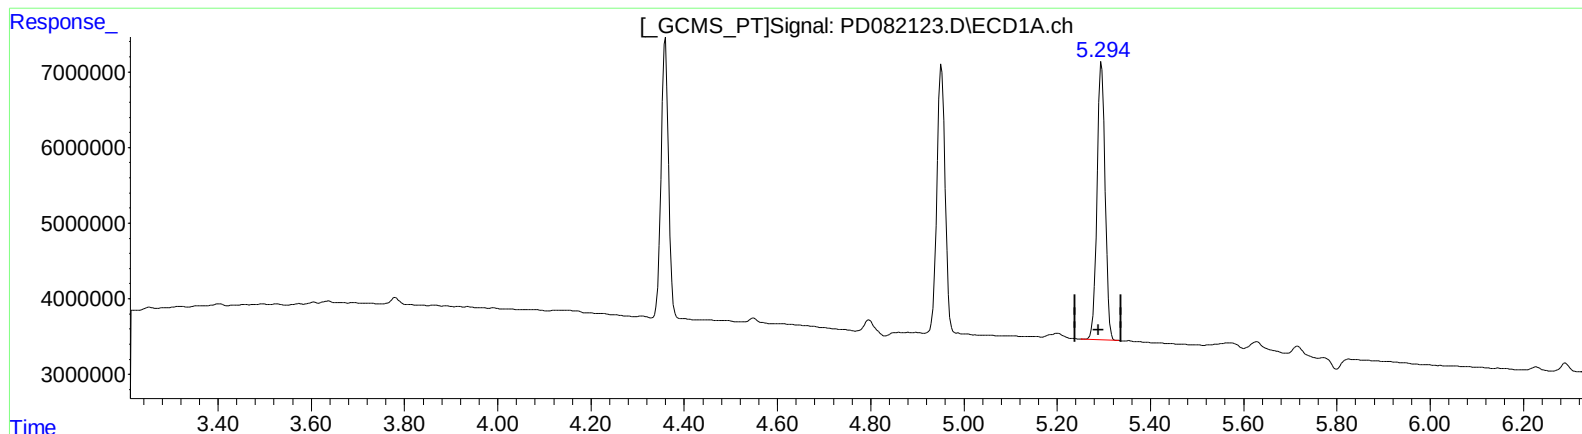

(5) Aldrin (MB)

5.296min 19.676 ng/ml

response 44184086

(5) Aldrin #2 (MB)

4.241min 21.156 ng/ml m

response 71754906

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

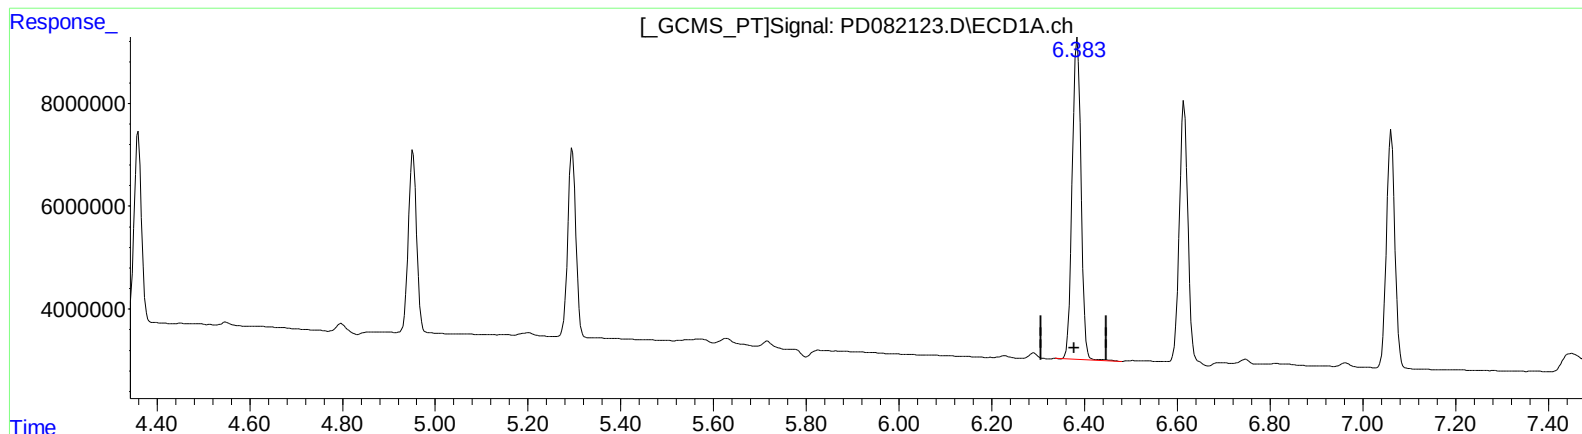

(13) Dieldrin (MA)
6.384min 37.796 ng/ml
response 82216314

(13) Dieldrin #2 (MA)
5.378min 41.692 ng/ml
response 137247512

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

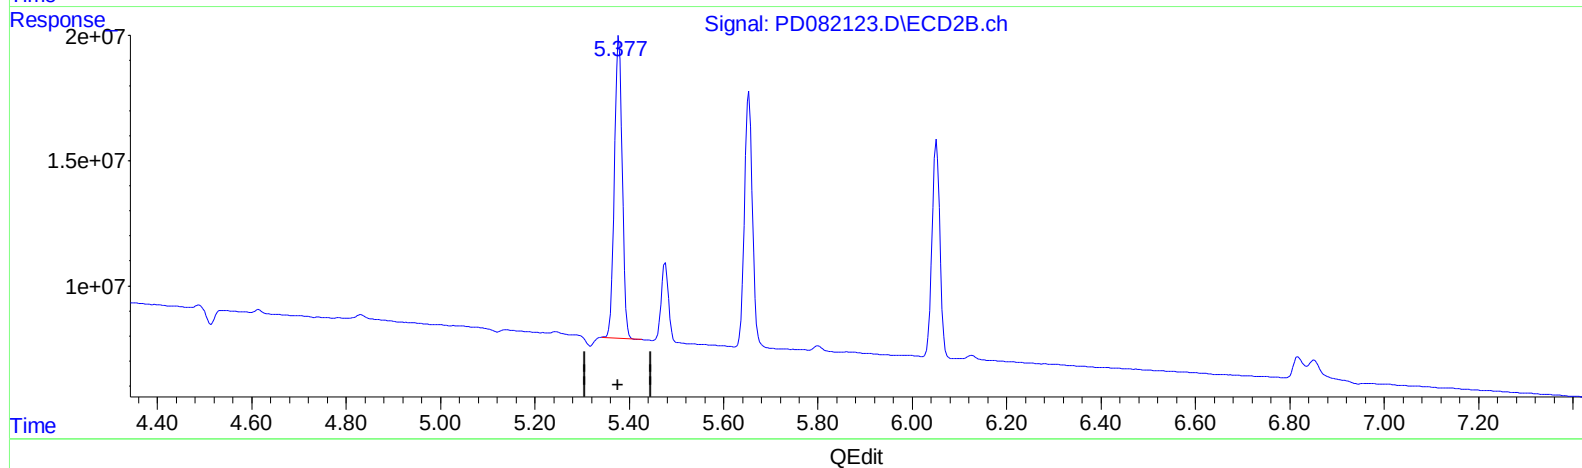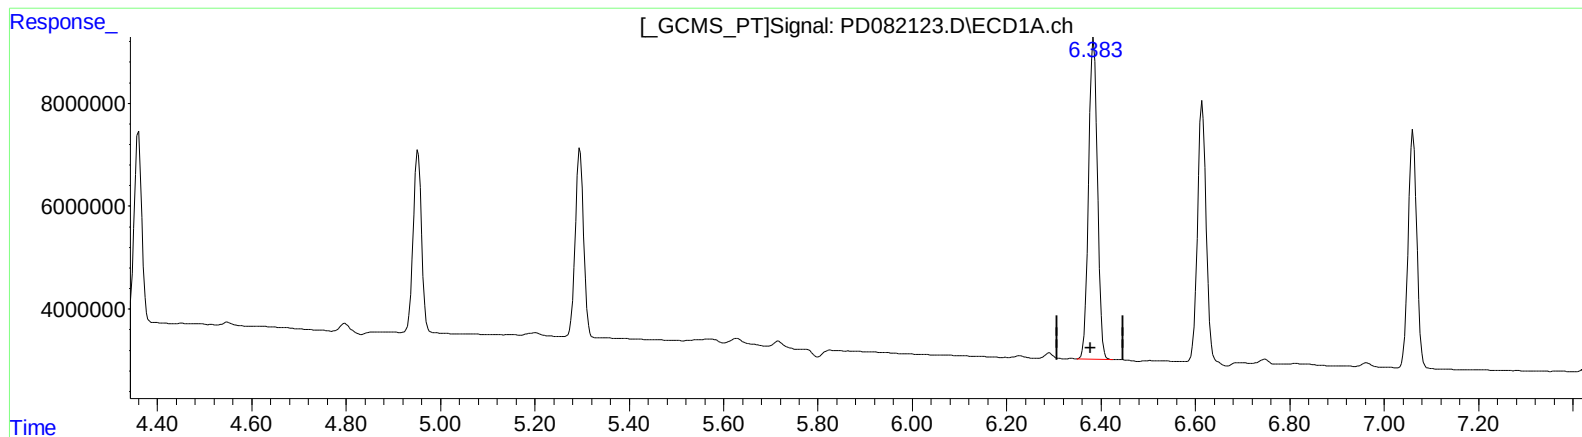

(13) Dieldrin (MA)
6.383min 37.453 ng/ml m
response 81469011

(13) Dieldrin #2 (MA)
5.378min 41.692 ng/ml
response 137247512

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
 Data File : PD082123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2024 13:20
 Operator : AR\AJ
 Sample : P1717-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
 Supervised By :Ankita Jodhani 03/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:19:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 09 04:31:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA gamma-BHC...	4.360	3.621	40908443	75865235	17.658	20.150m
4) MA Heptachlor	4.952	3.962	43352259	70661844	17.882	19.939
5) MB Aldrin	5.296	4.241	44184086	71754906	19.676	21.156m
13) MA Dieldrin	6.383	5.378	81469011	137.2E6	37.453m	41.692
14) MA Endrin	6.615	5.654	65222326	118.6E6	36.211	42.190
17) MA 4,4'-DDT	7.061	6.051	57964851	100.3E6	34.671	39.946

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031324\
Data File : PD082123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2024 13:20
Operator : AR\AJ
Sample : P1717-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
PEST-GPC2-BLANK-SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:19:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:31:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/13/2024
Supervised By :Ankita Jodhani 03/13/2024

