

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031325\
 Data File : PD087960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 15:25
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 05:55:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031325.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 18 05:48:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.884	35364148	278.3E6	19.528	20.466
28)	SA Decachlor...	9.080	8.080	61649897	322.2E6	20.652	20.620
Target Compounds							
9)	A Endosulfan I	6.079	5.253	28350542	169.7E6	8.972	10.164
10)	B gamma-Chl...	5.950	5.132	31960215	198.1E6	9.536	10.553
12)	B 4,4'-DDE	6.200	5.382	57360059	368.7E6	18.907	20.546
13)	MA Dieldrin	6.352	5.519	61908248	370.4E6	18.520	20.224
19)	B Endosulfa...	7.153	6.488	51712262	324.7E6	19.299	20.420
20)	A Methoxychlor	7.497	6.761	132.3E6	713.5E6	93.875	86.325
21)	B Endrin ke...	7.634	6.998	54976344	348.3E6	19.147	20.467



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031325\
Data File : PD087960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 15:25
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 05:55:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031325.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 05:48:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

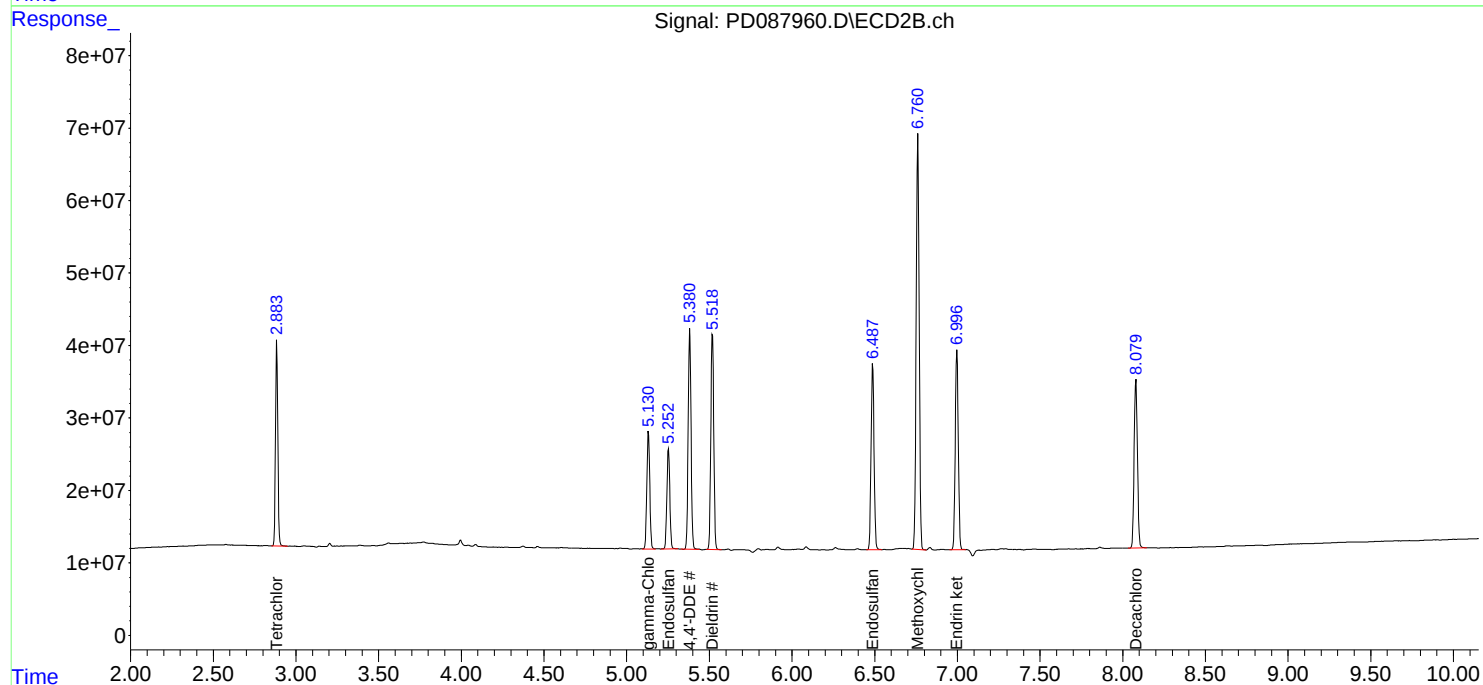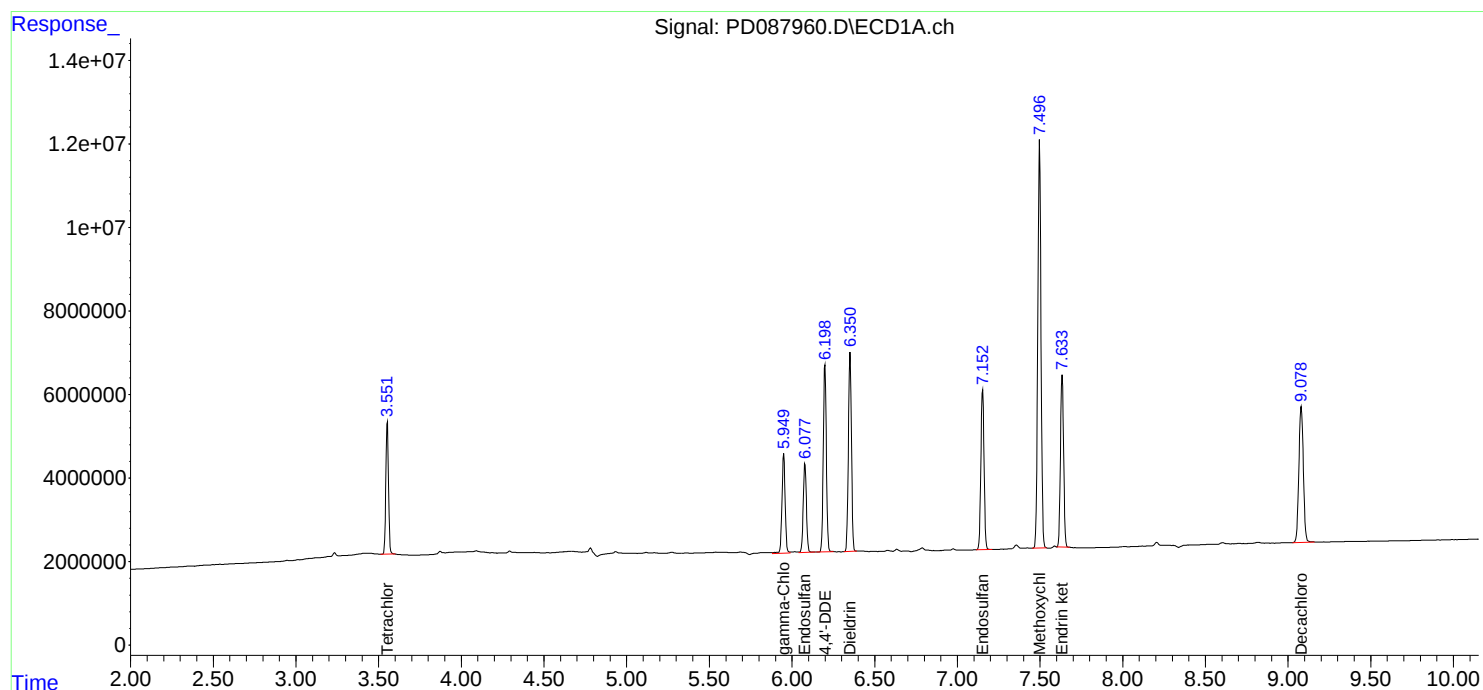


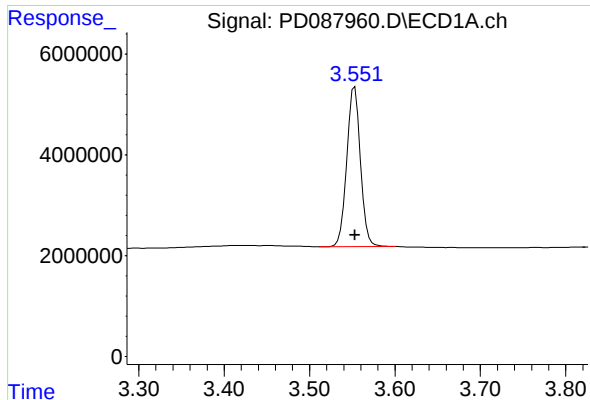

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 35364148
Conc: 19.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

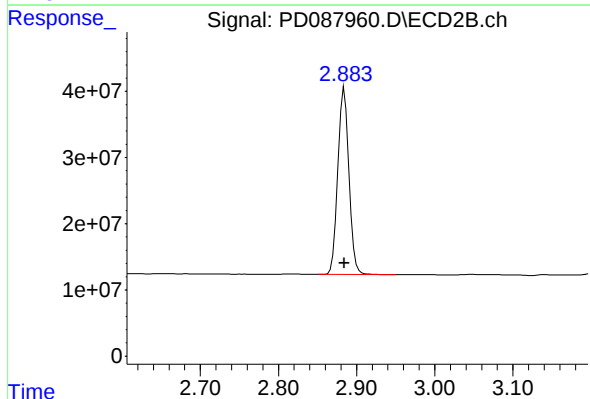


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 278312507
Conc: 20.47 ng/ml

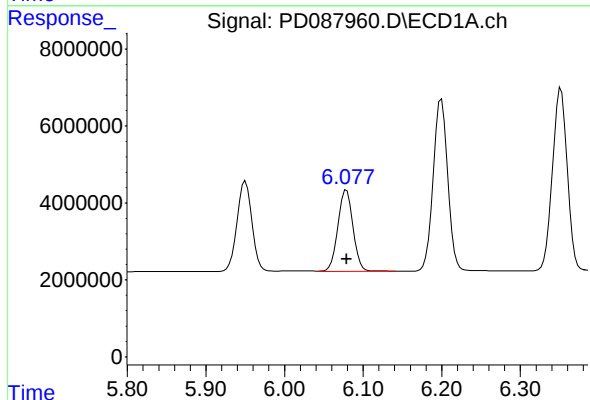


#9 Endosulfan I

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 28350542
Conc: 8.97 ng/ml

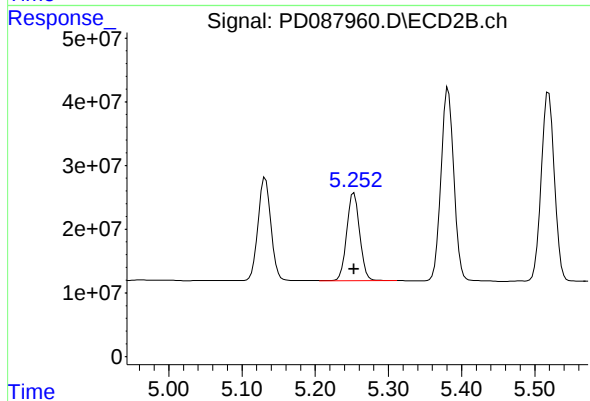

#9 Endosulfan I


R.T.: 5.253 min
Delta R.T.: 0.000 min
Response: 169712329
Conc: 10.16 ng/ml

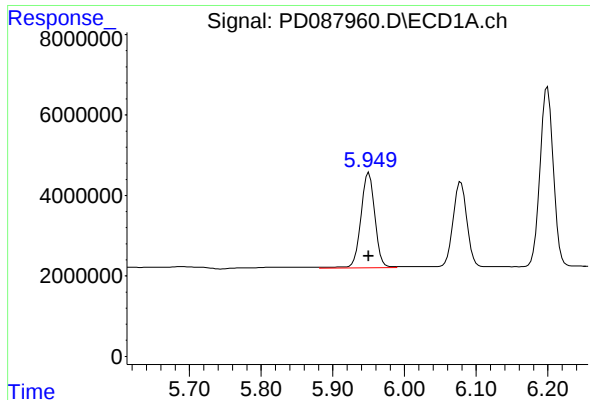

#10 gamma-Chlordane


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 31960215
Conc: 9.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

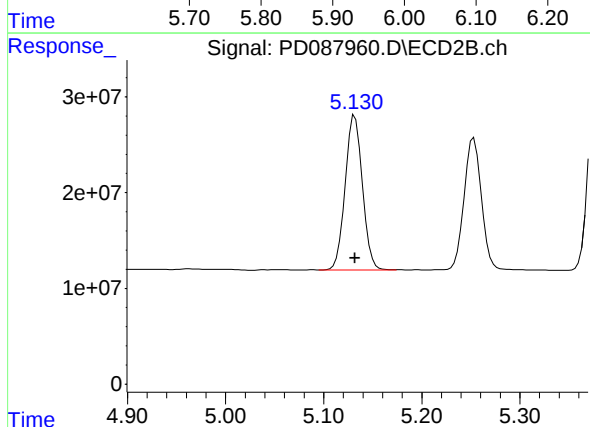


#10 gamma-Chlordane

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 198098262
Conc: 10.55 ng/ml

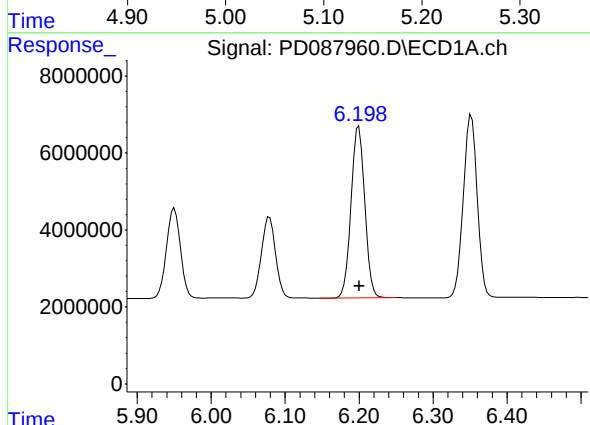


#12 4,4'-DDE

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 57360059
Conc: 18.91 ng/ml

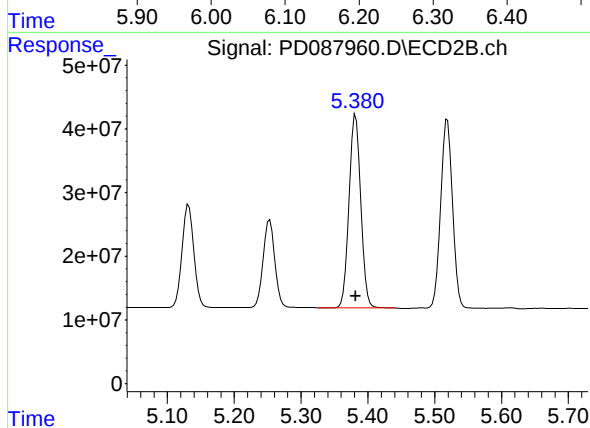

#12 4,4'-DDE


R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 368660041
Conc: 20.55 ng/ml

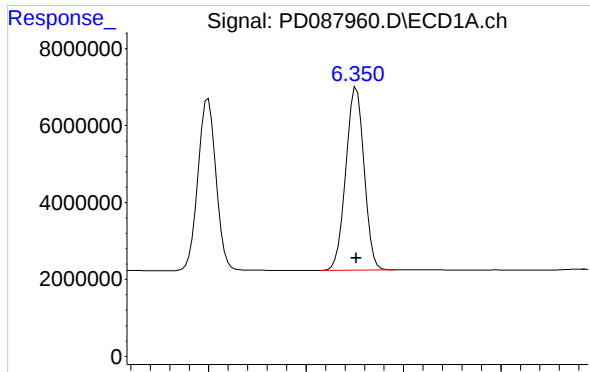

#13 Dieldrin


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 61908248
Conc: 18.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

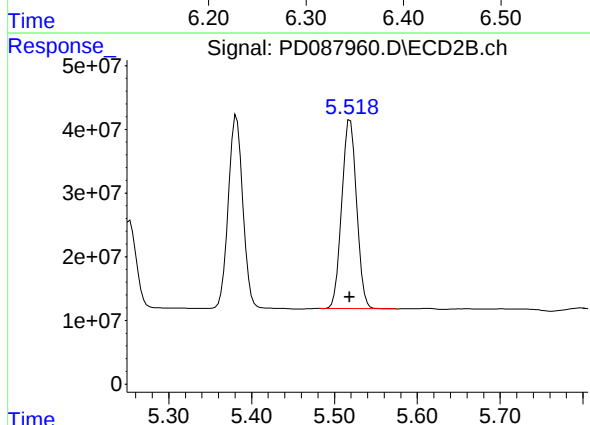


#13 Dieldrin

R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 370366068
Conc: 20.22 ng/ml

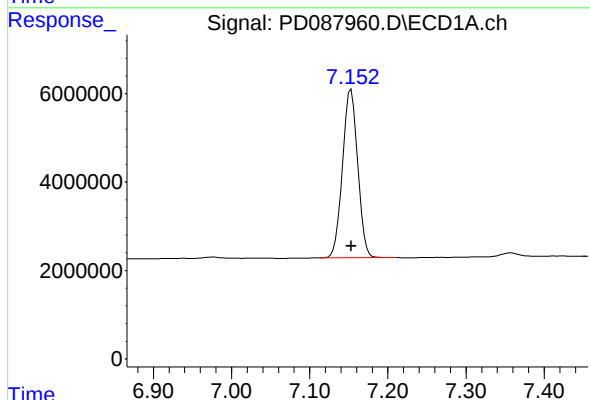


#19 Endosulfan Sulfate

R.T.: 7.153 min
Delta R.T.: 0.000 min
Response: 51712262
Conc: 19.30 ng/ml

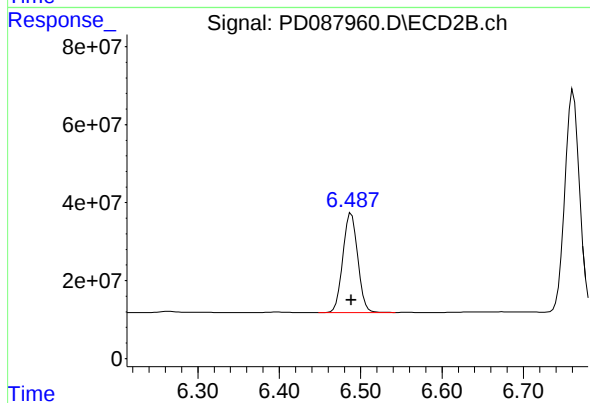

#19 Endosulfan Sulfate


R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 324723295
Conc: 20.42 ng/ml

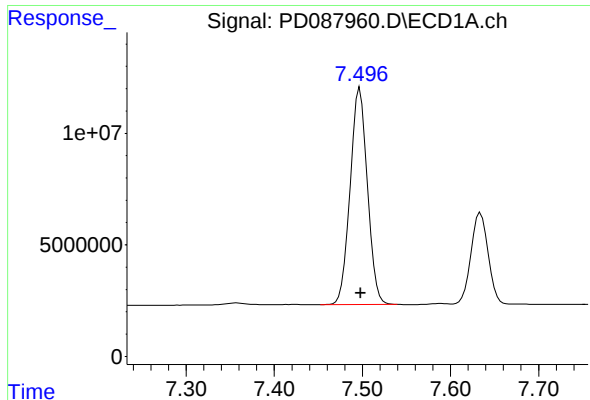

#20 Methoxychlor


R.T.: 7.497 min
Delta R.T.: -0.001 min
Response: 132275543
Conc: 93.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

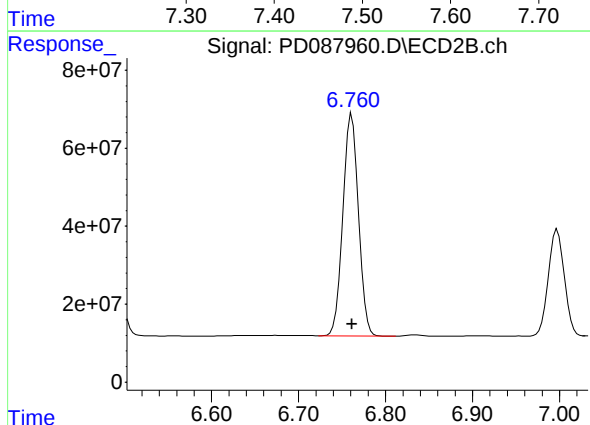


#20 Methoxychlor

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 713504879
Conc: 86.33 ng/ml

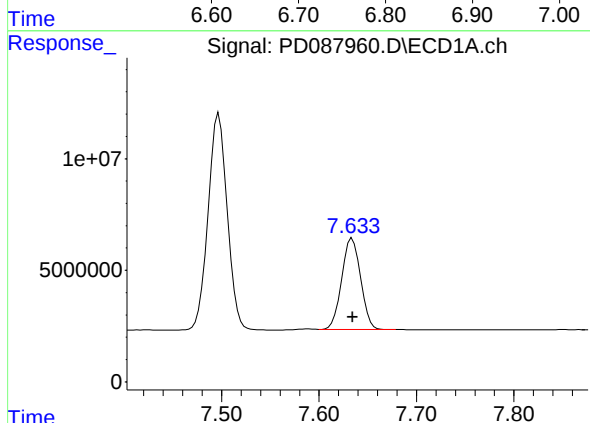


#21 Endrin ketone

R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 54976344
Conc: 19.15 ng/ml

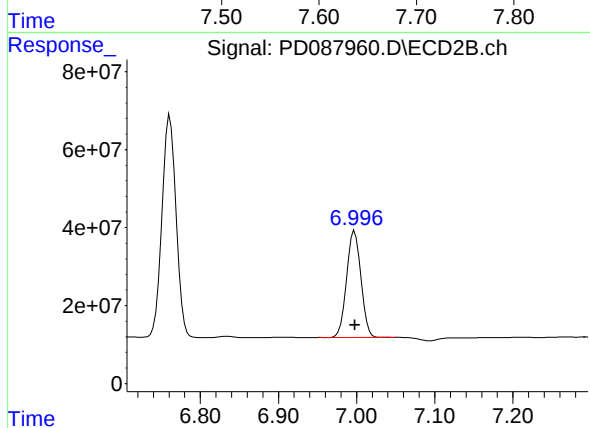

#21 Endrin ketone


R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 348288274
Conc: 20.47 ng/ml

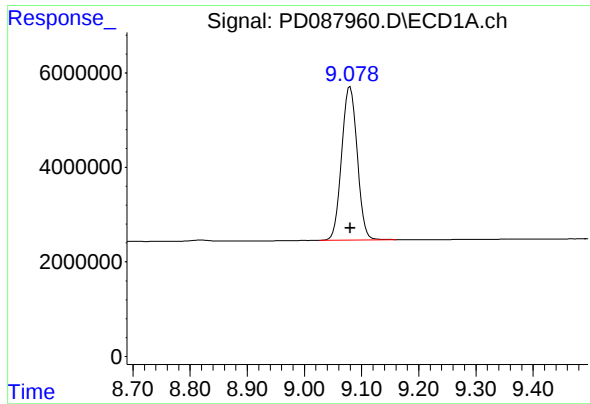

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.000 min
Response: 61649897
Conc: 20.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

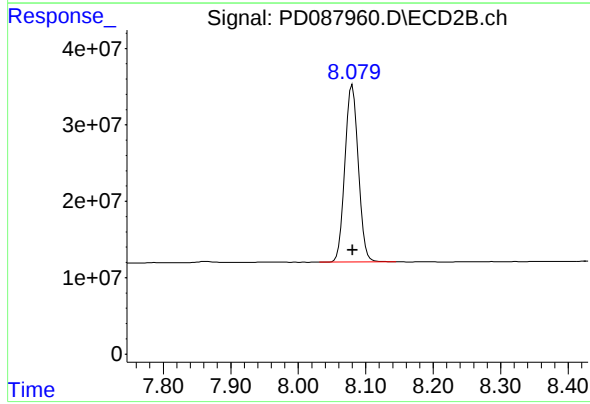

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: 0.000 min
Response: 322204135
Conc: 20.62 ng/ml