

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031419\
 Data File : PD051816.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Mar 2019 12:24
 Operator : AJ\SJ
 Sample : PIBLK34
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 03:22:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.223	4.043	35621920	775.9E6	24.789	25.114
27) SA	Decachlor...	7.822	9.156	52419349	781.6E6	43.587	41.228
Target Compounds							
6) B	beta-BHC	0.000	4.938f	0 41108049	N.D.	2.072	
8) B	Heptachlo...	0.000	5.924	0 123.7E6	N.D.	3.454	
10) B	trans-Chl...	0.000	6.115f	0 6604193	N.D.	0.183	
20) A	Methoxychlor	0.000	7.580f	0 10236317	N.D.	0.967	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031419\
Data File : PD051816.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Mar 2019 12:24
Operator : AJ\SJ
Sample : PIBLK34
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
PIBLK34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 03:22:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

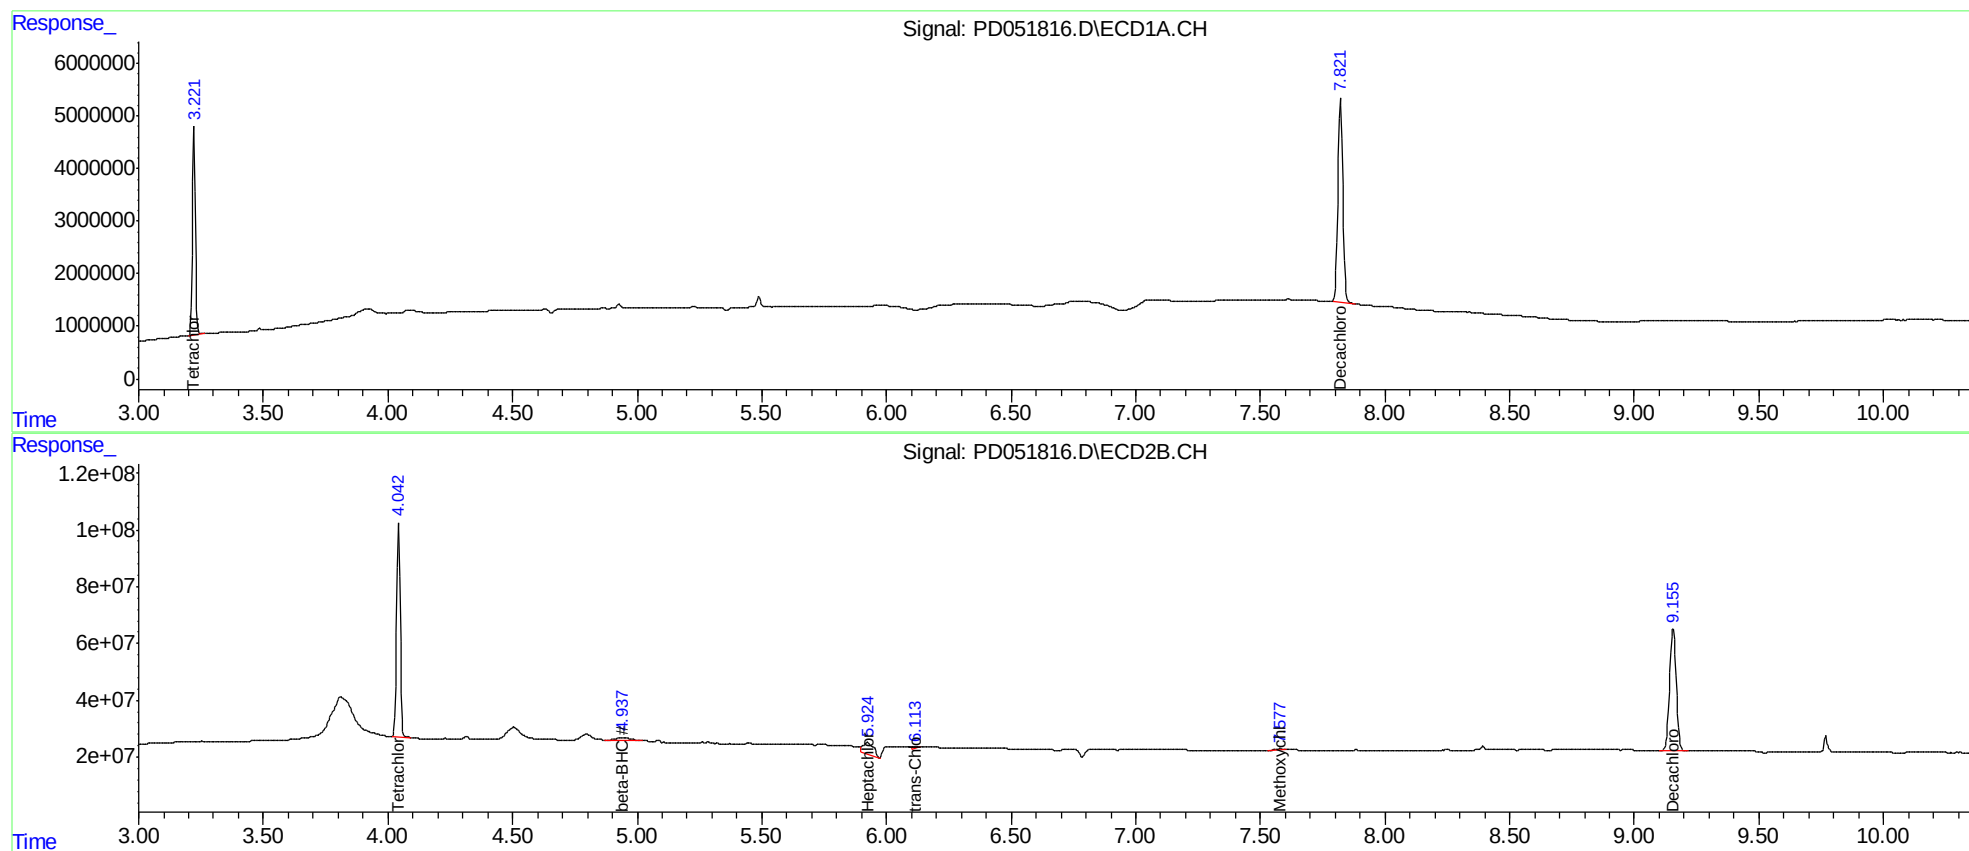


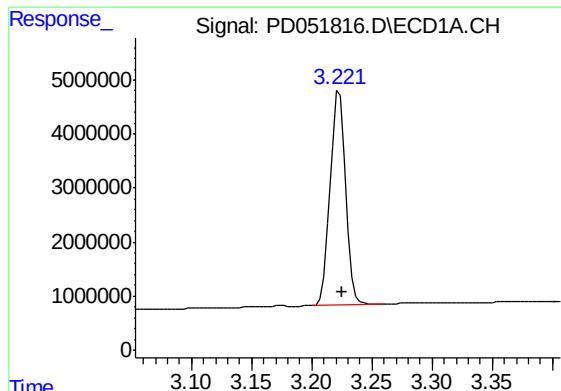

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.002 min
Response: 35621920
Conc: 24.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK34

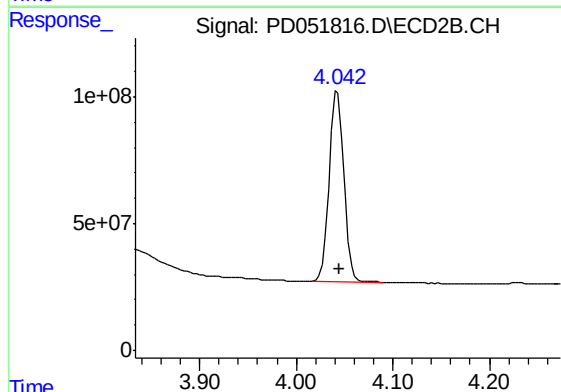


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 775921991
Conc: 25.11 ng/ml

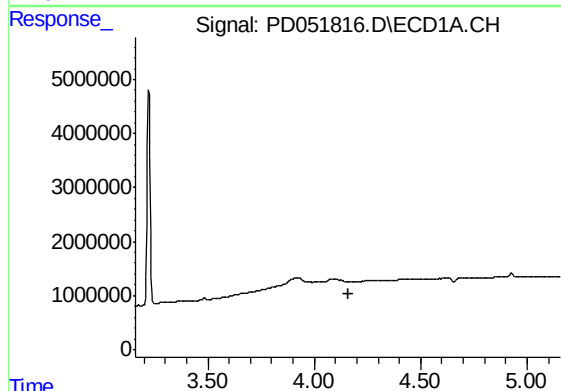


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

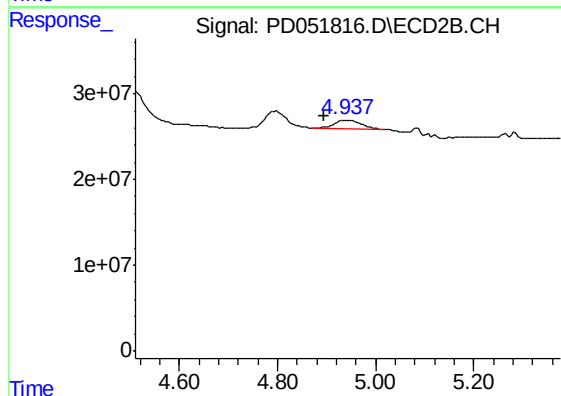

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.044 min
Response: 41108049
Conc: 2.07 ng/ml

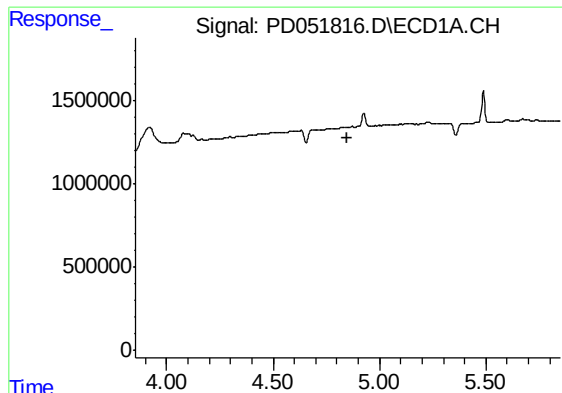

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

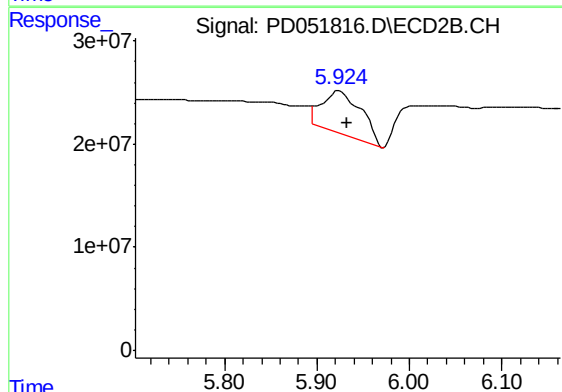


#8 Heptachlor epoxide

R.T.: 5.924 min
Delta R.T.: -0.009 min
Response: 123680250
Conc: 3.45 ng/ml

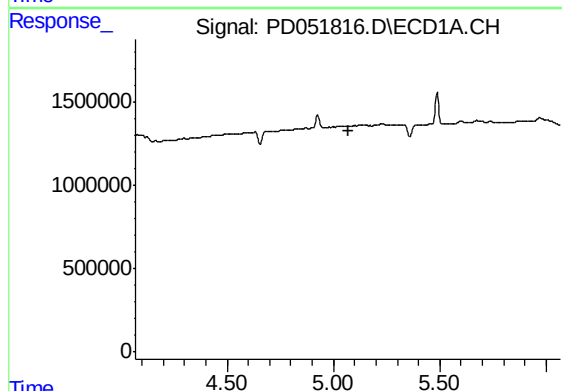


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.068 min
Response: 0
Conc: N.D.

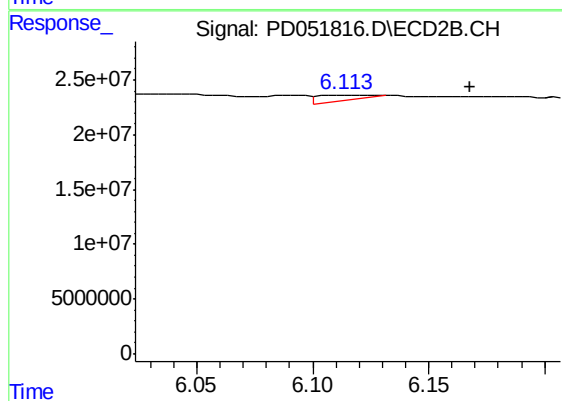

#10 trans-Chlordane


R.T.: 6.115 min
Delta R.T.: -0.053 min
Response: 6604193
Conc: 0.18 ng/ml

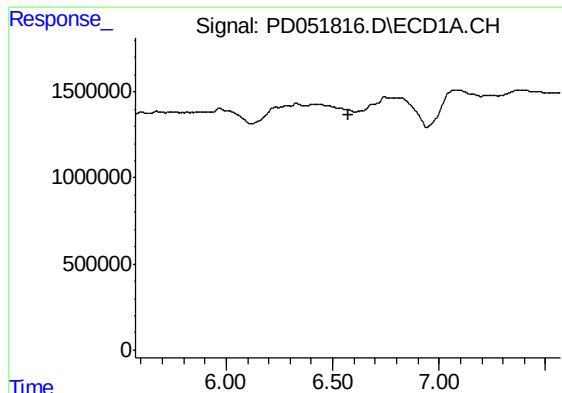

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

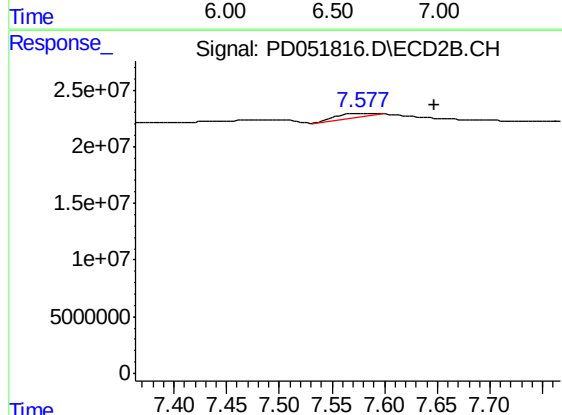


#20 Methoxychlor

R.T.: 7.580 min
Delta R.T.: -0.068 min
Response: 10236317
Conc: 0.97 ng/ml

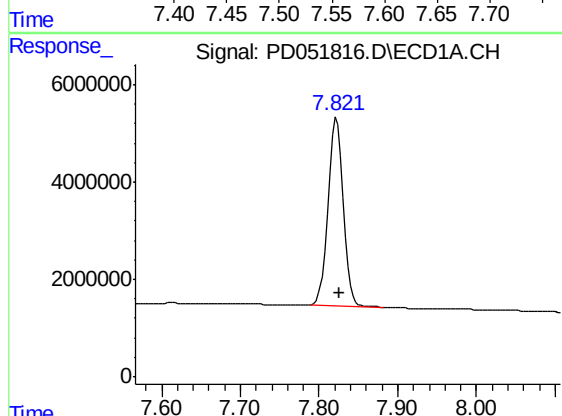

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: -0.004 min
Response: 52419349
Conc: 43.59 ng/ml

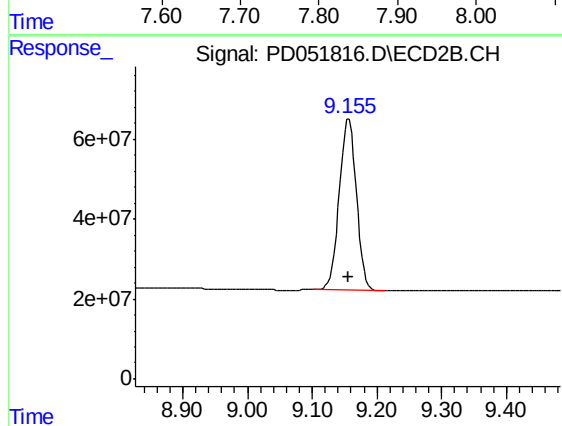

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 781571283
Conc: 41.23 ng/ml