

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684542.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 12:09
 Operator : AR\AJ
 Sample : N1818-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:13:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.172	18940525	148.2E6	13.909	13.536
27)	SA Decachlor...	8.207	9.366	33304860	154.8E6	23.951	24.545
Target Compounds							
2)	A alpha-BHC	0.000	4.533f	0	690176	N.D.	<MDL
3)	MA gamma-BHC...	4.132f	4.826f	-24671	659371	N.D.	<MDL
6)	B beta-BHC	4.387f	0.000	607104	0	0.729	N.D. #
7)	B delta-BHC	0.000	5.227	0	3474343	N.D.	0.245
8)	B Heptachlo...	0.000	6.154f	0	1545868	N.D.	0.128
9)	A Endosulfan I	0.000	6.402f	0	1412667	N.D.	0.130
11)	B cis-Chlor...	0.000	6.402	0	1412667	N.D.	0.123
13)	MA Dieldrin	0.000	6.709	0	1084063	N.D.	<MDL
14)	MA Endrin	0.000	6.996f	0	982396	N.D.	0.116
15)	B Endosulfa...	0.000	7.134	0	1515343	N.D.	0.169
16)	A 4,4'-DDD	0.000	6.996f	0	982396	N.D.	0.117


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684542.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 12:09
Operator : AR\AJ
Sample : N1818-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:13:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

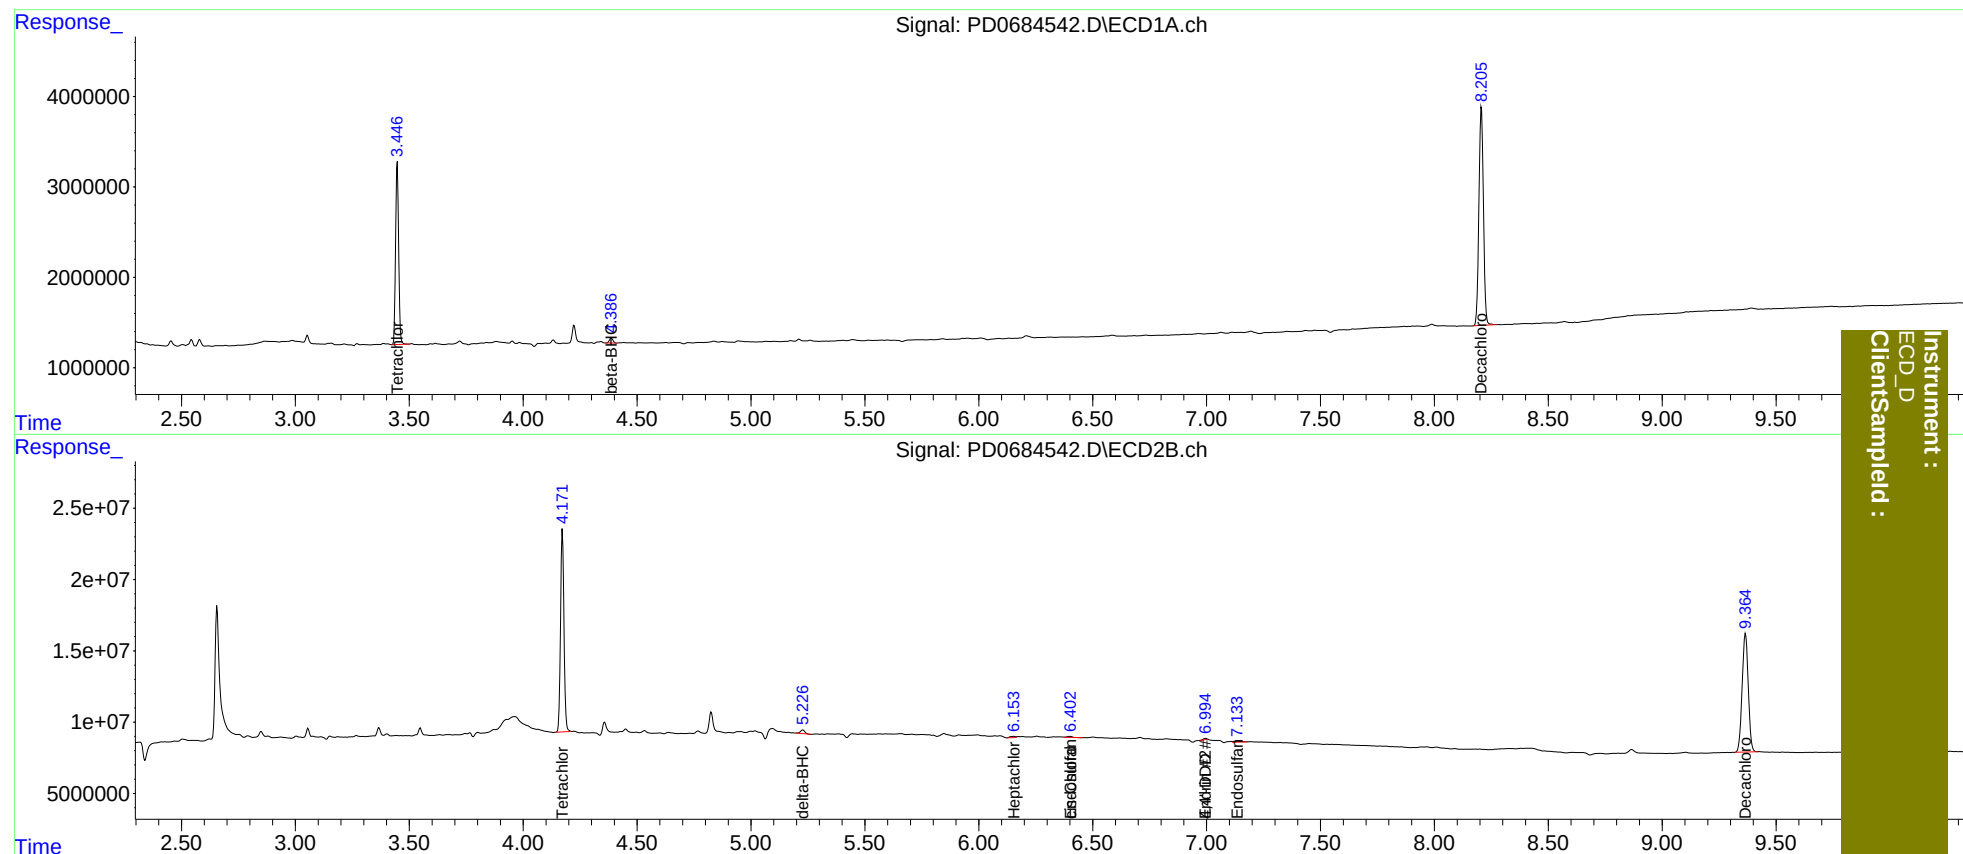


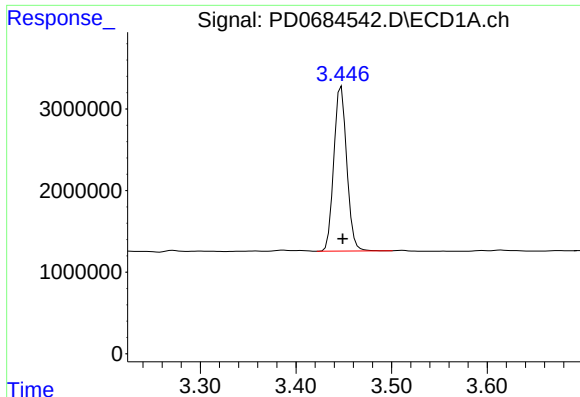

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: -0.002 min
Response: 18940525
Conc: 13.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

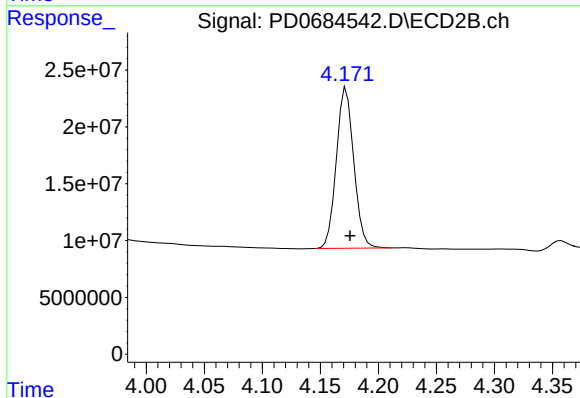


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.003 min
Response: 148152564
Conc: 13.54 ng/ml

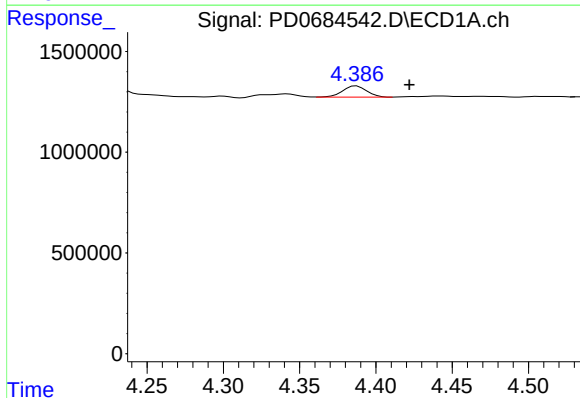


#6 beta-BHC

R.T.: 4.387 min
Delta R.T.: -0.035 min
Response: 607104
Conc: 0.73 ng/ml

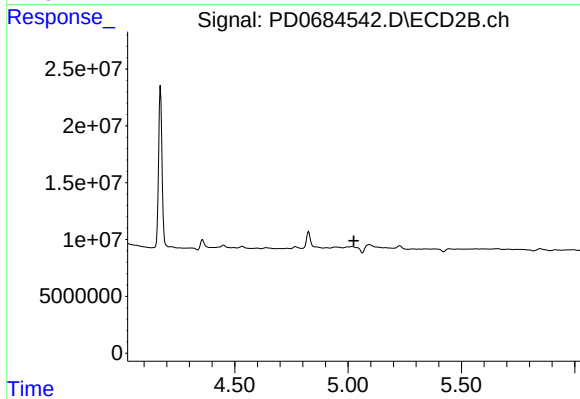

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 5.025 min
Response: 0
Conc: N.D.

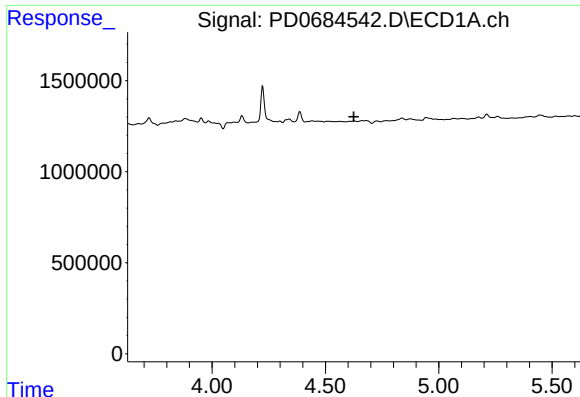

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

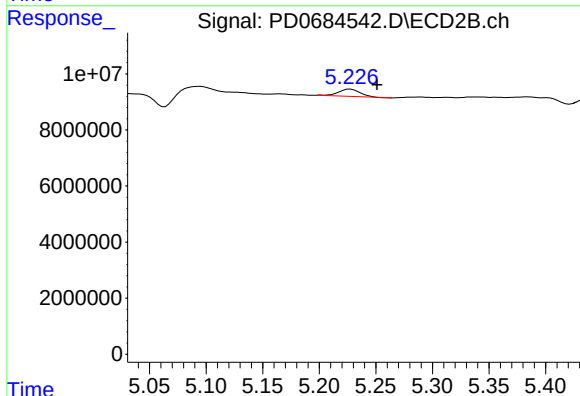


#7 delta-BHC

R.T.: 5.227 min
Delta R.T.: -0.023 min
Response: 3474343
Conc: 0.25 ng/ml

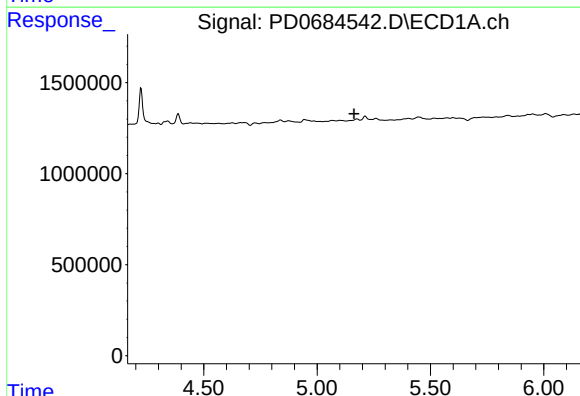


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

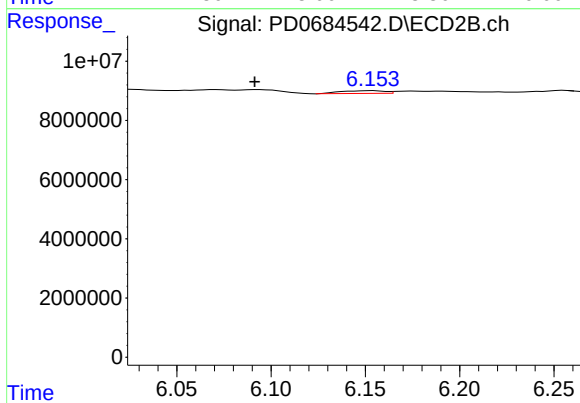

#8 Heptachlor epoxide


R.T.: 6.154 min
Delta R.T.: 0.062 min
Response: 1545868
Conc: 0.13 ng/ml

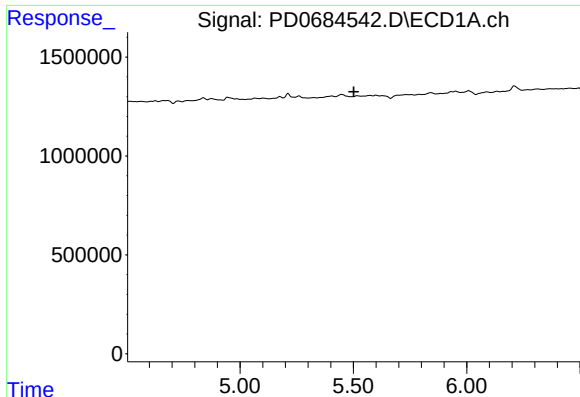

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

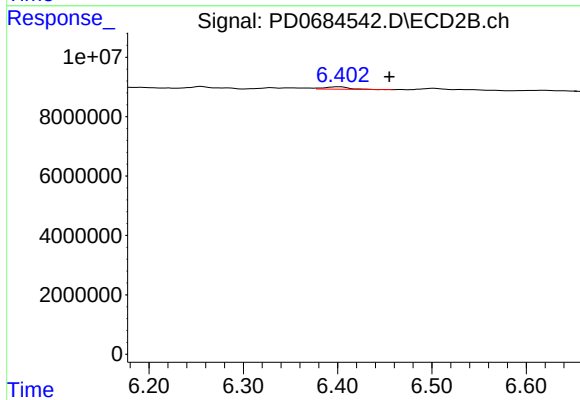


#9 Endosulfan I

R.T.: 6.402 min
Delta R.T.: -0.053 min
Response: 1412667
Conc: 0.13 ng/ml

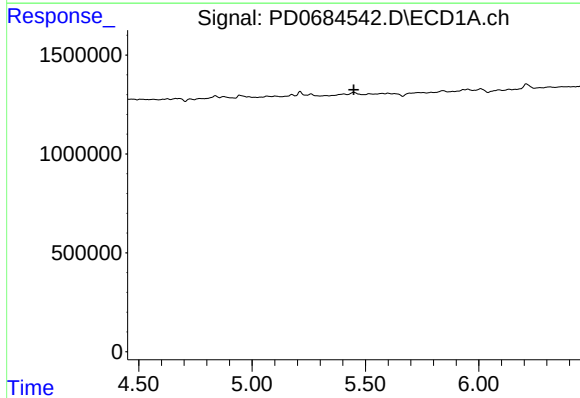


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

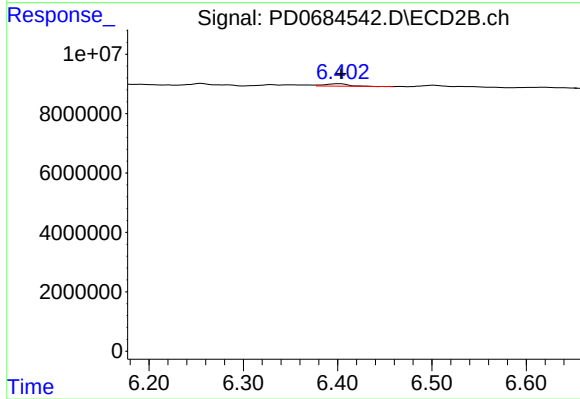

#11 cis-Chlordane


R.T.: 6.402 min
Delta R.T.: -0.002 min
Response: 1412667
Conc: 0.12 ng/ml

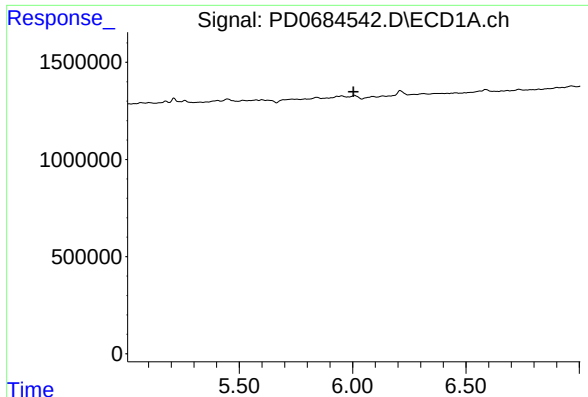

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

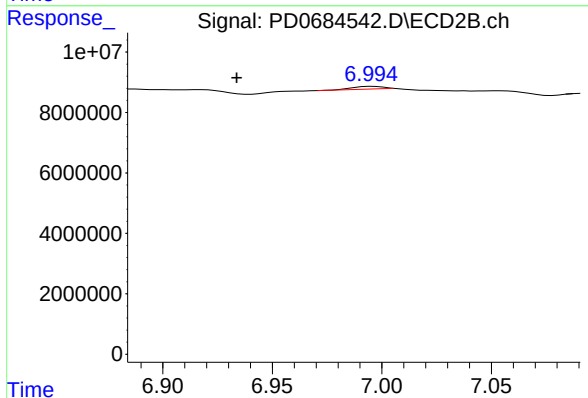


#14 Endrin

R.T.: 6.996 min
Delta R.T.: 0.062 min
Response: 982396
Conc: 0.12 ng/ml

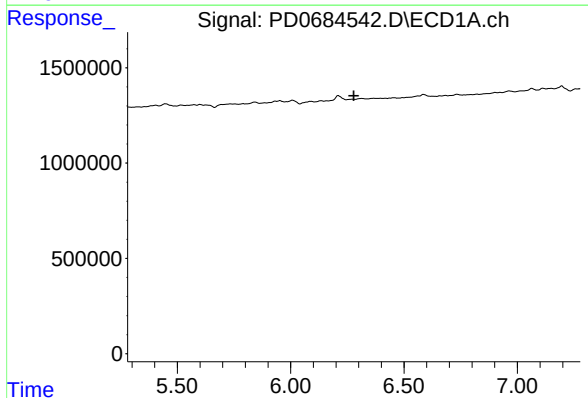


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

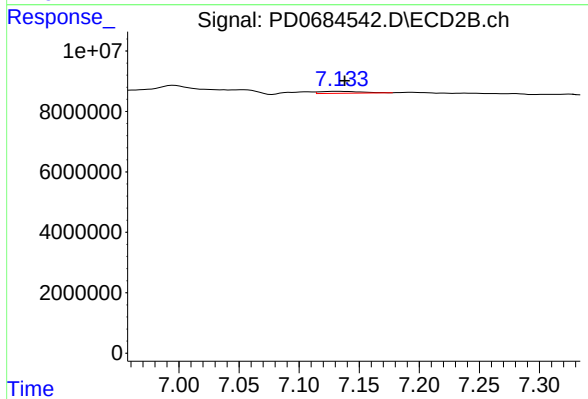

#15 Endosulfan II


R.T.: 7.134 min
Delta R.T.: -0.004 min
Response: 1515343
Conc: 0.17 ng/ml

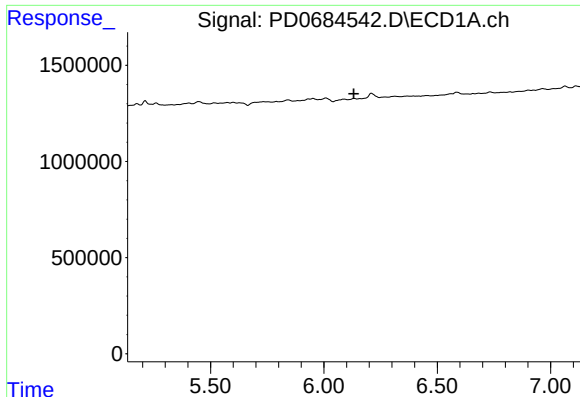

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

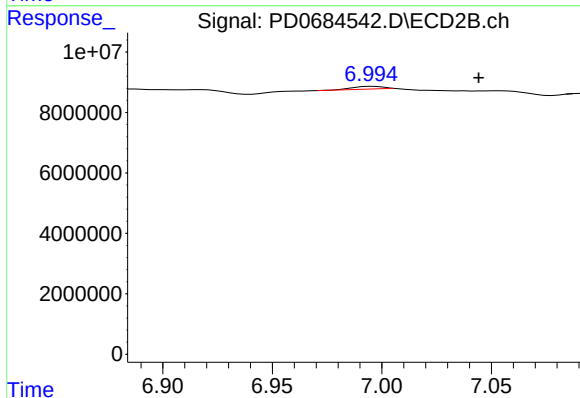


#16 4,4'-DDD

R.T.: 6.996 min
Delta R.T.: -0.049 min
Response: 982396
Conc: 0.12 ng/ml

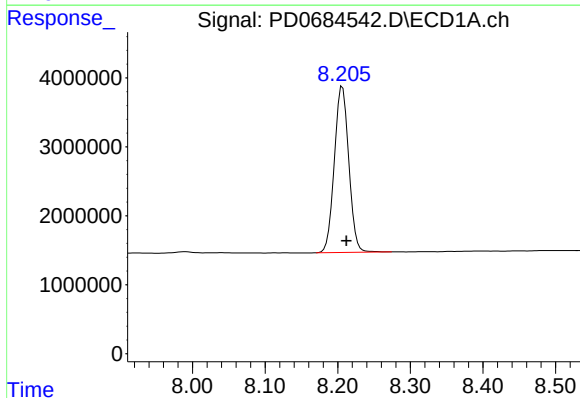

#27 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.006 min
Response: 33304860
Conc: 23.95 ng/ml

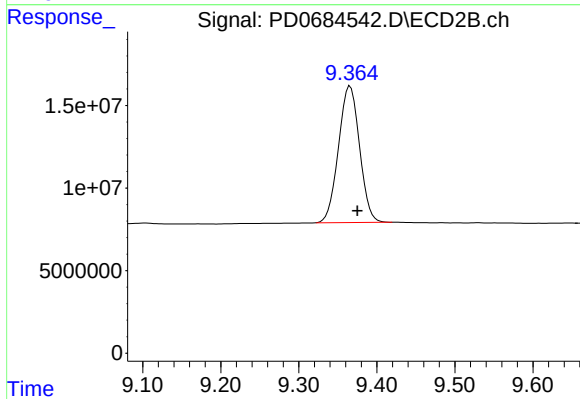

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 154810170
Conc: 24.55 ng/ml