

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 12:51
 Operator : AR\AJ
 Sample : N1818-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:14:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.173	25794365	202.2E6	18.942	18.472
27)	SA Decachlor...	8.219	9.364	48563296	218.7E6	34.924	34.678
Target Compounds							
2)	A alpha-BHC	0.000	4.533f	0	1413074	N.D.	<MDL
3)	MA gamma-BHC...	0.000	4.825f	0	3267119	N.D.	0.225
7)	B delta-BHC	0.000	5.227	0	2997260	N.D.	0.212
8)	B Heptachlo...	0.000	6.148f	0	3181346	N.D.	0.264
9)	A Endosulfan I	0.000	6.398f	0	3140968	N.D.	0.289
10)	B trans-Chl...	0.000	6.325	0	921297	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.398	0	3140968	N.D.	0.274
13)	MA Dieldrin	0.000	6.708	0	1354671	N.D.	0.122
14)	MA Endrin	0.000	6.995f	0	829666	N.D.	<MDL
15)	B Endosulfa...	0.000	7.130	0	3009279	N.D.	0.336
16)	A 4,4'-DDD	0.000	6.995f	0	829666	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 12:51
Operator : AR\AJ
Sample : N1818-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:14:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

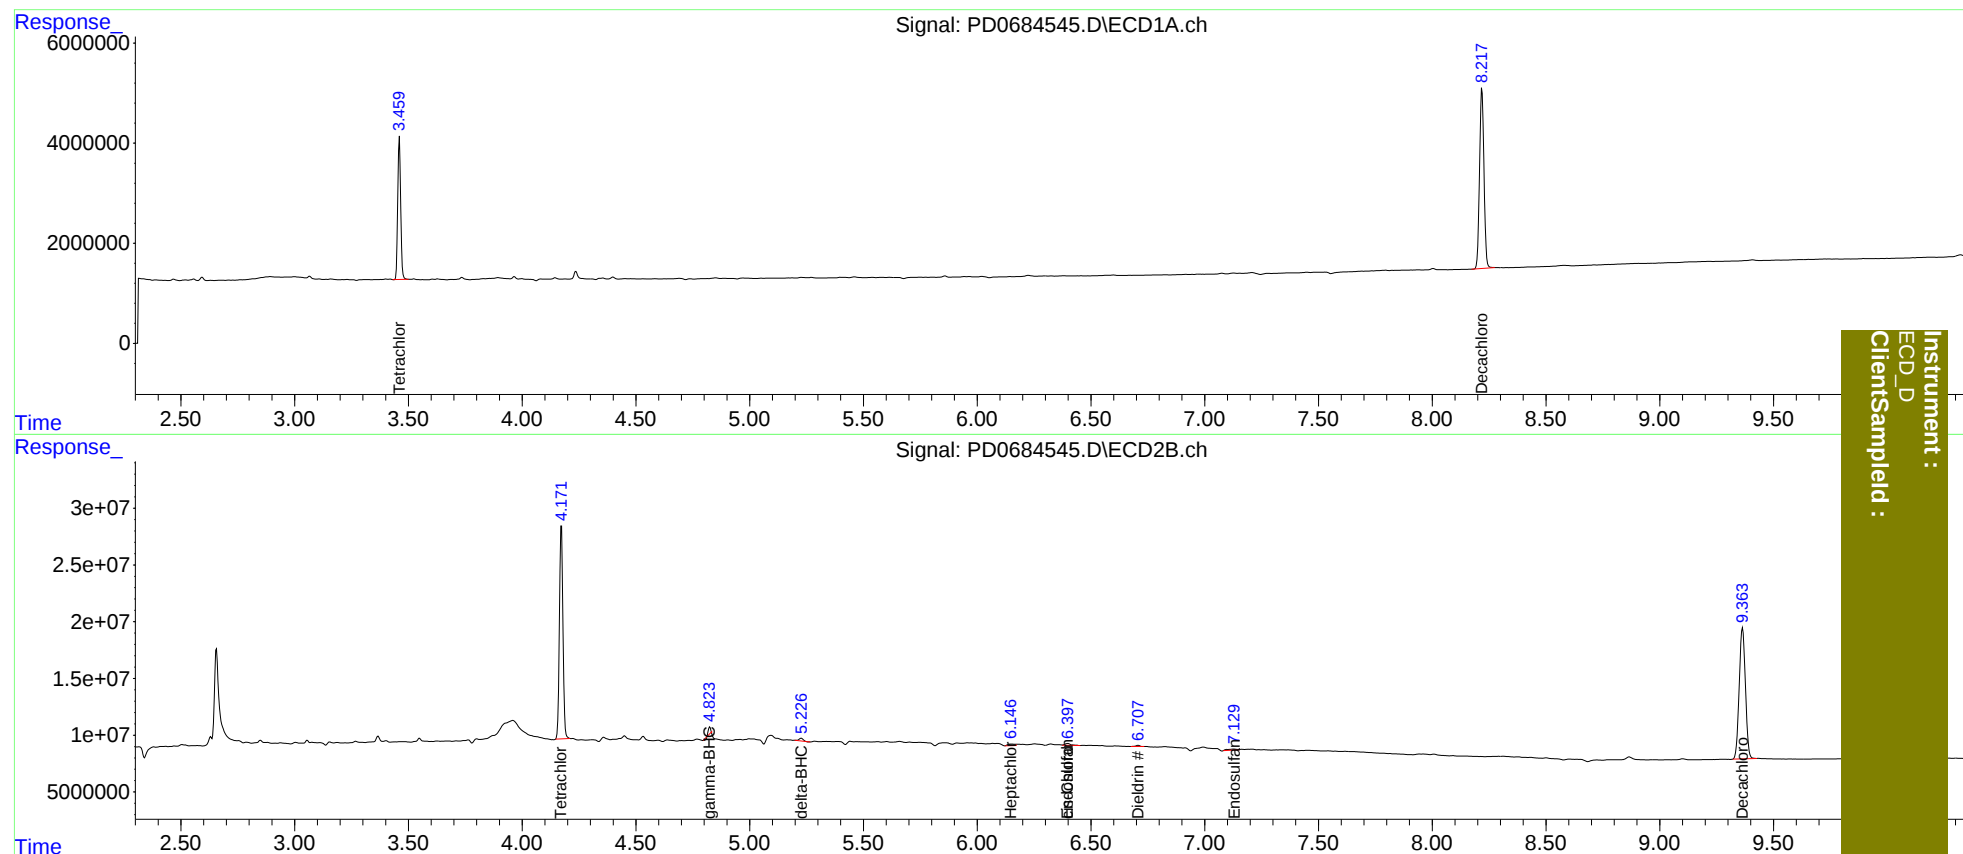


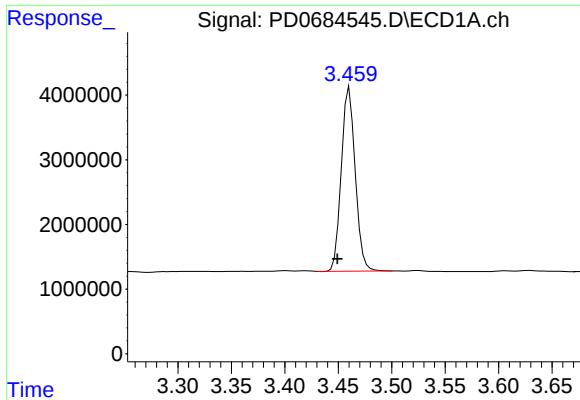

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.011 min
Response: 25794365
Conc: 18.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

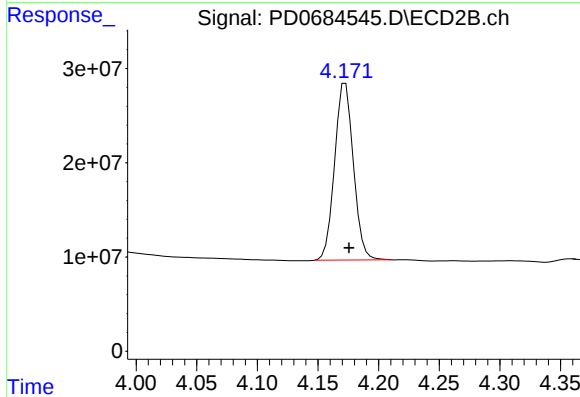


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 202182950
Conc: 18.47 ng/ml

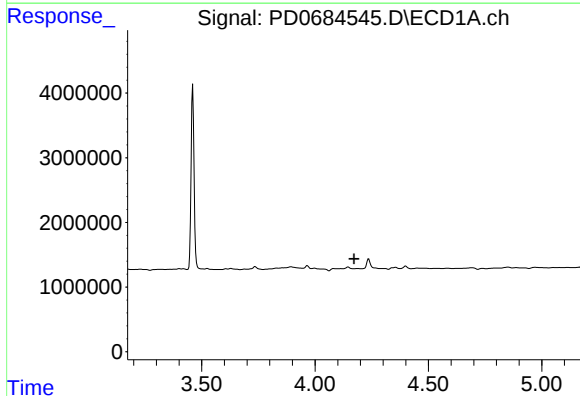


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.172 min
Response: 0
Conc: N.D.

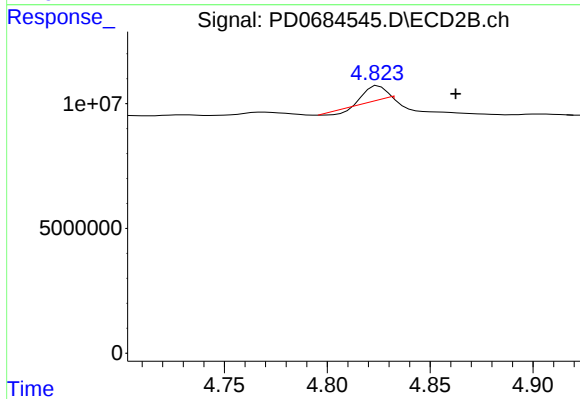

#3 gamma-BHC (Lindane)


R.T.: 4.825 min
Delta R.T.: -0.038 min
Response: 3267119
Conc: 0.23 ng/ml

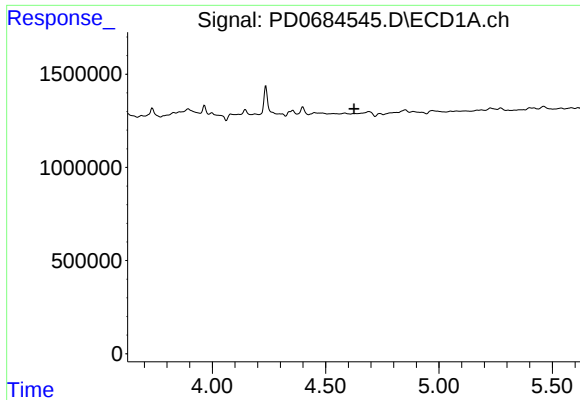

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

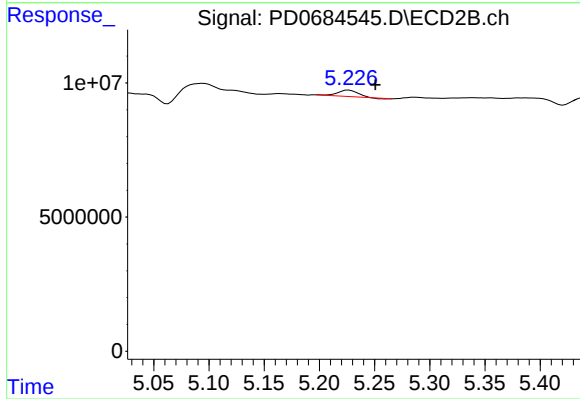


#7 delta-BHC

R.T.: 5.227 min
Delta R.T.: -0.024 min
Response: 2997260
Conc: 0.21 ng/ml

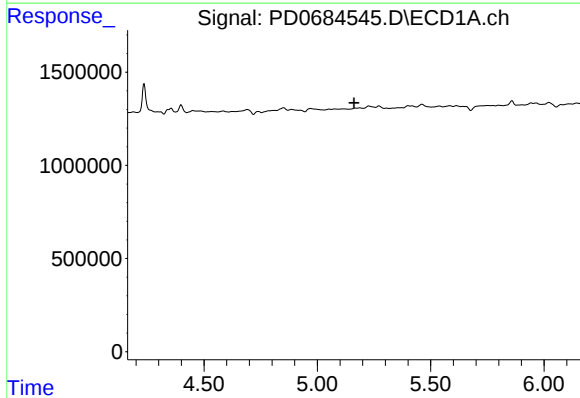


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

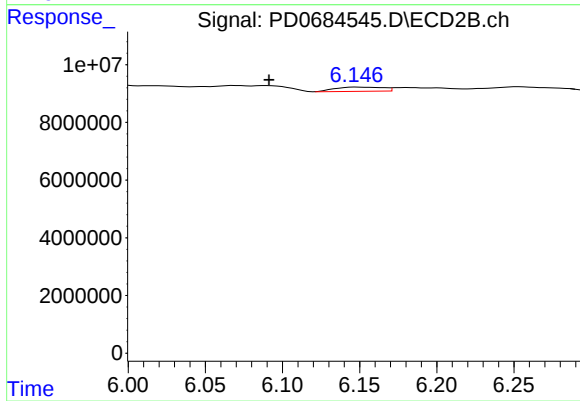

#8 Heptachlor epoxide


R.T.: 6.148 min
Delta R.T.: 0.057 min
Response: 3181346
Conc: 0.26 ng/ml

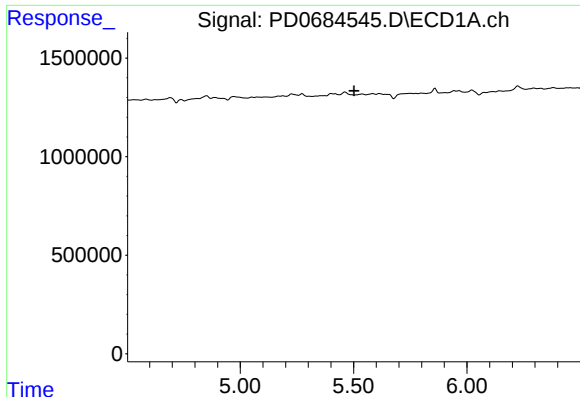

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

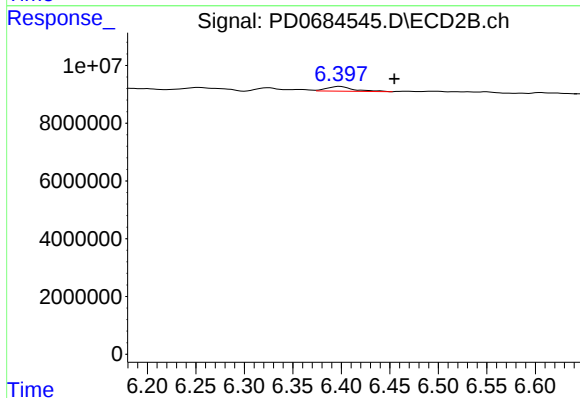


#9 Endosulfan I

R.T.: 6.398 min
Delta R.T.: -0.056 min
Response: 3140968
Conc: 0.29 ng/ml

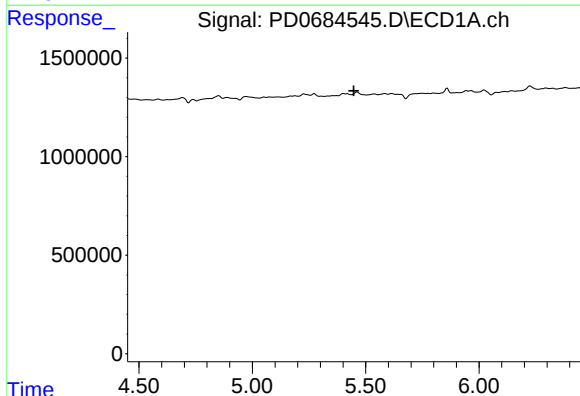


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

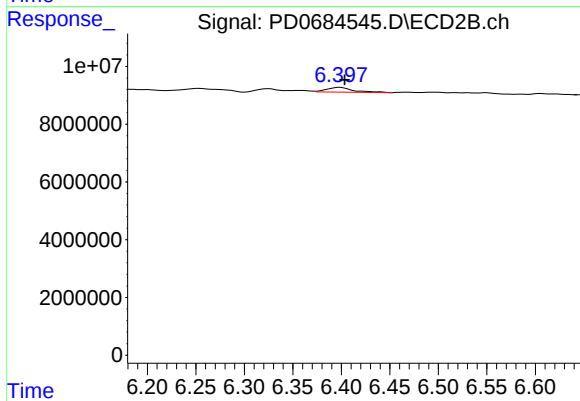

#11 cis-Chlordane


R.T.: 6.398 min
Delta R.T.: -0.005 min
Response: 3140968
Conc: 0.27 ng/ml

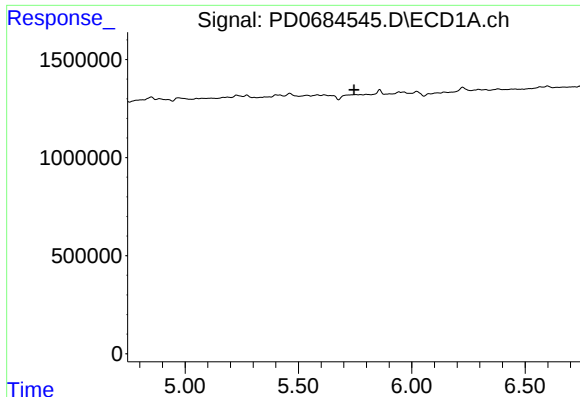

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

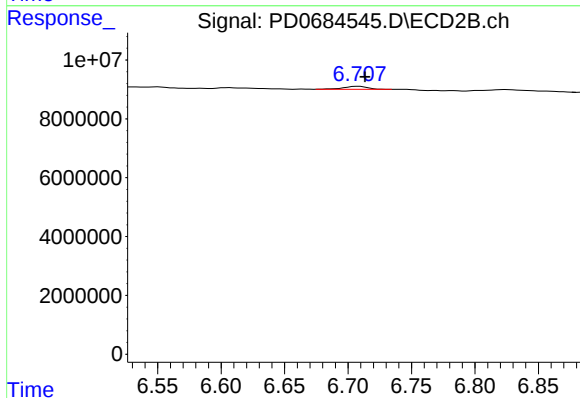


#13 Dieldrin

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 1354671
Conc: 0.12 ng/ml

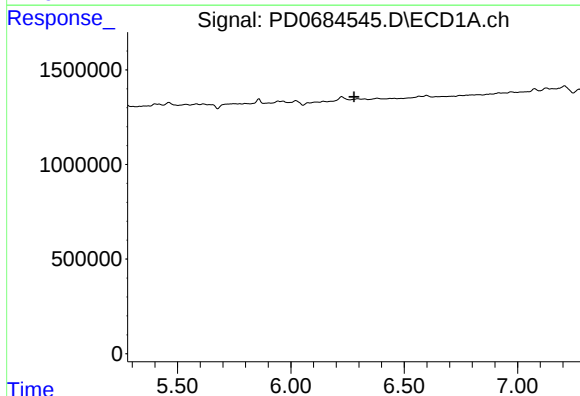


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

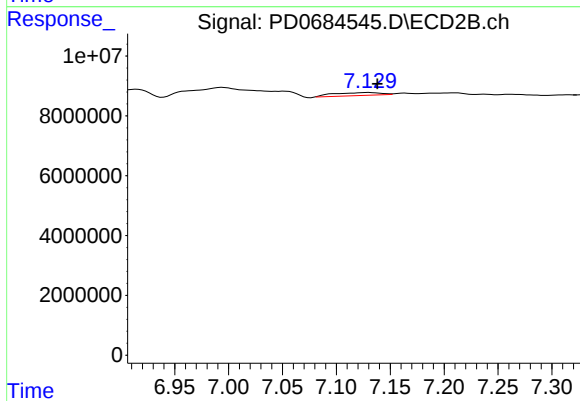

#15 Endosulfan II


R.T.: 7.130 min
Delta R.T.: -0.008 min
Response: 3009279
Conc: 0.34 ng/ml

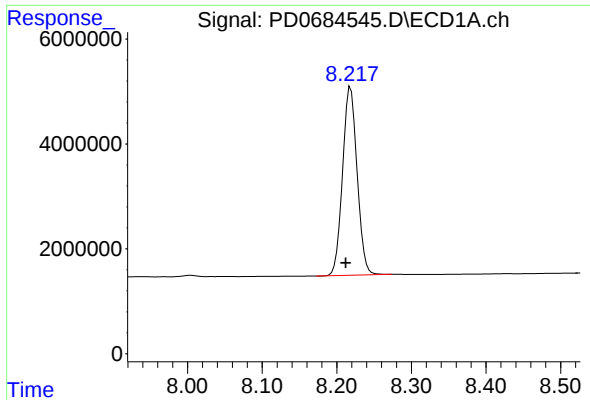

#27 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.006 min
Response: 48563296
Conc: 34.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

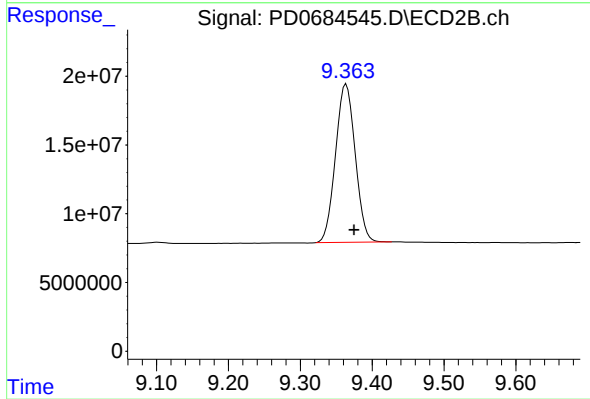

#27 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: -0.011 min
Response: 218718597
Conc: 34.68 ng/ml