

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 17:40
 Operator : AR\AJ
 Sample : N1818-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:18:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.173	22888432	177.8E6	16.808	16.245
2)	SA Decachlor...	8.206	9.365	46600655	207.0E6	33.512	32.817
Target Compounds							
2)	A alpha-BHC	0.000	4.533f	0	1375239	N.D.	<MDL
3)	MA gamma-BHC...	4.132f	4.825f	290388	2975241	0.160	0.205 #
7)	B delta-BHC	0.000	5.226	0	3369981	N.D.	0.238
8)	B Heptachlo...	0.000	6.148f	0	2920729	N.D.	0.242
9)	A Endosulfan I	0.000	6.504f	0	382670	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.350f	0	143326	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.504f	0	382670	N.D.	<MDL
13)	MA Dieldrin	0.000	6.708	0	1207199	N.D.	0.109
14)	MA Endrin	0.000	6.964	0	1549346	N.D.	0.183
15)	B Endosulfa...	0.000	7.130	0	2488932	N.D.	0.278
16)	A 4,4'-DDD	0.000	6.996f	0	969516	N.D.	0.116
21)	B Endrin ke...	0.000	7.965	0	1384477	N.D.	0.162


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 17:40
Operator : AR\AJ
Sample : N1818-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:18:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

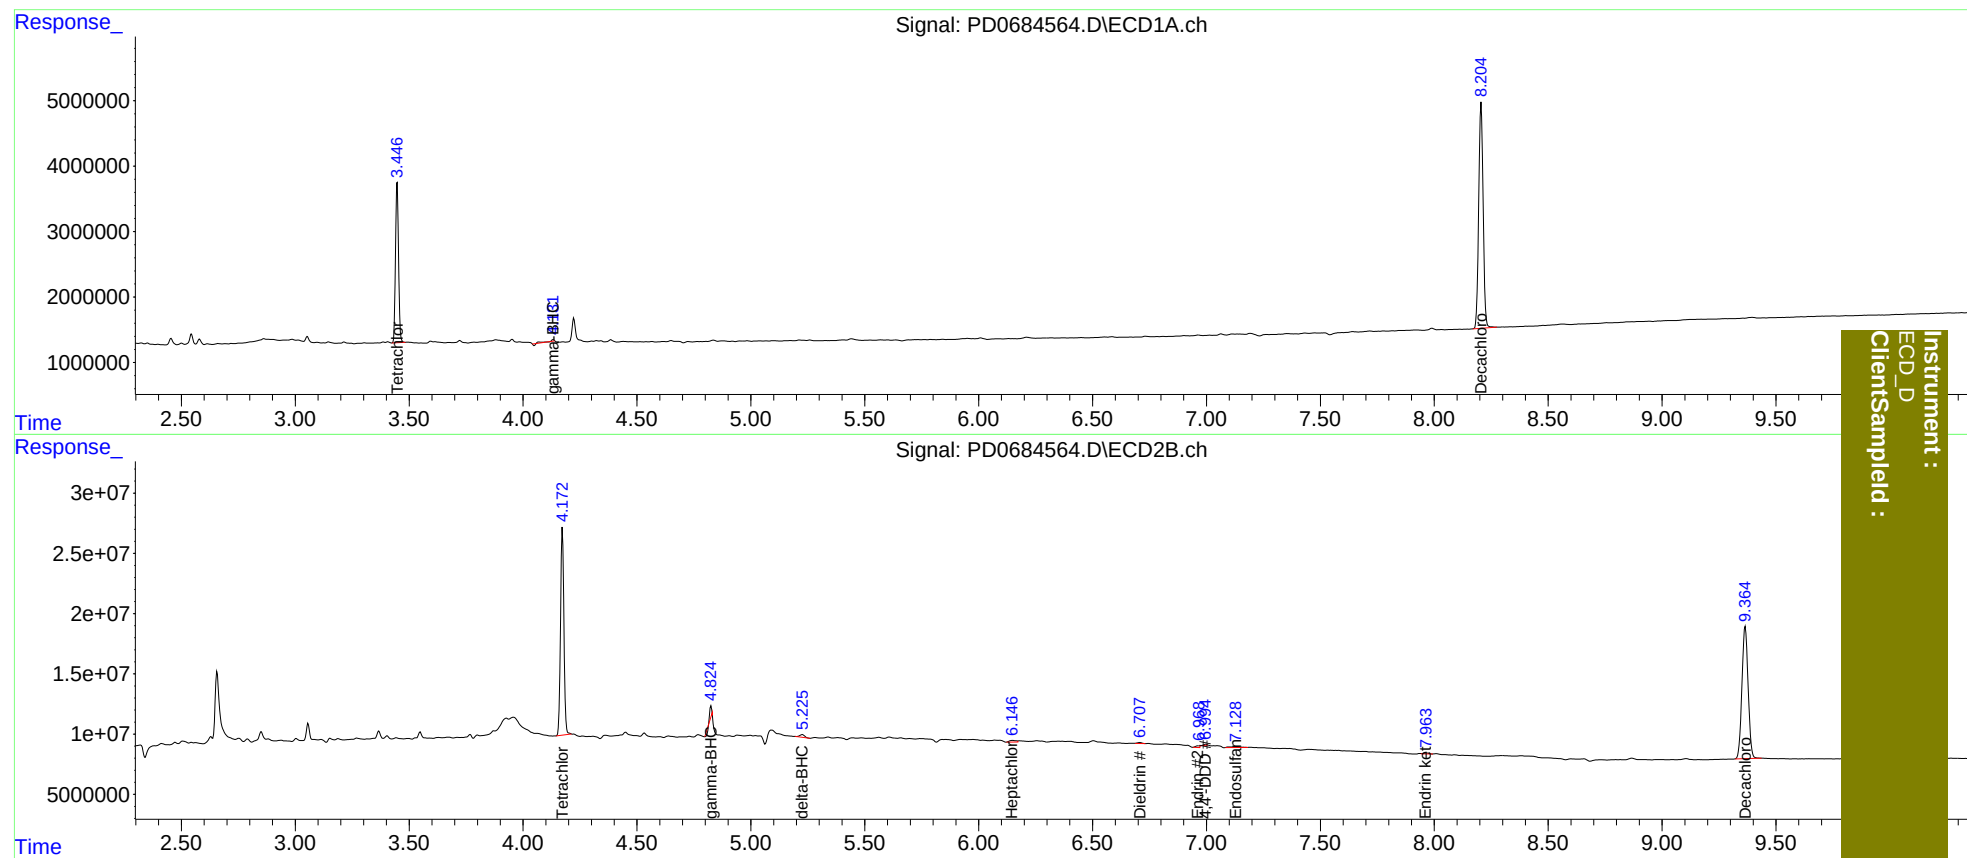


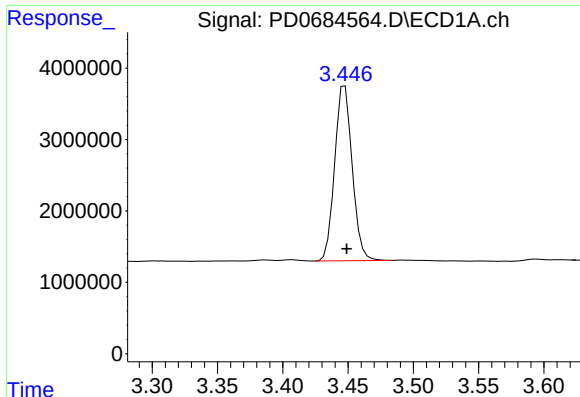

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: -0.001 min
Response: 22888432
Conc: 16.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

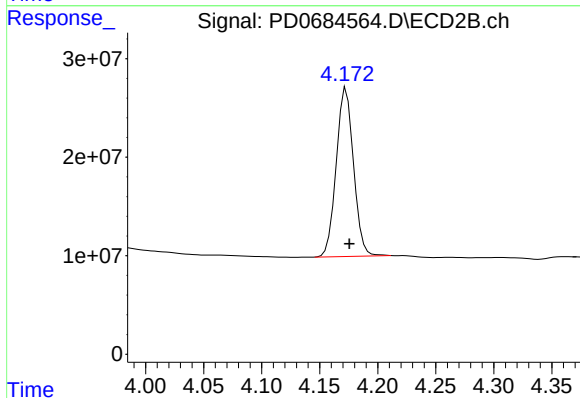


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 177809809
Conc: 16.25 ng/ml

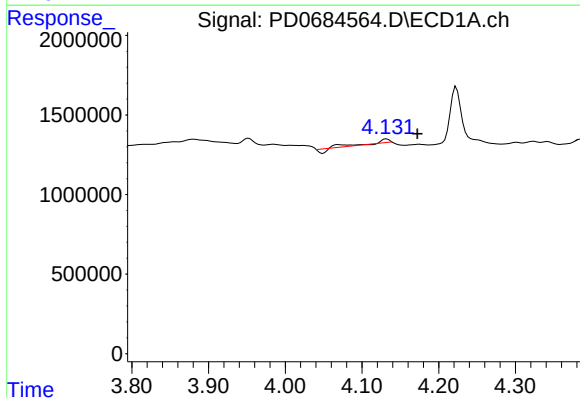


#3 gamma-BHC (Lindane)

R.T.: 4.132 min
Delta R.T.: -0.040 min
Response: 290388
Conc: 0.16 ng/ml

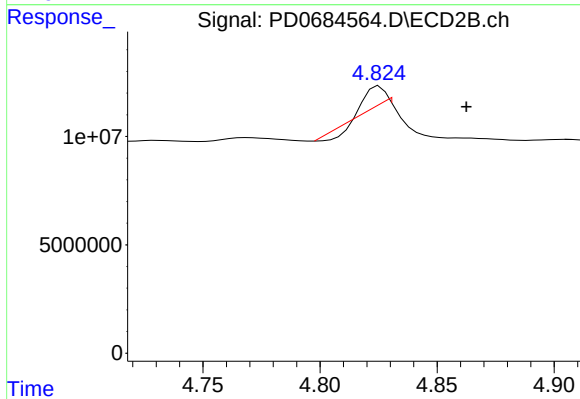

#3 gamma-BHC (Lindane)


R.T.: 4.825 min
Delta R.T.: -0.037 min
Response: 2975241
Conc: 0.21 ng/ml

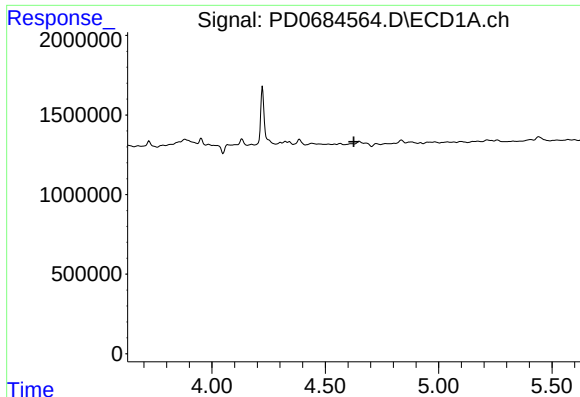

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

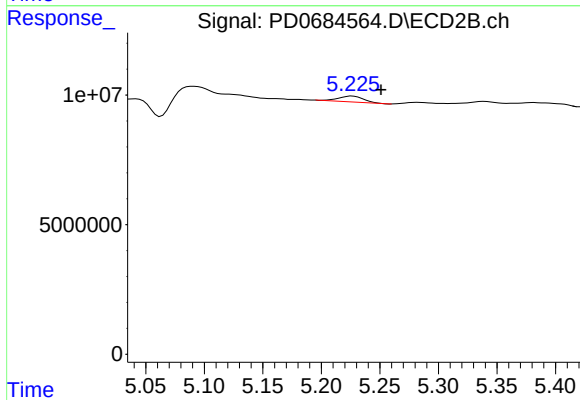


#7 delta-BHC

R.T.: 5.226 min
Delta R.T.: -0.025 min
Response: 3369981
Conc: 0.24 ng/ml

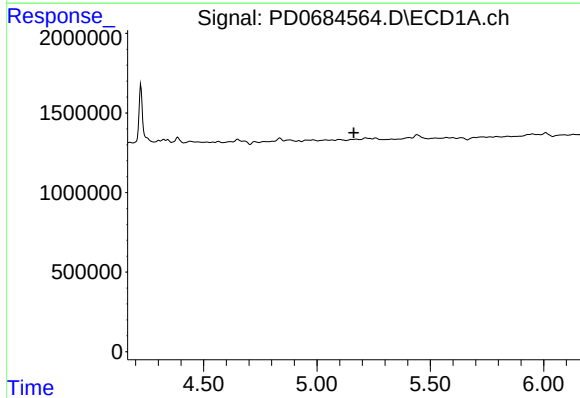


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

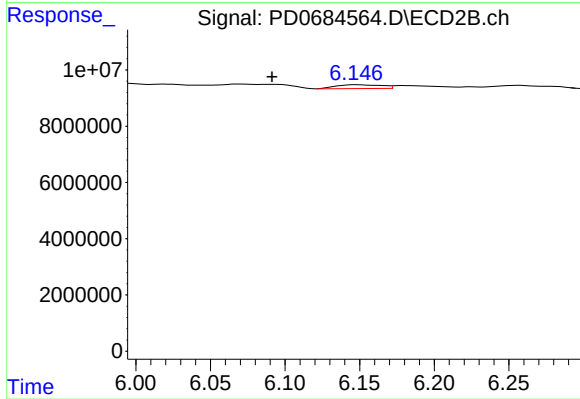

#8 Heptachlor epoxide


R.T.: 6.148 min
Delta R.T.: 0.057 min
Response: 2920729
Conc: 0.24 ng/ml

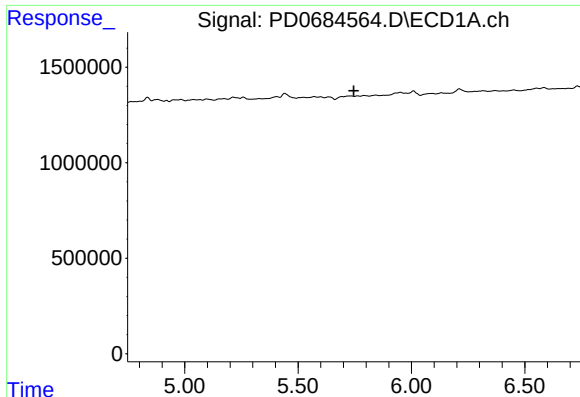

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

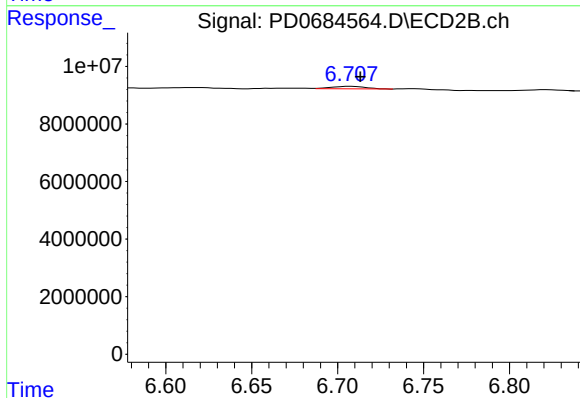


#13 Dieldrin

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 1207199
Conc: 0.11 ng/ml

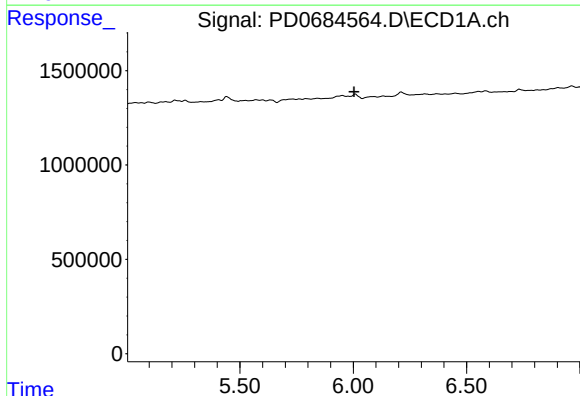


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.004 min
Response: 0
Conc: N.D.

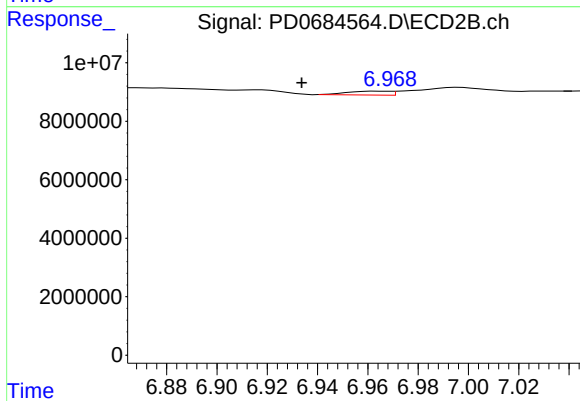

#14 Endrin


R.T.: 6.964 min
Delta R.T.: 0.030 min
Response: 1549346
Conc: 0.18 ng/ml

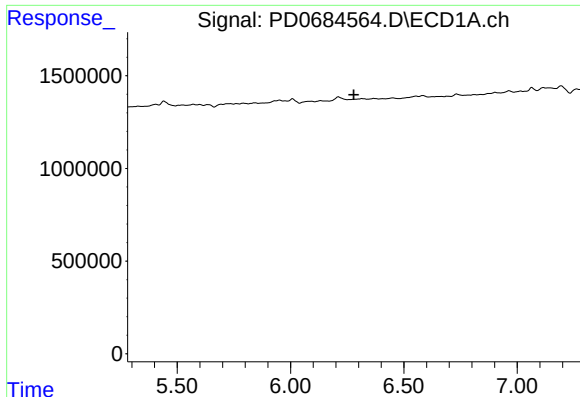

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

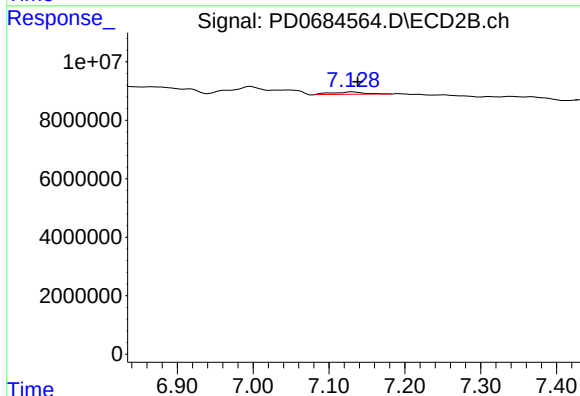


#15 Endosulfan II

R.T.: 7.130 min
Delta R.T.: -0.008 min
Response: 2488932
Conc: 0.28 ng/ml

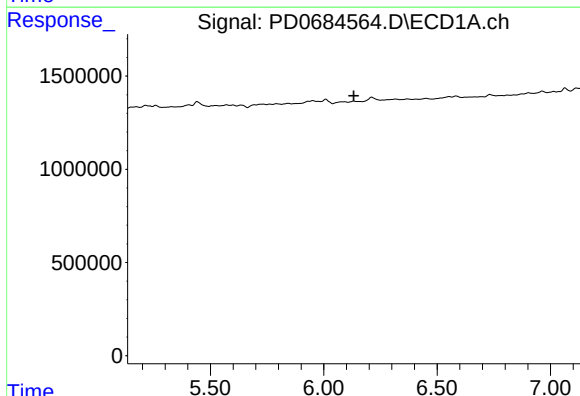


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.132 min
Response: 0
Conc: N.D.

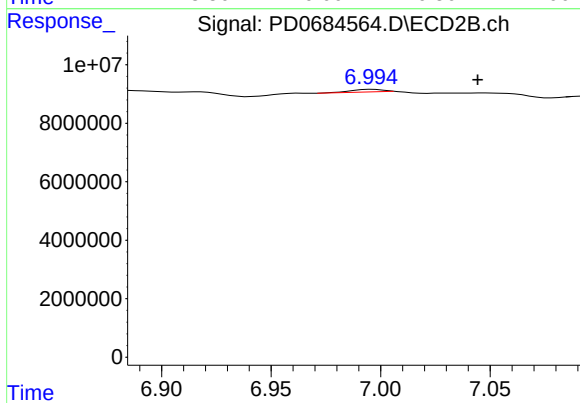

#16 4,4'-DDD


R.T.: 6.996 min
Delta R.T.: -0.048 min
Response: 969516
Conc: 0.12 ng/ml

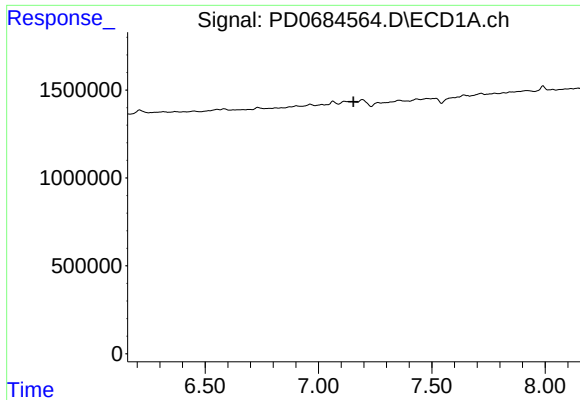

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

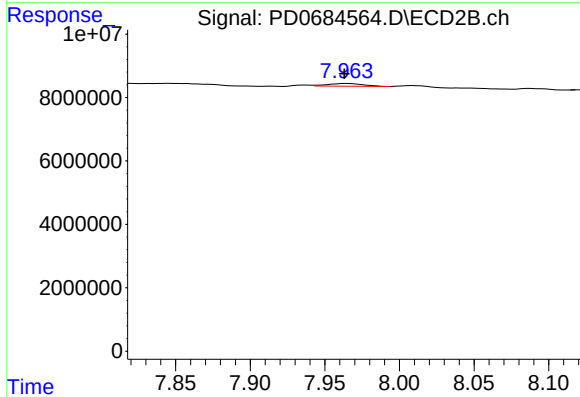


#21 Endrin ketone

R.T.: 7.965 min
Delta R.T.: 0.002 min
Response: 1384477
Conc: 0.16 ng/ml

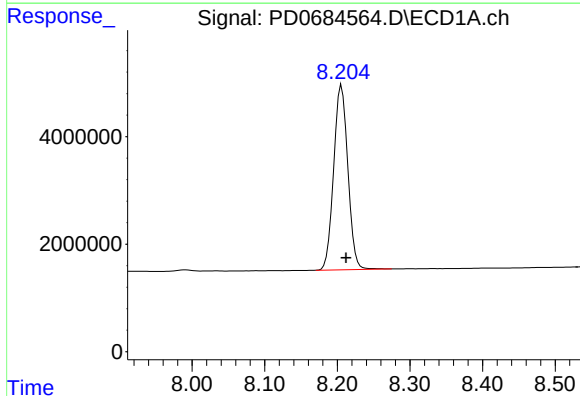

#27 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.006 min
Response: 46600655
Conc: 33.51 ng/ml

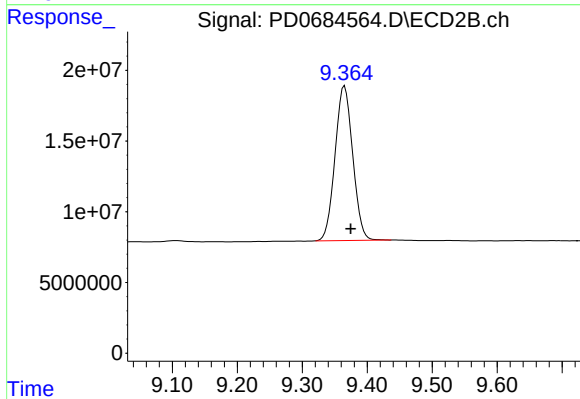

#27 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.010 min
Response: 206983591
Conc: 32.82 ng/ml