

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 20:00
 Operator : AR\AJ
 Sample : PIBLK242
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:20:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.173	27491460	210.0E6	20.188	19.185
27)	SA Decachlor...	8.206	9.366	55756927	244.1E6	40.097	38.699
Target Compounds							
8)	B Heptachlo...	0.000	6.073	0	3194193	N.D.	0.265
14)	MA Endrin	0.000	6.999f	0	700663	N.D.	<MDL
16)	A 4,4'-DDD	0.000	6.999f	0	700663	N.D.	<MDL
21)	B Endrin ke...	0.000	7.964	0	852047	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 20:00
Operator : AR\AJ
Sample : PIBLK242
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:20:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

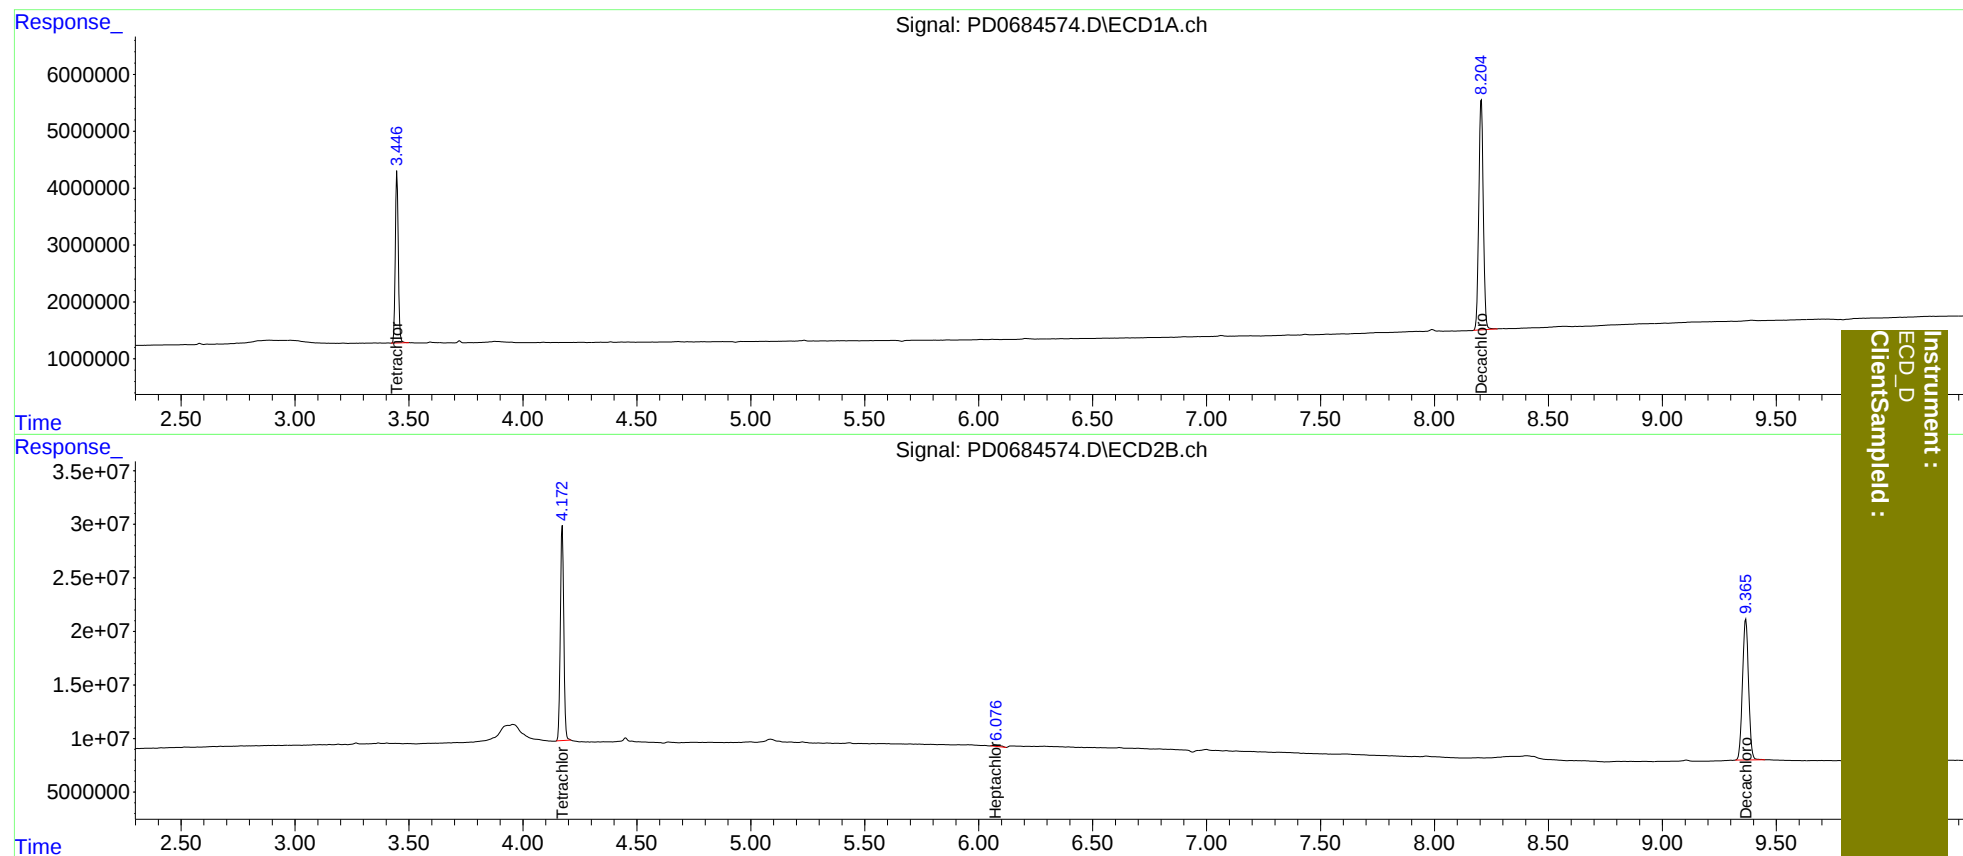


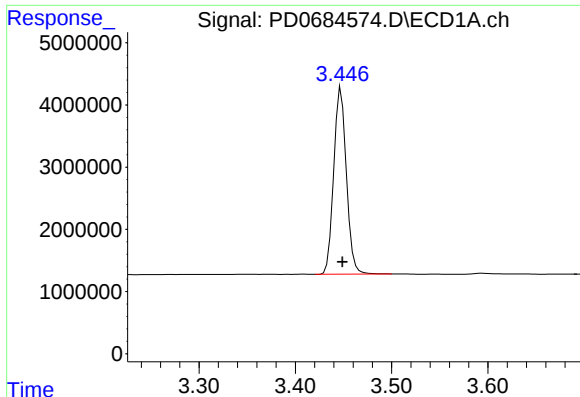

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: -0.001 min
Response: 27491460
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

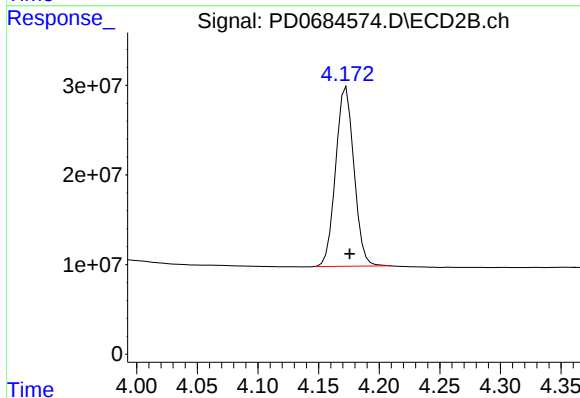


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 209993116
Conc: 19.19 ng/ml

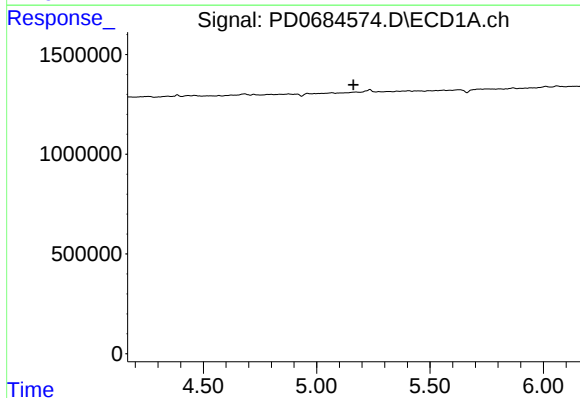


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

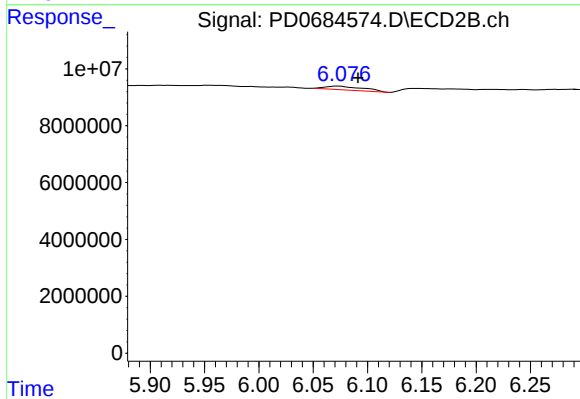

#8 Heptachlor epoxide


R.T.: 6.073 min
Delta R.T.: -0.018 min
Response: 3194193
Conc: 0.27 ng/ml

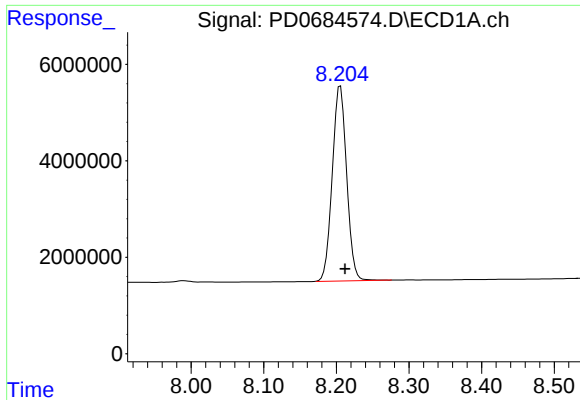

#27 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.006 min
Response: 55756927
Conc: 40.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

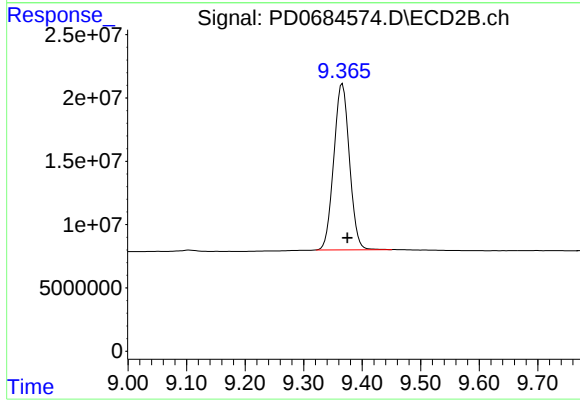

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 244081128
Conc: 38.70 ng/ml