

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 23:44
 Operator : AR\AJ
 Sample : PIBLK243
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:24:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	27214622	211.0E6	19.985	19.278
27)	SA Decachlor...	8.205	9.366	55920323	246.3E6	40.215	39.044
Target Compounds							
7)	B delta-BHC	0.000	5.228	0	1295318	N.D.	<MDL
8)	B Heptachlo...	0.000	6.073	0	9570565	N.D.	0.795
16)	A 4,4'-DDD	0.000	6.997f	0	708341	N.D.	<MDL
21)	B Endrin ke...	0.000	7.968	0	1347030	N.D.	0.158


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 23:44
Operator : AR\AJ
Sample : PIBLK243
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:24:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

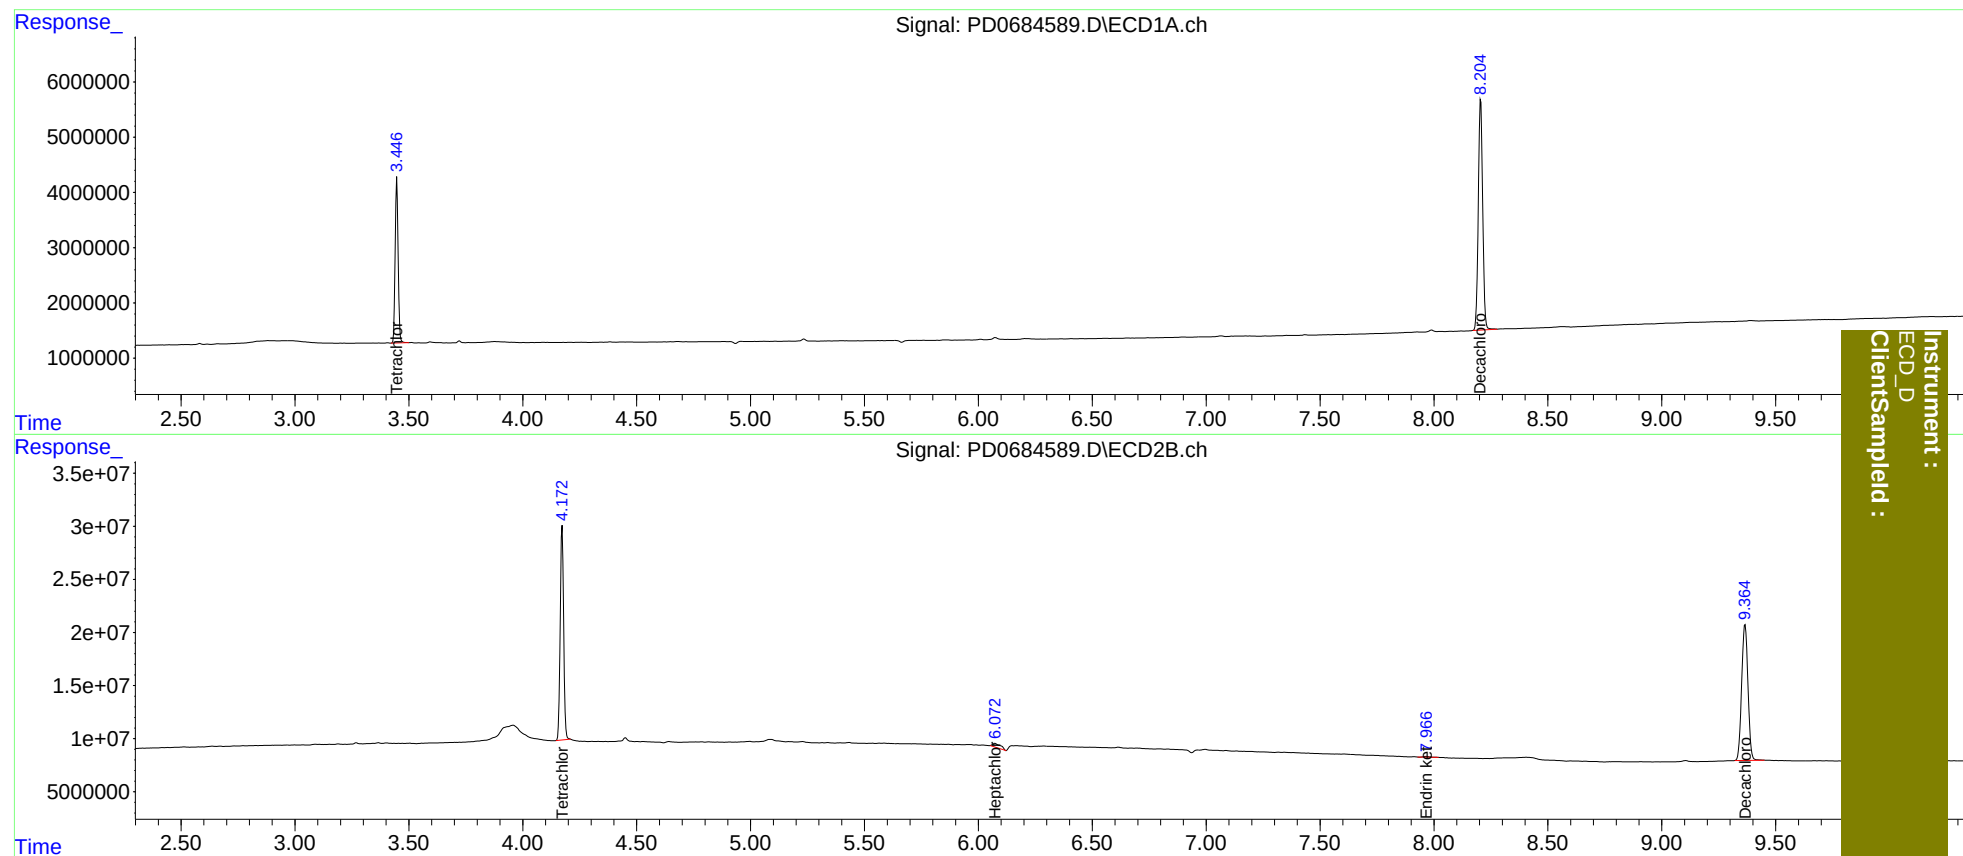


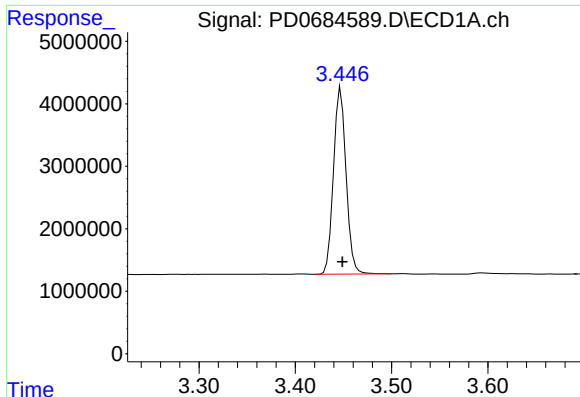

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: -0.002 min
Response: 27214622
Conc: 19.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

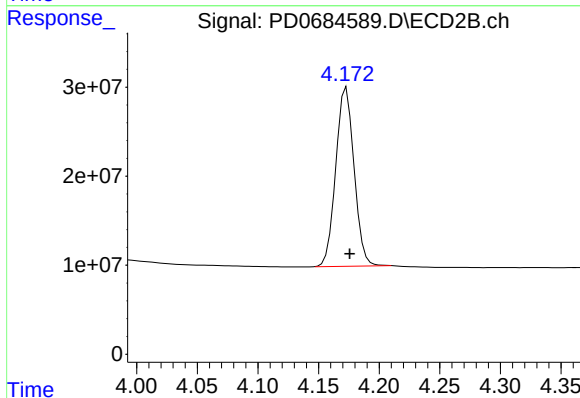


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 211004201
Conc: 19.28 ng/ml

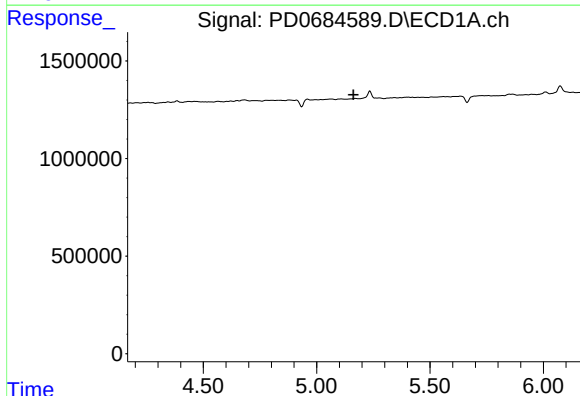


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

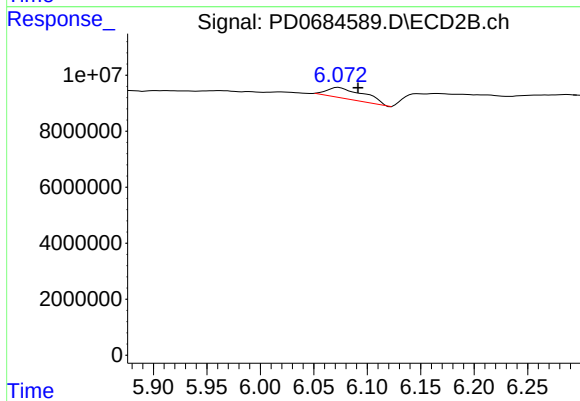

#8 Heptachlor epoxide


R.T.: 6.073 min
Delta R.T.: -0.018 min
Response: 9570565
Conc: 0.79 ng/ml

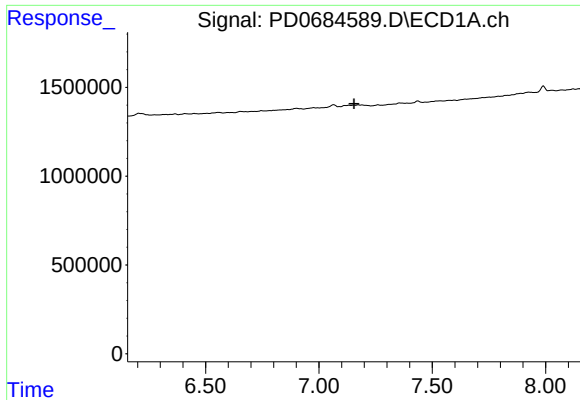

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

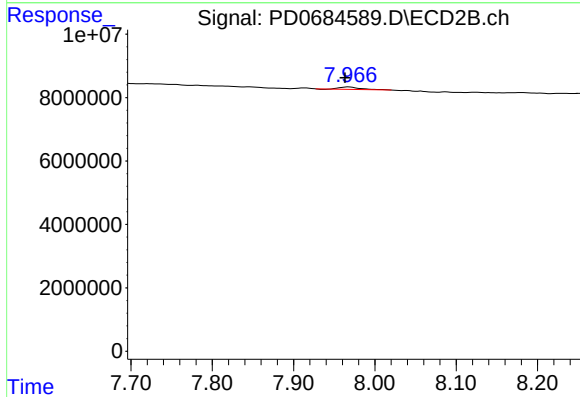


#21 Endrin ketone

R.T.: 7.968 min
Delta R.T.: 0.005 min
Response: 1347030
Conc: 0.16 ng/ml

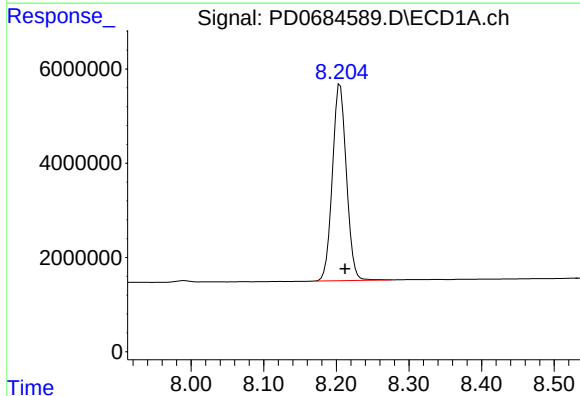

#27 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.007 min
Response: 55920323
Conc: 40.21 ng/ml

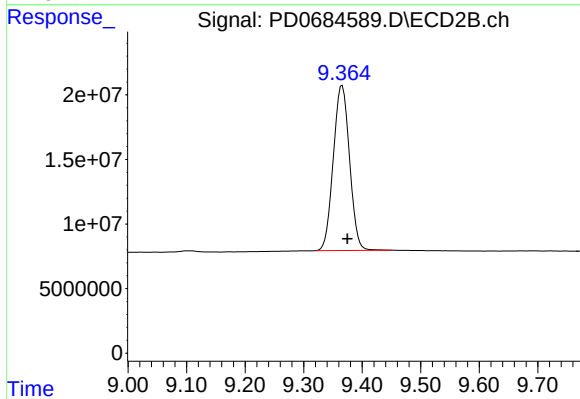

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 246254692
Conc: 39.04 ng/ml