

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD0684595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 01:36
 Operator : AR\AJ
 Sample : N1882-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:26:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	19465489	156.6E6	14.294	14.308
27)	SA Decachlor...	8.205	9.366	35765929	164.3E6	25.721	26.044
Target Compounds							
2)	A alpha-BHC	0.000	4.599f	0	658044	N.D.	<MDL
4)	MA Heptachlor	0.000	5.383	0	2321480	N.D.	0.169
6)	B beta-BHC	0.000	5.004	0	1630076	N.D.	0.255
7)	B delta-BHC	0.000	5.227	0	1543920	N.D.	0.109
8)	B Heptachlo...	0.000	6.071	0	2153096	N.D.	0.179
14)	MA Endrin	0.000	6.998f	0	574130	N.D.	<MDL
15)	B Endosulfa...	0.000	7.135	0	3551342	N.D.	0.397
16)	A 4,4'-DDD	0.000	6.998f	0	574130	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD0684595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 01:36
Operator : AR\AJ
Sample : N1882-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:26:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

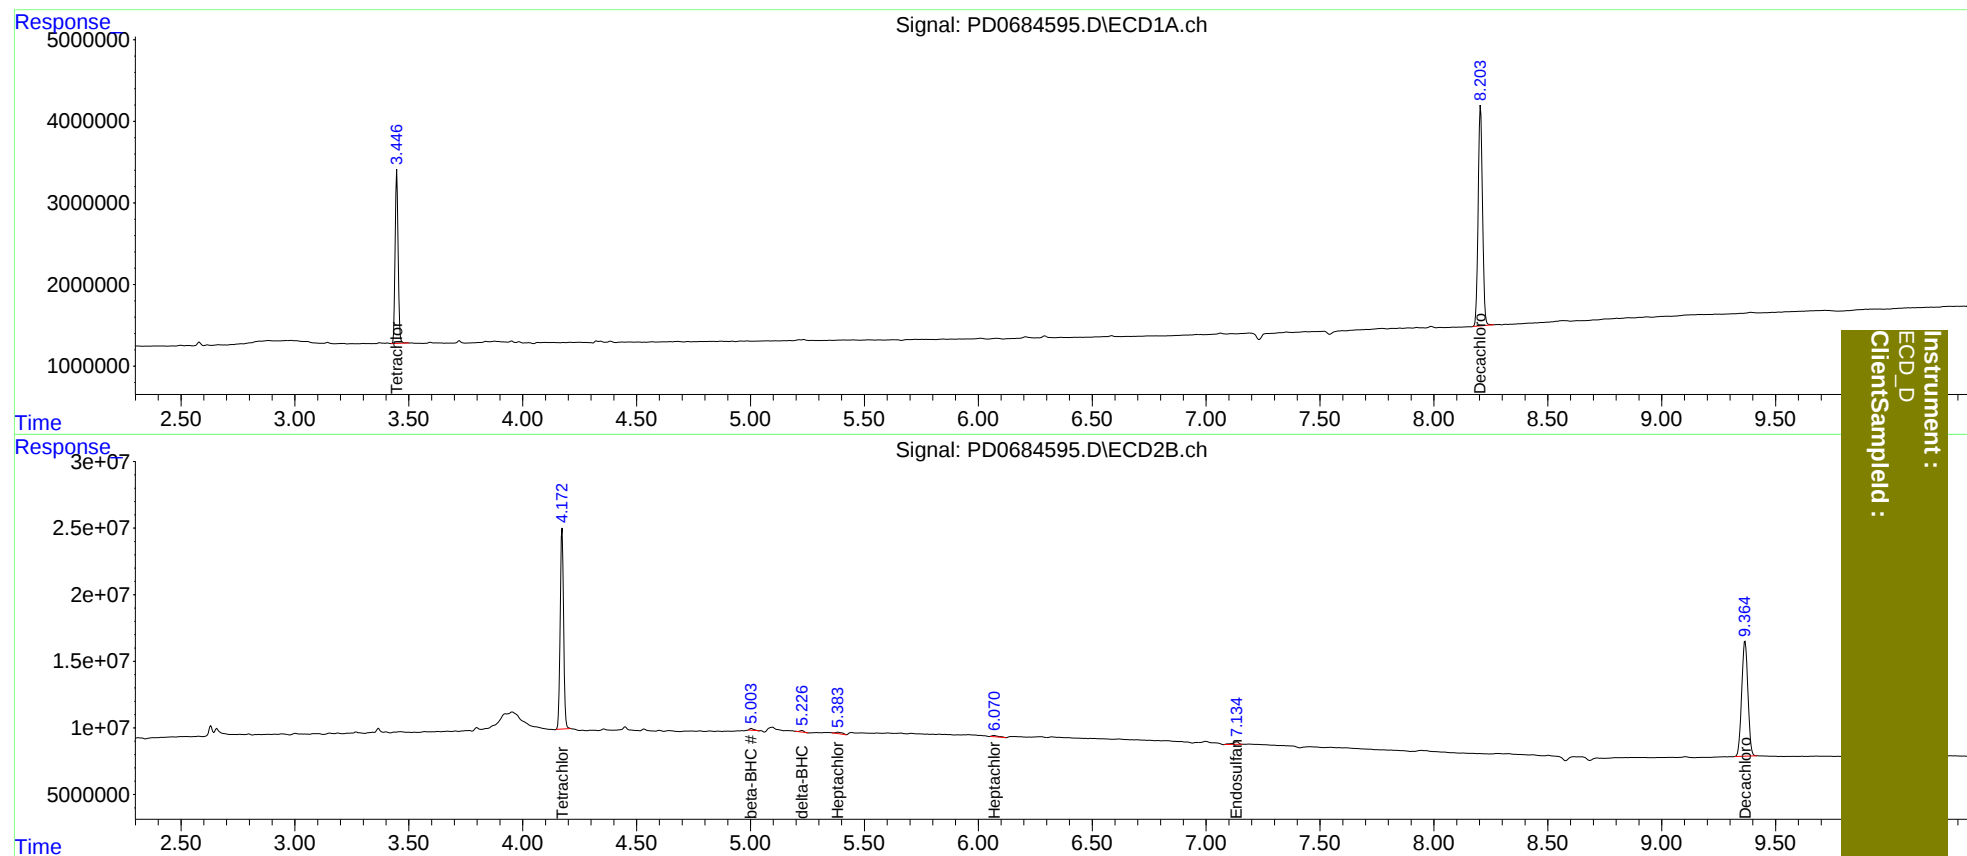


Instrument :
ECD_D
ClientSampled :
N1882-13

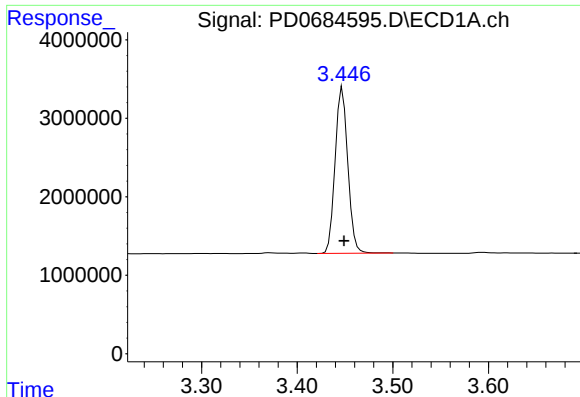

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: -0.002 min
Response: 19465489
Conc: 14.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

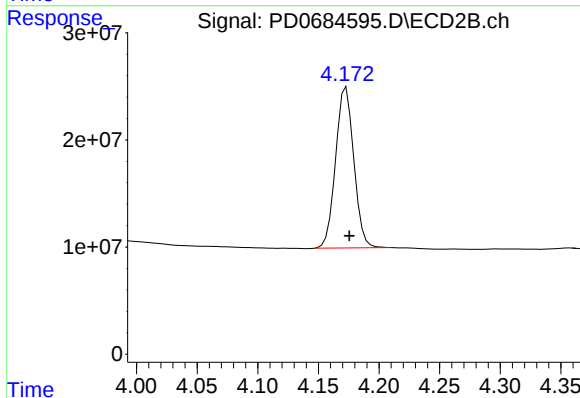


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 156605980
Conc: 14.31 ng/ml

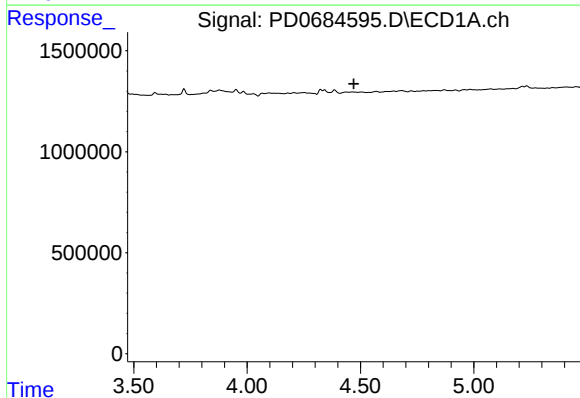


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.471 min
Response: 0
Conc: N.D.

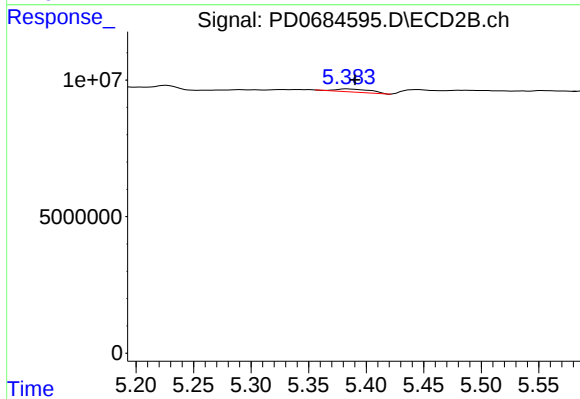

#4 Heptachlor


R.T.: 5.383 min
Delta R.T.: -0.007 min
Response: 2321480
Conc: 0.17 ng/ml

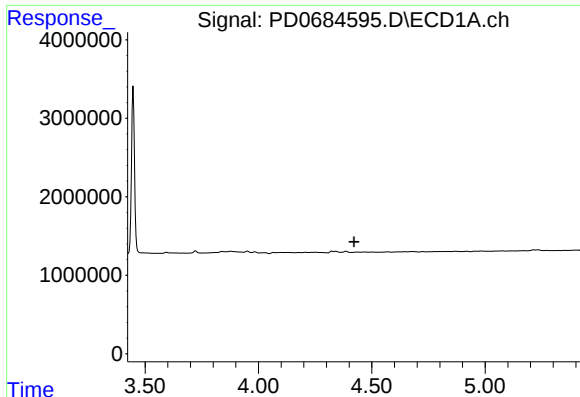

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

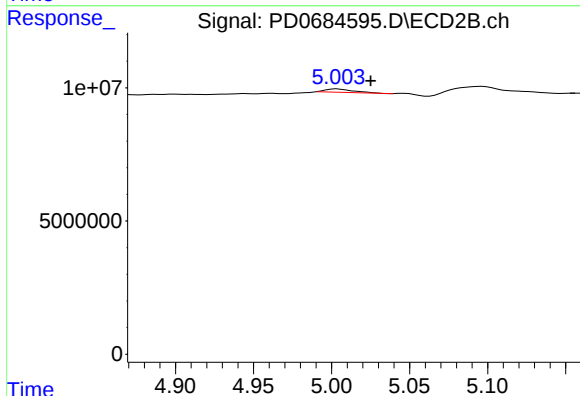


#6 beta-BHC

R.T.: 5.004 min
Delta R.T.: -0.021 min
Response: 1630076
Conc: 0.26 ng/ml

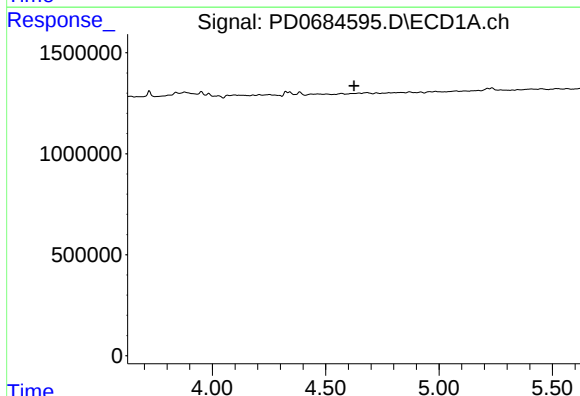


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

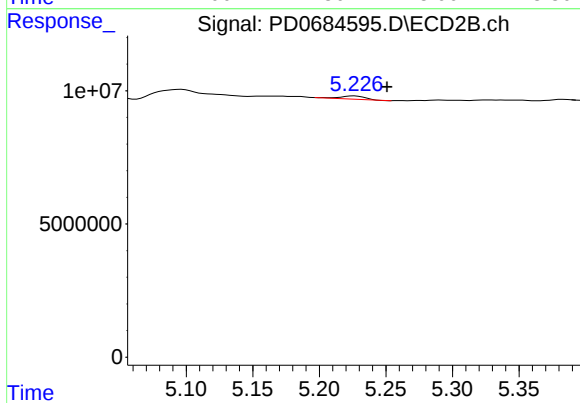

#7 delta-BHC


R.T.: 5.227 min
Delta R.T.: -0.024 min
Response: 1543920
Conc: 0.11 ng/ml

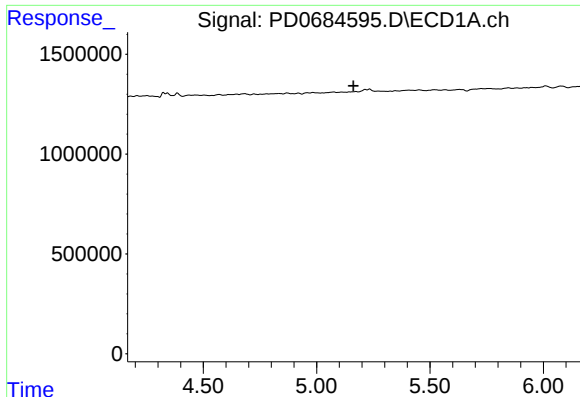

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

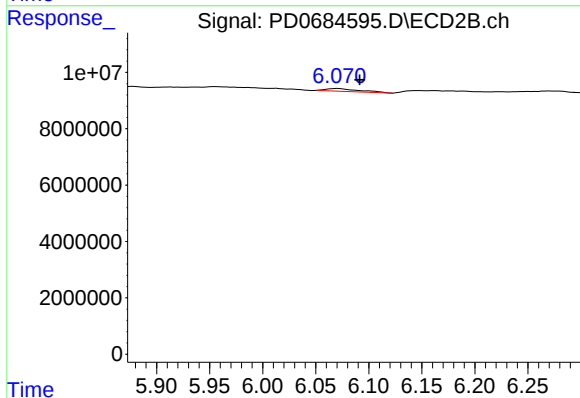


#8 Heptachlor epoxide

R.T.: 6.071 min
Delta R.T.: -0.020 min
Response: 2153096
Conc: 0.18 ng/ml

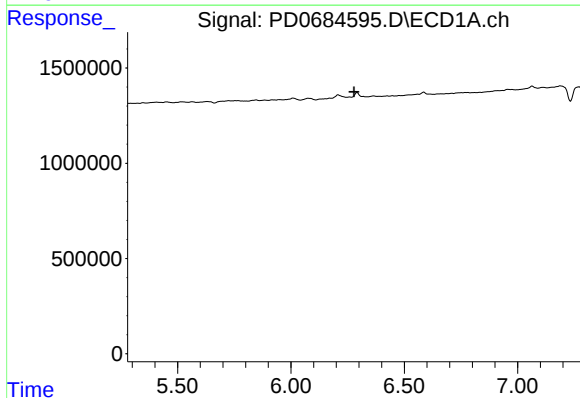


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

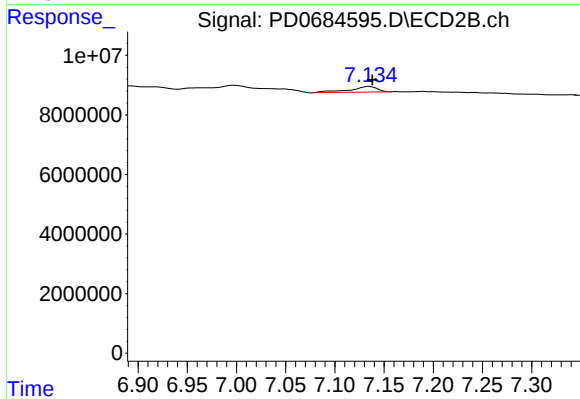

#15 Endosulfan II


R.T.: 7.135 min
Delta R.T.: -0.003 min
Response: 3551342
Conc: 0.40 ng/ml

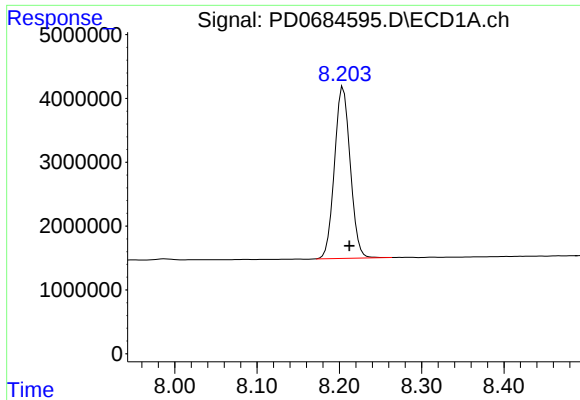

#27 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.007 min
Response: 35765929
Conc: 25.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

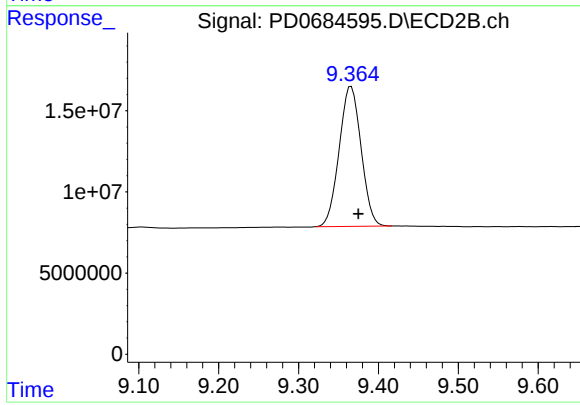

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 164262928
Conc: 26.04 ng/ml