

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031422\  
 Data File : PD068543.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Mar 2022 12:23  
 Operator : AR\AJ  
 Sample : N1818-23  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 DBSJ9

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022  
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 15 07:13:57 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031322CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Mar 14 07:24:04 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|----------|
| -----                       |                 |       |       |          |         |         |          |
| System Monitoring Compounds |                 |       |       |          |         |         |          |
| 1)                          | SA Tetrachlo... | 3.448 | 4.173 | 19767392 | 154.3E6 | 14.516  | 14.098   |
| 27)                         | SA Decachlor... | 8.206 | 9.365 | 40777693 | 185.7E6 | 29.325  | 29.444   |
| Target Compounds            |                 |       |       |          |         |         |          |
| 4)                          | MA Heptachlor   | 4.469 | 5.386 | 48078017 | 347.3E6 | 26.839  | 25.232   |
| 6)                          | B beta-BHC      | 4.420 | 5.022 | 42144975 | 296.5E6 | 50.575  | 46.429   |
| 9)                          | A Endosulfan I  | 5.500 | 6.450 | 79692606 | 482.2E6 | 51.762  | 44.303   |
| 10)                         | B trans-Chl...  | 5.387 | 6.322 | 81918674 | 509.6E6 | 49.085  | 42.849m  |
| 11)                         | B cis-Chlor...  | 5.446 | 6.398 | 56981197 | 363.5E6 | 34.711  | 31.689   |
| 12)                         | B 4,4'-DDE      | 5.612 | 6.548 | 14039931 | 100.8E6 | 9.439   | 9.863    |
| 13)                         | MA Dieldrin     | 5.743 | 6.707 | 158.2E6  | 929.5E6 | 94.703  | 83.654   |
| 14)                         | MA Endrin       | 6.002 | 6.927 | 178.6E6  | 727.8E6 | 126.351 | 86.077m# |
| 15)                         | B Endosulfa...  | 6.275 | 7.133 | 133.9E6  | 743.0E6 | 92.298  | 83.032   |
| 16)                         | A 4,4'-DDD      | 6.129 | 7.039 | 53916586 | 334.3E6 | 41.019  | 39.840   |
| 17)                         | MA 4,4'-DDT     | 6.369 | 7.339 | 63719646 | 469.1E6 | 47.716  | 59.519m  |
| 18)                         | B Endrin al...  | 6.444 | 7.257 | 29171758 | 175.9E6 | 26.602  | 26.493   |
| 21)                         | B Endrin ke...  | 7.150 | 7.956 | 78809128 | 403.6E6 | 49.392  | 47.269   |
| -----                       |                 |       |       |          |         |         |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031422\  
Data File : PD068543.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Mar 2022 12:23  
Operator : AR\AJ  
Sample : N1818-23  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 15 07:13:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031322CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Mar 14 07:24:04 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

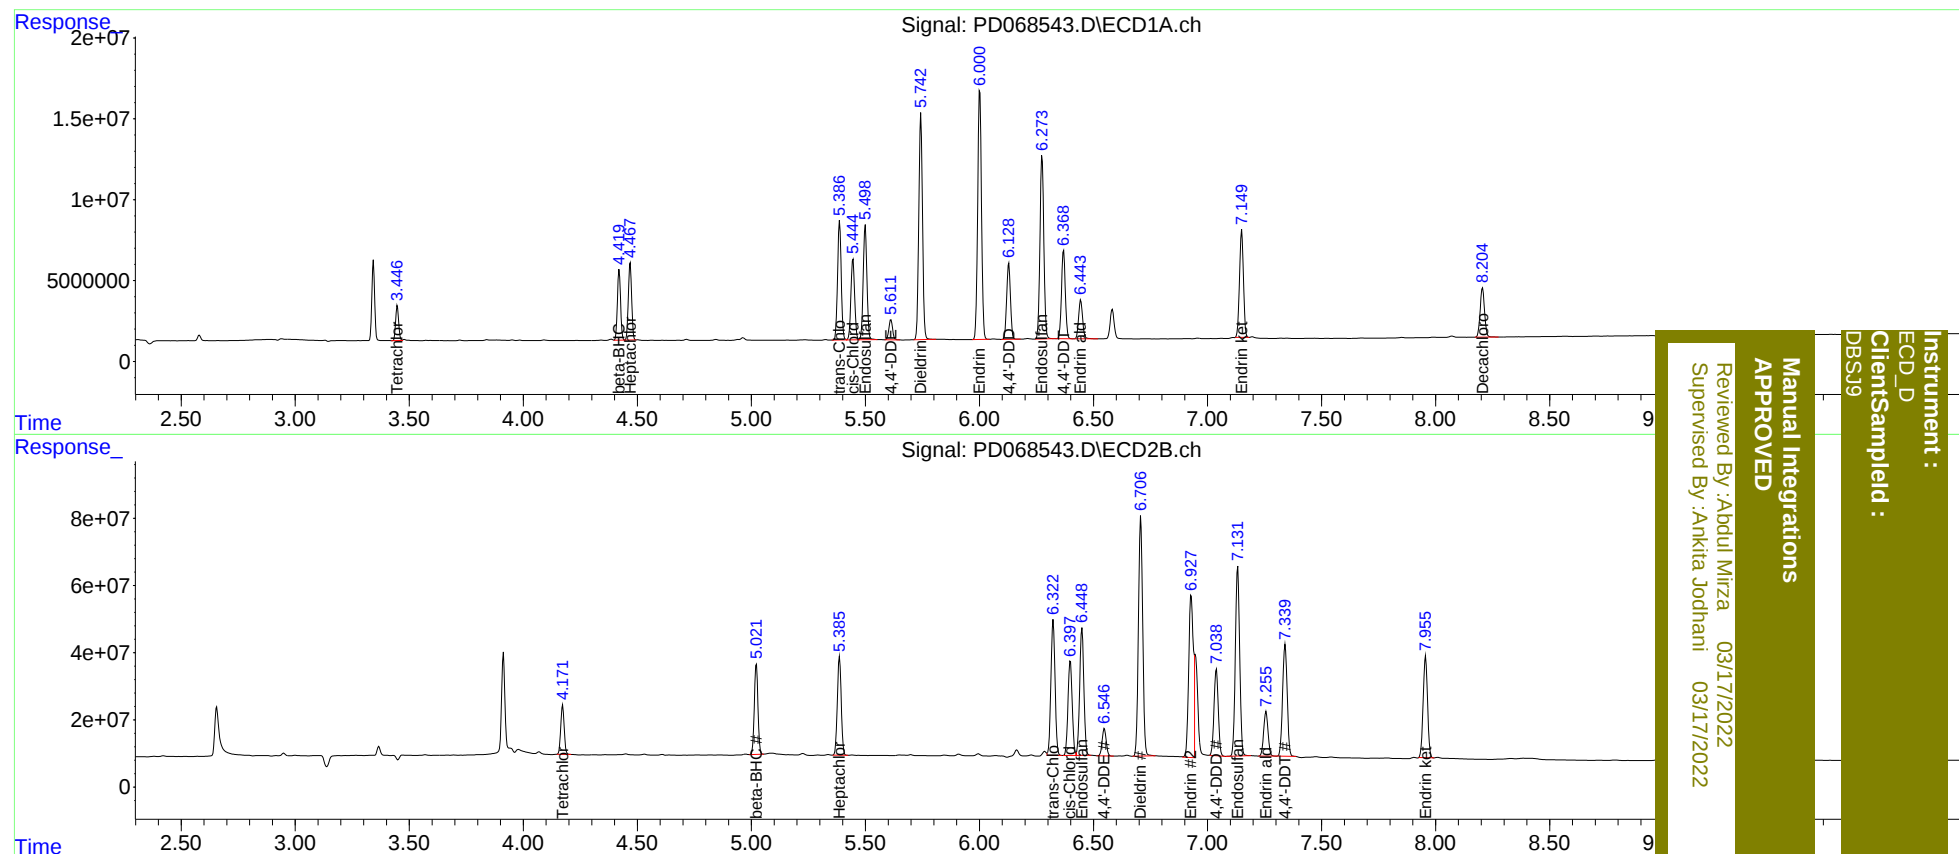

Reviewed By: Abdul Mirza 03/17/2022  
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
ClientSampled :  
DBSJ9