

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
 Data File : PD068550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 14:04
 Operator : AR\AJ
 Sample : N1818-09MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBSF4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:15:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	4.173	23780613	191.0E6	17.463	17.448
27)	SA Decachlor...	8.210	9.367	55884386	247.6E6	40.189	39.256
Target Compounds							
2)	A alpha-BHC	3.891	4.569	89349069	636.8E6	46.675	40.725
3)	MA gamma-BHC...	4.175	4.858	83624301	589.3E6	46.068	40.643m
4)	MA Heptachlor	4.473	5.386	79225931	548.2E6	44.227	39.827
5)	MB Aldrin	4.721	5.699	77576218	546.1E6	44.109	40.470
6)	B beta-BHC	4.425	5.022	36694174	274.7E6	44.034	43.004
7)	B delta-BHC	4.629	5.248	81177471	571.9E6	45.910	40.397
8)	B Heptachlo...	5.165	6.088	74090515	488.2E6	45.622	40.529
9)	A Endosulfan I	5.504	6.450	69057145	437.1E6	44.854	40.167
10)	B trans-Chl...	5.391	6.323	75928067	476.9E6	45.496	40.096
11)	B cis-Chlor...	5.450	6.399	73906727	463.2E6	45.022	40.385
12)	B 4,4'-DDE	5.616	6.549	147.2E6	879.8E6	98.964	86.121
13)	MA Dieldrin	5.747	6.708	158.4E6	934.6E6	94.804	84.114
14)	MA Endrin	6.005	6.929	133.2E6	716.0E6	94.234	84.689
15)	B Endosulfa...	6.279	7.133	134.0E6	743.2E6	92.395	83.051
16)	A 4,4'-DDD	6.133	7.040	120.1E6	686.0E6	91.404	81.767
17)	MA 4,4'-DDT	6.374	7.342	129.2E6	703.4E6	96.787	89.249
18)	B Endrin al...	6.449	7.258	100.0E6	555.5E6	91.218	83.658
19)	B Endosulfa...	6.661	7.482	126.4E6	666.3E6	90.468	81.348
20)	A Methoxychlor	6.924	7.795	332.0E6	1515.4E6	469.028	432.597
21)	B Endrin ke...	7.154	7.957	156.4E6	742.9E6	98.038	87.010

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031422\
Data File : PD068550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 14:04
Operator : AR\AJ
Sample : N1818-09MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:15:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

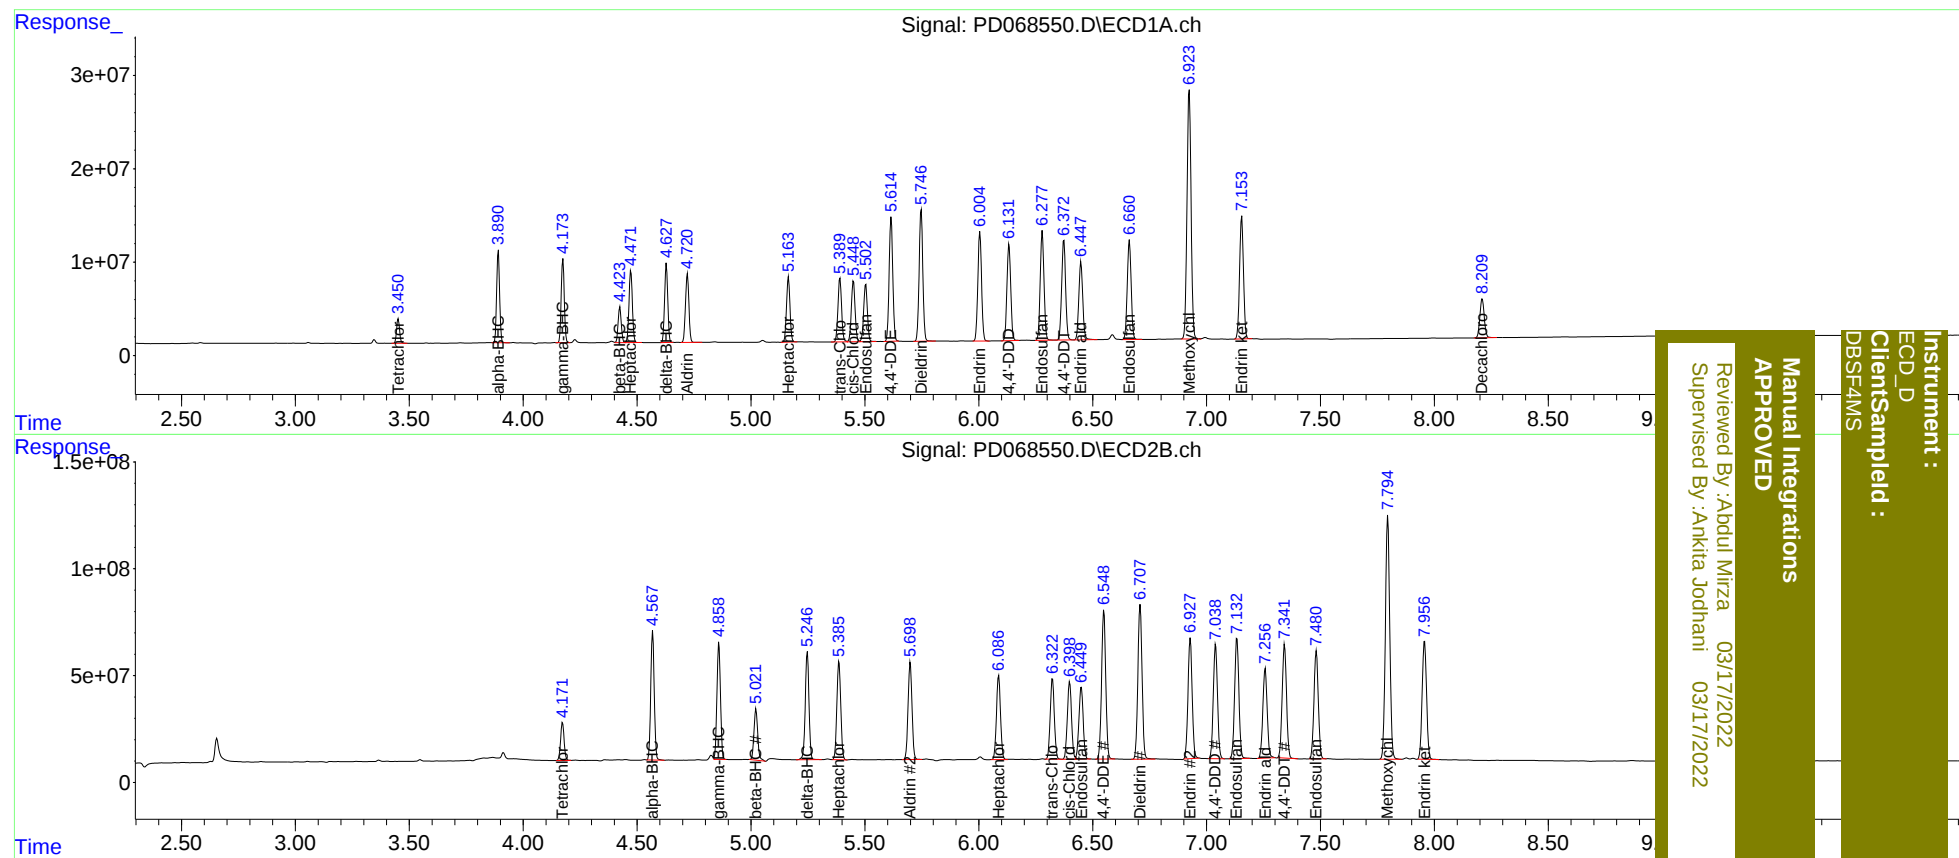

Reviewed By: Abdul Miza 03/17/2022
Supervised By: Ankita Jodhani 03/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBSF4MS